


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040722\
 Data File : VL038833.D
 Acq On : 7 Apr 2022 9:01
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL040522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Apr 06 06:12:53 2022
 Last Update : Wed Apr 06 06:12:53 2022

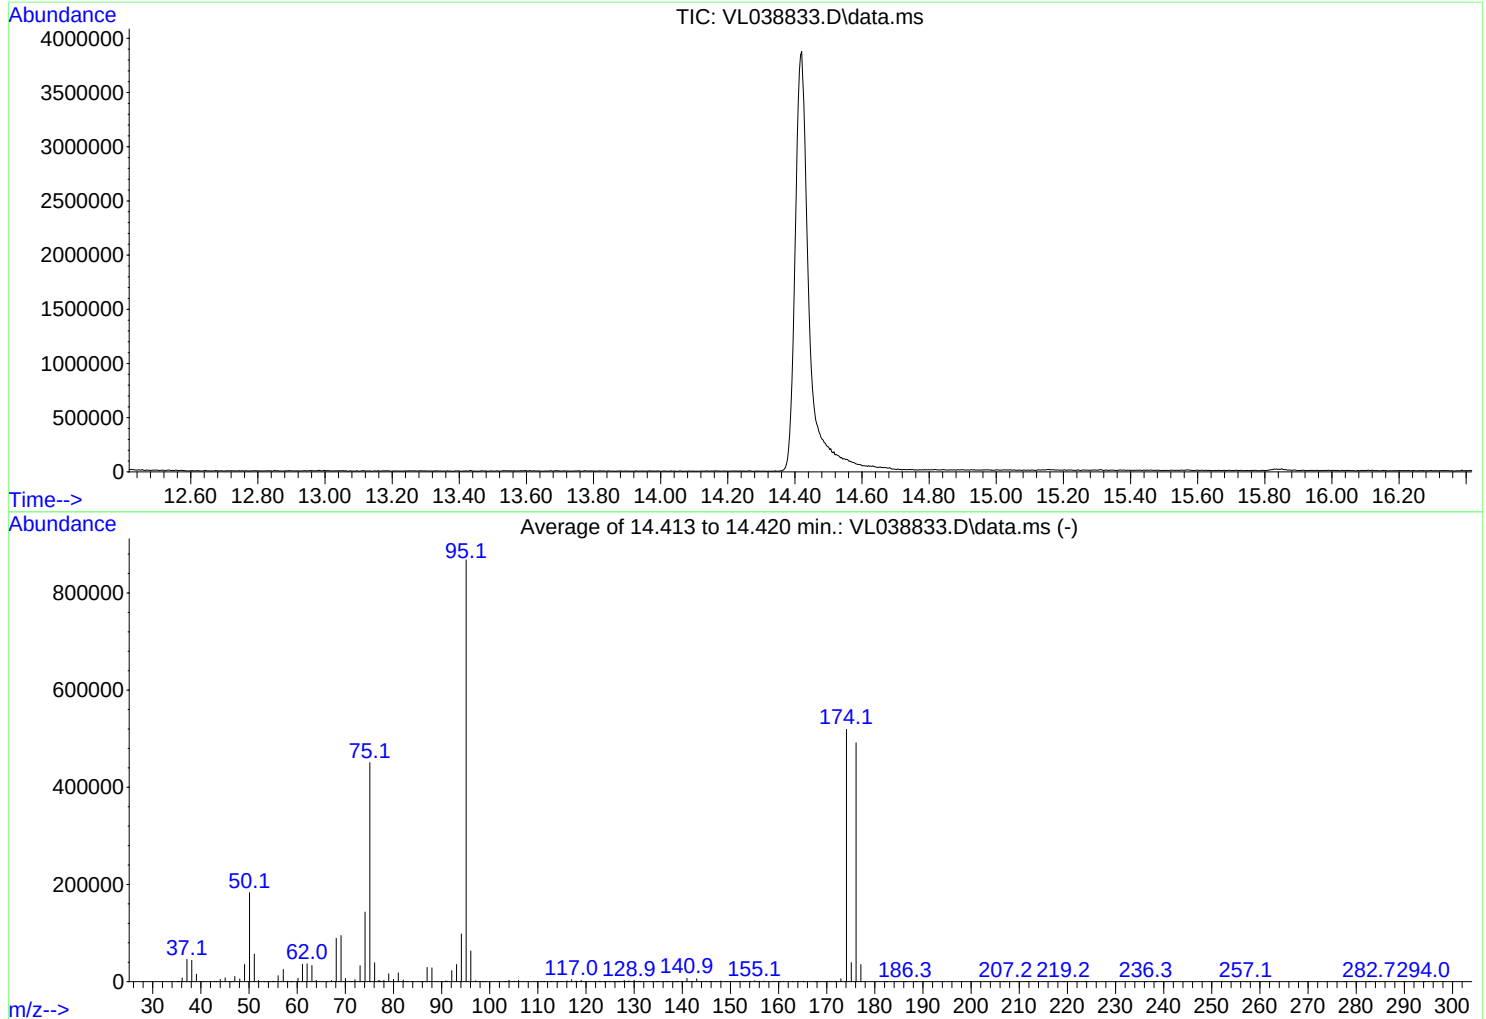

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.1	183125	PASS
75	95	30	66	51.9	450688	PASS
95	95	100	100	100.0	868139	PASS
96	95	5	9	7.3	63369	PASS
173	174	0.00	2	1.1	5825	PASS
174	95	50	120	59.8	519445	PASS
175	174	4	9	7.5	39085	PASS
176	174	93	101	94.7	491797	PASS
177	176	5	9	7.2	35192	PASS

Average of 14.413 to 14.420 min.: VL038833.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	96	46.00	449	54.90	723	65.15	50
36.10	7510	46.30	123	55.15	1116	66.10	9
37.10	45712	47.05	10713	56.05	12208	67.10	235
38.10	43987	48.05	5667	57.10	25189	68.10	8917
39.05	15623	49.05	35269	58.05	977	69.10	94752
39.95	728	50.10	183125	58.75	130	70.05	6594
40.40	243	51.10	56685	60.15	6822	70.95	298
42.85	264	52.00	2244	61.10	35909	71.20	132
43.10	123	53.10	151	62.05	36445	72.00	4214
44.00	4763	53.90	57	63.05	33331	73.05	32525
45.05	8063	54.15	203	63.95	2601	74.10	143339

Average of 14.413 to 14.420 min.: VL038833.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	450688	82.70	347	93.10	35405	105.10	923
76.10	38845	82.95	443	94.10	98171	106.00	2692
76.95	2392	85.70	259	95.10	868139	106.95	597
77.10	1640	85.90	291	96.05	63369	109.80	222
77.30	877	86.20	194	97.10	1998	110.00	246
77.80	1106	87.00	29445	98.50	50	110.80	801
78.00	2566	88.00	28464	99.10	142	111.20	155
79.00	16288	90.20	195	102.75	308	111.90	205
80.00	4546	90.90	1697	103.10	97	112.80	516
81.00	18301	91.20	788	104.00	3100	113.10	222
82.05	3486	92.10	22904	104.80	518	114.10	87

Average of 14.413 to 14.420 min.: VL038833.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.90	309	123.15	390	130.90	651	139.80	588
115.10	438	123.75	185	131.20	136	140.95	6850
115.90	1009	124.00	171	133.80	234	141.90	392
116.10	1262	124.80	87	134.50	158	142.10	352
117.00	3842	125.70	140	134.80	258	143.00	6079
117.90	1493	126.40	170	135.10	730	143.80	382
118.10	706	126.90	95	136.10	467	144.00	244
119.00	2807	127.95	2537	136.70	309	145.05	733
120.10	219	128.80	483	137.00	869	145.75	597
121.75	176	128.95	1574	138.80	154	146.15	495
122.80	58	130.00	2940	139.10	440	147.05	562

Average of 14.413 to 14.420 min.: VL038833.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.00	1429	157.00	1404	169.90	271	178.05	671
149.10	544	158.85	662	170.15	529	182.40	56
149.30	217	160.30	115	170.60	417	186.30	58
149.95	584	161.05	751	171.05	759	188.40	52
151.80	247	162.90	170	171.50	419	206.60	58
152.10	234	164.20	351	171.70	645	207.20	65
152.80	201	165.10	79	172.95	5825	219.20	68
153.10	626	167.70	63	174.10	519445	223.70	64
154.10	875	168.60	336	175.10	39085	236.30	73
155.05	1940	169.15	378	176.10	491797	238.30	51
155.95	514	169.65	320	177.10	35192	257.10	84

Average of 14.413 to 14.420 min.: VL038833.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
277.45	128						
282.70	139						
294.00	52						