
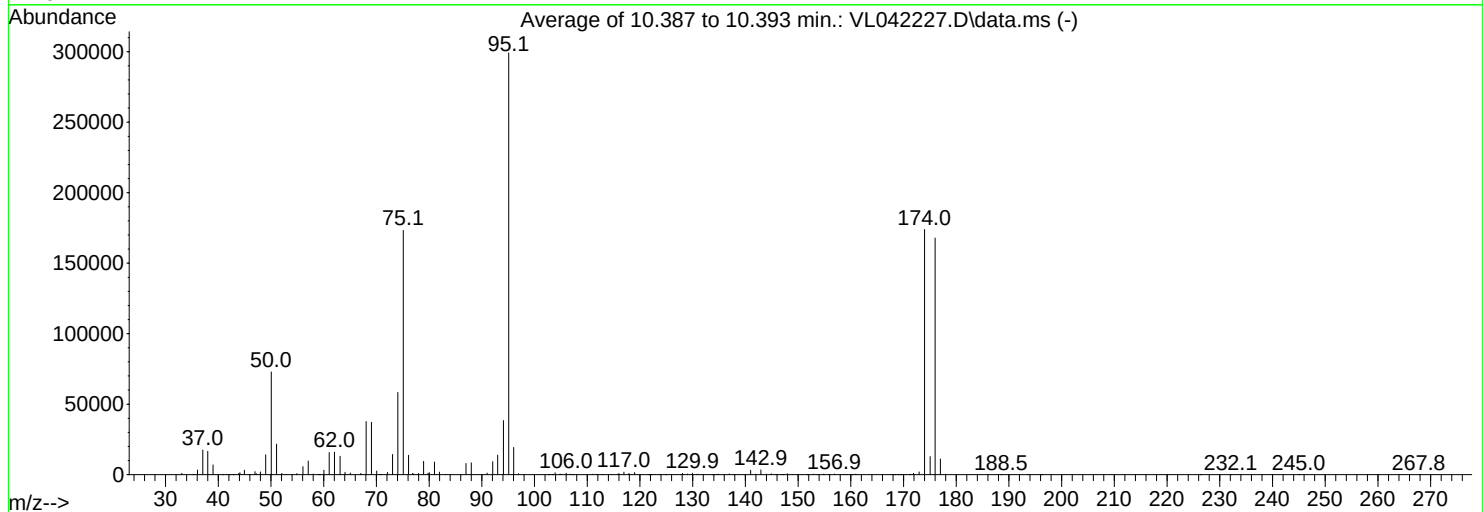


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040725\
Data File : VL042227.D
Acq On : 07 Apr 2025 08:46
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

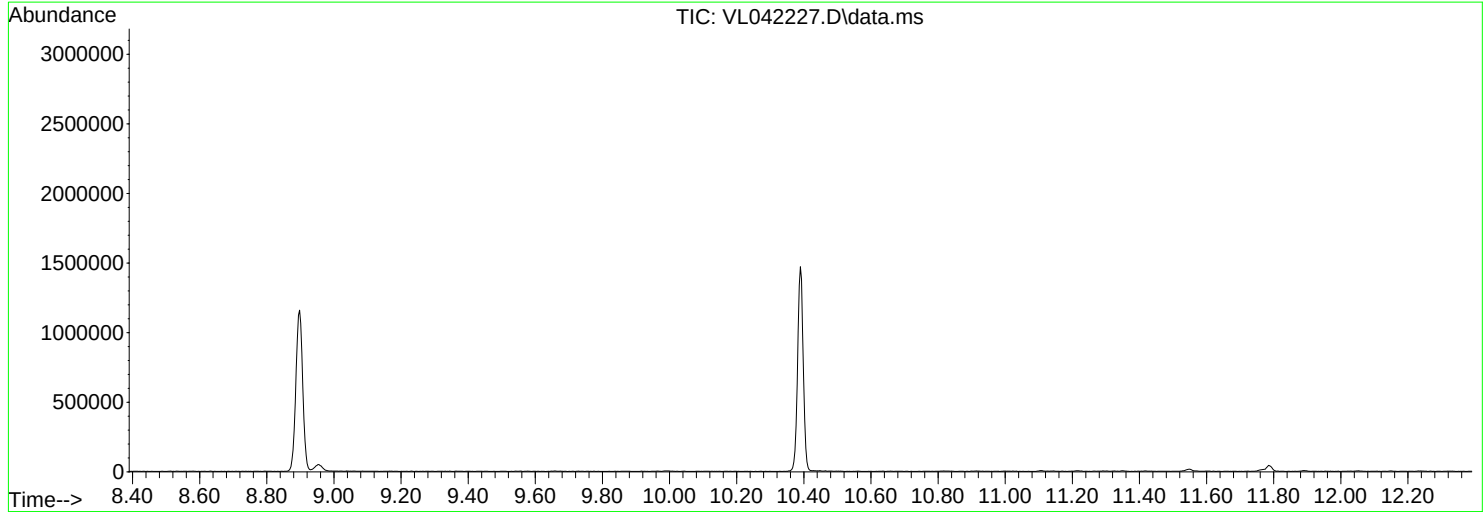

AutoFind: Scans 3182, 3183, 3184; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	72901	PASS
75	95	30	66	57.9	173376	PASS
95	95	100	100	100.0	299221	PASS
96	95	5	9	6.4	19264	PASS
173	174	0.00	2	1.1	1915	PASS
174	95	50	120	58.1	173867	PASS
175	174	4	9	7.4	12863	PASS
176	174	93	101	96.5	167851	PASS
177	176	5	9	6.6	11132	PASS

Average of 10.387 to 10.393 min.: VL042227.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	965	43.05	112	51.05	21688	62.05	16071
35.20	41	43.90	959	52.05	943	63.10	1305
36.05	3249	44.10	1347	52.90	152	64.05	167
37.05	17465	44.95	3167	54.90	818	65.05	113
38.00	16570	45.80	46	56.05	5729	65.95	77
39.00	6896	46.10	148	57.05	9702	67.05	943
39.90	152	46.95	2161	58.00	446	68.05	37715
40.85	43	47.20	647	59.00	93	69.05	37165
41.70	79	48.00	1984	59.20	29	70.05	2638
42.10	18	49.00	14071	60.05	3193	70.70	65
42.80	56	50.05	72901	61.05	15725	70.95	142

Average of 10.387 to 10.393 min.: VL042227.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
72.10	1599	81.00	9008	96.05	19264	110.00	155
73.05	14308	81.95	1879	96.95	735	111.05	377
74.05	58405	83.10	252	102.70	44	111.75	246
75.10	173376	86.05	180	102.95	89	112.10	209
76.10	13734	87.00	7976	103.40	40	112.80	74
76.90	932	88.00	8390	103.90	1363	113.05	159
77.10	516	91.00	1190	104.85	452	114.75	174
77.95	962	92.05	9244	105.10	163	115.80	297
78.95	9378	93.00	13914	106.00	1042	116.00	828
79.80	1120	94.10	38397	106.75	293	116.95	1830
80.05	1367	95.10	299221	107.20	60	117.80	436

Average of 10.387 to 10.393 min.: VL042227.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.95	676	127.70	161	136.95	598	146.75	125
119.00	1521	128.05	936	137.80	47	147.10	35
121.70	21	129.00	465	138.70	73	147.95	663
121.95	151	129.95	1048	140.00	204	149.05	144
122.20	33	130.70	172	141.00	3029	149.90	255
122.95	159	131.00	360	141.90	297	151.70	38
123.70	92	133.70	18	142.95	3397	152.00	196
123.85	131	134.05	37	143.95	292	152.85	326
124.85	49	134.60	172	144.90	544	153.60	89
126.00	163	134.85	305	145.80	286	153.90	138
127.00	71	135.90	56	146.00	135	154.80	340

Average of 10.387 to 10.393 min.: VL042227.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.00	152	167.80	104	175.05	12863		
155.80	170	168.00	18	176.00	167851		
156.90	434	168.40	18	177.00	11132		
158.10	103	169.00	22	178.00	383		
158.75	251	169.50	45	188.50	38		
159.10	149	169.65	89	193.50	22		
159.30	73	170.60	82	196.20	26		
159.80	19	171.20	57	226.30	26		
160.20	62	171.90	867	232.10	53		
160.80	324	172.95	1915	245.00	28		
161.00	251	174.00	173867	267.80	45		