
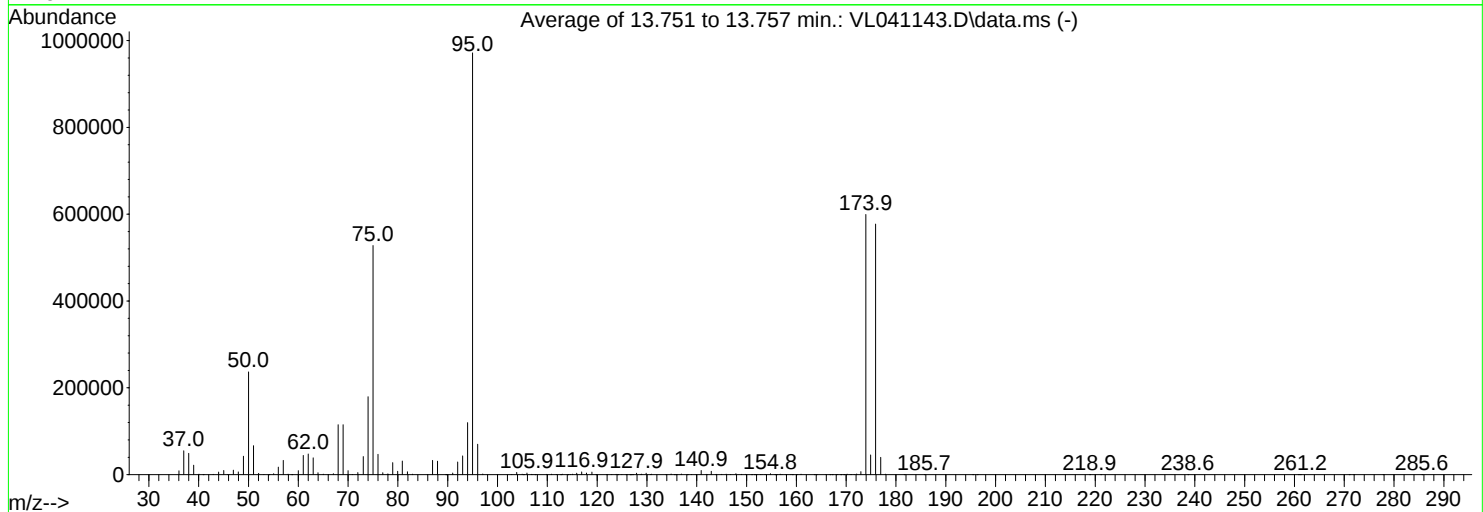


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040824\
Data File : VL041143.D
Acq On : 8 Apr 2024 9:48
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL040424AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Apr 09 01:10:08 2024

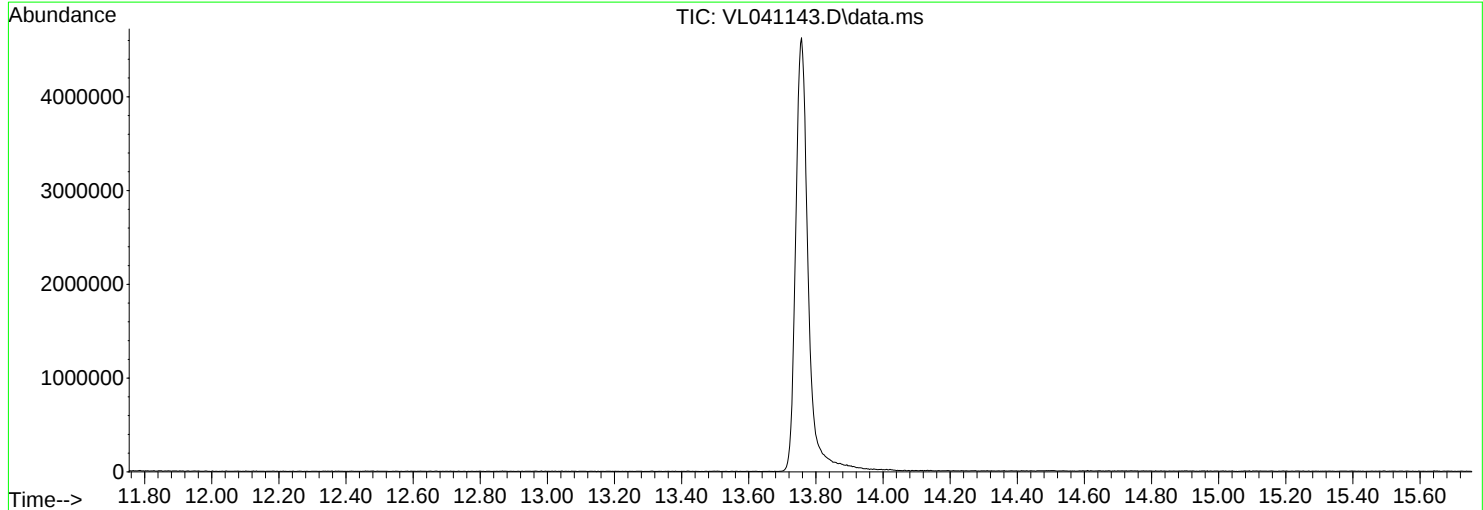

AutoFind: Scans 3467, 3468, 3469; Background Corrected with Scan 3438

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.4	236672	PASS
75	95	30	66	54.3	527723	PASS
95	95	100	100	100.0	971776	PASS
96	95	5	9	7.2	69976	PASS
173	174	0.00	2	1.2	6919	PASS
174	95	50	120	61.7	599339	PASS
175	174	4	9	7.6	45411	PASS
176	174	93	101	96.3	577152	PASS
177	176	5	9	6.9	39907	PASS

Average of 13.751 to 13.757 min.: VL041143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8877	46.95	10213	57.95	1149	69.00	11507
37.00	54787	47.95	6124	58.70	56	70.00	925
38.00	48928	49.00	42363	60.00	9222	70.85	31
39.00	21759	50.00	236672	61.00	44317	71.95	477
40.05	1180	51.00	66584	62.00	47403	73.05	41667
40.90	98	52.05	2798	63.00	38712	74.00	179605
42.90	790	53.10	344	63.95	4508	75.00	527723
44.00	6001	54.10	130	65.00	978	76.00	47000
45.05	9526	55.05	2192	66.05	317	76.95	4547
45.85	456	56.00	17407	67.05	2244	77.90	1678
46.10	372	57.00	32800	68.00	114888	78.10	996

Average of 13.751 to 13.757 min.: VL041143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	27832	92.00	29173	106.80	825	115.90	3253
79.95	7959	93.00	43131	107.10	224	116.90	6229
80.90	31520	94.00	119781	107.50	106	117.85	3719
81.90	6723	95.00	971776	109.90	766	118.95	6024
82.95	973	96.00	69976	110.85	997	119.75	129
85.95	476	97.05	1544	111.80	454	121.90	157
86.95	32744	102.85	417	112.70	138	122.95	471
87.95	31112	103.85	5155	113.00	1049	123.80	636
89.60	142	104.95	1007	114.10	123	124.10	120
89.80	89	105.20	209	114.60	244	124.95	234
91.00	3854	105.90	3846	115.05	1029	125.80	144

Average of 13.751 to 13.757 min.: VL041143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.00	262	134.85	1471	142.90	7956	151.90	216
126.60	109	135.50	143	143.80	123	152.80	455
126.80	57	135.80	193	143.95	714	153.10	517
127.10	118	136.05	375	145.00	850	153.70	280
127.90	3243	136.90	1661	145.90	1308	153.90	287
128.80	668	138.10	60	146.80	527	154.80	2358
128.95	1109	138.95	318	147.85	2196	155.70	75
129.85	3188	139.85	397	149.00	680	156.00	66
130.70	236	140.90	9646	149.85	956	156.75	1041
130.90	993	141.90	728	151.00	144	157.10	342
133.80	211	142.10	519	151.60	83	157.90	163

Average of 13.751 to 13.757 min.: VL041143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.90	855	168.90	58	175.90	577152	261.20	122
159.20	208	169.10	227	176.95	39907	271.00	52
160.00	198	169.50	77	177.85	1000	271.90	56
160.95	1095	170.20	987	181.65	197	277.80	54
163.60	55	170.80	464	185.70	60	285.60	71
164.00	61	171.10	247	195.40	56		
165.95	240	171.60	283	196.30	52		
166.75	150	172.10	1492	218.90	56		
167.20	162	172.95	6919	221.10	56		
167.95	166	173.95	599339	238.60	58		
168.30	337	174.90	45411	260.80	59		