


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041222\
 Data File : VL038888.D
 Acq On : 12 Apr 2022 11:38
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL040522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Apr 06 06:12:53 2022
 Last Update : Wed Apr 06 06:12:53 2022

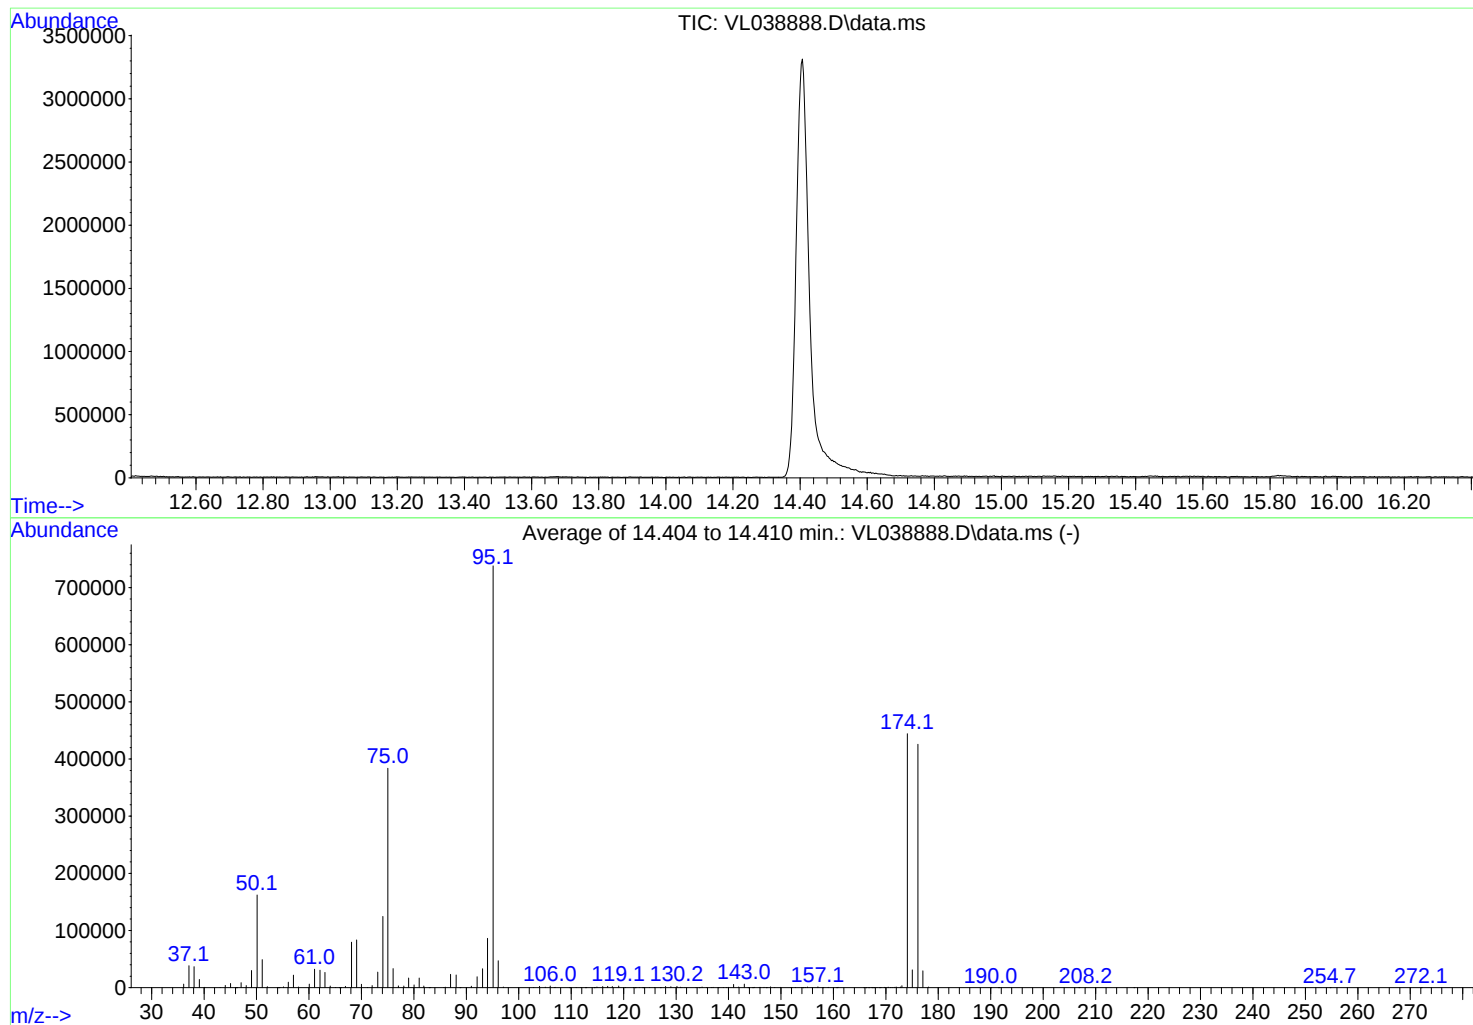

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	162197	PASS
75	95	30	66	52.0	383763	PASS
95	95	100	100	100.0	738069	PASS
96	95	5	9	6.4	46973	PASS
173	174	0.00	2	0.8	3462	PASS
174	95	50	120	60.2	444203	PASS
175	174	4	9	7.0	31075	PASS
176	174	93	101	95.8	425728	PASS
177	176	5	9	6.9	29507	PASS

Average of 14.404 to 14.410 min.: VL038888.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	6069	48.05	3700	60.05	6214	70.00	5821
37.10	38480	49.05	30067	61.05	32211	71.15	2118
38.10	36597	50.10	162197	62.10	30613	72.05	3711
39.10	14415	51.10	48936	63.05	26536	73.10	2715
40.10	580	52.05	1670	64.05	2921	74.10	124731
43.05	296	54.00	144	65.10	361	75.05	383763
44.05	4009	54.30	102	65.80	104	76.05	33237
45.05	7416	55.15	1417	66.00	95	77.05	3081
46.00	94	56.05	9613	66.95	2263	78.10	2764
46.20	100	57.05	21875	68.10	79677	79.00	16843
47.05	8698	58.00	1196	69.10	83515	80.05	4911

Average of 14.404 to 14.410 min.: VL038888.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.00	16736	93.10	32928	109.70	118	119.05	2947
81.90	2899	94.05	86232	109.85	293	120.30	164
82.90	110	95.10	738069	110.95	219	121.90	206
83.20	426	96.10	46973	111.85	419	122.20	85
85.70	196	97.05	1210	112.70	154	123.00	227
86.00	775	102.85	228	112.95	306	123.65	117
87.00	23237	103.95	2319	114.40	107	124.00	186
88.05	22235	105.05	858	114.90	1003	124.95	268
88.80	66	106.00	2808	116.00	1984	125.90	327
90.95	2413	106.80	299	116.95	2126	127.00	117
92.05	19147	106.95	487	117.85	2105	128.00	2006

Average of 14.404 to 14.410 min.: VL038888.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.00	1660	138.00	99	145.85	498	154.20	159
130.15	2393	139.00	376	146.05	454	154.70	172
130.85	747	139.60	183	146.75	562	155.05	1198
131.10	259	140.00	662	147.20	113	157.05	1422
131.70	180	140.95	5619	148.00	1324	157.95	156
133.80	178	141.95	998	148.80	367	159.00	713
134.40	57	143.00	6101	149.90	678	160.60	109
134.95	1062	143.70	155	151.90	337	160.90	698
135.85	233	144.00	364	152.10	222	165.80	71
136.80	275	144.60	51	152.75	393	166.20	105
137.05	655	144.95	629	154.00	304	166.70	66

Average of 14.404 to 14.410 min.: VL038888.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
167.20	173	171.60	552	206.80	70		
167.40	137	171.95	1220	208.15	166		
167.70	74	172.80	1205	217.30	53		
168.30	161	173.05	3462	254.70	69		
168.80	125	174.10	444203	272.10	84		
169.10	163	175.05	31075				
169.70	476	176.10	425728				
169.90	315	177.05	29507				
170.45	749	178.15	1143				
170.90	174	190.00	84				
171.20	328	191.50	55				