


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041922\
 Data File : VL038942.D
 Acq On : 19 Apr 2022 9:17
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL040522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Apr 06 06:12:53 2022
 Last Update : Wed Apr 06 06:12:53 2022

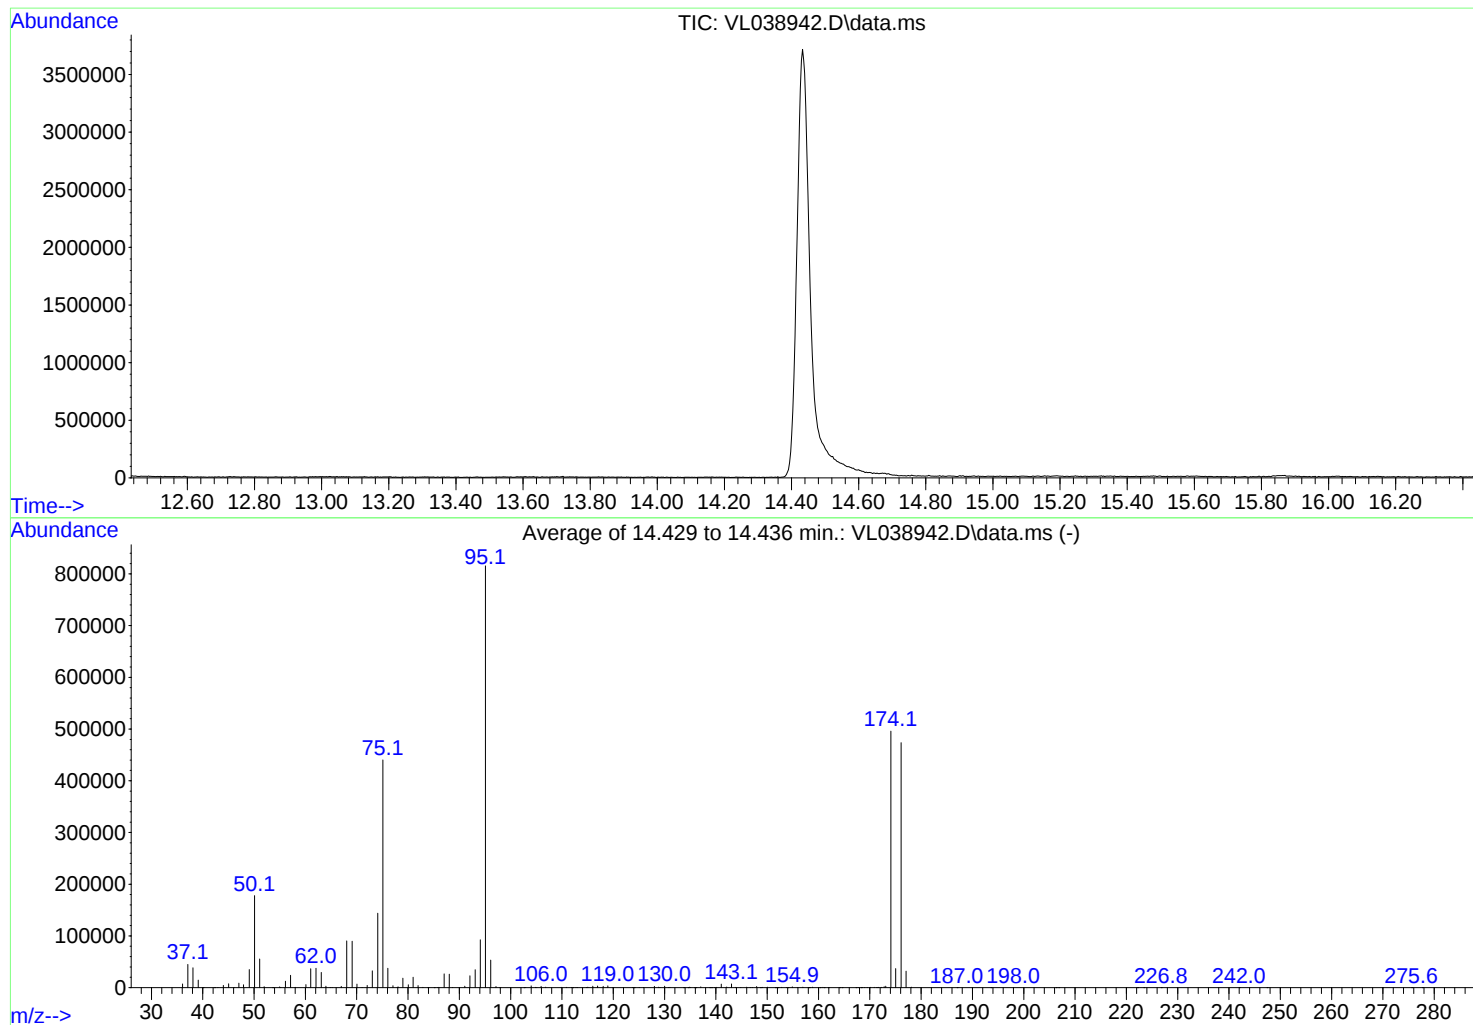

AutoFind: Scans 3621, 3622, 3623; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.8	177877	PASS
75	95	30	66	54.0	440363	PASS
95	95	100	100	100.0	815573	PASS
96	95	5	9	6.5	53099	PASS
173	174	0.00	2	0.5	2724	PASS
174	95	50	120	60.8	496085	PASS
175	174	4	9	7.4	36731	PASS
176	174	93	101	95.5	473707	PASS
177	176	5	9	6.7	31781	PASS

Average of 14.429 to 14.436 min.: VL038942.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7171	47.95	5460	60.10	6017	71.05	261
37.10	44933	49.05	34915	61.05	36517	72.05	433
38.10	38253	50.10	177877	62.05	37421	73.05	3244
39.10	14620	51.10	55312	63.10	29389	74.10	14395
40.05	100	51.95	1912	64.00	2836	75.10	440363
42.30	136	53.60	87	64.85	381	76.05	37448
42.95	291	55.00	1492	65.20	222	77.05	3871
44.00	4269	55.20	405	67.00	2547	77.90	577
45.05	7416	56.10	12498	68.05	90376	78.05	1724
46.10	405	57.10	23853	69.10	89691	79.00	18130
47.05	8722	58.00	697	70.05	6701	80.05	5502

Average of 14.429 to 14.436 min.: VL038942.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.00	20213	92.05	22819	105.10	433	116.00	2790
81.95	4138	93.10	34637	105.95	2649	116.95	3169
82.90	785	94.10	92576	106.85	1008	118.05	2590
83.90	52	95.10	815573	109.85	638	118.95	3466
85.10	132	96.10	53099	110.85	481	119.90	152
85.70	338	97.15	2078	111.85	409	121.95	365
86.00	620	97.90	74	112.10	153	123.75	357
87.05	26731	102.60	135	112.75	382	123.90	120
88.05	26016	102.95	234	113.00	381	124.10	133
88.70	350	104.00	3381	114.80	346	125.05	469
91.05	2917	104.85	711	115.05	902	125.90	366

Average of 14.429 to 14.436 min.: VL038942.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.00	2359	135.85	182	144.85	412	152.85	616
128.85	1009	136.10	143	146.00	919	153.75	216
129.10	356	137.05	1475	146.70	359	154.05	57
130.00	2768	138.80	152	147.10	431	154.90	1563
130.80	464	139.15	175	147.95	2066	155.95	195
131.05	653	139.70	217	148.70	129	156.95	890
133.70	86	140.15	491	149.05	503	158.00	221
133.90	281	141.05	6699	150.05	1005	158.20	54
134.60	70	142.10	1170	151.60	96	158.85	954
134.90	926	143.05	7190	151.90	360	160.30	60
135.10	306	143.90	589	152.10	94	160.85	546

Average of 14.429 to 14.436 min.: VL038942.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
161.10	113	170.85	605	178.10	864	269.90	54
161.90	81	171.30	469	187.00	50	275.60	94
164.10	51	171.50	401	193.60	56	277.70	56
164.60	61	171.70	513	198.00	215		
167.30	53	172.30	732	206.30	58		
167.75	290	172.80	1841	206.80	58		
168.30	161	173.10	2724	222.20	82		
168.55	290	174.10	496085	223.40	60		
169.00	400	175.05	36731	226.80	85		
169.50	309	176.10	473707	242.00	90		
170.10	704	177.05	31781	247.40	85		