
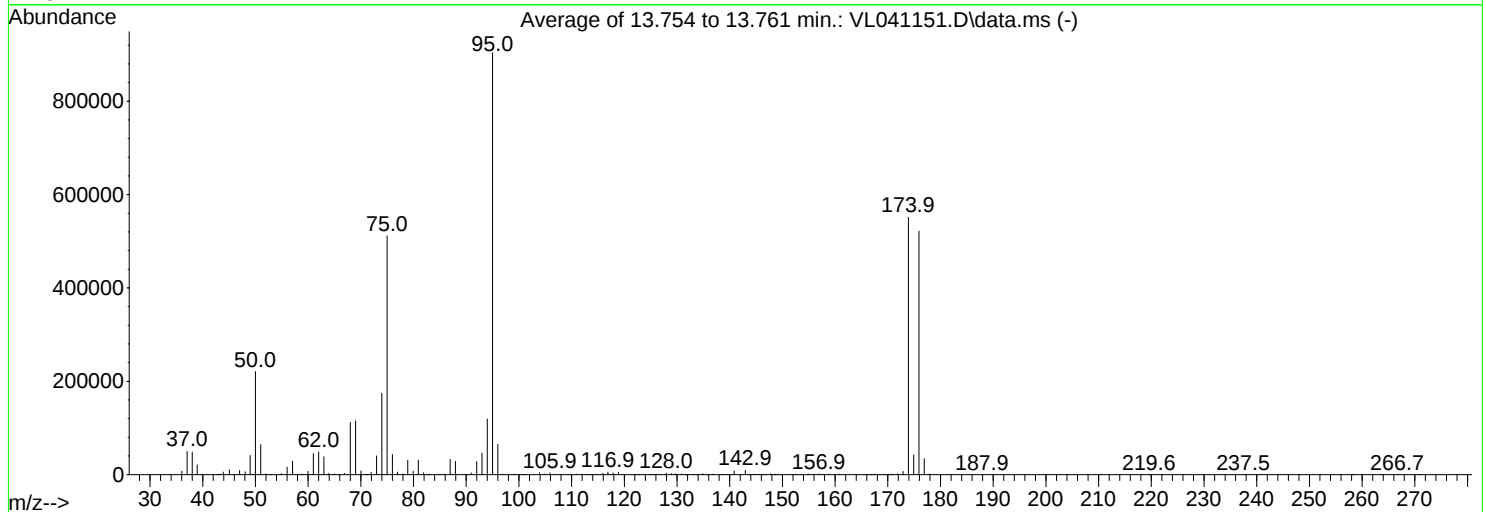


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042324\
Data File : VL041151.D
Acq On : 23 Apr 2024 8:20
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL040424AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Apr 24 02:47:46 2024

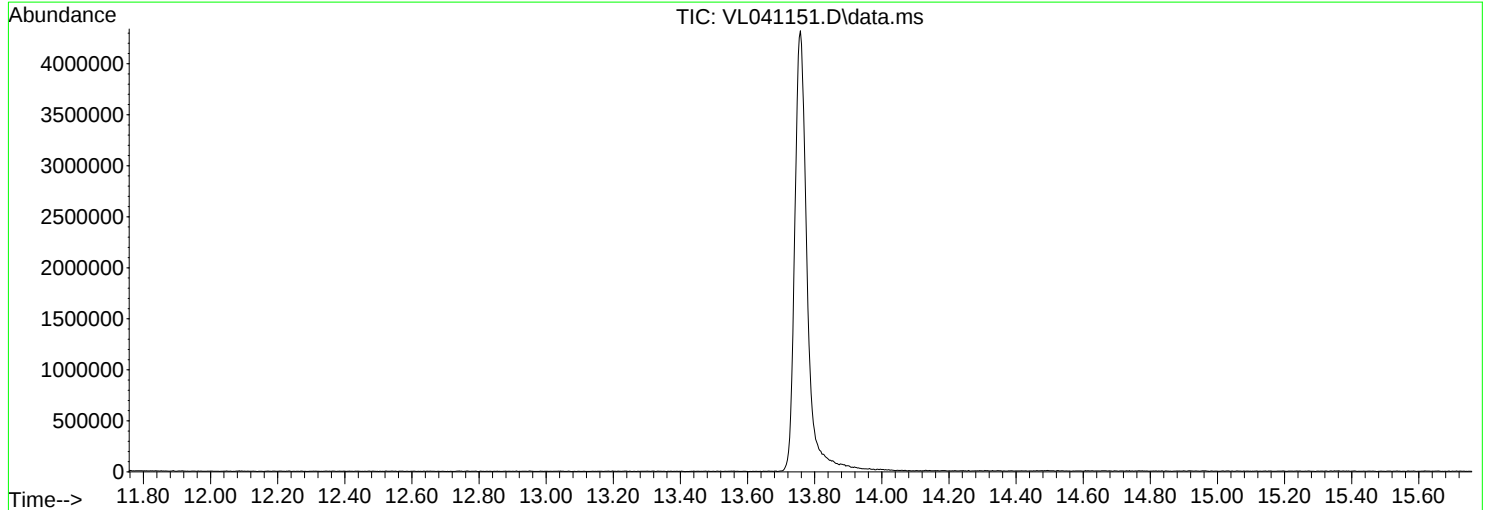

AutoFind: Scans 3468, 3469, 3470; Background Corrected with Scan 3444

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.4	220843	PASS
75	95	30	66	56.6	511787	PASS
95	95	100	100	100.0	903765	PASS
96	95	5	9	7.2	64803	PASS
173	174	0.00	2	1.3	6914	PASS
174	95	50	120	61.0	551360	PASS
175	174	4	9	7.7	42304	PASS
176	174	93	101	94.7	521899	PASS
177	176	5	9	6.6	34323	PASS

Average of 13.754 to 13.761 min.: VL041151.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7624	47.00	8790	58.05	1463	69.00	11529
37.05	49813	48.05	6109	58.80	72	70.05	823
38.00	48661	49.00	41091	59.95	7270	70.90	21
38.95	21070	50.00	220843	61.00	44885	71.20	17
40.00	1088	51.00	64629	62.00	48411	71.95	4768
42.80	101	52.00	1894	63.00	38536	73.00	40168
43.00	229	52.90	129	63.85	2578	74.00	174635
43.20	73	53.85	452	65.00	1266	75.00	511787
43.90	5490	54.95	2013	65.70	87	76.00	43107
45.05	10330	56.00	16194	66.90	2826	76.95	5624
46.10	858	57.05	29197	68.00	112043	77.95	1760

Average of 13.754 to 13.761 min.: VL041151.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	30829	89.95	148	103.90	4260	114.85	746
79.95	7534	90.95	3670	104.80	1313	115.95	2963
80.90	31107	92.00	28037	105.90	3689	116.90	5563
81.90	4234	93.00	46357	106.85	997	117.85	3316
82.70	135	94.00	119251	109.80	793	118.90	4826
83.10	533	95.00	903765	110.90	969	120.00	84
84.70	78	96.00	64803	111.90	890	121.70	139
85.10	268	96.95	1202	112.80	393	122.10	154
85.85	924	99.00	119	113.00	246	122.70	125
86.95	32432	100.80	124	113.60	98	123.75	379
87.95	28547	102.85	768	114.60	438	124.90	57

Average of 13.754 to 13.761 min.: VL041151.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.60	93	133.10	191	140.00	374	146.70	403
125.85	388	133.70	91	140.85	8221	146.95	428
126.65	280	134.00	313	142.00	777	147.75	1640
127.70	812	134.90	2084	142.95	9295	148.50	128
127.95	2982	135.75	186	143.70	56	148.75	537
128.95	1924	136.10	285	144.00	398	149.00	298
129.80	2227	136.80	1102	144.70	266	149.70	306
130.00	743	137.00	530	145.00	704	149.95	576
130.90	1312	138.50	87	145.60	592	151.90	473
131.60	57	138.95	377	145.95	586	152.45	327
131.90	59	139.70	205	146.20	154	152.90	310

Average of 13.754 to 13.761 min.: VL041151.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.60	228	166.70	154	171.85	1720	258.20	102
153.90	459	166.90	160	172.90	6914	263.60	152
154.90	1433	167.30	128	173.90	551360	266.70	167
155.65	394	167.75	242	174.90	42304	270.80	79
156.95	1811	168.45	418	175.90	521899		
157.80	129	168.90	370	176.90	34323		
158.80	961	169.40	436	177.85	1363		
159.95	244	169.55	323	187.90	105		
160.80	955	170.10	796	219.60	91		
165.40	50	170.60	182	222.00	54		
166.10	74	171.10	716	237.50	88		