

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042524\
 Data File : VL041165.D
 Acq On : 25 Apr 2024 10:22
 Operator : SY/MD
 Sample : VL0425ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0425ABL01

Quant Time: Apr 26 03:10:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL040424AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Apr 26 03:09:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	5.176	49	1254975	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.629	114	3103858	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.436	117	2725049	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.744	95	2112901	9.642	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.400%
Target Compounds						
					Qvalue	
15) Acetone	3.484	43	46588	0.343	ppbv #	88
20) Methylene Chloride	3.928	84	19110	0.341	ppbv #	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042524\
Data File : VL041165.D
Acq On : 25 Apr 2024 10:22
Operator : SY/MD
Sample : VL0425ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0425ABL01

Quant Time: Apr 26 03:10:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL040424AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Apr 26 03:09:28 2024
Response via : Initial Calibration




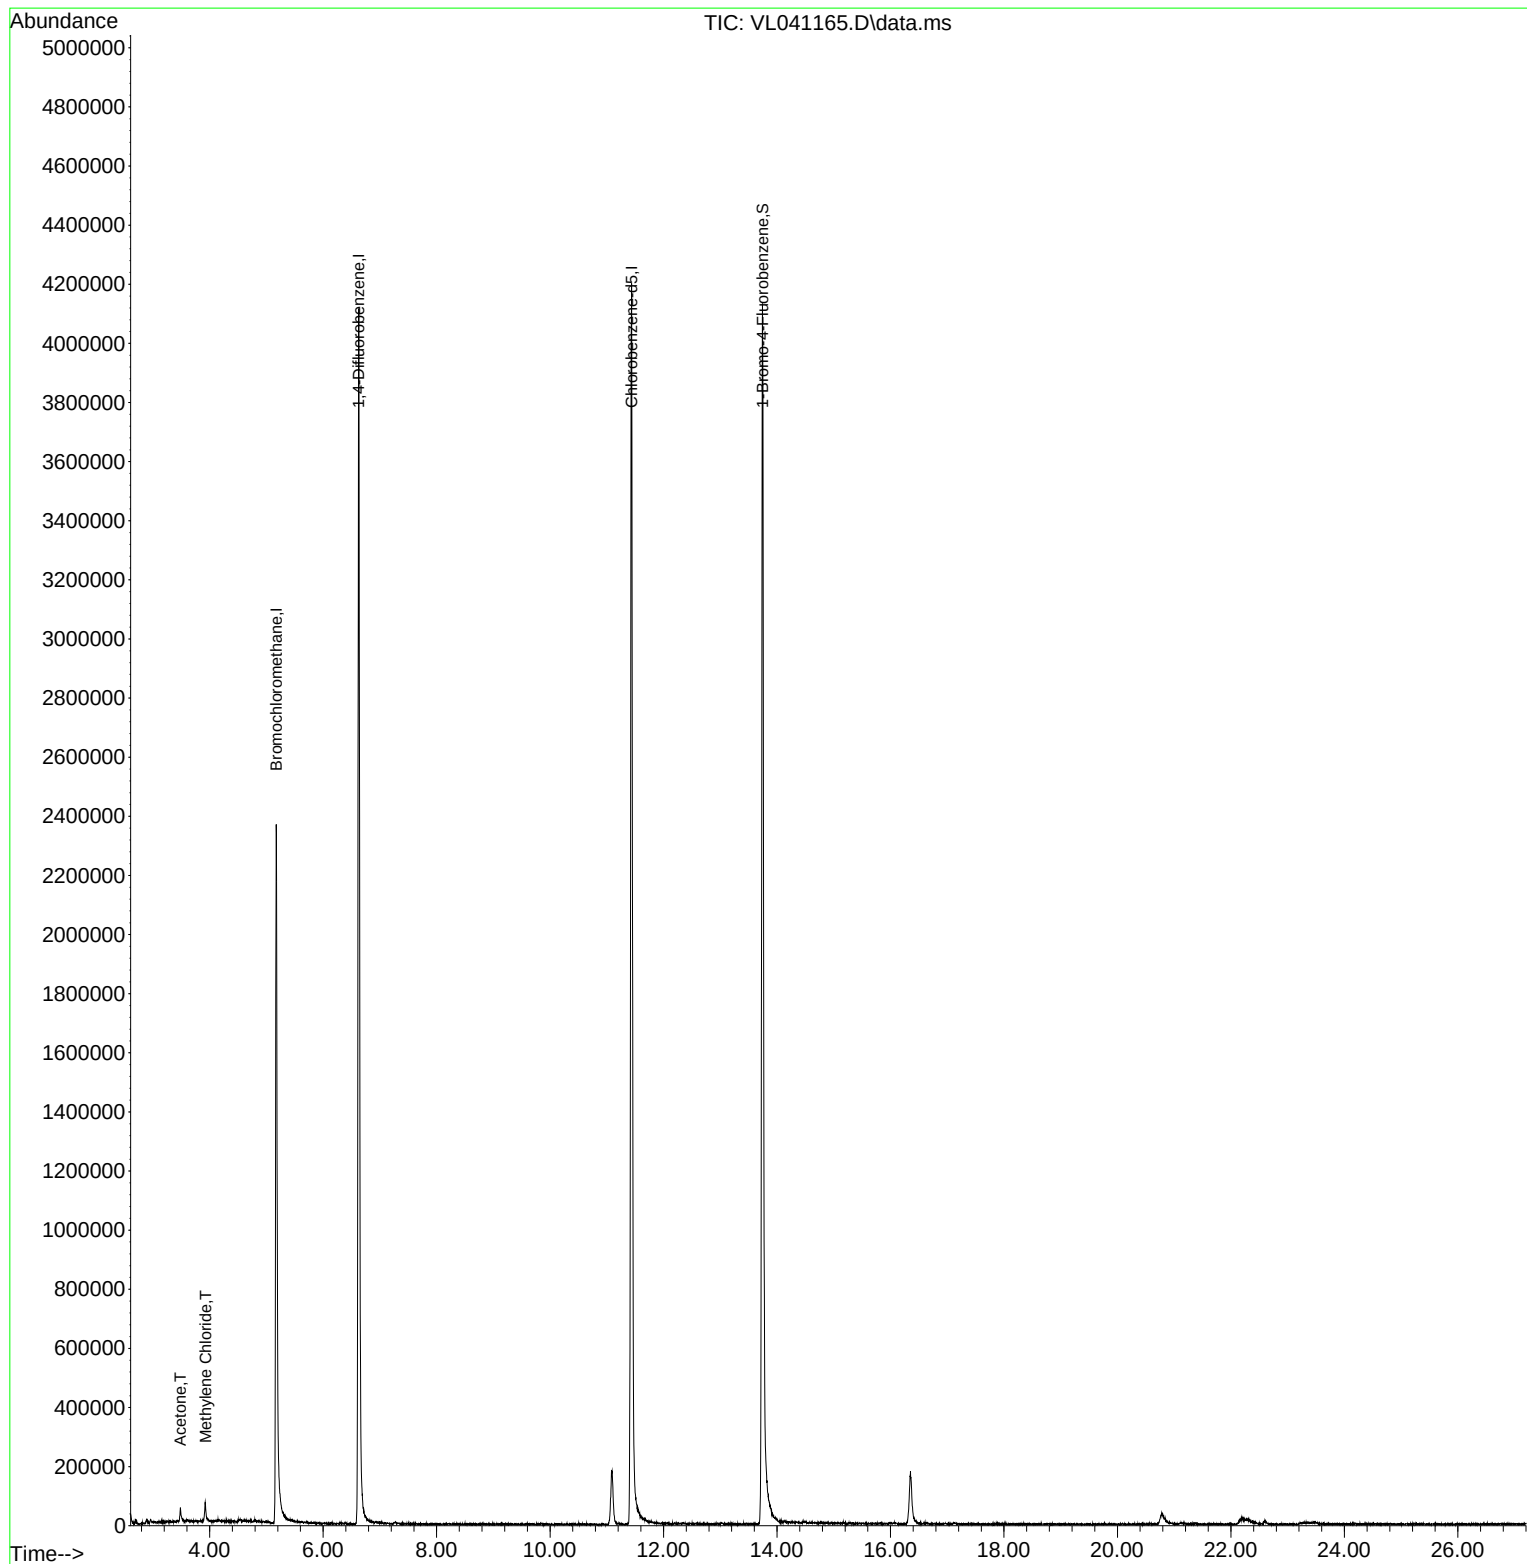


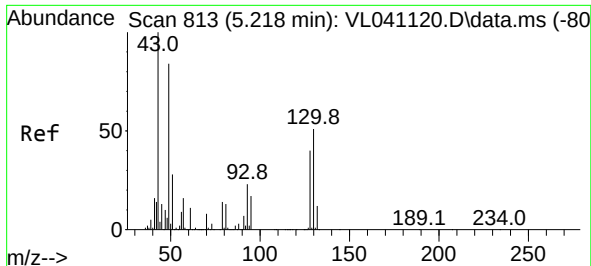

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.176 min Scan# 80
Delta R.T. -0.003 min
Lab File: VL041165.D
Acq: 25 Apr 2024 10:22




Instrument :
MSVOA_L
ClientSampleId :
VL0425ABL01


Tgt Ion: 49 Resp: 1254975
Ion Ratio Lower Upper
49 100
128 45.7 23.6 71.0
130 60.3 30.1 90.5

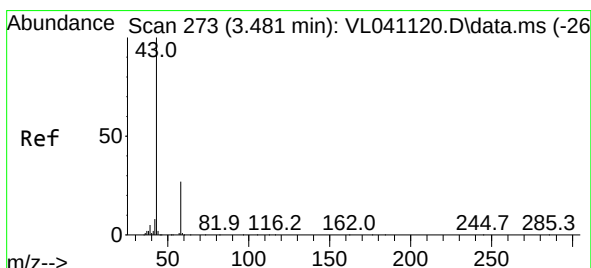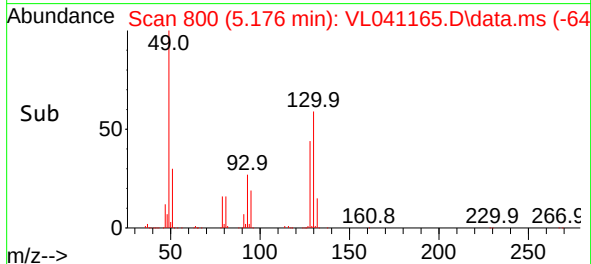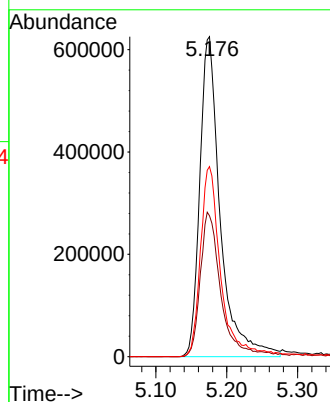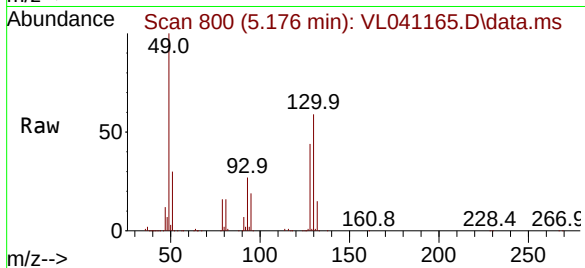

#15
Acetone
Concen: 0.343 ppbv
RT: 3.484 min Scan# 274
Delta R.T. 0.026 min
Lab File: VL041165.D
Acq: 25 Apr 2024 10:22

Tgt Ion: 43 Resp: 46588
Ion Ratio Lower Upper
43 100
58 32.6 21.1 31.7#


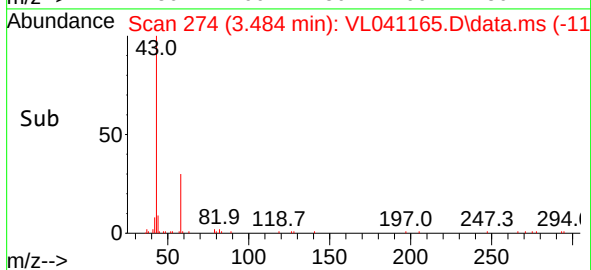
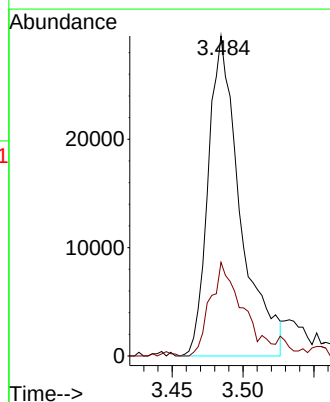
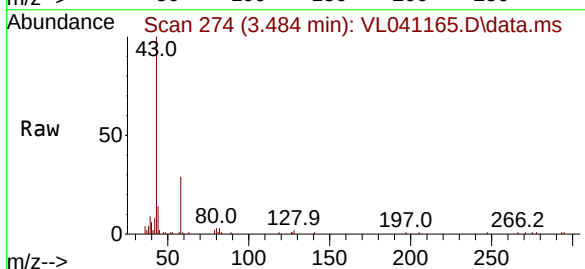


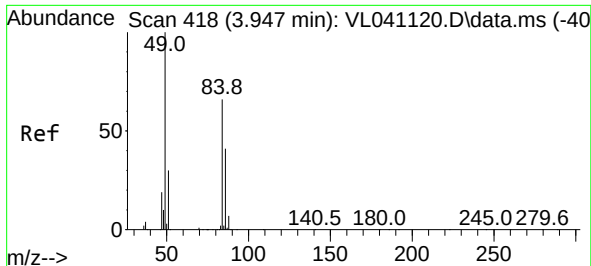

#20
Methylene Chloride
Concen: 0.341 ppbv
RT: 3.928 min Scan# 41
Delta R.T. 0.003 min
Lab File: VL041165.D
Acq: 25 Apr 2024 10:22




Instrument :
MSVOA_L
ClientSampleId :
VL0425ABL01


Tgt Ion: 84 Resp: 19110
Ion Ratio Lower Upper
84 100
49 109.3 120.7 181.1#
51 31.2 36.6 54.8#
86 52.5 49.2 73.8

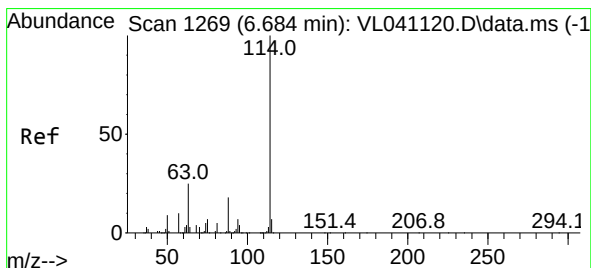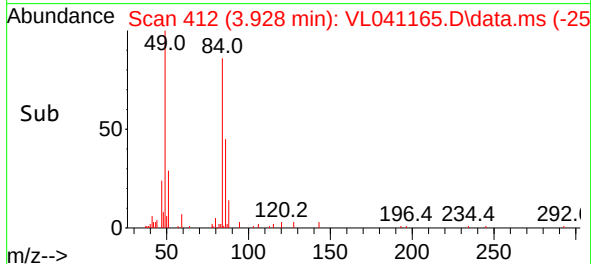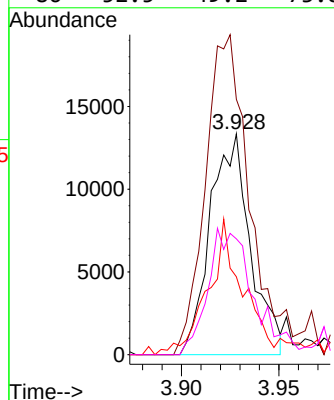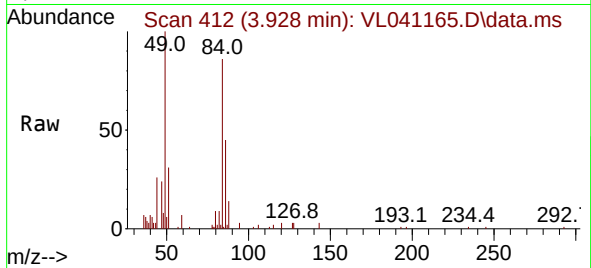

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.629 min Scan# 1252
Delta R.T. -0.006 min
Lab File: VL041165.D
Acq: 25 Apr 2024 10:22

Tgt Ion: 114 Resp: 3103858
Ion Ratio Lower Upper
114 100
63 25.6 20.9 31.3
88 18.0 14.5 21.7


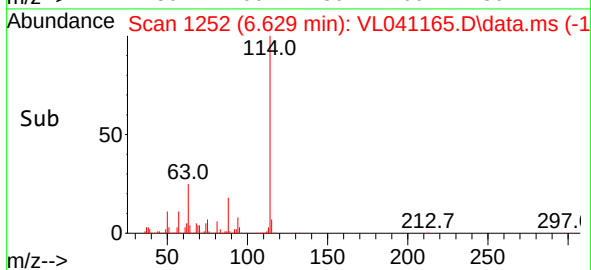
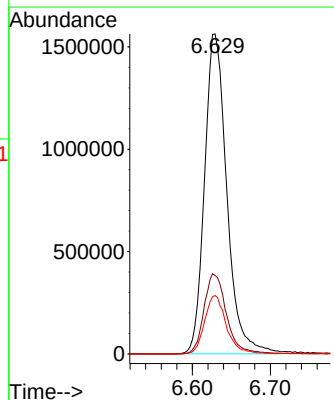
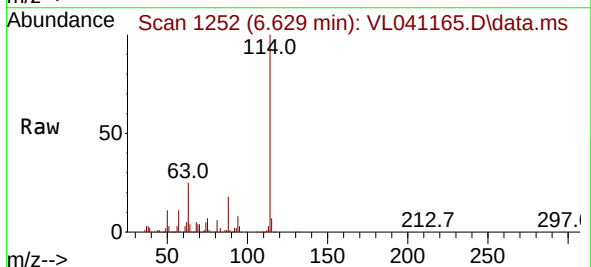


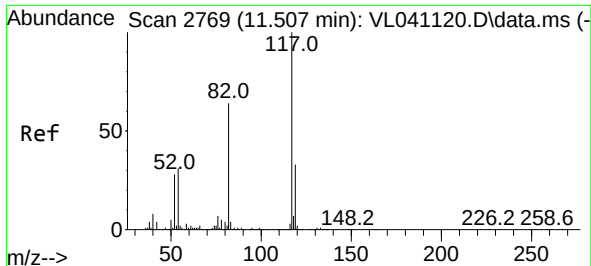

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.436 min Scan# 21
Delta R.T. -0.006 min
Lab File: VL041165.D
Acq: 25 Apr 2024 10:22

Instrument :
MSVOA_L
ClientSampleId :
VL0425ABL01

Tgt Ion:117 Resp: 2725049
Ion Ratio Lower Upper
117 100
82 67.8 51.0 76.6
119 33.7 25.2 37.8

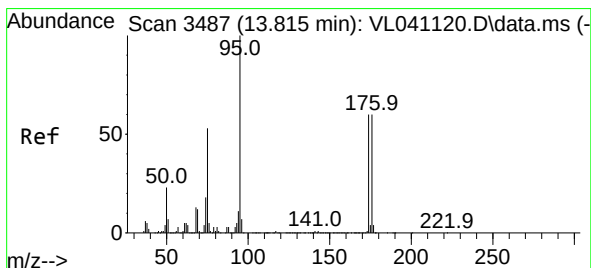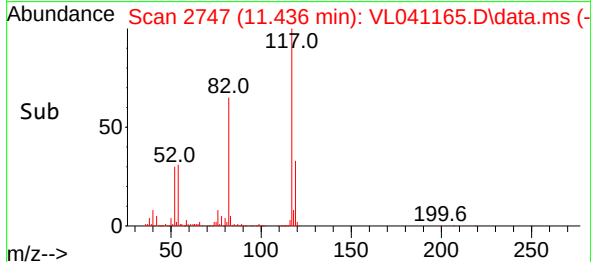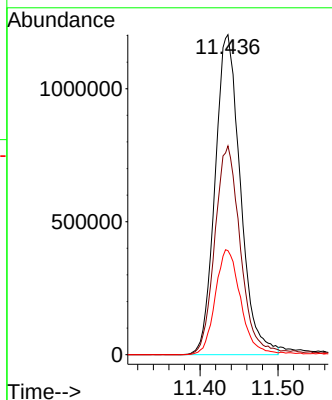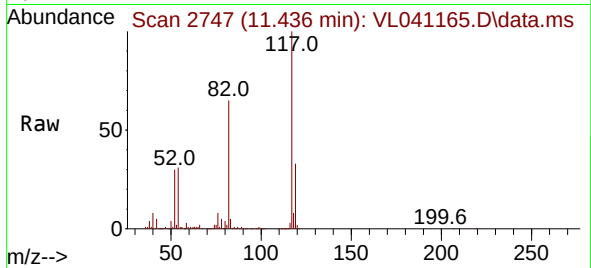

#68
1-Bromo-4-Fluorobenzene
Concen: 9.642 ppbv
RT: 13.744 min Scan# 3465
Delta R.T. -0.003 min
Lab File: VL041165.D
Acq: 25 Apr 2024 10:22

Tgt Ion: 95 Resp: 2112901
Ion Ratio Lower Upper
95 100
174 61.7 49.3 73.9
175 4.6 3.6 5.4

