

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042524\
 Data File : VL041167.D
 Acq On : 25 Apr 2024 12:37
 Operator : SY/MD
 Sample : VIBLK
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VIBLK

Quant Time: Apr 26 03:11:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL040424AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Apr 26 03:09:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.176	49	1211743	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.632	114	3060879	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.439	117	2664311	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.751	95	2086646	9.740	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042524\
Data File : VL041167.D
Acq On : 25 Apr 2024 12:37
Operator : SY/MD
Sample : VIBLK
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Apr 26 03:11:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL040424AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Apr 26 03:09:28 2024
Response via : Initial Calibration




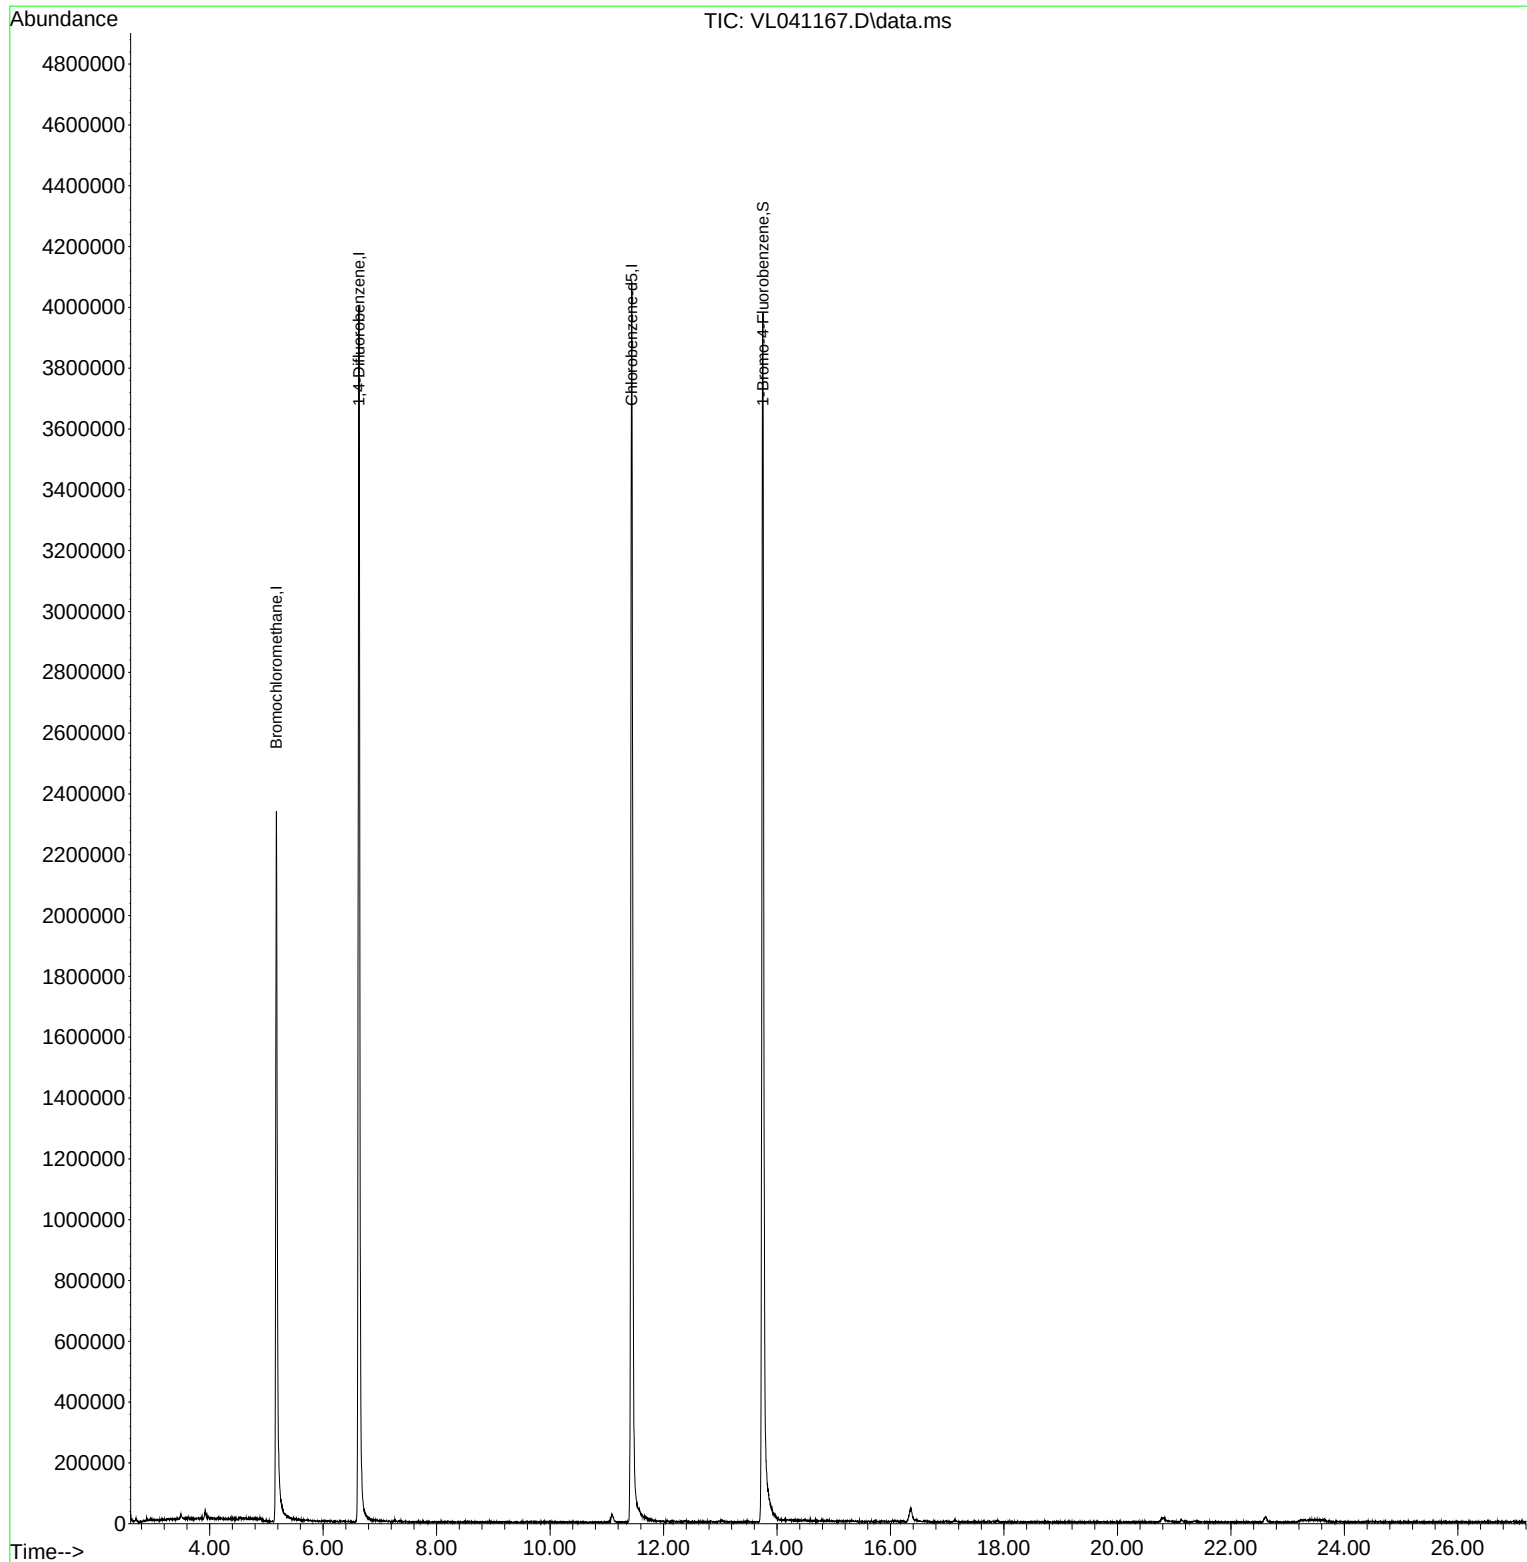


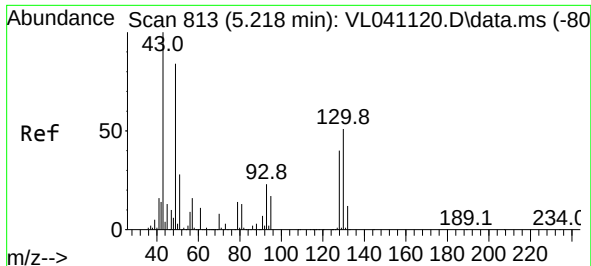

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.176 min Scan# 80
Delta R.T. -0.003 min
Lab File: VL041167.D
Acq: 25 Apr 2024 12:37




Instrument :
MSVOA_L
ClientSampleId :
VIBLK


Tgt Ion: 49 Resp: 1211743
Ion Ratio Lower Upper
49 100
128 48.0 23.6 71.0
130 61.9 30.1 90.5

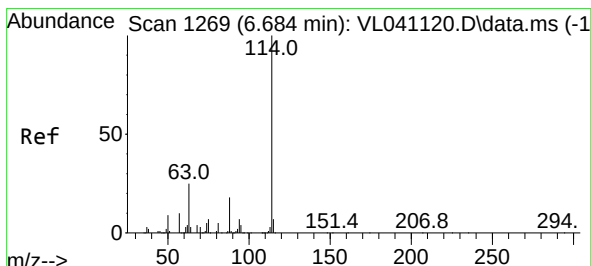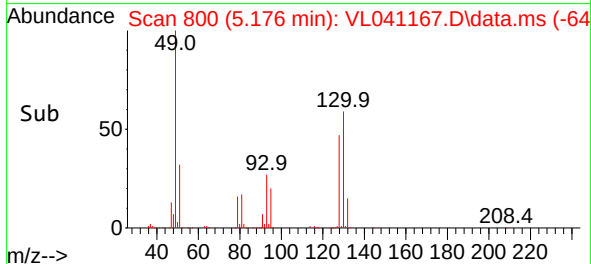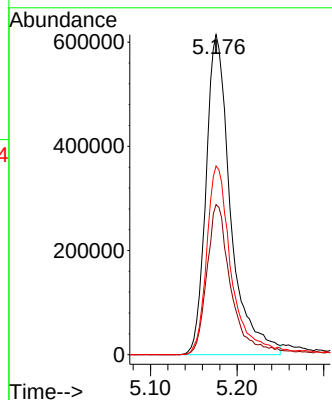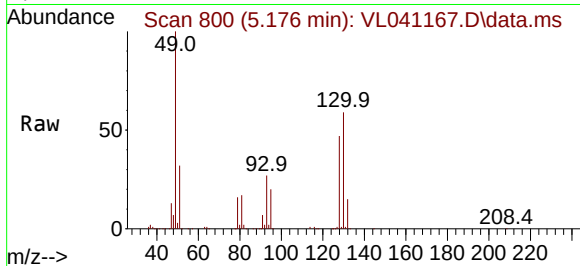

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.632 min Scan# 1253
Delta R.T. -0.003 min
Lab File: VL041167.D
Acq: 25 Apr 2024 12:37

Tgt Ion: 114 Resp: 3060879
Ion Ratio Lower Upper
114 100
63 25.7 20.9 31.3
88 18.0 14.5 21.7


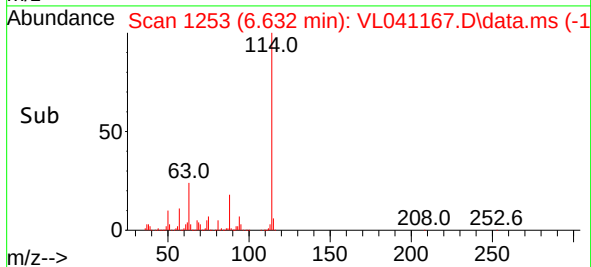
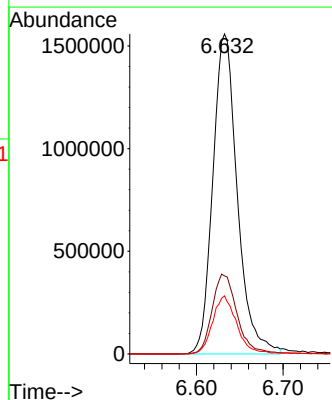
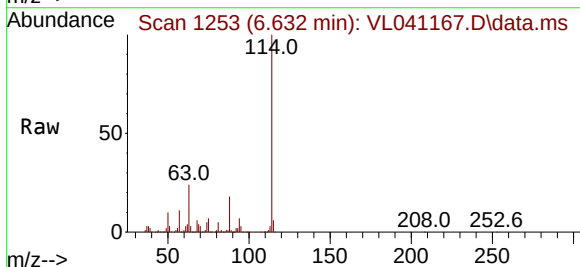


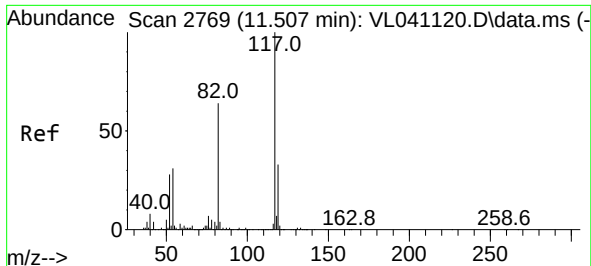

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.439 min Scan# 21
Delta R.T. -0.003 min
Lab File: VL041167.D
Acq: 25 Apr 2024 12:37

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 2664311
Ion Ratio Lower Upper
117 100
82 66.5 51.0 76.6
119 32.8 25.2 37.8

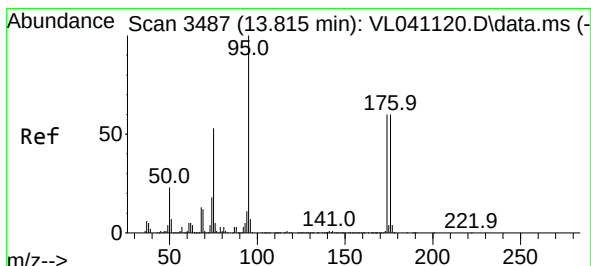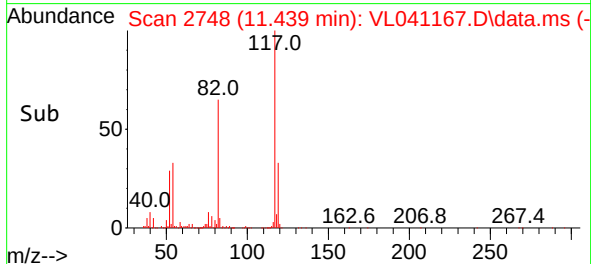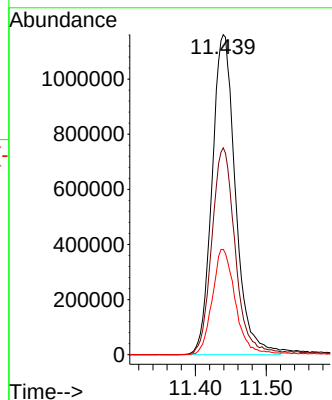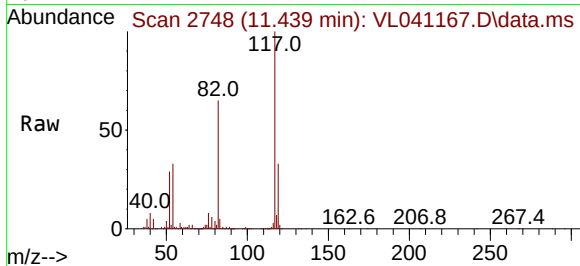

#68
1-Bromo-4-Fluorobenzene
Concen: 9.740 ppbv
RT: 13.751 min Scan# 3467
Delta R.T. 0.003 min
Lab File: VL041167.D
Acq: 25 Apr 2024 12:37

Tgt Ion: 95 Resp: 2086646
Ion Ratio Lower Upper
95 100
174 61.3 49.3 73.9
175 4.6 3.6 5.4

