


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042524\
Data File : VL041163.D
Acq On : 25 Apr 2024 8:43
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL040424AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Apr 26 03:09:28 2024

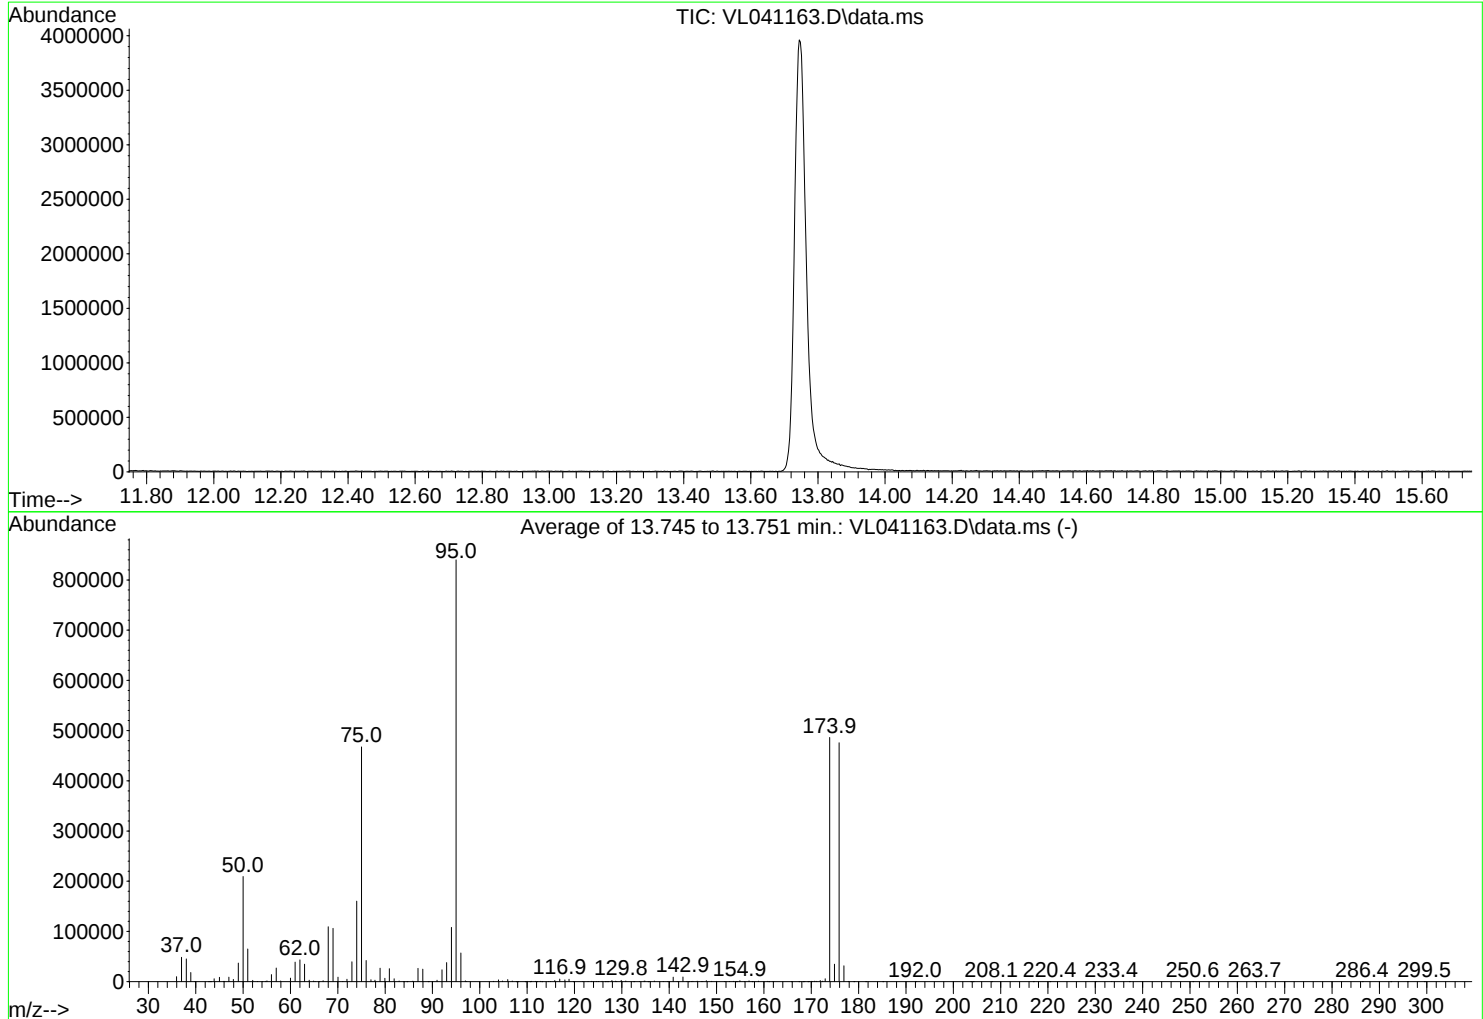

AutoFind: Scans 3465, 3466, 3467; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	209344	PASS
75	95	30	66	55.7	467563	PASS
95	95	100	100	100.0	840085	PASS
96	95	5	9	6.8	56936	PASS
173	174	0.00	2	1.2	5642	PASS
174	95	50	120	57.9	486251	PASS
175	174	4	9	7.1	34723	PASS
176	174	93	101	97.8	475776	PASS
177	176	5	9	6.6	31480	PASS

Average of 13.745 to 13.751 min.: VL041163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	9949	47.00	9098	57.00	27072	68.00	10939
37.00	48483	47.95	4393	57.95	1256	69.00	10600
38.00	45367	49.00	37005	60.00	7162	70.05	890
38.95	18094	50.00	209344	61.00	38952	71.05	31
39.85	312	51.00	65085	62.00	43517	71.95	4876
42.70	64	52.05	2577	63.00	34741	73.00	39421
43.10	177	53.05	373	63.95	3009	74.00	160320
43.90	5615	54.05	263	64.90	1371	75.00	467563
45.00	8634	54.80	677	65.20	305	76.00	41960
45.85	521	55.05	1743	65.95	168	77.00	3870
46.10	683	56.00	14147	66.90	1934	77.85	3033

Average of 13.745 to 13.751 min.: VL041163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	26848	90.95	2984	105.90	4176	112.80	571
79.95	6795	92.00	23619	106.85	1178	113.10	133
80.90	25963	93.00	38024	107.70	58	114.55	497
81.90	5801	94.00	108219	108.00	156	114.95	504
82.95	1405	95.00	840085	109.60	131	115.85	2339
83.90	155	96.00	56936	109.90	452	116.90	5130
84.60	52	96.95	1691	110.00	552	117.95	3492
85.85	853	97.20	488	110.60	71	118.85	4707
86.95	26403	102.90	536	110.90	694	119.75	166
87.95	25024	103.95	3405	111.75	750	121.75	315
89.10	166	104.80	1358	112.00	181	122.85	243

Average of 13.745 to 13.751 min.: VL041163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.65	663	130.85	1249	140.85	8970	147.85	1982
124.00	455	132.50	100	141.70	347	149.00	522
124.65	322	133.70	238	142.00	426	149.95	779
125.05	212	134.70	1006	142.90	9378	151.65	252
125.80	728	134.85	1159	143.75	607	151.95	334
126.50	78	135.55	161	144.10	110	152.75	440
127.00	180	135.90	269	144.70	314	153.60	742
127.90	2385	136.85	1337	145.00	583	154.20	106
128.70	939	138.75	414	145.90	980	154.95	1959
128.90	278	139.70	484	146.85	481	155.90	469
129.85	2703	139.95	405	147.10	195	156.85	1723

Average of 13.745 to 13.751 min.: VL041163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.50	54	170.05	704	177.80	396	230.00	92
158.85	1079	170.30	208	177.95	712	233.45	212
160.70	640	170.75	832	179.00	74	237.20	108
161.00	153	171.15	826	181.50	172	250.60	57
161.90	90	171.90	2190	185.10	145	263.70	130
165.80	51	172.40	875	192.00	71	286.40	85
167.40	88	172.95	5642	203.70	65	292.40	58
168.30	135	173.90	486251	204.20	83	295.90	56
168.65	295	174.90	34723	208.10	92	299.50	81
169.30	161	175.90	475776	216.90	60		
169.60	324	176.90	31480	220.40	75		