
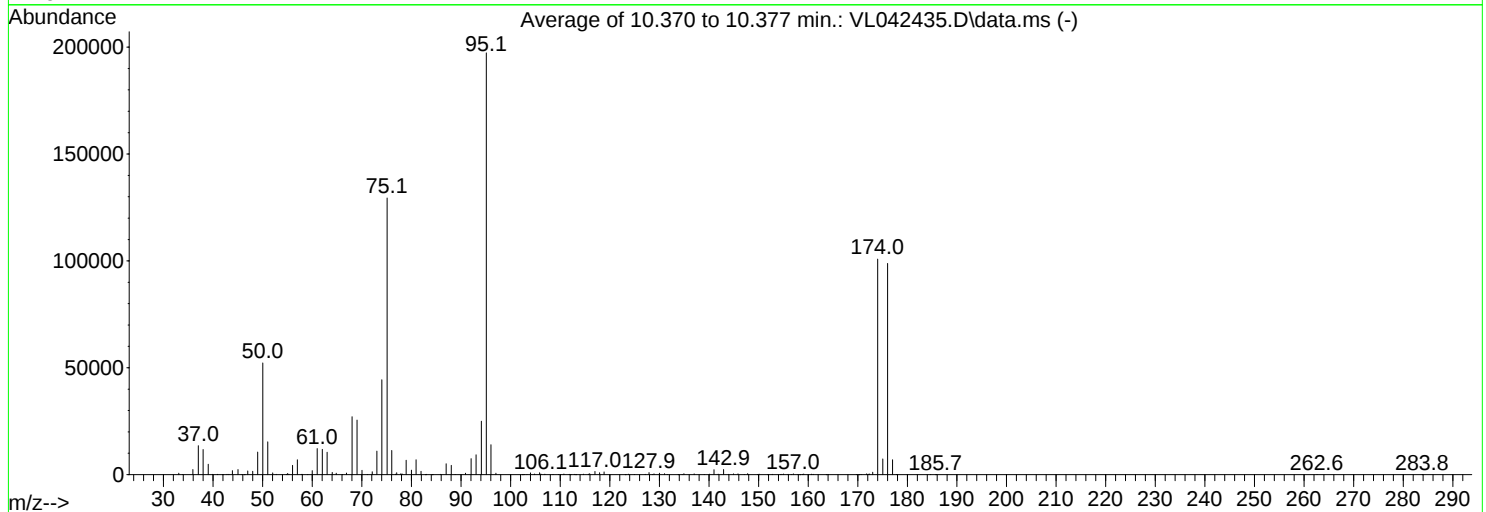


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042925\
Data File : VL042435.D
Acq On : 29 Apr 2025 07:55
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Apr 18 02:14:00 2025

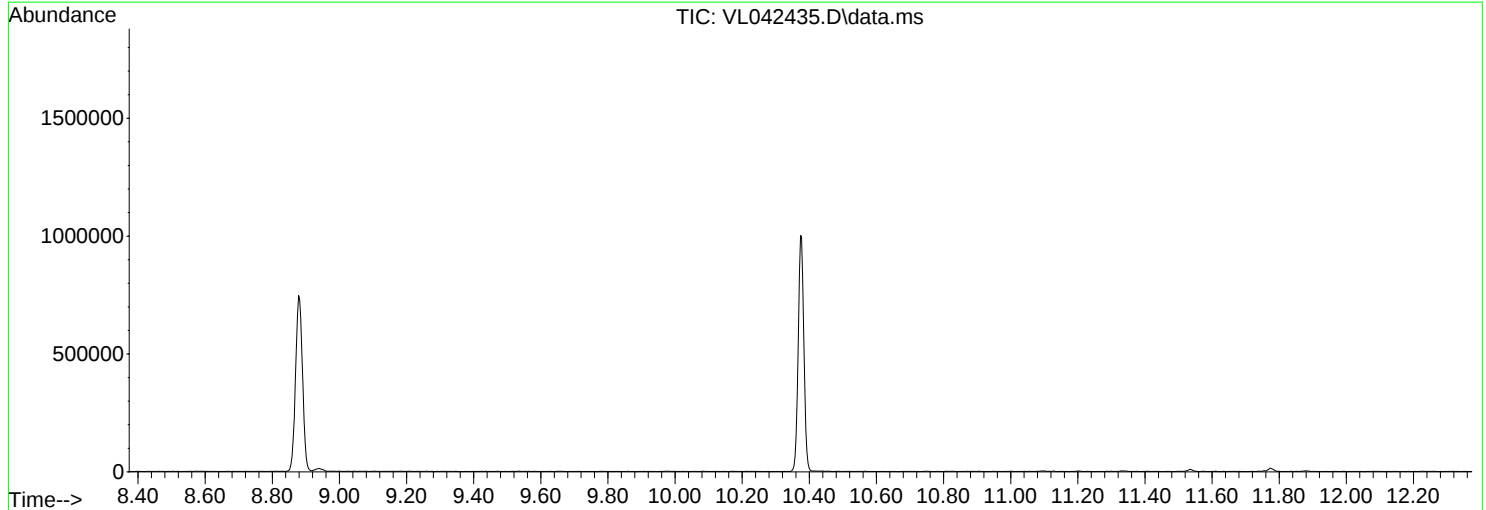

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.5	52245	PASS
75	95	30	66	65.6	129440	PASS
95	95	100	100	100.0	197333	PASS
96	95	5	9	7.1	14000	PASS
173	174	0.00	2	1.1	1121	PASS
174	95	50	120	51.1	100867	PASS
175	174	4	9	7.3	7342	PASS
176	174	93	101	98.0	98848	PASS
177	176	5	9	7.0	6939	PASS

Average of 10.370 to 10.377 min.: VL042435.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	714	43.90	1851	54.80	126	63.00	1048
33.90	68	45.05	2416	55.05	511	64.05	104
35.95	2417	45.85	54	55.30	193	64.85	71
37.05	13537	46.30	32	56.05	4376	66.10	5
38.00	11741	47.00	1705	57.00	6959	66.90	731
39.05	4836	48.00	1585	57.80	154	68.05	27091
39.95	153	49.00	10586	58.00	156	69.05	25563
40.90	123	50.05	52245	59.10	80	70.05	2028
41.90	19	51.05	15372	60.00	1903	71.15	62
42.80	178	52.05	824	61.00	12203	72.10	1333
43.20	122	52.75	183	62.05	11832	73.05	11010

Average of 10.370 to 10.377 min.: VL042435.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.05	44413	82.80	30	95.10	197333	108.55	60
75.10	129440	83.05	167	96.05	14000	109.70	112
76.05	11301	84.20	26	97.05	641	110.10	43
76.80	261	85.90	176	102.40	20	110.75	309
77.05	913	87.00	5065	102.80	59	111.80	122
77.85	347	88.05	4373	103.30	48	112.00	37
78.10	350	88.80	65	104.00	827	112.85	189
78.95	6718	90.90	688	104.85	297	113.10	34
80.00	2065	92.05	7462	105.85	911	114.70	193
80.95	6957	93.05	9289	106.10	276	115.70	254
81.95	1614	94.10	24989	106.90	244	115.95	432

Average of 10.370 to 10.377 min.: VL042435.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.00	1501	131.05	431	143.95	172	154.70	147
117.95	866	131.60	86	144.95	407	155.05	292
118.85	1300	133.80	30	145.85	387	155.95	124
123.10	17	134.60	57	147.10	90	156.60	42
123.75	238	134.95	433	147.80	478	157.00	394
124.95	43	137.00	365	148.00	169	157.95	107
127.15	148	139.05	59	149.80	98	158.30	35
127.90	953	140.10	228	150.10	201	158.90	143
128.60	76	141.00	2360	151.85	38	159.10	311
128.90	384	141.85	270	152.75	124	160.65	217
130.00	664	142.95	2375	154.40	47	161.00	136

Average of 10.370 to 10.377 min.: VL042435.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
163.65	39	176.00	98848				
164.10	45	177.00	6939				
169.80	75	177.80	93				
170.20	24	178.00	89				
170.70	42	184.70	71				
171.80	400	185.70	21				
172.10	268	262.60	63				
172.40	291	283.80	21				
173.00	1121						
174.00	100867						
175.05	7342						

Instrument :

MSVOA_L

ClientSampleId :

BFB