
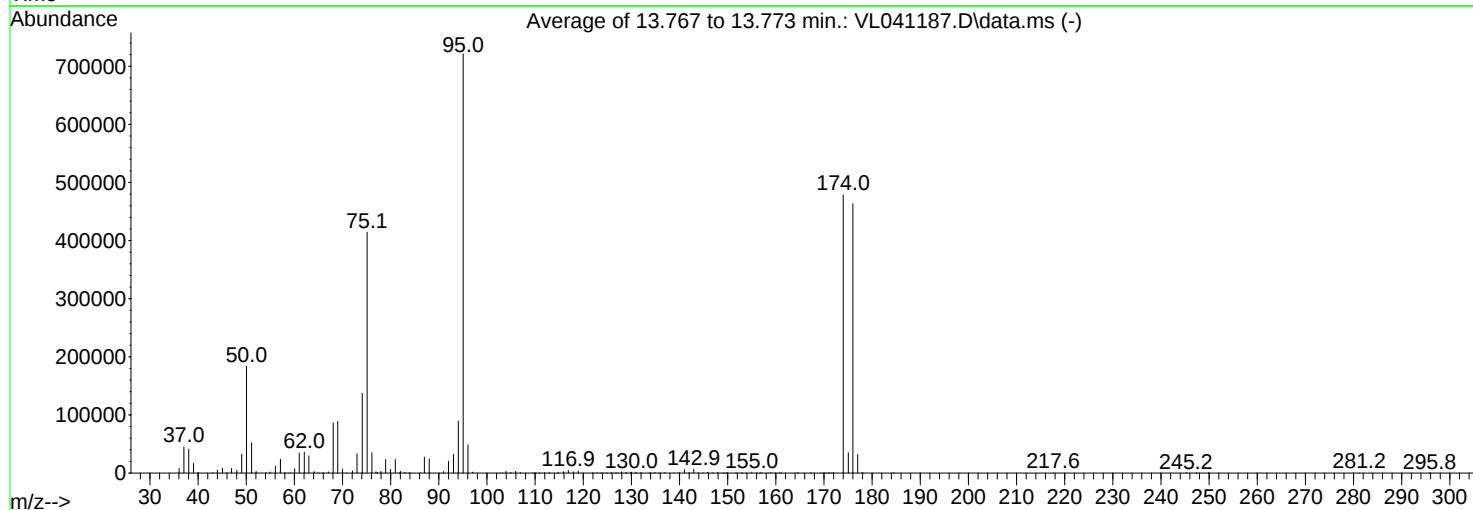


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050224\
Data File : VL041187.D
Acq On : 2 May 2024 8:39
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue May 07 05:19:44 2024

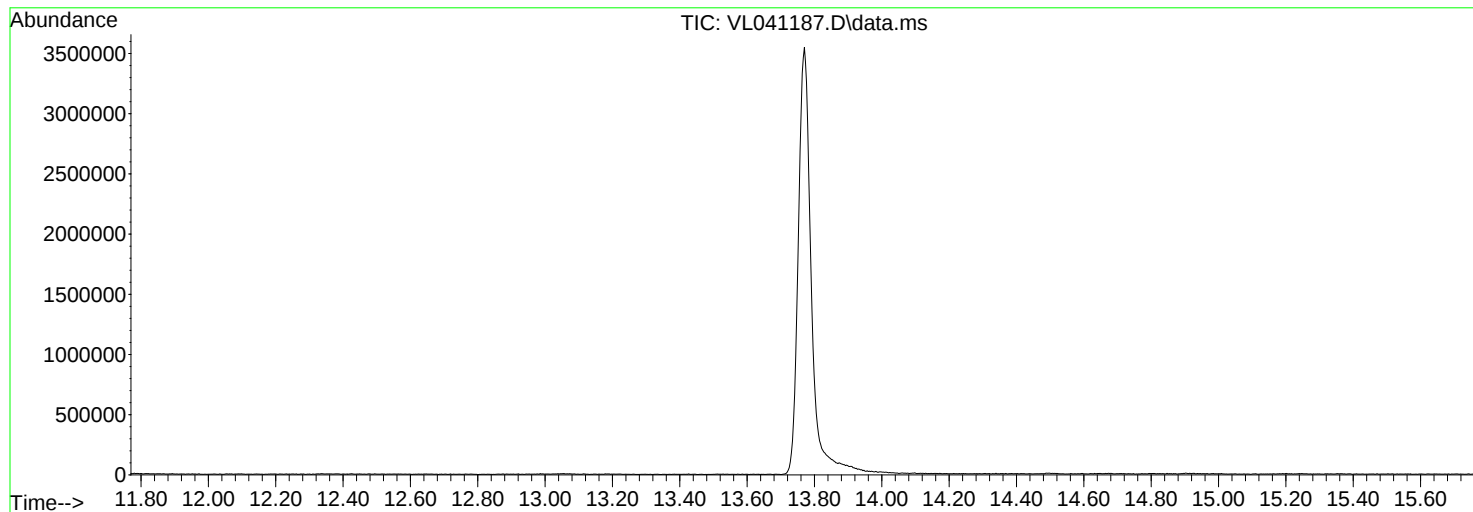

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.5	184000	PASS
75	95	30	66	57.4	414379	PASS
95	95	100	100	100.0	721579	PASS
96	95	5	9	6.8	48779	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	66.3	478763	PASS
175	174	4	9	7.3	35075	PASS
176	174	93	101	96.8	463381	PASS
177	176	5	9	6.9	31880	PASS

Average of 13.767 to 13.773 min.: VL041187.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7946	49.05	32653	60.05	7612	70.00	7153
37.05	44965	50.05	184000	61.00	34403	70.90	141
38.05	41315	51.10	52341	62.05	35955	72.05	3772
39.05	16956	52.05	2849	63.00	29704	73.00	33408
40.05	487	54.05	235	64.10	2652	74.10	137301
43.05	501	54.95	1922	64.80	89	75.10	414379
44.00	4944	56.05	11752	65.15	114	76.10	35165
45.05	8366	57.10	23845	65.90	58	76.95	2433
46.00	791	58.05	666	67.05	2142	77.20	1054
46.95	8009	58.70	157	68.05	86389	77.95	2922
48.05	5001	59.20	265	69.00	88955	78.95	23315

Average of 13.767 to 13.773 min.: VL041187.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	6491	92.00	20389	105.95	3035	115.90	2413
80.95	23302	93.05	32200	106.95	747	116.90	4374
81.90	1616	94.05	89813	109.50	127	117.90	2400
82.05	3092	95.05	721579	109.85	258	118.95	3668
82.90	661	96.05	48779	110.20	175	121.90	78
83.10	257	97.05	1631	110.95	669	122.25	115
83.80	59	102.70	374	112.00	593	122.85	396
86.10	199	103.20	76	112.90	241	123.60	76
87.00	27592	103.95	3338	113.05	534	123.90	361
88.00	24373	104.80	610	114.60	239	124.10	143
91.00	2733	105.10	263	114.85	589	124.70	308

Average of 13.767 to 13.773 min.: VL041187.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.00	108	130.90	417	140.00	456	148.85	312
125.70	86	131.05	510	141.00	6092	149.20	90
125.90	438	131.90	52	141.95	842	149.40	146
126.70	56	133.70	277	142.95	6693	149.70	302
127.25	190	133.90	59	143.85	425	149.90	511
127.95	2229	134.90	1113	144.90	353	151.70	176
128.80	465	135.70	339	145.80	877	151.95	289
128.95	889	136.10	146	146.00	169	152.90	368
129.80	624	136.95	1077	146.80	160	153.10	136
130.00	1621	138.85	272	147.00	73	153.95	267
130.80	100	139.70	118	147.95	1236	155.00	1534

Average of 13.767 to 13.773 min.: VL041187.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.10	166	167.20	60	176.00	463381		
156.60	106	169.25	162	177.00	31880		
156.80	316	169.75	219	177.90	237		
157.10	599	170.15	416	178.10	581		
158.40	97	170.50	349	184.40	52		
158.95	943	171.00	607	217.60	122		
159.90	78	171.20	262	245.20	63		
160.75	316	171.60	290	247.30	51		
161.00	188	171.95	1120	249.80	63		
161.20	135	174.00	478763	281.20	102		
164.50	57	175.05	35075	295.80	61		

Instrument :

MSVOA.L

ClientSampleId :

BFB