
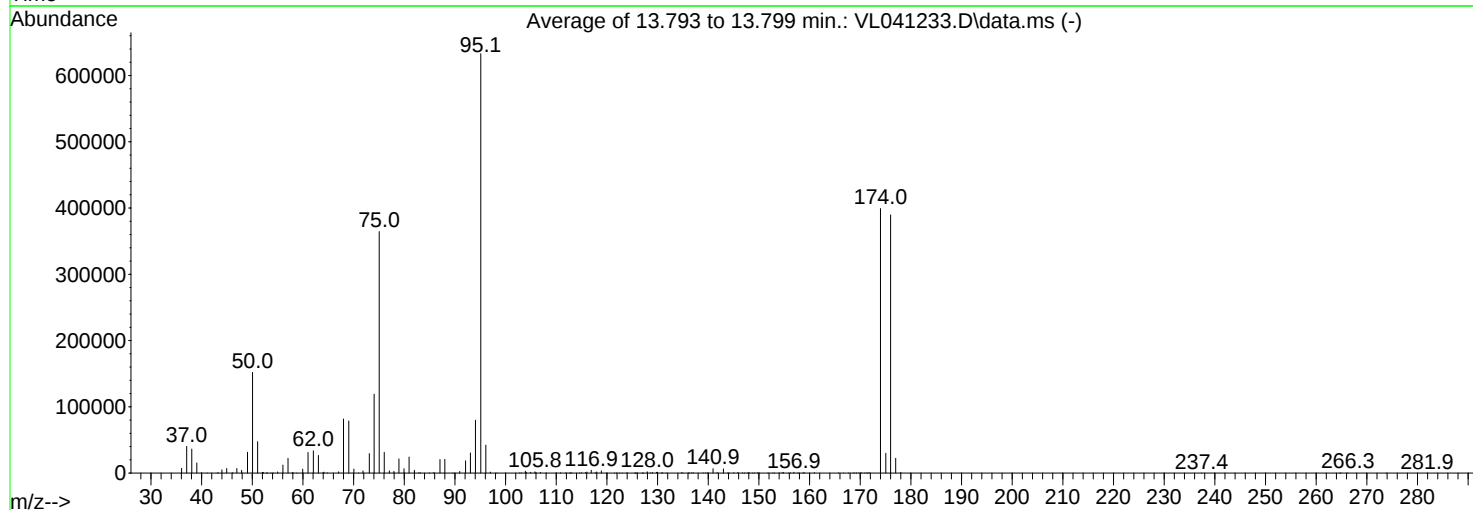


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050824\
Data File : VL041233.D
Acq On : 8 May 2024 7:56
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu May 09 02:43:03 2024

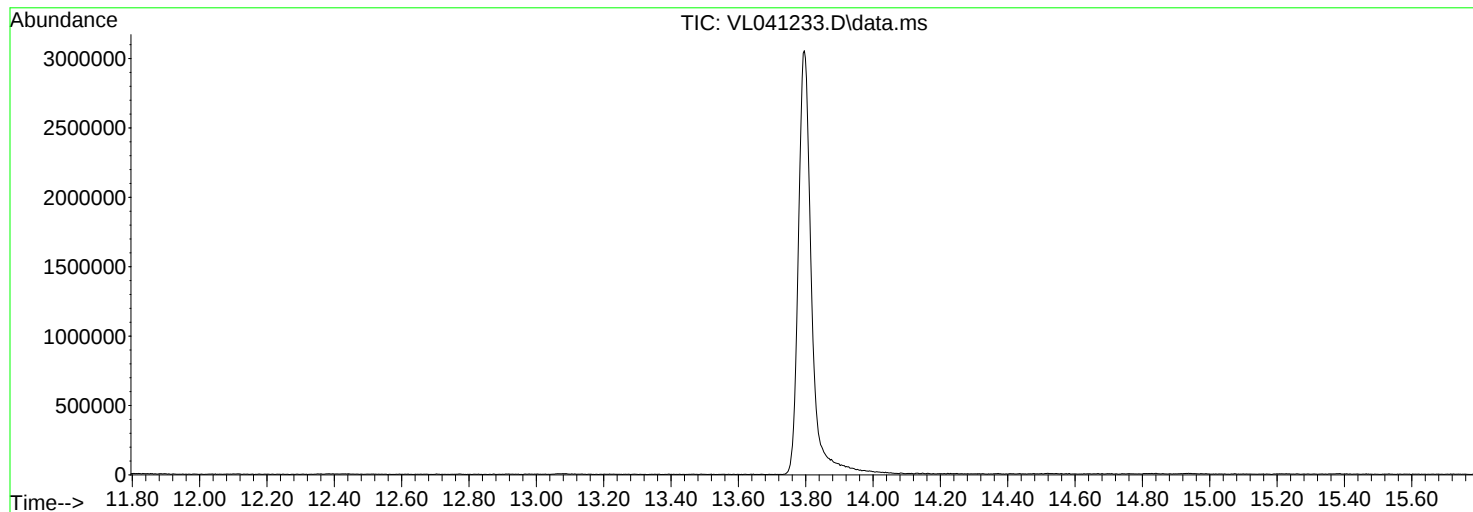

AutoFind: Scans 3480, 3481, 3482; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	151905	PASS
75	95	30	66	57.6	364565	PASS
95	95	100	100	100.0	632896	PASS
96	95	5	9	6.7	42296	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.1	399275	PASS
175	174	4	9	7.5	29907	PASS
176	174	93	101	97.6	389696	PASS
177	176	5	9	5.7	22307	PASS

Average of 13.793 to 13.799 min.: VL041233.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7166	46.95	6963	56.05	12114	64.80	432
37.05	40237	47.90	4201	57.05	22280	67.05	1877
38.05	36331	49.05	31496	57.90	717	68.00	81578
39.05	15396	50.05	151905	58.10	219	69.05	78635
40.00	516	51.05	47395	58.80	72	70.05	6142
41.10	116	52.00	1155	59.95	6127	71.00	175
43.10	228	52.20	831	61.00	31187	71.85	3264
43.30	157	52.80	57	62.05	33600	73.10	29456
44.00	4856	53.70	115	63.05	26584	74.05	119109
44.95	6965	54.20	126	64.00	824	75.05	364565
46.15	580	55.00	1752	64.15	1459	76.05	31381

Average of 13.793 to 13.799 min.: VL041233.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	3482	87.05	20461	102.80	309	111.95	376
77.95	2598	88.00	20779	103.10	227	112.60	84
78.95	21453	89.60	85	103.90	2890	112.80	342
79.95	6650	90.95	2496	104.10	1120	113.05	544
80.95	24205	92.10	18563	104.95	1187	114.60	131
82.00	4325	93.05	30464	105.80	1967	114.95	489
82.90	676	94.05	79856	106.00	854	115.80	774
83.20	326	95.10	632896	106.90	1014	116.05	1627
85.00	203	96.10	42296	108.05	209	116.90	4264
85.75	474	97.00	1509	110.00	316	117.70	530
86.00	98	98.30	74	110.85	560	118.00	1788

Average of 13.793 to 13.799 min.: VL041233.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.90	3362	127.95	2021	136.75	479	145.85	966
120.00	158	128.60	189	137.05	511	146.75	275
121.50	74	128.95	981	139.00	263	147.20	343
121.90	108	129.80	1077	139.50	253	147.70	222
122.50	117	130.00	1289	139.90	486	148.05	1031
123.00	109	130.80	296	140.95	6692	148.70	153
123.95	502	131.00	595	141.75	660	149.10	321
125.50	58	131.70	126	143.00	6332	149.70	576
125.80	107	134.75	628	143.80	118	150.10	139
126.05	158	135.00	311	144.10	369	151.80	285
127.00	57	136.10	52	145.05	619	152.75	170

Average of 13.793 to 13.799 min.: VL041233.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.10	121	160.95	691	171.30	214	273.80	109
154.00	304	165.70	152	171.50	210	281.90	68
154.60	455	166.70	101	171.75	599		
154.85	839	167.65	169	174.00	399275		
155.80	97	168.60	90	175.05	29907		
156.25	270	168.90	79	176.00	389696		
156.90	1302	169.25	295	177.00	22307		
157.70	79	169.70	71	178.00	882		
157.90	237	170.00	163	237.40	69		
158.75	609	170.30	371	264.70	55		
159.00	334	170.90	200	266.25	186		

Instrument :

MSVOA_L

ClientSampleId :

BFB