

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050922\
 Data File : VL038993.D
 Acq On : 9 May 2022 19:04
 Operator : SY/AP
 Sample : N2724-02
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/10/2022
 Supervised By : Mahesh Dadoda 05/11/2022

Quant Time: May 10 05:46:00 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022

QLast Update : Thu May 05 10:12:15 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.648	49	1097733	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.153	114	2511161	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.056	117	2090526	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.384	95	1726910	10.431	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	104.300%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	3.044	85	52710	0.306	ppbv	100
3) Chlorodifluoromethane	2.976	51	72670m	0.533	ppbv	
4) Chloromethane	3.137	50	34576m	0.507	ppbv	
9) Propene	3.015	41	72043m	1.211	ppbv	
10) Heptane	8.098	43	140375	0.962	ppbv	98
11) Trichlorofluoromethane	3.944	101	43936	0.298	ppbv	86
13) Ethanol	3.590	45	373720m	88.776	ppbv	
15) Acetone	3.832	43	2426268m	23.431	ppbv	
19) Isopropyl Alcohol	3.954	45	239065	4.856	ppbv #	1
20) Methylene Chloride	4.330	84	282198	7.231	ppbv	97
26) Hexane	5.668	57	677741	6.154	ppbv #	39
29) Chloroform	5.735	83	21473m	0.121	ppbv	
30) Cyclohexane	7.111	84	63876m	0.693	ppbv	
34) 2-Butanone	5.230	43	88965	0.694	ppbv #	90
35) Carbon Tetrachloride	7.002	117	10365m	0.063	ppbv	
36) Benzene	6.867	78	386201	1.797	ppbv	96
44) 2,2,4-Trimethylpentane	7.848	57	112658	0.299	ppbv #	65
52) Tetrachloroethene	11.201	164	8973m	0.117	ppbv	
53) Toluene	9.780	91	1599821	6.642	ppbv	99
58) Ethyl Benzene	12.677	91	270433m	0.899	ppbv	
59) m/p-Xylene	12.934	91	901807m	3.511	ppbv	
60) o-Xylene	13.661	91	292354	1.209	ppbv	96
61) Styrene	13.494	104	19468m	0.151	ppbv	
64) n-propylbenzene	15.526	120	22497m	0.263	ppbv	
69) p-Isopropyltoluene	17.629	119	45854m	0.128	ppbv	
72) 4-Ethyltoluene	15.805	105	151144	0.549	ppbv #	96
73) 1,3,5-Trimethylbenzene	15.960	105	111106m	0.448	ppbv	
74) 1,2,4-Trimethylbenzene	16.731	105	398487m	1.468	ppbv	
76) 1,4-Dichlorobenzene	17.101	146	20917m	0.143	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050922\
Data File : VL038993.D
Acq On : 9 May 2022 19:04
Operator : SY/AP
Sample : N2724-02
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
IA1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022


Quant Time: May 10 05:46:00 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LThu May
QLast Update : Thu May 05 10:12:15 2022
Response via : Initial Calibration

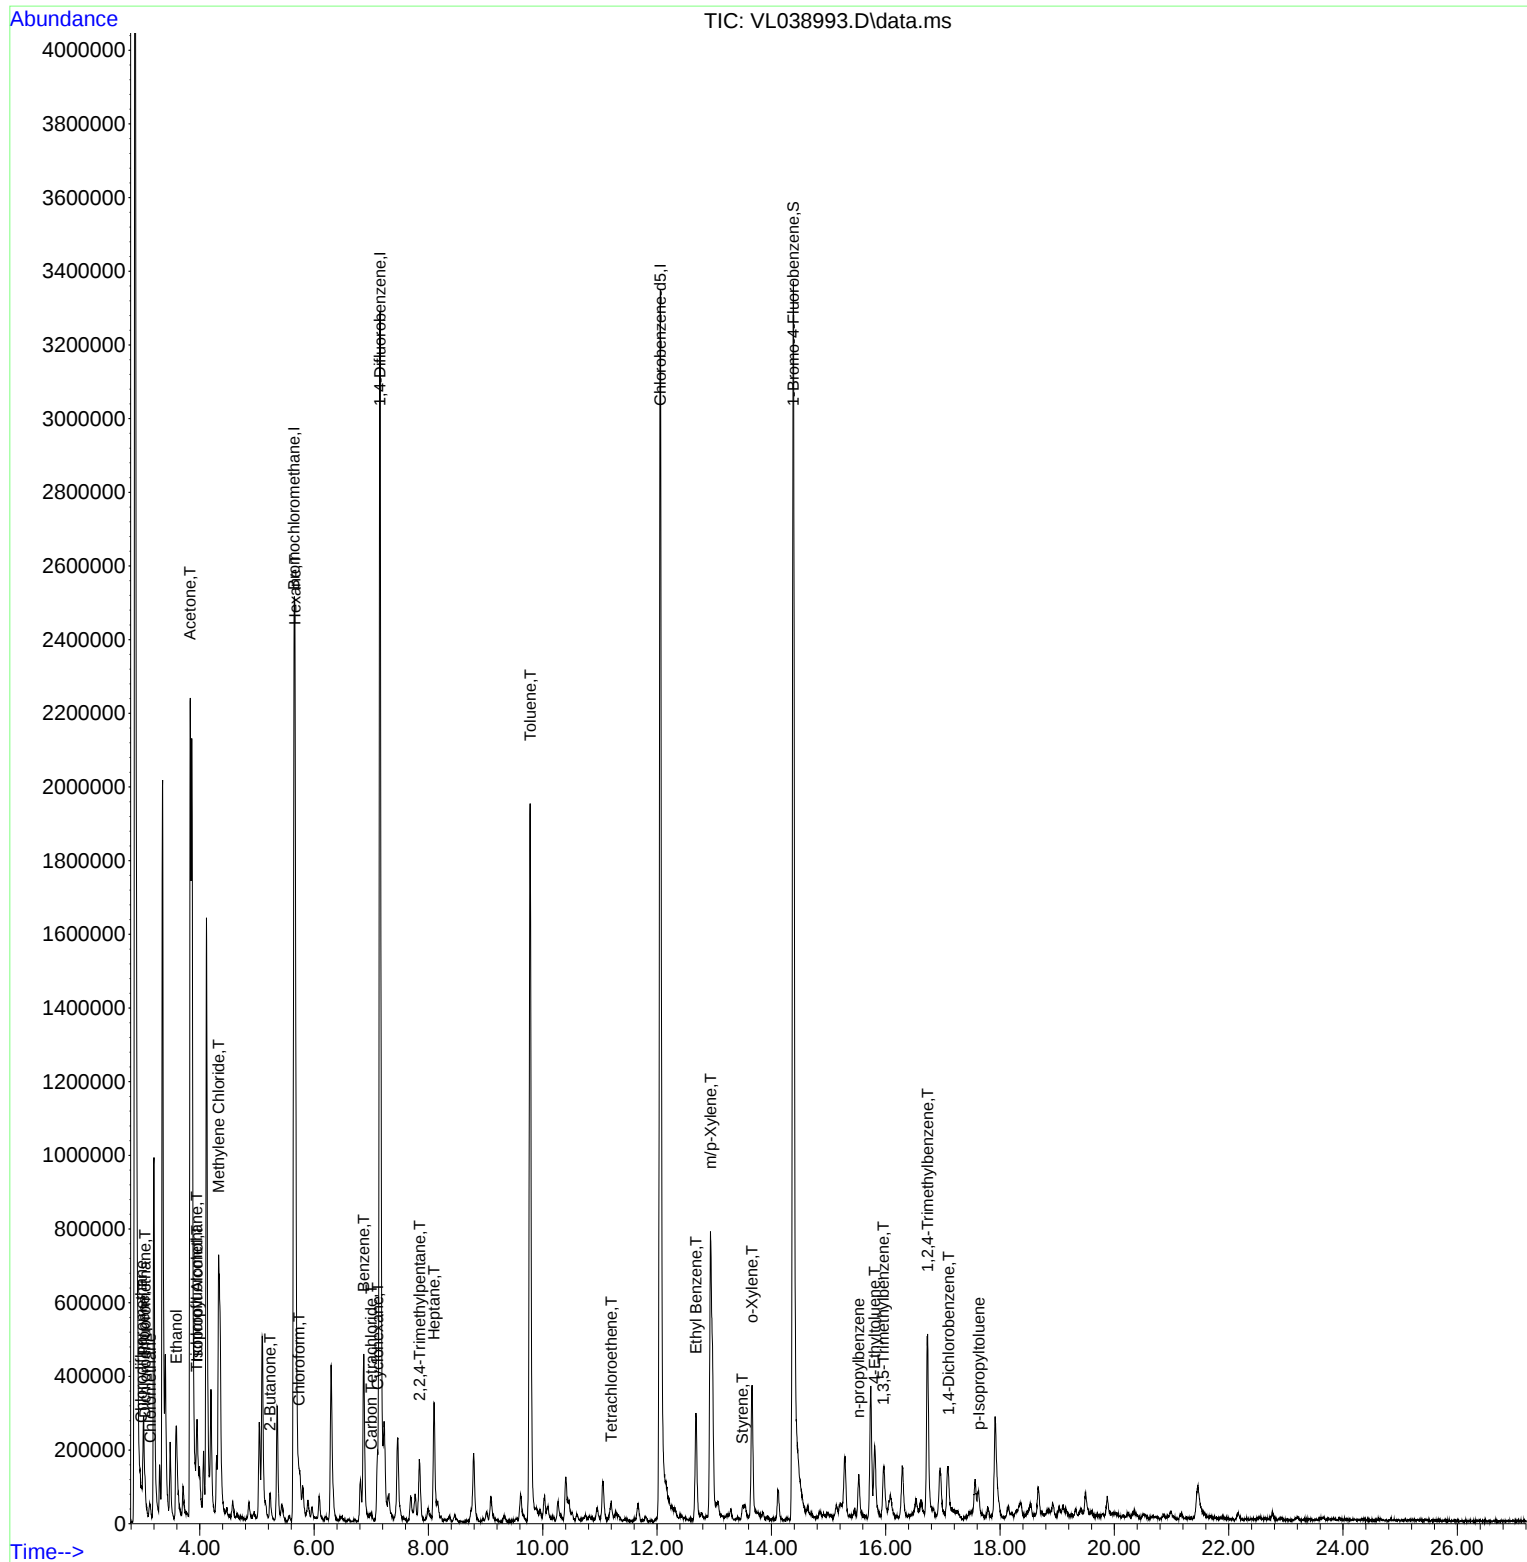

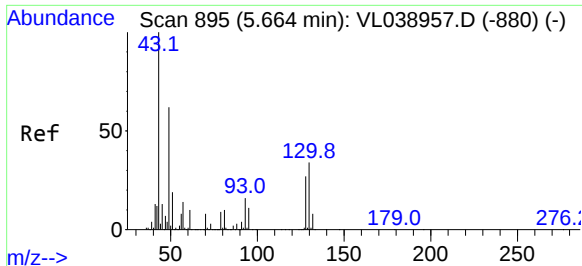

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.648 min Scan# 80
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1

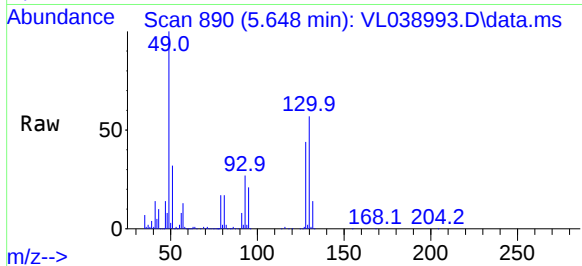

Tgt Ion: 49 Resp: 109773
Ion Ratio Lower Upper
49 100
128 45.8 23.3 69.8
130 58.9 29.8 89.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

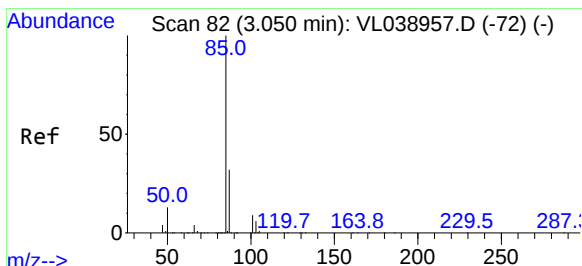

#2
Dichlorodifluoromethane
Concen: 0.306 ppbv
RT: 3.044 min Scan# 80
Delta R.T. -0.006 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

Tgt Ion: 85 Resp: 52710
Ion Ratio Lower Upper
85 100
87 32.4 25.7 38.5

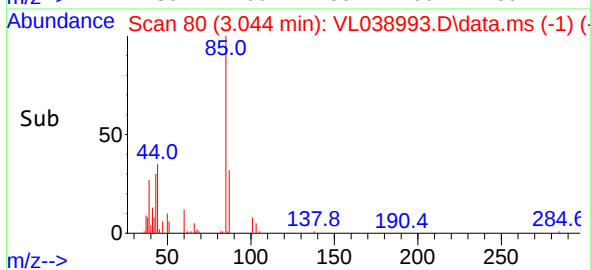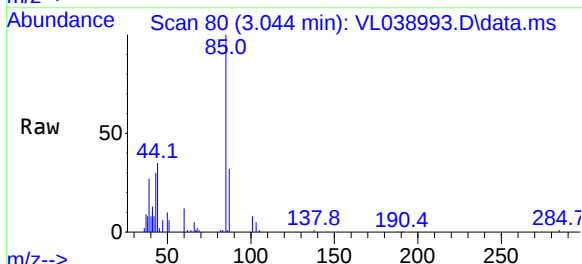

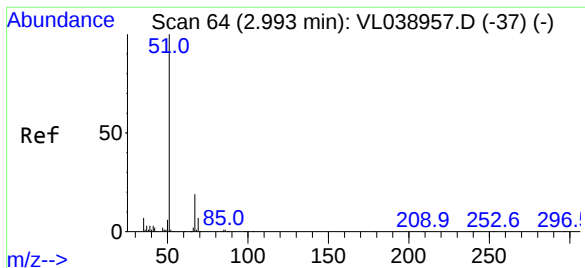





#3
Chlorodifluoromethane
Concen: 0.533 ppbv m
RT: 2.976 min Scan# 51
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion: 51 Resp: 72670
Ion Ratio Lower Upper
51 100
67 18.3 15.8 23.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

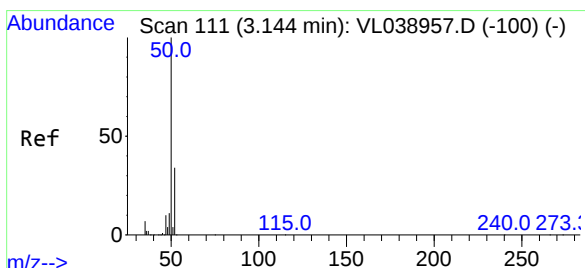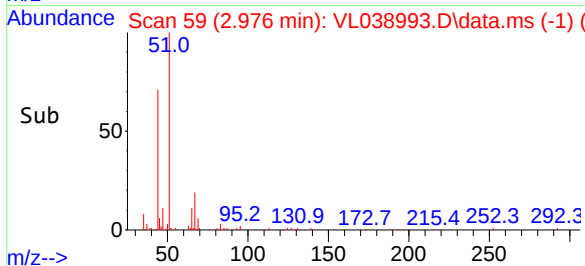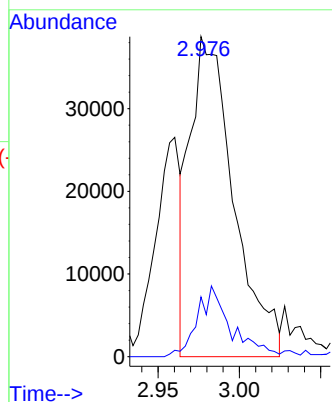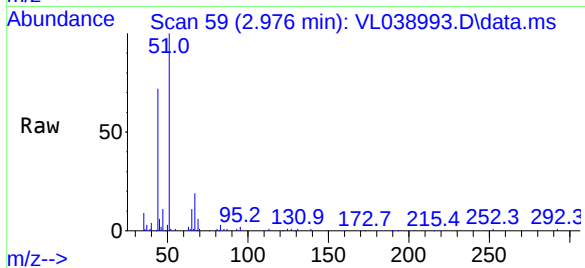

#4
Chloromethane
Concen: 0.507 ppbv m
RT: 3.137 min Scan# 109
Delta R.T. -0.006 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04


Tgt Ion: 50 Resp: 34576
Ion Ratio Lower Upper
50 100
52 34.5 27.3 40.9

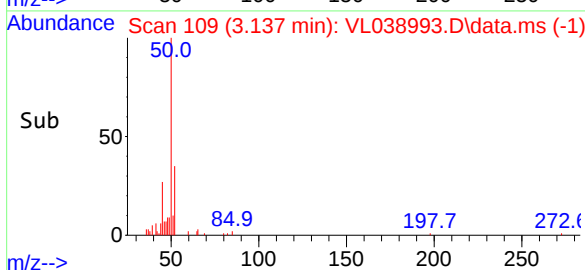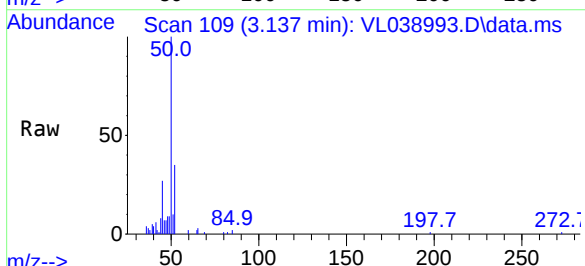

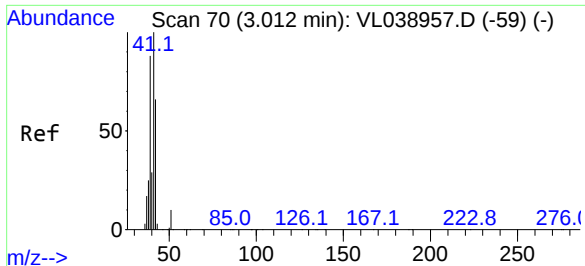

#9
Propene
Concen: 1.211 ppbv m
RT: 3.015 min Scan# 71
Delta R.T. 0.003 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1

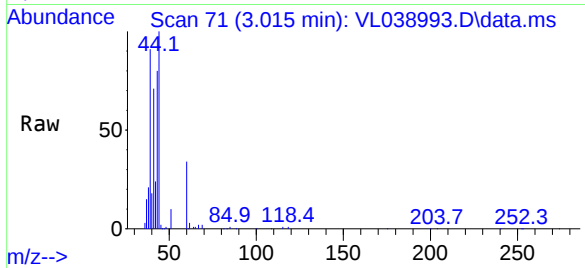


Tgt Ion: 41 Resp: 7204
Ion Ratio Lower Upper
41 100
42 323.1 58.3 87.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

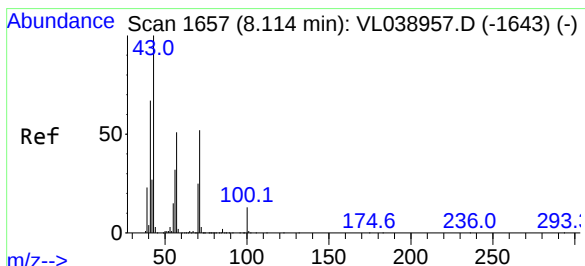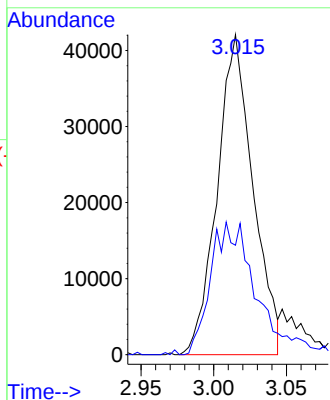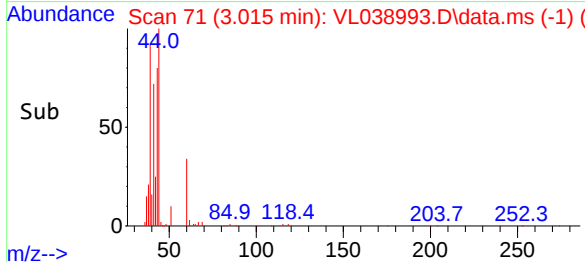


#10
Heptane
Concen: 0.962 ppbv
RT: 8.098 min Scan# 1652
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

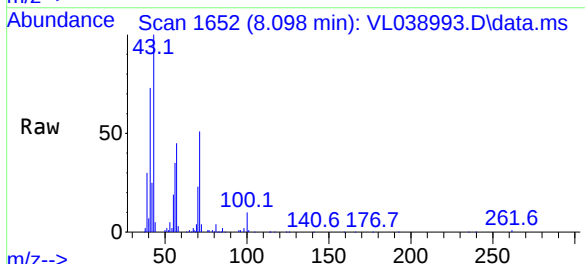


Tgt Ion: 43 Resp: 140375
Ion Ratio Lower Upper
43 100
57 52.2 40.5 60.7

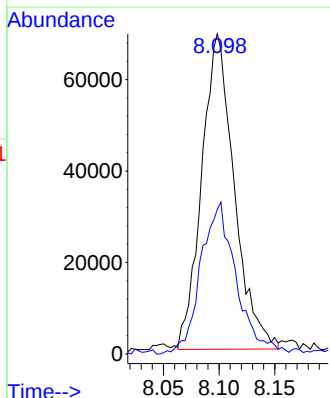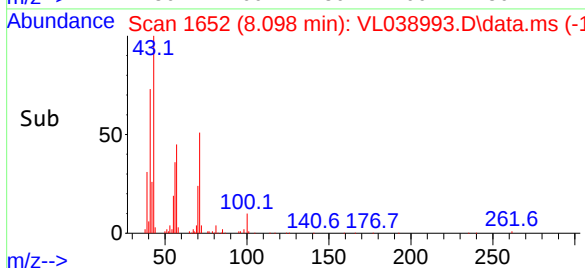

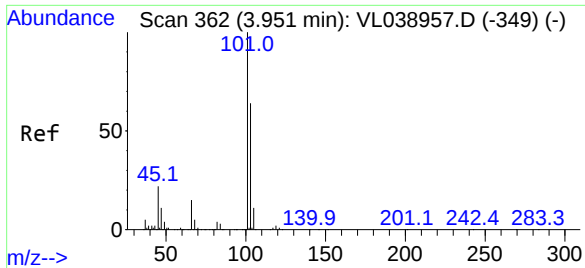

#11
 Trichlorofluoromethane
 Concen: 0.298 ppbv
 RT: 3.944 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VL038993.D
 Acq: 9 May 2022 19:04




Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

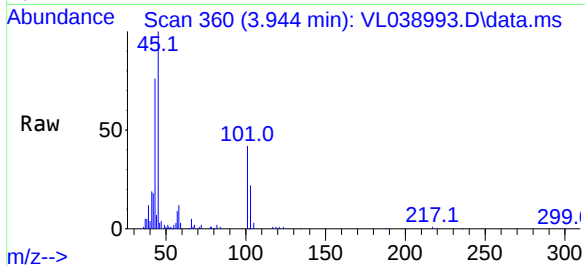


Tgt Ion:101 Resp: 43930
 Ion Ratio Lower Upper
 101 100
 103 53.2 51.5 77.3

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/11/2022

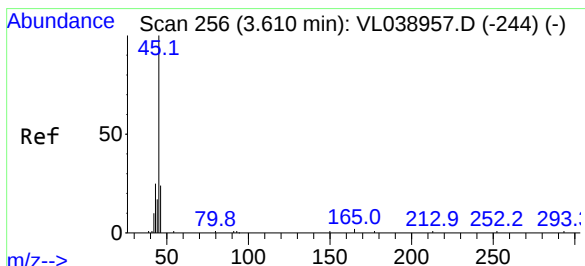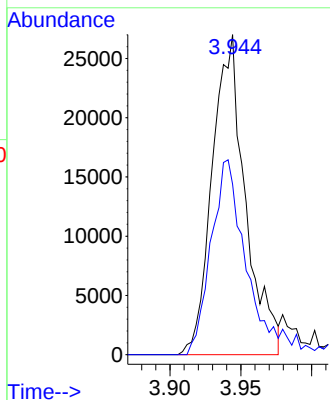


#13
 Ethanol
 Concen: 88.776 ppbv m
 RT: 3.590 min Scan# 250
 Delta R.T. -0.019 min
 Lab File: VL038993.D
 Acq: 9 May 2022 19:04

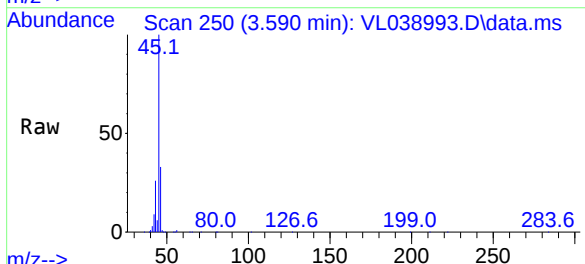


Tgt Ion: 45 Resp: 373720
 Ion Ratio Lower Upper
 45 100
 46 38.1 18.0 72.2

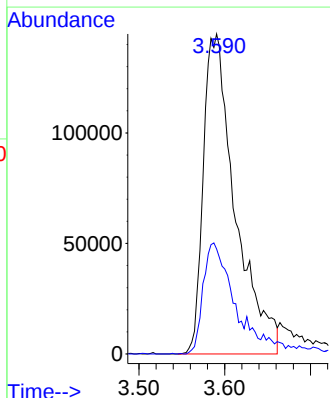

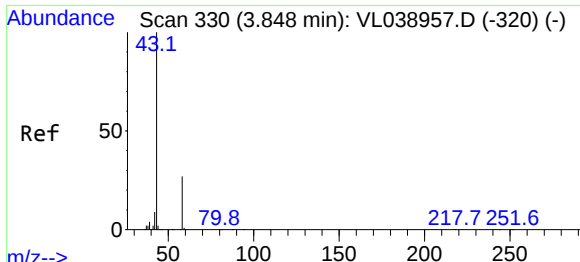

#15
Acetone
Concen: 23.431 ppbv m
RT: 3.832 min Scan# 31
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 43 Resp: 242626
Ion Ratio Lower Upper
43 100
58 34.5 21.3 31.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

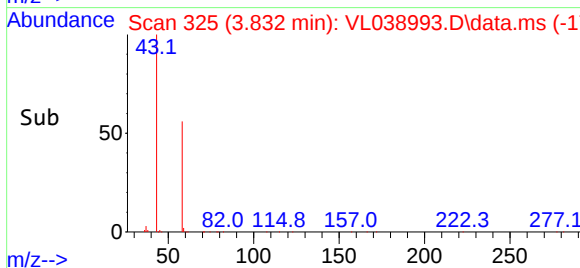

#19
Isopropyl Alcohol
Concen: 4.856 ppbv
RT: 3.954 min Scan# 363
Delta R.T. -0.003 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04


Tgt Ion: 45 Resp: 239065
Ion Ratio Lower Upper
45 100
58 349.8 1.4 2.2

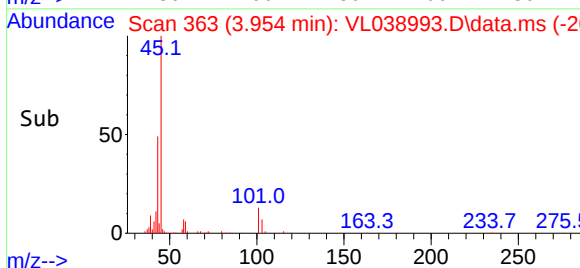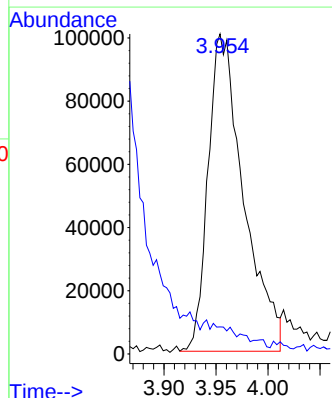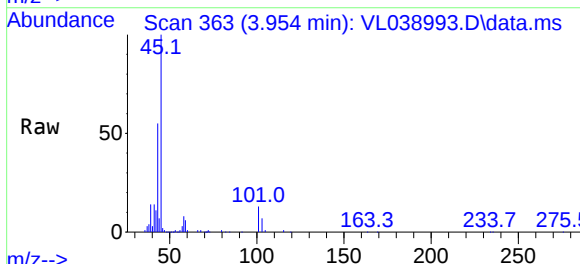



#20
Methylene Chloride
Concen: 7.231 ppbv
RT: 4.330 min Scan# 41
Delta R.T. -0.013 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1

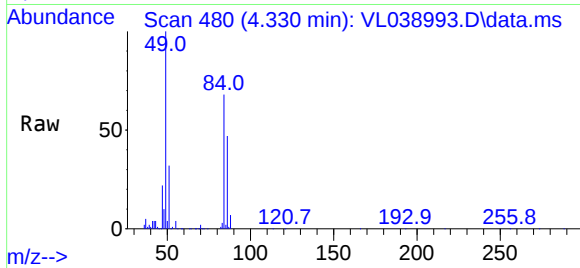


Tgt Ion: 84 Resp: 282198
Ion Ratio Lower Upper
84 100
49 146.0 119.9 179.9
51 46.3 35.7 53.5
86 68.4 53.8 80.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

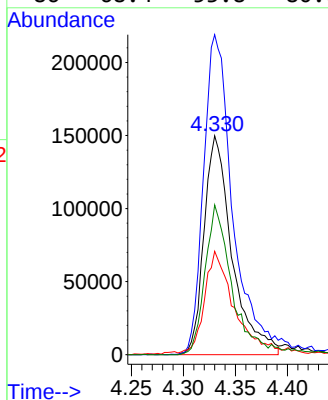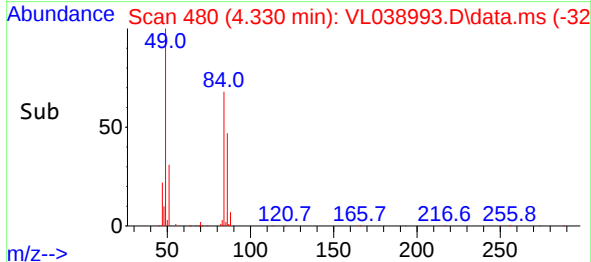


#26
Hexane
Concen: 6.154 ppbv
RT: 5.668 min Scan# 896
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

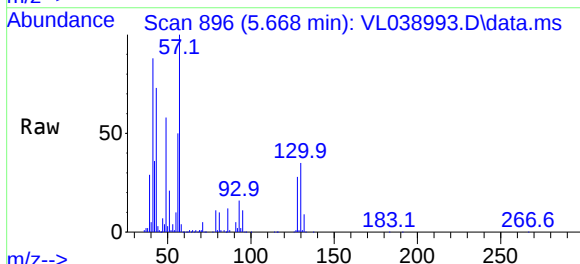


Tgt Ion: 57 Resp: 677741
Ion Ratio Lower Upper
57 100
41 97.4 75.2 112.8
43 74.5 190.8 286.2#
56 55.3 43.0 64.6

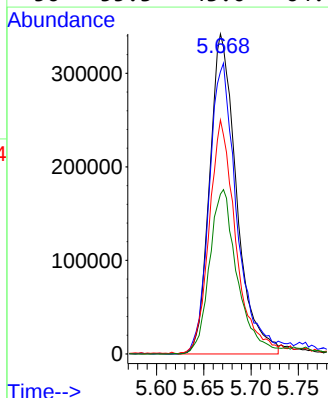



#29
Chloroform
Concen: 0.121 ppbv m
RT: 5.735 min Scan# 917
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1

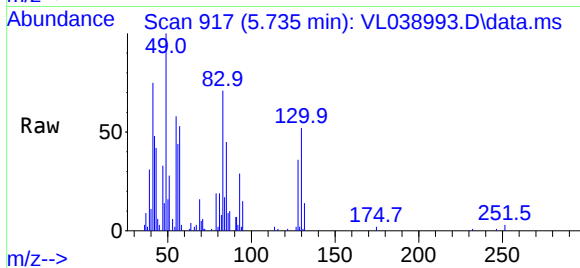


Tgt Ion: 83 Resp: 2147
Ion Ratio Lower Upper
83 100
85 63.9 51.8 77.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

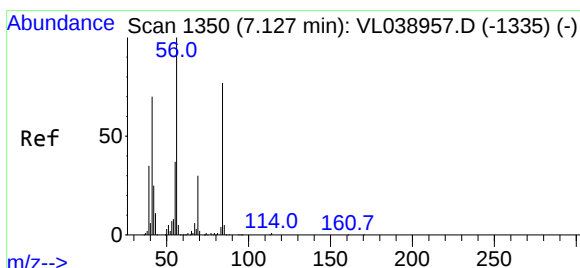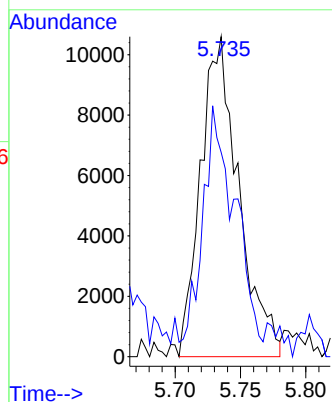


#30
Cyclohexane
Concen: 0.693 ppbv m
RT: 7.111 min Scan# 1345
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Tgt Ion: 84 Resp: 63876
Ion Ratio Lower Upper
84 100
56 114.0 115.3 172.9#
41 88.6 72.0 108.0

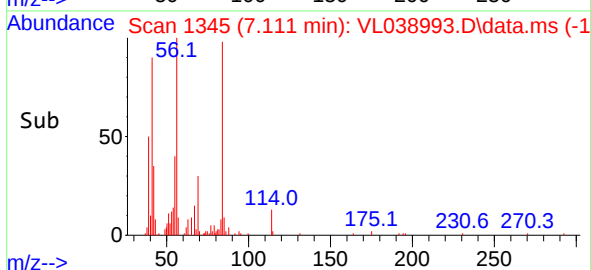



#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.153 min Scan# 11
Delta R.T. -0.019 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion:114 Resp: 251116
Ion Ratio Lower Upper
114 100
63 29.2 22.6 33.8
88 19.6 15.4 23.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022




#34
2-Butanone
Concen: 0.694 ppbv
RT: 5.230 min Scan# 760
Delta R.T. -0.010 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

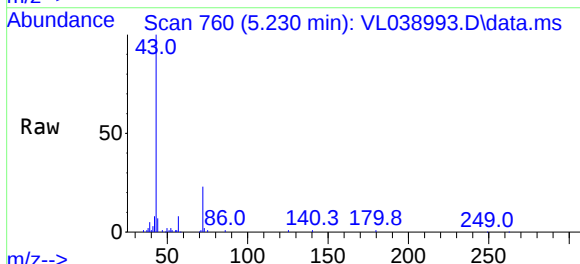


Tgt Ion: 43 Resp: 88965
Ion Ratio Lower Upper
43 100
72 27.1 17.8 26.6#

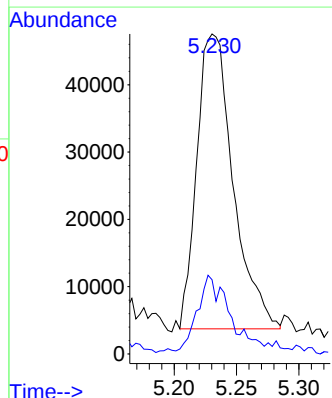

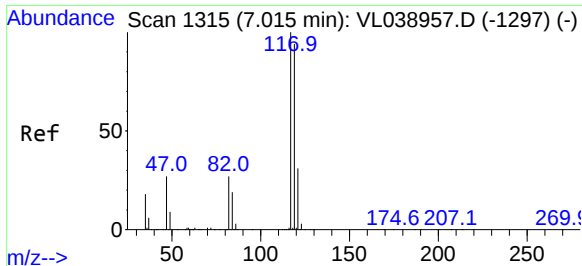

#35
Carbon Tetrachloride
Concen: 0.063 ppbv m
RT: 7.002 min Scan# 117
Delta R.T. -0.013 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1

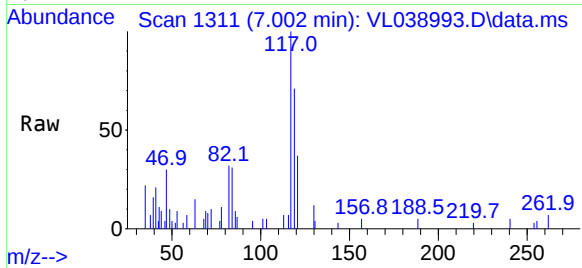


Tgt Ion: 117 Resp: 1036
Ion Ratio Lower Upper
117 100
119 70.7 75.2 112.8
121 36.8 24.6 37.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

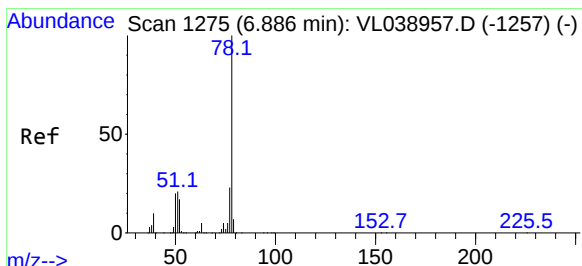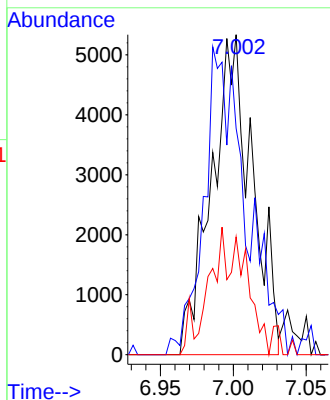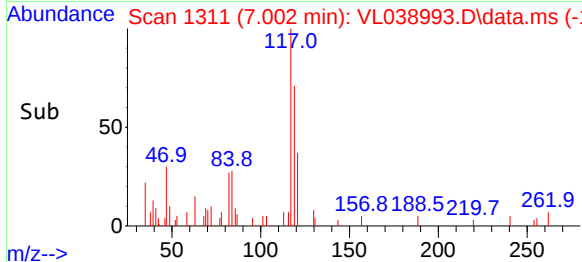


#36
Benzene
Concen: 1.797 ppbv
RT: 6.867 min Scan# 1269
Delta R.T. -0.019 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

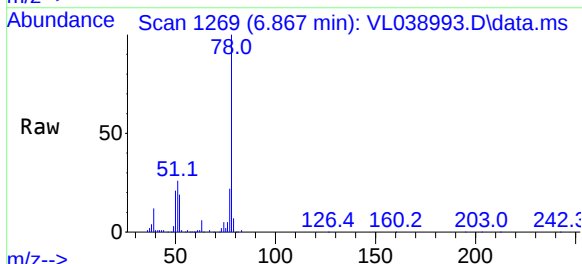


Tgt Ion: 78 Resp: 386201
Ion Ratio Lower Upper
78 100
77 21.0 18.6 28.0
50 20.7 15.6 23.4

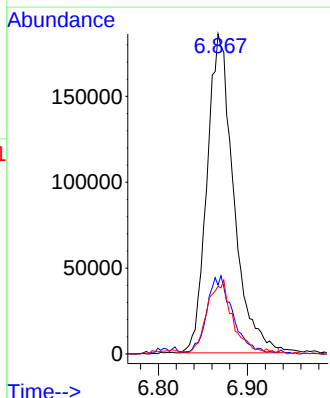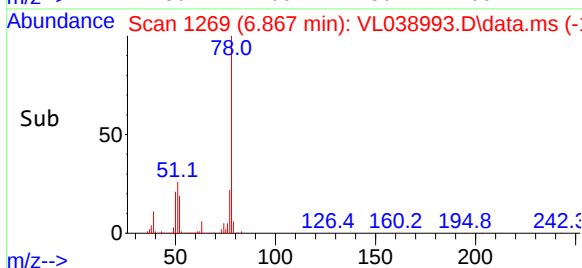



#44
2,2,4-Trimethylpentane
Concen: 0.299 ppbv
RT: 7.848 min Scan# 11265
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion: 57 Resp: 11265
Ion Ratio Lower Upper
57 100
41 51.3 26.3 39.5
56 51.1 24.6 37.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

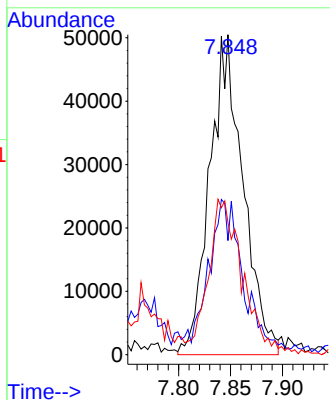


#52
Tetrachloroethene
Concen: 0.117 ppbv m
RT: 11.201 min Scan# 2617
Delta R.T. -0.010 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

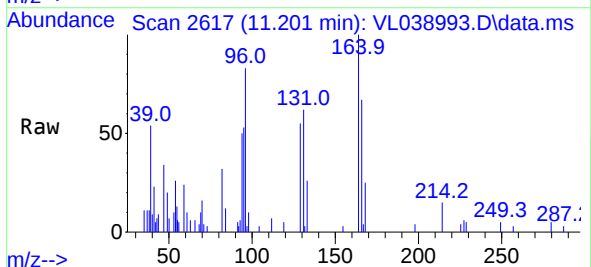


Tgt Ion:164 Resp: 8973
Ion Ratio Lower Upper
164 100
166 67.0 102.5 153.7#
129 54.7 90.1 135.1#
131 62.0 84.8 127.2#

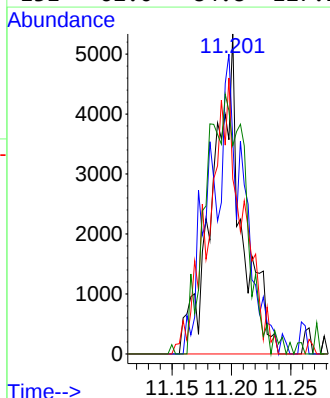

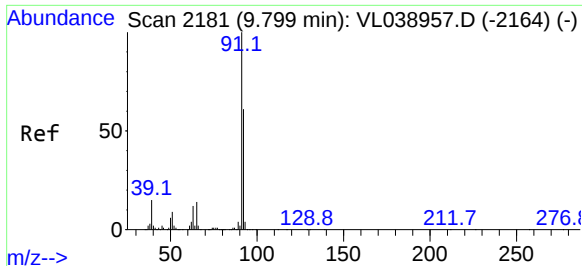

#53
Toluene
Concen: 6.642 ppbv
RT: 9.780 min Scan# 2181
Delta R.T. -0.019 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1

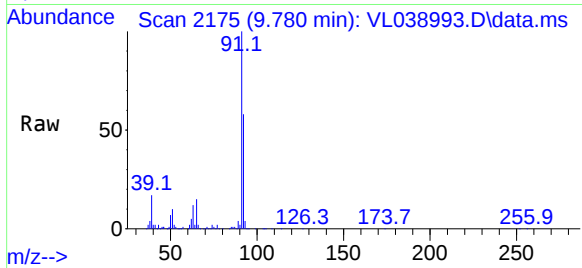


Tgt Ion: 91 Resp: 159982
Ion Ratio Lower Upper
91 100
92 59.6 48.2 72.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

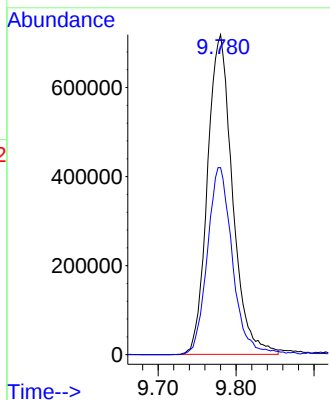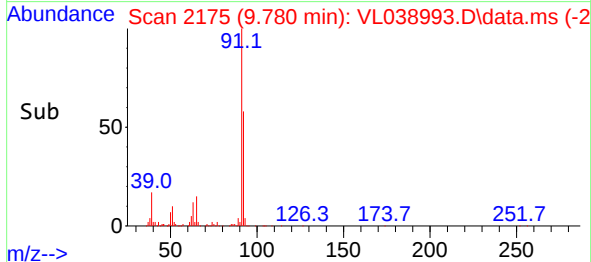


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.056 min Scan# 2883
Delta R.T. -0.019 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

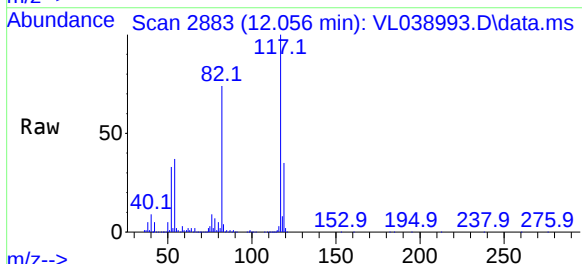


Tgt Ion:117 Resp: 2090526
Ion Ratio Lower Upper
117 100
82 77.7 57.0 85.6
119 35.2 27.2 40.8

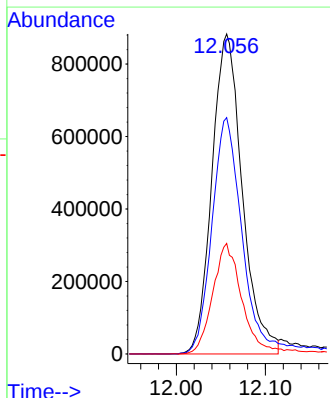



#58
Ethyl Benzene
Concen: 0.899 ppbv m
RT: 12.677 min Scan# 3083
Delta R.T. -0.023 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion: 91 Resp: 27043
Ion Ratio Lower Upper
91 100
106 27.2 24.2 36.4

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

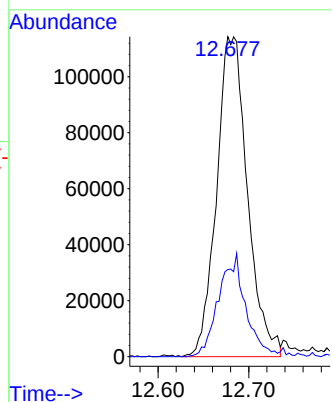


#59
m/p-Xylene
Concen: 3.511 ppbv m
RT: 12.934 min Scan# 3156
Delta R.T. -0.052 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

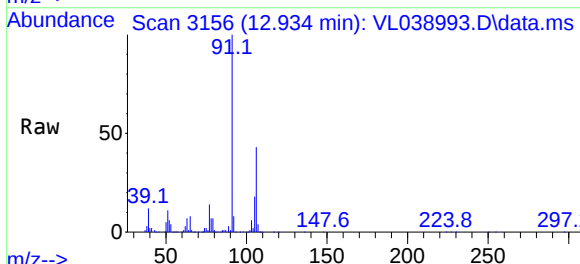

Tgt Ion: 91 Resp: 901807
Ion Ratio Lower Upper
91 100
106 0.0 34.6 52.0#









#60
o-Xylene
Concen: 1.209 ppbv
RT: 13.661 min Scan# 31
Delta R.T. -0.019 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion: 91 Resp: 292354
Ion Ratio Lower Upper
91 100
106 42.1 22.2 66.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022



#61
Styrene
Concen: 0.151 ppbv m
RT: 13.494 min Scan# 3330
Delta R.T. -0.023 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

Tgt Ion:104 Resp: 19468
Ion Ratio Lower Upper
104 100
78 0.0 46.4 69.6#
103 0.0 39.3 58.9#

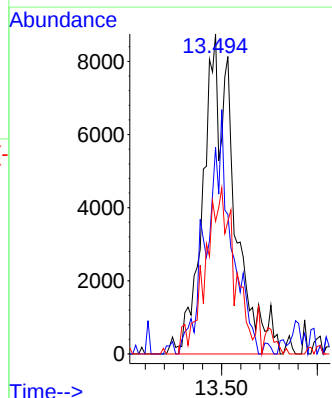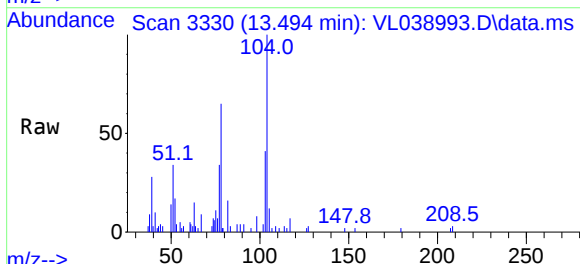







#64
n-propylbenzene
Concen: 0.263 ppbv m
RT: 15.526 min Scan# 3962
Delta R.T. -0.023 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion:120 Resp: 2249
Ion Ratio Lower Upper
120 100
91 541.3 400.6 601.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

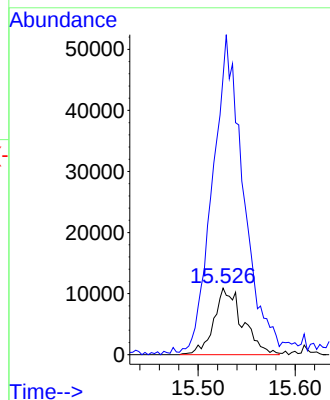

#68
1-Bromo-4-Fluorobenzene
Concen: 10.431 ppbv
RT: 14.384 min Scan# 3607
Delta R.T. -0.019 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04


Tgt Ion: 95 Resp: 1726910
Ion Ratio Lower Upper
95 100
174 65.1 50.8 76.2
175 4.5 3.8 5.6

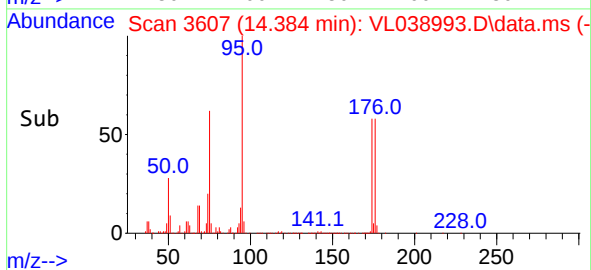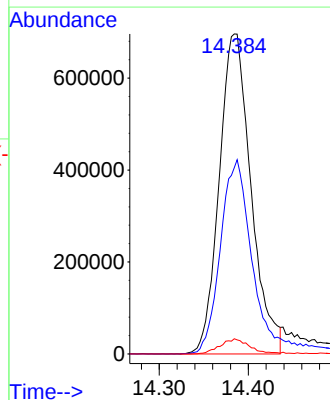



#69
p-Isopropyltoluene
Concen: 0.128 ppbv m
RT: 17.629 min Scan# 4616
Delta R.T. -0.010 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion:119 Resp: 45854
Ion Ratio Lower Upper
119 100
134 30.8 20.0 30.0
91 35.1 24.8 37.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

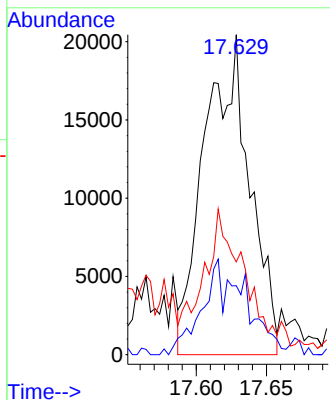


#72
4-Ethyltoluene
Concen: 0.549 ppbv
RT: 15.805 min Scan# 4049
Delta R.T. -0.023 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

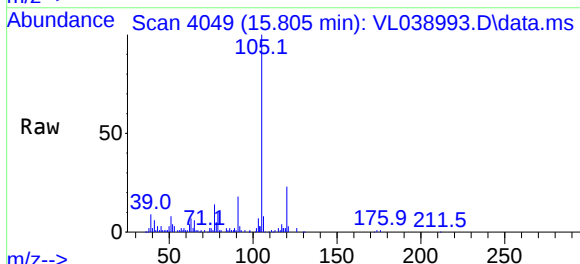

Tgt Ion:105 Resp: 151144
Ion Ratio Lower Upper
105 100
120 30.0 23.4 35.0
91 16.8 10.6 16.0
77 17.3 12.5 18.7

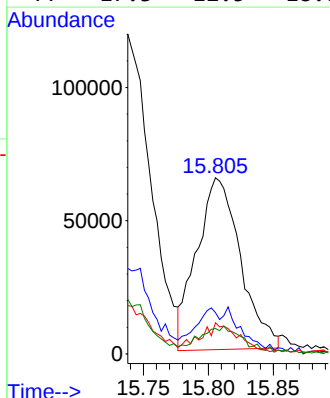







#73
1,3,5-Trimethylbenzene
Concen: 0.448 ppbv m
RT: 15.960 min Scan# 4097
Delta R.T. -0.026 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion:105 Resp: 111100
Ion Ratio Lower Upper
105 100
120 32.6 34.4 51.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022



#74
1,2,4-Trimethylbenzene
Concen: 1.468 ppbv m
RT: 16.731 min Scan# 4337
Delta R.T. -0.016 min
Lab File: VL038993.D
Acq: 9 May 2022 19:04


Tgt Ion:105 Resp: 398487
Ion Ratio Lower Upper
105 100
120 43.0 36.9 55.3
91 13.6 45.0 67.4#
77 15.9 19.2 28.8#

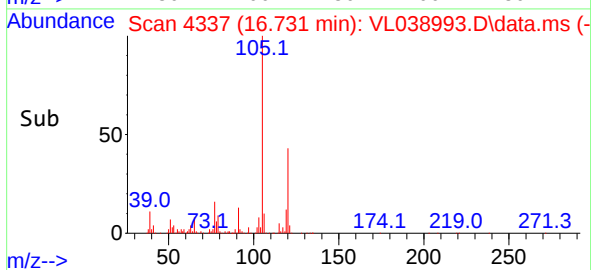



#76
 1,4-Dichlorobenzene
 Concen: 0.143 ppbv m
 RT: 17.101 min Scan# 44
 Delta R.T. -0.019 min
 Lab File: VL038993.D
 Acq: 9 May 2022 19:04

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

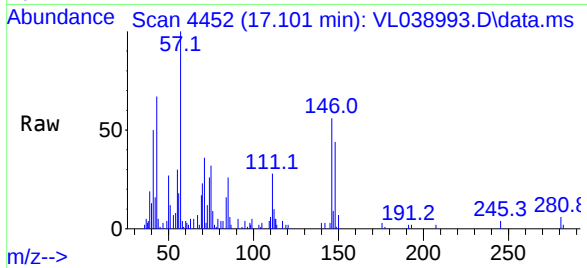

Tgt Ion:	146	Resp:	2091
Ion	Ratio	Lower	Upper
146	100		
111	0.0	23.6	71.0
148	73.1	32.2	96.6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/11/2022

