

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050922\
 Data File : VL038997.D
 Acq On : 9 May 2022 21:43
 Operator : SY/AP
 Sample : N2744-01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/11/2022

Quant Time: May 10 05:47:17 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LThu May 05 10:12:15 2022

QLast Update : Thu May 05 10:12:15 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Bromochloromethane	5.648	49	1231637	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.156	114	3372337	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.057	117	3000810	10.000	ppbv	-0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 14.384 95 2389639 10.055 ppbv -0.02
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.600%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	3.044	85	31097	0.161	ppbv #	87
4) Chloromethane	3.131	50	58121	0.759	ppbv	93
9) Propene	3.002	41	7515403	112.604	ppbv	91
10) Heptane	8.105	43	6009232	36.700	ppbv	100
11) Trichlorofluoromethane	3.938	101	45522m	0.275	ppbv	
13) Ethanol	3.623	45	26091019	5524.023	ppbv	99
15) Acetone	3.832	43	2274051	19.574	ppbv #	26
20) Methylene Chloride	4.333	84	271912	6.210	ppbv	98
26) Hexane	5.674	57	8082027	65.413	ppbv #	40
27) Carbon Disulfide	4.536	76	514288	4.382	ppbv #	93
30) Cyclohexane	7.111	84	2014687	19.476	ppbv	93
34) 2-Butanone	5.221	43	3782821	21.987	ppbv	99
36) Benzene	6.870	78	4517025	15.652	ppbv	98
41) Tetrahydrofuran	6.028	42	364589	3.153	ppbv	98
44) 2,2,4-Trimethylpentane	7.854	57	18360748	36.257	ppbv #	78
50) 4-Methyl-2-Pentanone	8.719	43	1041098	3.451	ppbv	99
51) 2-Hexanone	10.095	43	2538840	11.530	ppbv #	61
52) Tetrachloroethene	11.211	164	11129852	107.919	ppbv	90
53) Toluene	9.790	91	18911538	58.465	ppbv #	84
58) Ethyl Benzene	12.684	91	7625419	17.657	ppbv	95
59) m/p-Xylene	12.941	91	16229264	44.021	ppbv #	86
60) o-Xylene	13.661	91	6607269	19.041	ppbv	94
61) Styrene	13.497	104	61580m	0.332	ppbv	
62) Isopropylbenzene	14.638	105	784650	1.546	ppbv	99
64) n-propylbenzene	15.536	120	382625m	3.119	ppbv	
70) n-Butylbenzene	18.526	91	292700m	0.537	ppbv	
72) 4-Ethyltoluene	15.806	105	1724667	4.362	ppbv	98
73) 1,3,5-Trimethylbenzene	15.960	105	1215114	3.414	ppbv	99
74) 1,2,4-Trimethylbenzene	16.728	105	3752374	9.627	ppbv #	67
79) Naphthalene	22.162	128	35277m	0.111	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050922\
Data File : VL038997.D
Acq On : 9 May 2022 21:43
Operator : SY/AP
Sample : N2744-01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SV1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022


Quant Time: May 10 05:47:17 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LThu May
QLast Update : Thu May 05 10:12:15 2022
Response via : Initial Calibration

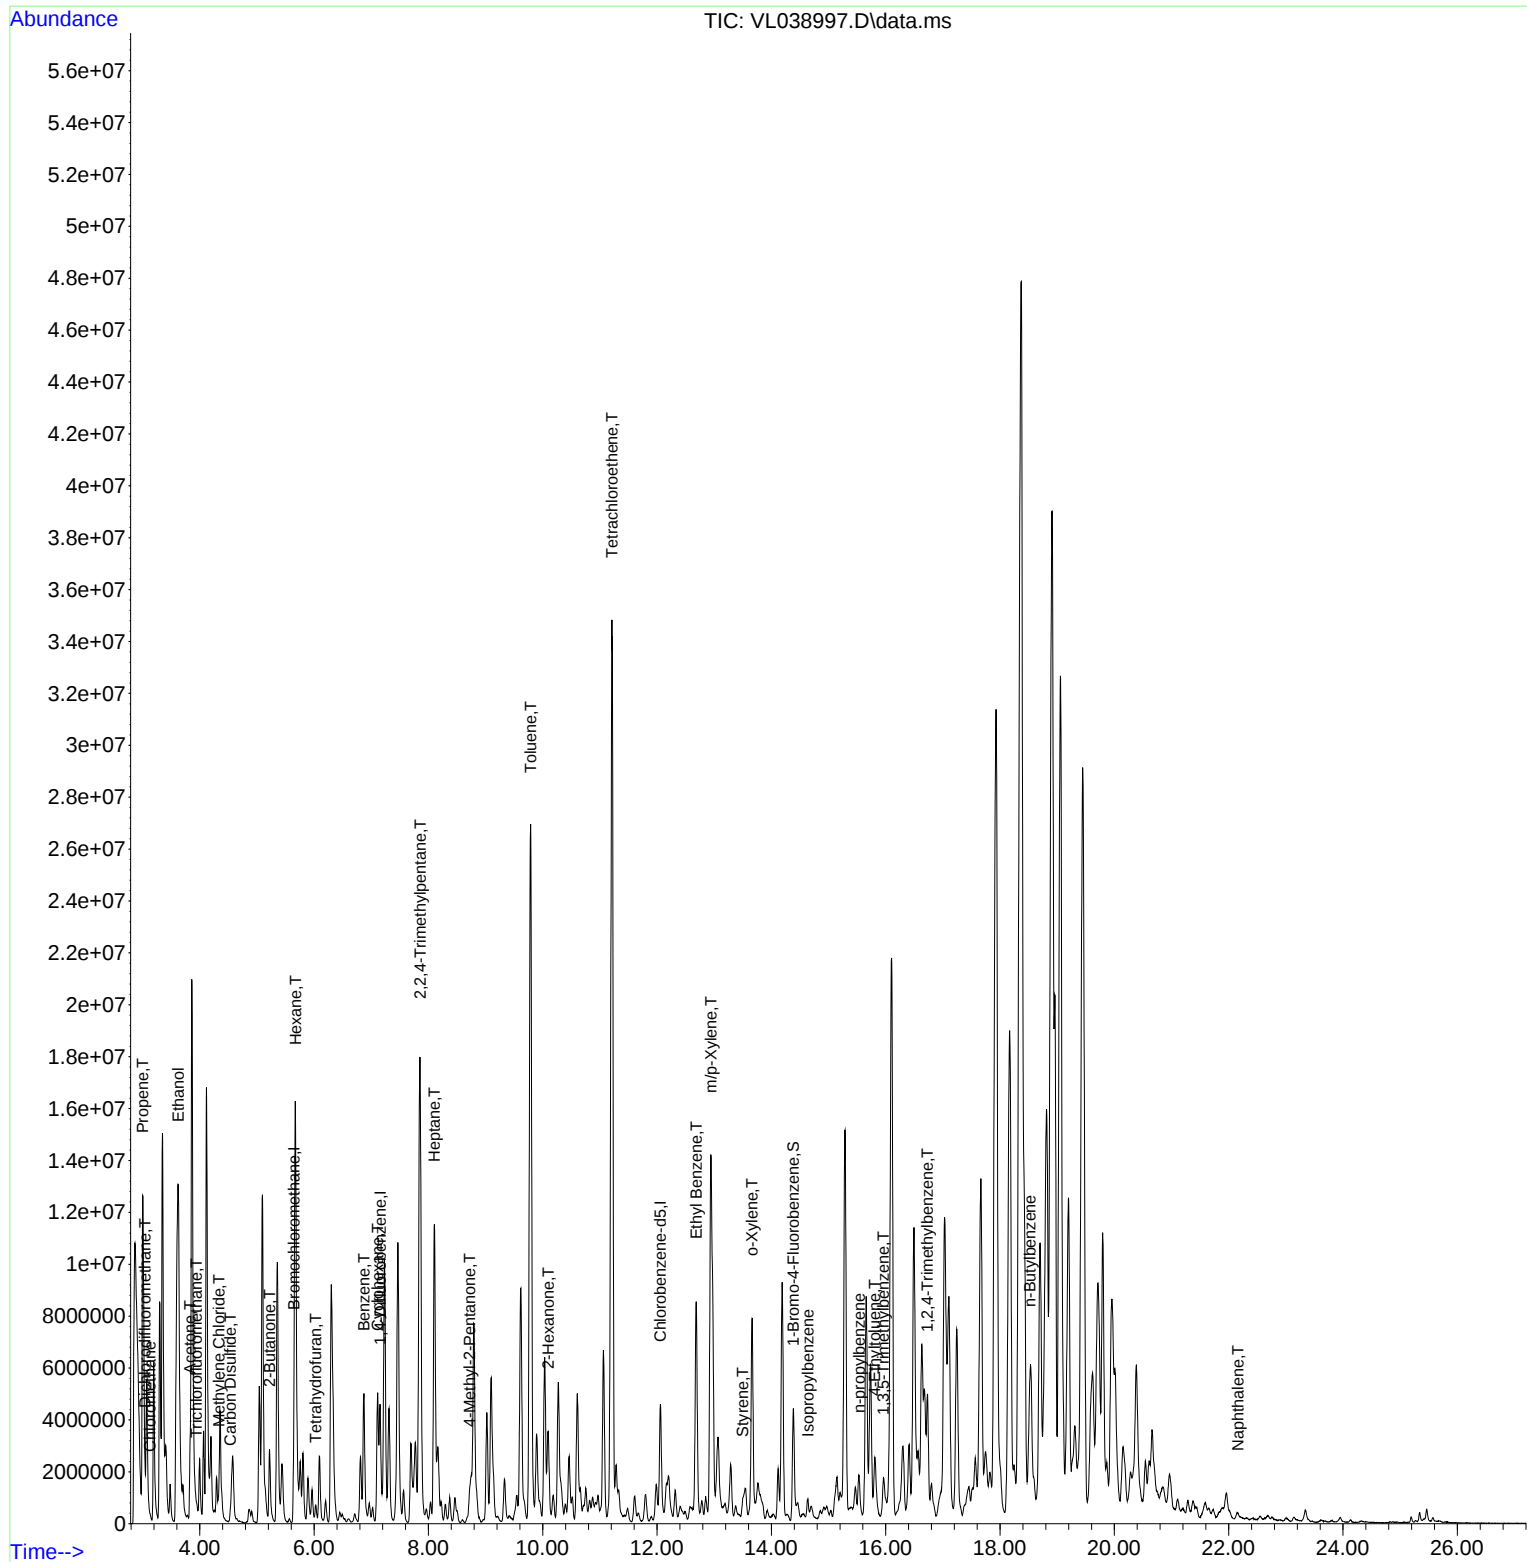



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.648 min Scan# 80
Delta R.T. -0.016 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1



Tgt Ion: 49 Resp: 123163
Ion Ratio Lower Upper
49 100
128 48.1 23.3 69.8
130 60.7 29.8 89.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022



#2
Dichlorodifluoromethane
Concen: 0.161 ppbv
RT: 3.044 min Scan# 80
Delta R.T. -0.006 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Tgt Ion: 85 Resp: 31097
Ion Ratio Lower Upper
85 100
87 39.6 25.7 38.5

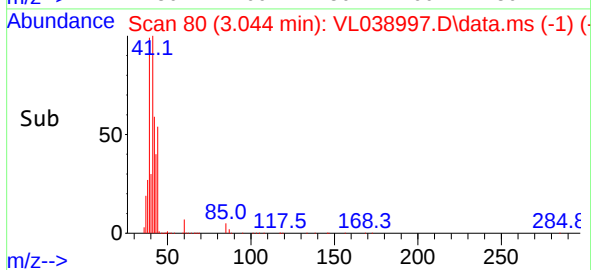

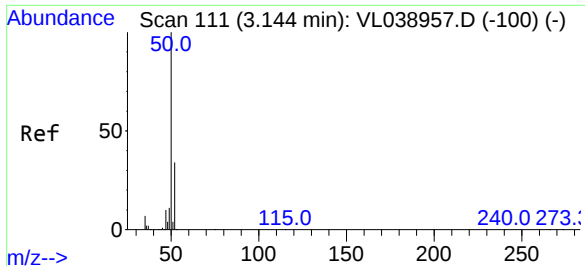





#4
Chloromethane
Concen: 0.759 ppbv
RT: 3.131 min Scan# 107
Delta R.T. -0.013 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion: 50 Resp: 5812
Ion Ratio Lower Upper
50 100
52 30.4 27.3 40.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

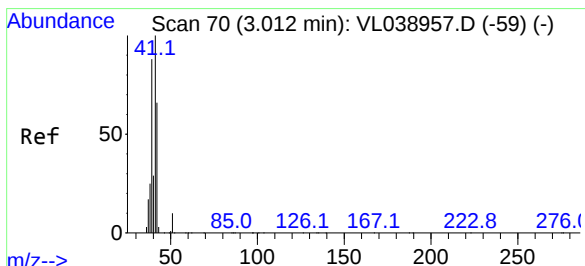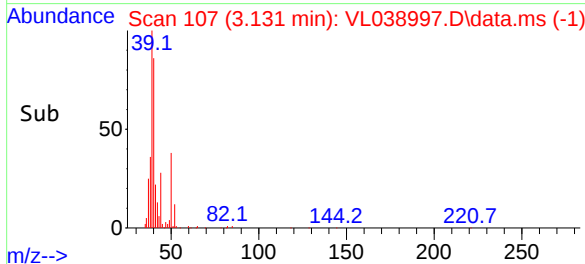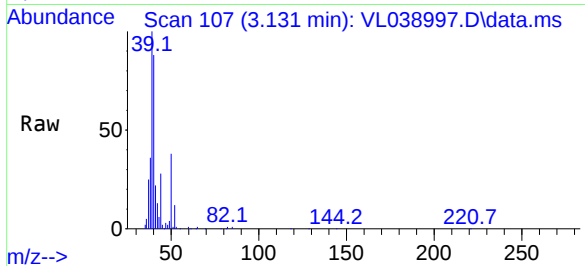

#9
Propene
Concen: 112.604 ppbv
RT: 3.002 min Scan# 67
Delta R.T. -0.010 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43


Tgt Ion: 41 Resp: 7515403
Ion Ratio Lower Upper
41 100
42 65.1 58.3 87.5

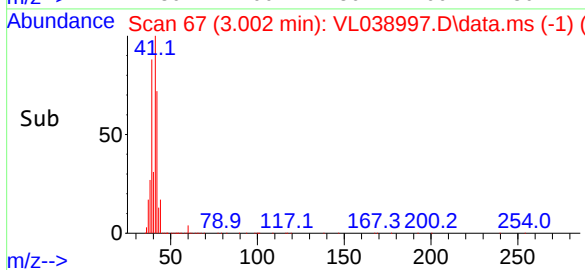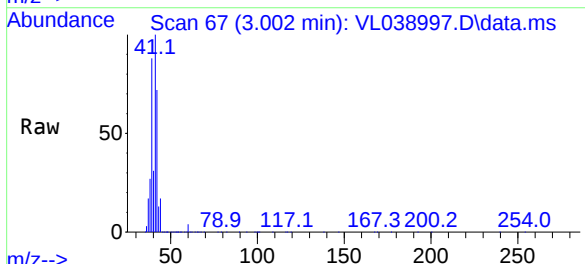



#10
Heptane
Concen: 36.700 ppbv
RT: 8.105 min Scan# 11
Delta R.T. -0.010 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1



Tgt Ion: 43 Resp: 600923
Ion Ratio Lower Upper
43 100
57 50.6 40.5 60.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022



#11
Trichlorofluoromethane
Concen: 0.275 ppbv m
RT: 3.938 min Scan# 358
Delta R.T. -0.013 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Tgt Ion:101 Resp: 45522
Ion Ratio Lower Upper
101 100
103 56.3 51.5 77.3

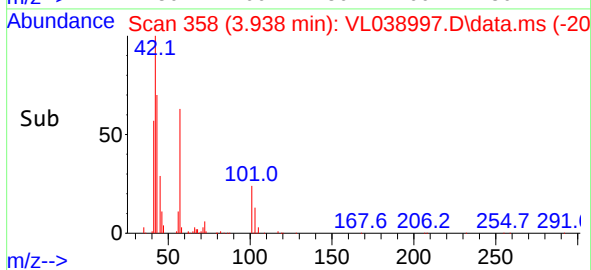







#13
Ethanol
Concen: 5524.023 ppbv
RT: 3.623 min Scan# 210
Delta R.T. 0.013 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion: 45 Resp: 26091019
Ion Ratio Lower Upper
45 100
46 45.8 18.0 72.2




Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 05/10/2022
Supervised By : Mahesh Dadoda 05/11/2022



#15
Acetone
Concen: 19.574 ppbv
RT: 3.832 min Scan# 325
Delta R.T. -0.016 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43


Tgt Ion: 43 Resp: 2274051
Ion Ratio Lower Upper
43 100
58 64.8 21.3 31.9#

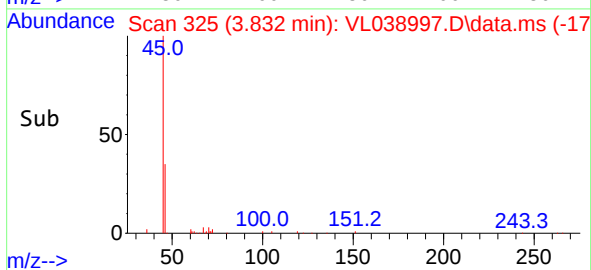

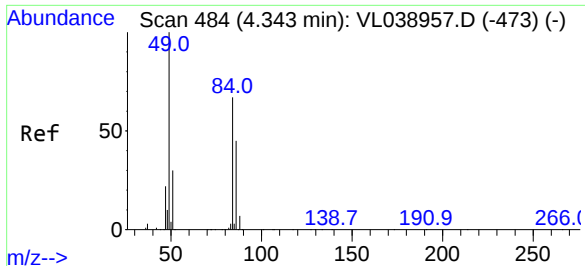

#20
Methylene Chloride
Concen: 6.210 ppbv
RT: 4.333 min Scan# 481
Delta R.T. -0.010 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1

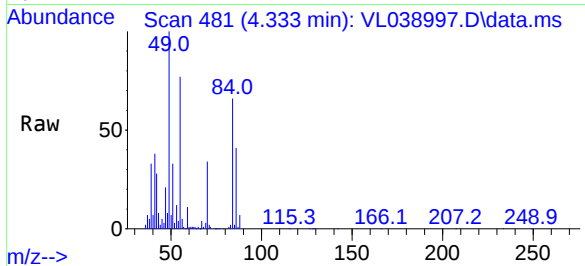


Tgt Ion: 84 Resp: 271912
Ion Ratio Lower Upper
84 100
49 149.9 119.9 179.9
51 43.8 35.7 53.5
86 62.0 53.8 80.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

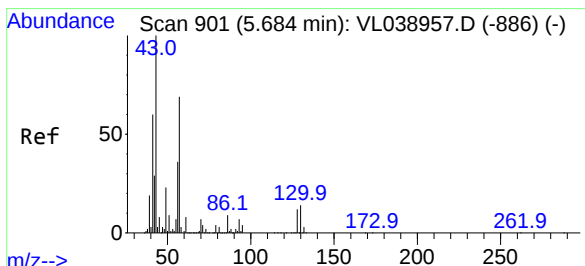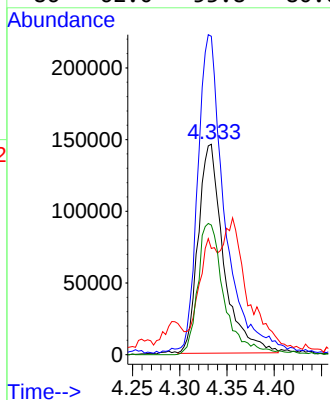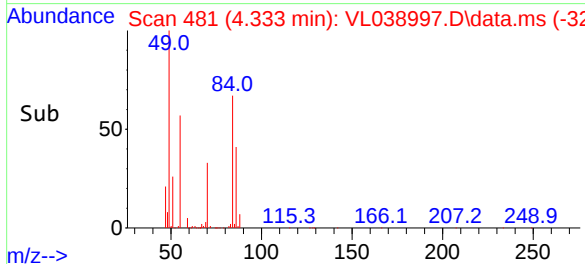


#26
Hexane
Concen: 65.413 ppbv
RT: 5.674 min Scan# 898
Delta R.T. -0.010 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

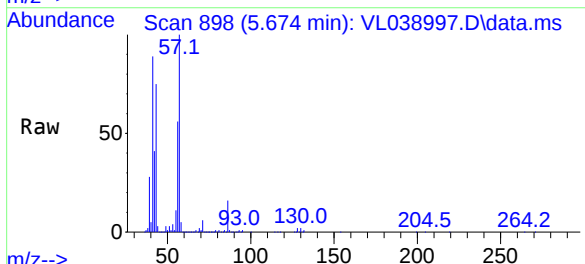


Tgt Ion: 57 Resp: 8082027
Ion Ratio Lower Upper
57 100
41 91.9 75.2 112.8
43 77.4 190.8 286.2#
56 55.5 43.0 64.6

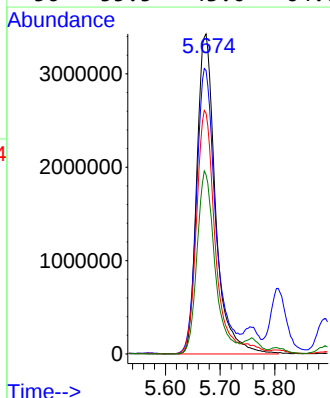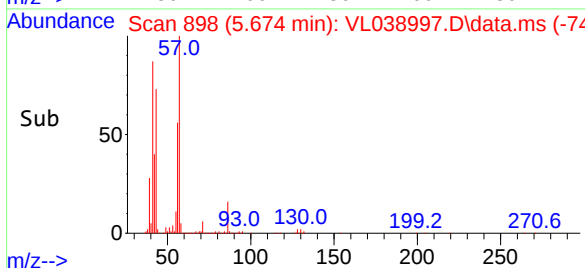

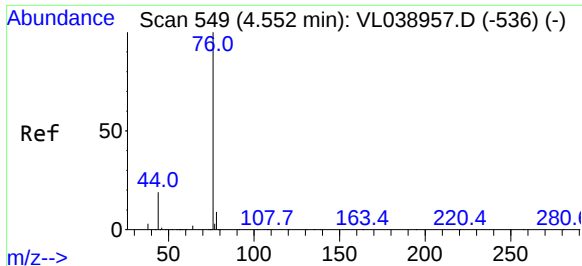

#27
Carbon Disulfide
Concen: 4.382 ppbv
RT: 4.536 min Scan# 54
Delta R.T. -0.016 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1

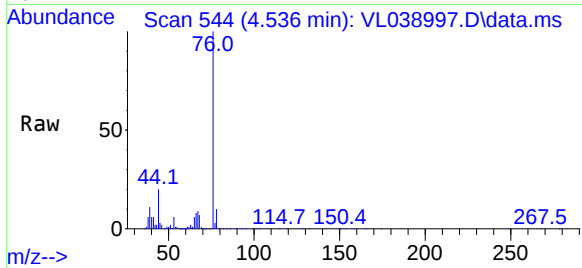


Tgt Ion: 76 Resp: 51428
Ion Ratio Lower Upper
76 100
44 23.8 15.3 22.9
78 10.0 8.2 12.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

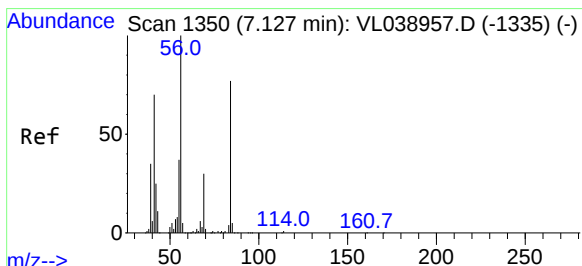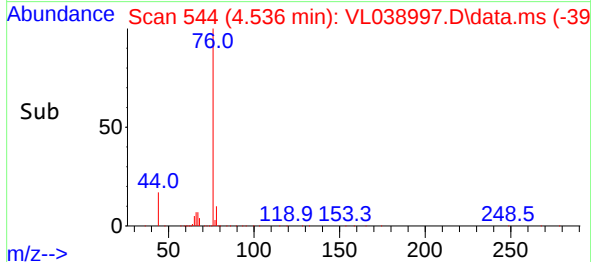


#30
Cyclohexane
Concen: 19.476 ppbv
RT: 7.111 min Scan# 1345
Delta R.T. -0.016 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

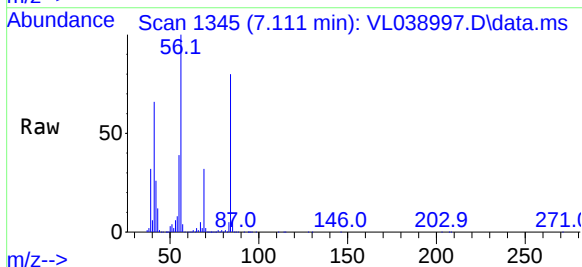


Tgt Ion: 84 Resp: 2014687
Ion Ratio Lower Upper
84 100
56 134.7 115.3 172.9
41 83.3 72.0 108.0

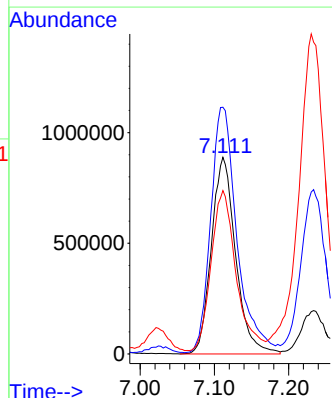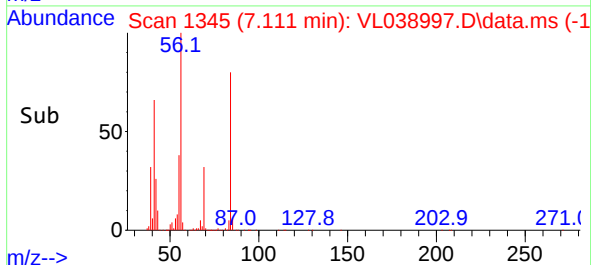



#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.156 min Scan# 11
Delta R.T. -0.016 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1




Tgt Ion:114 Resp: 337233
Ion Ratio Lower Upper
114 100
63 26.0 22.6 33.8
88 18.0 15.4 23.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022




#34
2-Butanone
Concen: 21.987 ppbv
RT: 5.221 min Scan# 757
Delta R.T. -0.019 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Tgt Ion: 43 Resp: 3782821
Ion Ratio Lower Upper
43 100
72 22.7 17.8 26.6

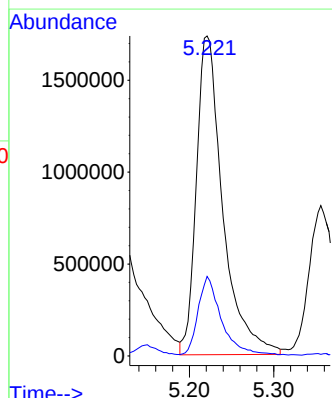

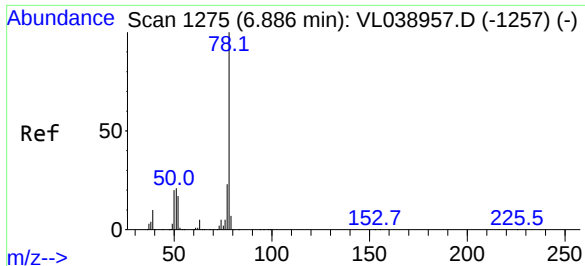

#36
Benzene
Concen: 15.652 ppbv
RT: 6.870 min Scan# 1008
Delta R.T. -0.016 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Instrument :
MSVOA_L
ClientSampleId :
SV1



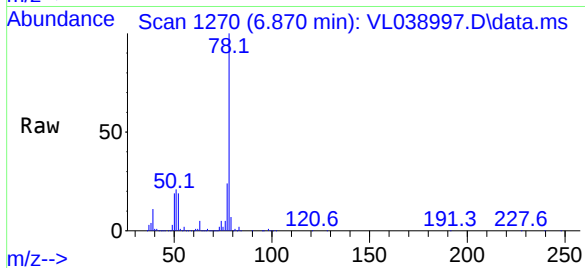


Tgt Ion: 78 Resp: 451702

Ion	Ratio	Lower	Upper
78	100		
77	23.9	18.6	28.0
50	18.6	15.6	23.4

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

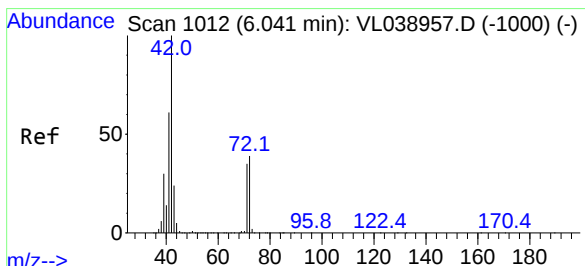


#41
Tetrahydrofuran
Concen: 3.153 ppbv
RT: 6.028 min Scan# 1008
Delta R.T. -0.013 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Tgt Ion: 42 Resp: 364589


Ion	Ratio	Lower	Upper
42	100		
72	41.4	31.8	47.6
71	39.2	30.6	45.8

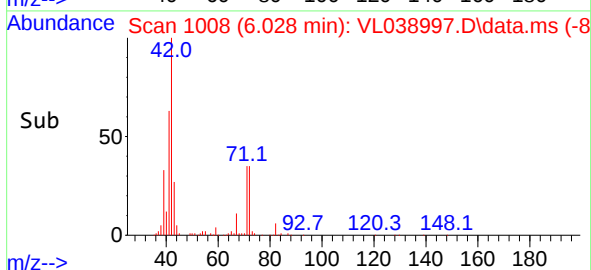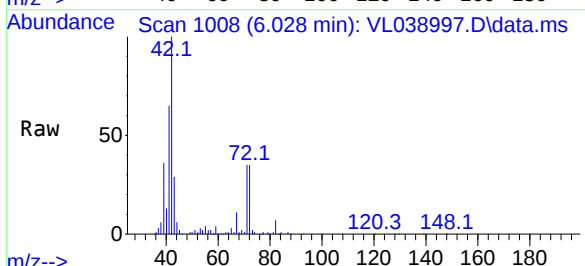



#44
2,2,4-Trimethylpentane
Concen: 36.257 ppbv
RT: 7.854 min Scan# 11
Delta R.T. -0.010 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Instrument :
MSVOA_L
ClientSampleId :
SV1






Tgt Ion: 57 Resp:1836074


Ion	Ratio	Lower	Upper
57	100		
41	43.4	26.3	39.5
56	44.9	24.6	37.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

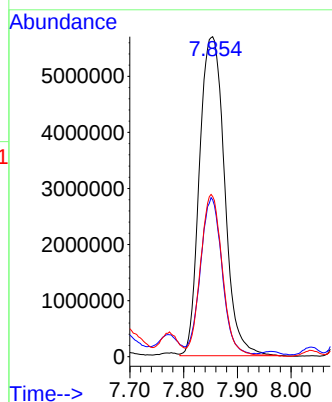




#50
4-Methyl-2-Pentanone
Concen: 3.451 ppbv
RT: 8.719 min Scan# 1845
Delta R.T. -0.013 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43



Tgt Ion: 43 Resp: 1041098

Ion	Ratio	Lower	Upper
43	100		
58	35.8	28.4	42.6

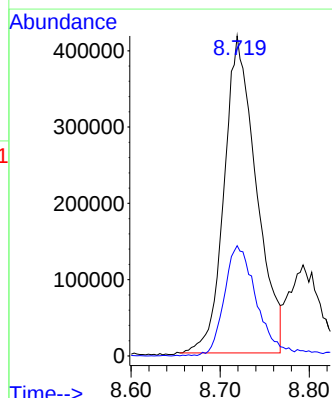







#51
2-Hexanone
Concen: 11.530 ppbv
RT: 10.095 min Scan# 21
Delta R.T. -0.026 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion: 43 Resp: 2538840
Ion Ratio Lower Upper
43 100
58 22.6 39.3 58.9
98 0.0 0.2 0.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

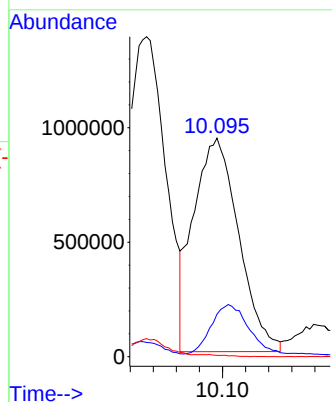

#52
Tetrachloroethene
Concen: 107.919 ppbv
RT: 11.211 min Scan# 2620
Delta R.T. 0.000 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43


Tgt Ion:164 Resp:11129852
Ion Ratio Lower Upper
164 100
166 117.3 102.5 153.7
129 99.0 90.1 135.1
131 96.7 84.8 127.2

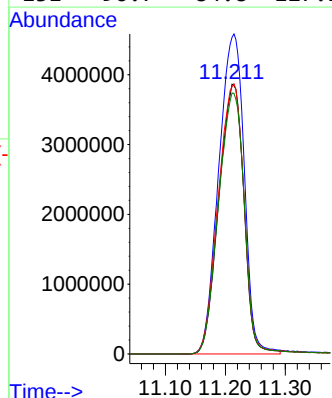



#53
Toluene
Concen: 58.465 ppbv
RT: 9.790 min Scan# 2181
Delta R.T. -0.010 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1




Tgt Ion: 91 Resp: 18911538
Ion Ratio Lower Upper
91 100
92 72.3 48.2 72.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.057 min Scan# 2883
Delta R.T. -0.019 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43



Tgt Ion: 117 Resp: 3000810
Ion Ratio Lower Upper
117 100
82 65.6 57.0 85.6
119 34.2 27.2 40.8

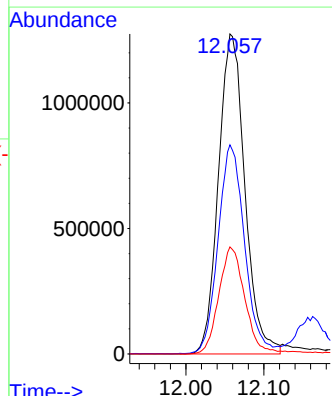



#58

Ethyl Benzene

Concen: 17.657 ppbv

RT: 12.684 min Scan# 3083

Delta R.T. -0.016 min

Lab File: VL038997.D

Acq: 9 May 2022 21:43

Instrument :

MSVOA_L

ClientSampleId :

SV1

Tgt Ion: 91 Resp: 7625419

Ion Ratio Lower Upper

91 100





106 33.2 24.2 36.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022

Supervised By :Mahesh Dadoda 05/11/2022

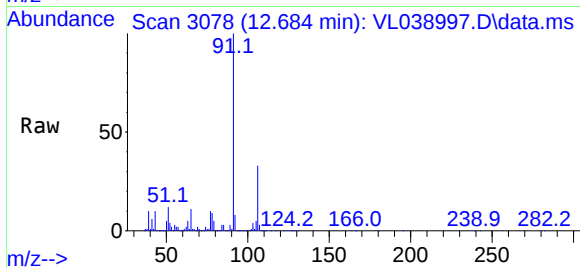

#59

m/p-Xylene

Concen: 44.021 ppbv

RT: 12.941 min Scan# 3158

Delta R.T. -0.045 min

Lab File: VL038997.D




Acq: 9 May 2022 21:43


Tgt Ion: 91 Resp:16229264

Ion Ratio Lower Upper

91 100

106 52.3 34.6 52.0#

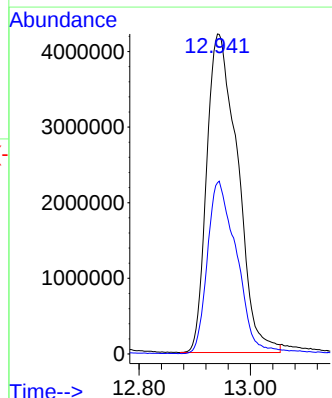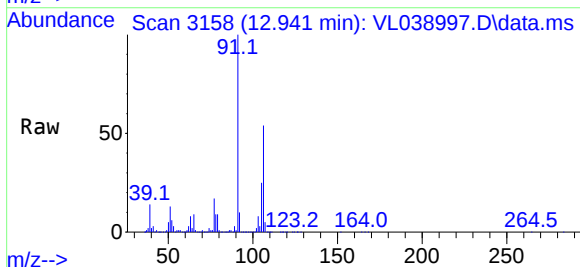







#60
o-Xylene
Concen: 19.041 ppbv
RT: 13.661 min Scan# 3382
Delta R.T. -0.019 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion: 91 Resp: 6607269
Ion Ratio Lower Upper
91 100
106 48.2 22.2 66.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022



#61
Styrene
Concen: 0.332 ppbv m
RT: 13.497 min Scan# 3331
Delta R.T. -0.019 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43


Tgt Ion:104 Resp: 61580
Ion Ratio Lower Upper
104 100
78 56.8 46.4 69.6
103 0.0 39.3 58.9#

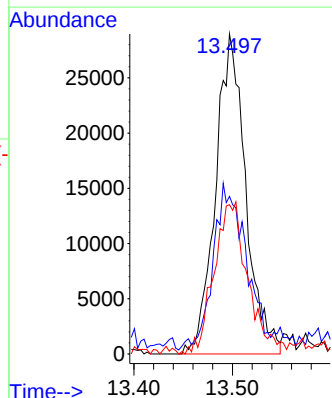



#62
Isopropylbenzene
Concen: 1.546 ppbv
RT: 14.638 min Scan# 30
Delta R.T. -0.016 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1




Tgt Ion:105 Resp: 784650
Ion Ratio Lower Upper
105 100
120 24.9 20.5 30.7

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

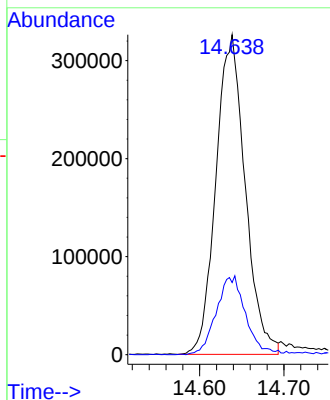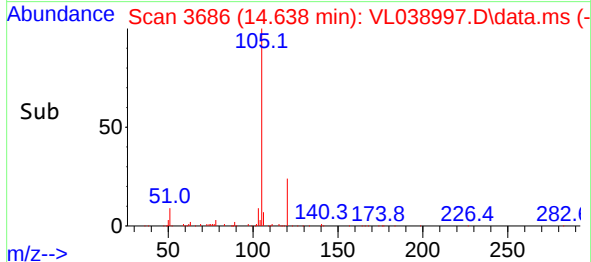


#64
n-propylbenzene
Concen: 3.119 ppbv m
RT: 15.536 min Scan# 3965
Delta R.T. -0.013 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Tgt Ion:120 Resp: 382625
Ion Ratio Lower Upper
120 100
91 0.0 400.6 601.0#

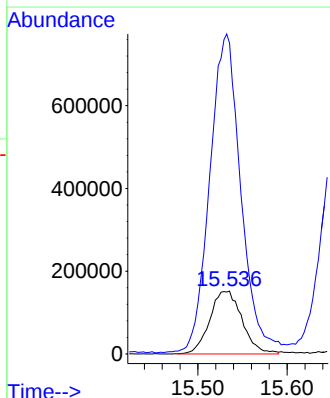



#68
1-Bromo-4-Fluorobenzene
Concen: 10.055 ppbv
RT: 14.384 min Scan# 30
Delta R.T. -0.019 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1




Tgt Ion: 95 Resp: 2389639
Ion Ratio Lower Upper
95 100
174 64.9 50.8 76.2
175 4.6 3.8 5.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

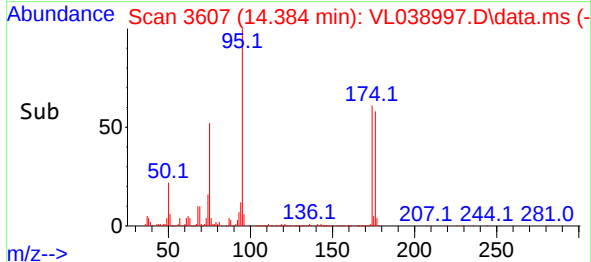


#70
n-Butylbenzene
Concen: 0.537 ppbv m
RT: 18.526 min Scan# 4895
Delta R.T. -0.010 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Tgt Ion: 91 Resp: 292700
Ion Ratio Lower Upper
91 100
92 0.0 43.1 64.7#
134 0.0 17.0 25.4#

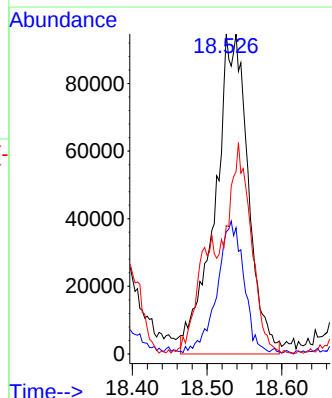



#72
4-Ethyltoluene
Concen: 4.362 ppbv
RT: 15.806 min Scan# 4056
Delta R.T. -0.022 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1




Tgt Ion:105 Resp: 172466
Ion Ratio Lower Upper
105 100
120 29.7 23.4 35.0
91 13.3 10.6 16.0
77 13.8 12.5 18.7

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022




#73
1,3,5-Trimethylbenzene
Concen: 3.414 ppbv
RT: 15.960 min Scan# 4097
Delta R.T. -0.026 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Tgt Ion:105 Resp: 1215114
Ion Ratio Lower Upper
105 100
120 43.3 34.4 51.6





#74
1,2,4-Trimethylbenzene
Concen: 9.627 ppbv
RT: 16.728 min Scan# 41
Delta R.T. -0.019 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43




Instrument :
MSVOA_L
ClientSampleId :
SV1




Tgt Ion:105 Resp: 3752374
Ion Ratio Lower Upper
105 100
120 42.5 36.9 55.3
91 11.5 45.0 67.4
77 13.7 19.2 28.8#

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/11/2022

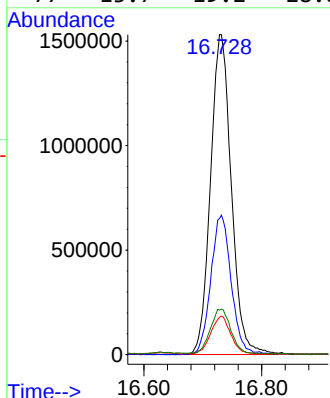

#79
Naphthalene
Concen: 0.111 ppbv m
RT: 22.162 min Scan# 6026
Delta R.T. -0.010 min
Lab File: VL038997.D
Acq: 9 May 2022 21:43



Tgt Ion:128 Resp: 35277
Ion Ratio Lower Upper
128 100
127 22.9 10.2 15.2#
129 4.4 8.9 13.3#

