

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050922\
 Data File : VL039000.D
 Acq On : 9 May 2022 23:42
 Operator : SY/AP
 Sample : N2744-02DL 5X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV2DL

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/11/2022

Quant Time: May 10 05:48:14 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LThu May 05 10:12:15 2022

QLast Update : Thu May 05 10:12:15 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Bromochloromethane	5.648	49	1278246	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.150	114	3437787	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.053	117	2948964	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.378	95	2244696	9.611	ppbv	-0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.100%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	3.041	85	21287m	0.106	ppbv	
9) Propene	3.002	41	794821	11.475	ppbv	87
10) Heptane	8.095	43	604168	3.555	ppbv	99
13) Ethanol	3.584	45	3375798	688.667	ppbv	89
15) Acetone	3.835	43	703366	5.833	ppbv #	64
17) tert-Butyl alcohol	4.282	59	75461m	0.814	ppbv	
20) Methylene Chloride	4.333	84	81946	1.803	ppbv	94
26) Hexane	5.671	57	884288	6.896	ppbv #	39
27) Carbon Disulfide	4.539	76	44518	0.365	ppbv #	88
30) Cyclohexane	7.108	84	182993	1.704	ppbv #	83
34) 2-Butanone	5.221	43	940309	5.361	ppbv	100
35) Carbon Tetrachloride	7.002	117	6827m	0.030	ppbv	
36) Benzene	6.864	78	444662	1.511	ppbv	97
41) Tetrahydrofuran	6.034	42	123066	1.044	ppbv	92
44) 2,2,4-Trimethylpentane	7.841	57	2496107	4.835	ppbv #	93
50) 4-Methyl-2-Pentanone	8.725	43	125164	0.407	ppbv	95
51) 2-Hexanone	10.105	43	390632m	1.740	ppbv	
52) Tetrachloroethene	11.188	164	910829	8.664	ppbv	94
53) Toluene	9.774	91	3224171	9.778	ppbv	99
58) Ethyl Benzene	12.677	91	1027464	2.421	ppbv	97
59) m/p-Xylene	12.934	91	2711580	7.484	ppbv	93
60) o-Xylene	13.658	91	1006216	2.951	ppbv	99
62) Isopropylbenzene	14.629	105	92751	0.186	ppbv	97
64) n-propylbenzene	15.529	120	63491	0.527	ppbv	94
70) n-Butylbenzene	18.526	91	73281m	0.137	ppbv	
72) 4-Ethyltoluene	15.802	105	367277	0.945	ppbv #	97
73) 1,3,5-Trimethylbenzene	15.963	105	275029	0.786	ppbv	97
74) 1,2,4-Trimethylbenzene	16.722	105	1025187	2.677	ppbv #	66
79) Naphthalene	22.159	128	51075m	0.164	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050922\
Data File : VL039000.D
Acq On : 9 May 2022 23:42
Operator : SY/AP
Sample : N2744-02DL 5X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SV2DL

Quant Time: May 10 05:48:14 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May
QLast Update : Thu May 05 10:12:15 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 05/11/2022
Supervised By : Mahesh Dadoda 05/11/2022

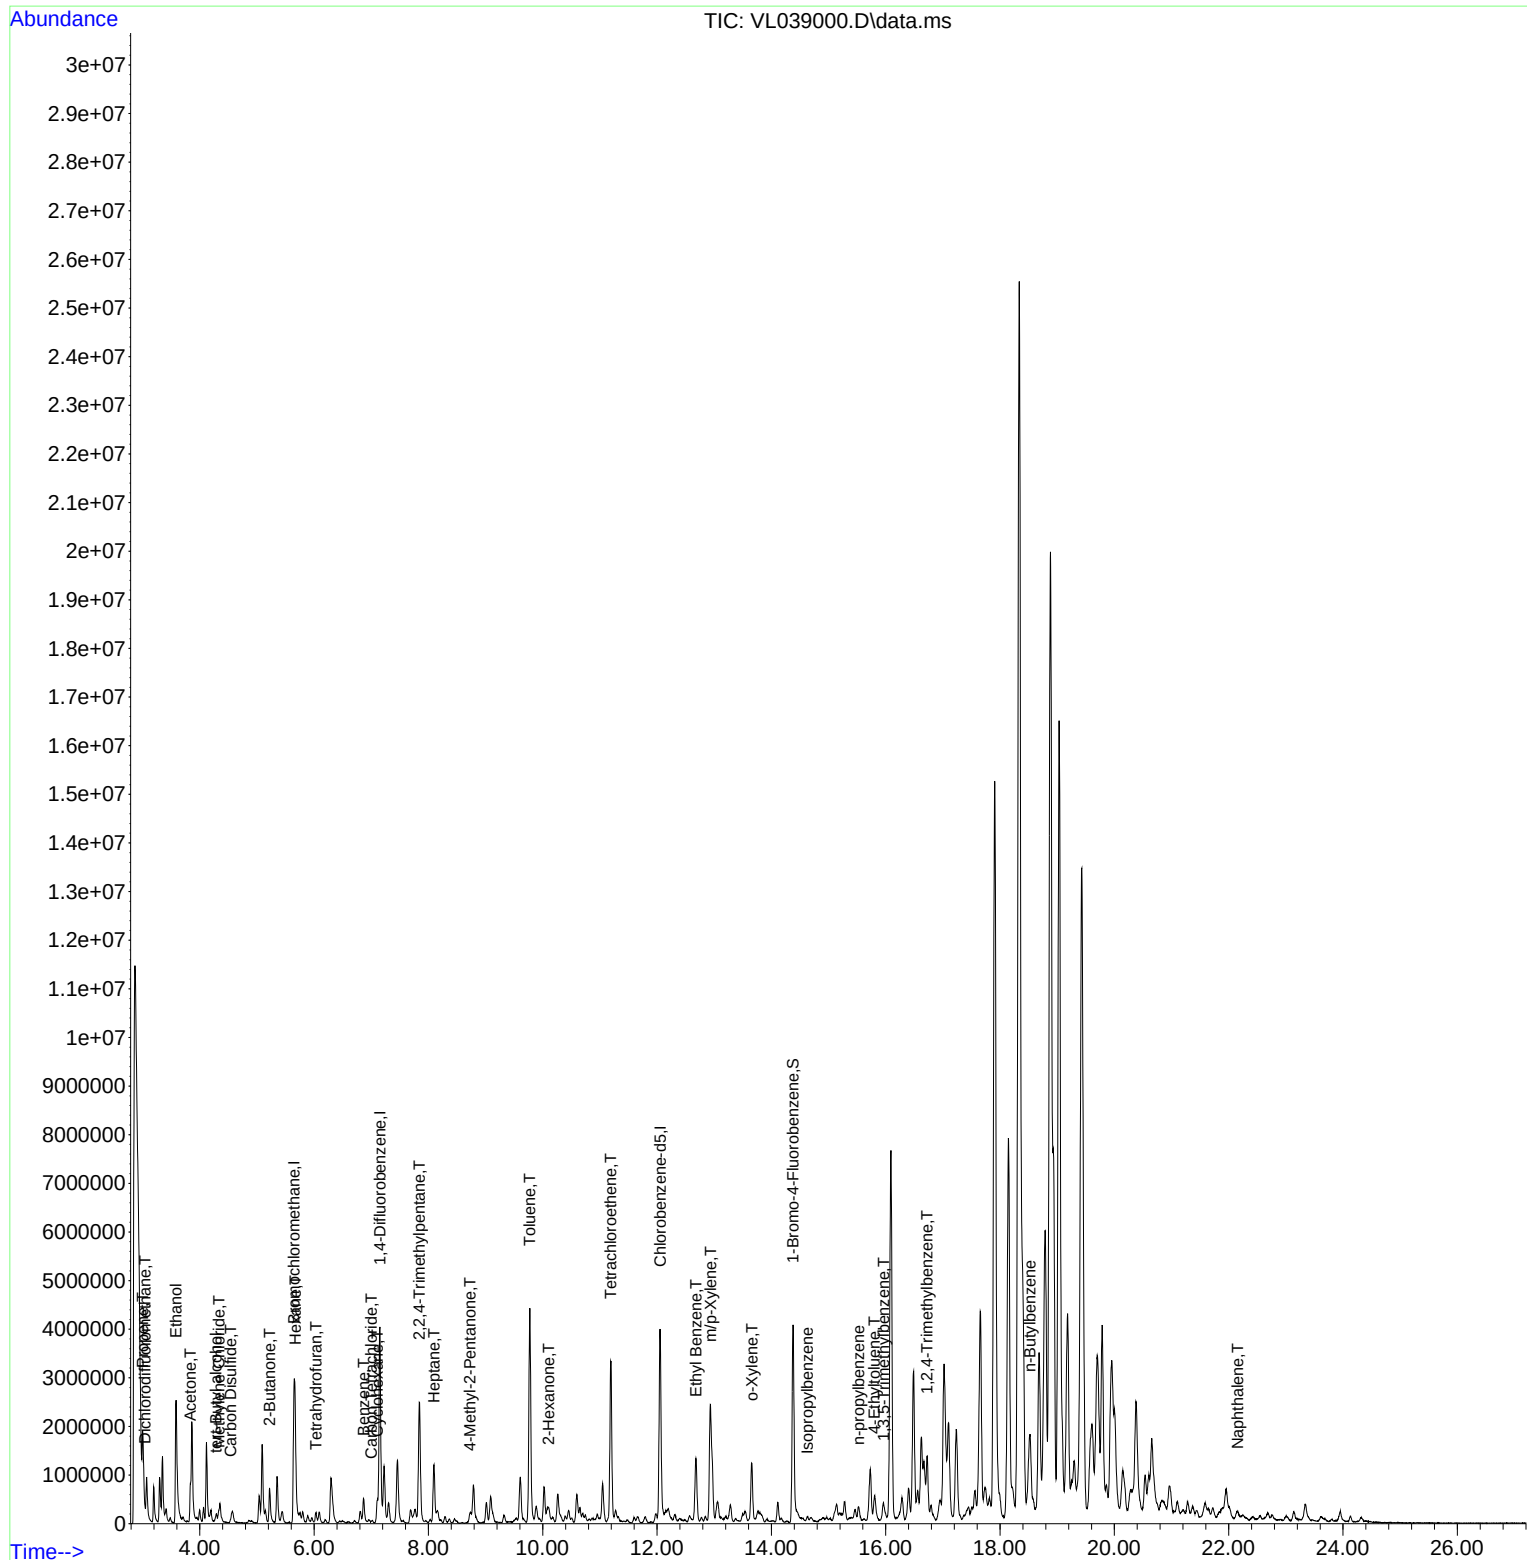

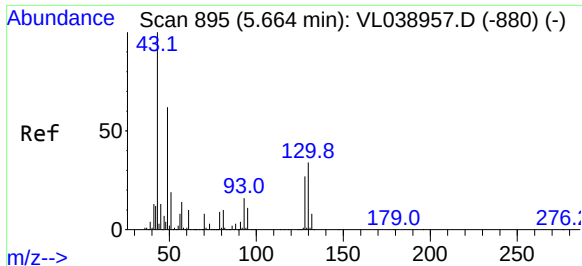

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.648 min Scan# 89
Delta R.T. -0.016 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL

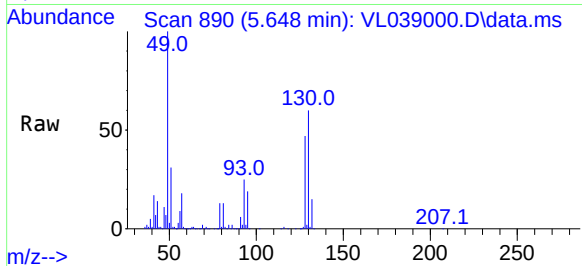

Tgt Ion: 49 Resp: 1278240
Ion Ratio Lower Upper
49 100
128 48.9 23.3 69.8
130 62.6 29.8 89.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

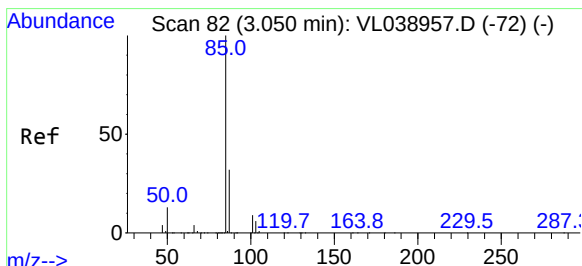

#2
Dichlorodifluoromethane
Concen: 0.106 ppbv m
RT: 3.041 min Scan# 79
Delta R.T. -0.010 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42


Tgt Ion: 85 Resp: 21287
Ion Ratio Lower Upper
85 100
87 40.9 25.7 38.5#

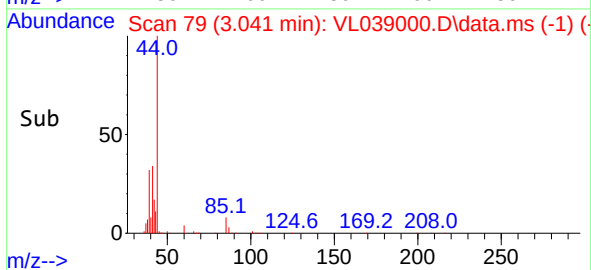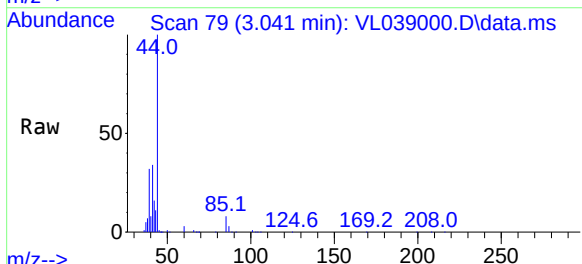

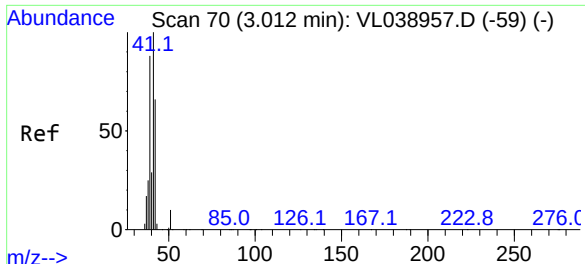

#9
Propene
Concen: 11.475 ppbv
RT: 3.002 min Scan# 61
Delta R.T. -0.010 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL

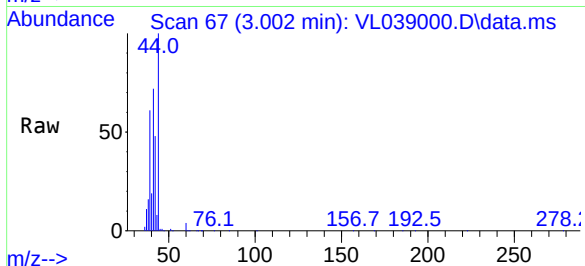

Tgt Ion: 41 Resp: 79482
Ion Ratio Lower Upper
41 100
42 61.9 58.3 87.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

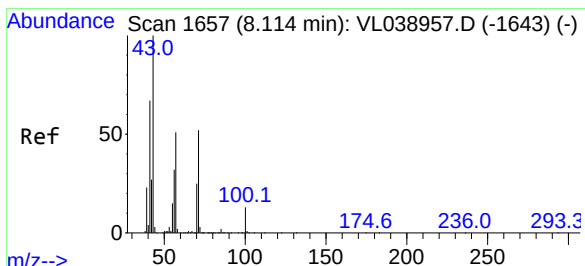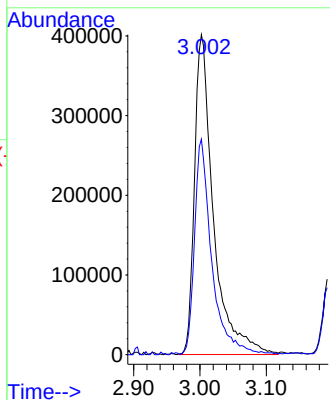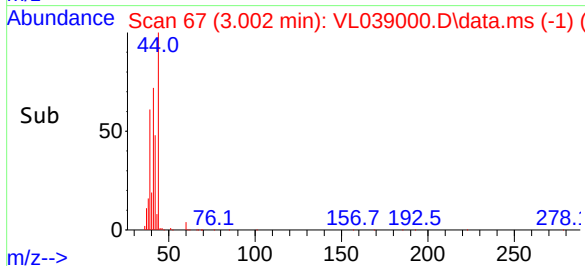

#10
Heptane
Concen: 3.555 ppbv
RT: 8.095 min Scan# 1651
Delta R.T. -0.019 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42



Tgt Ion: 43 Resp: 604168
Ion Ratio Lower Upper
43 100
57 49.6 40.5 60.7

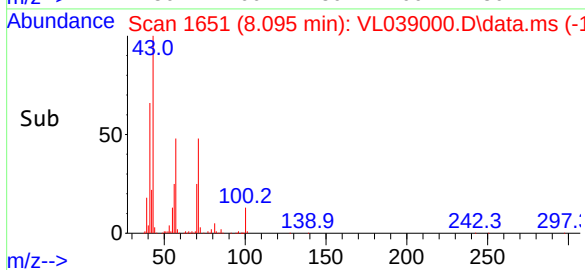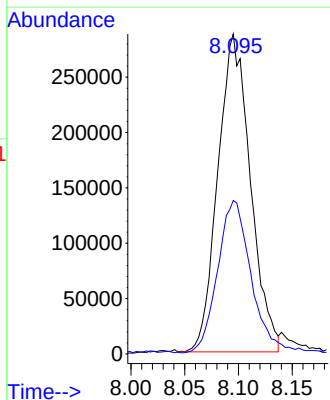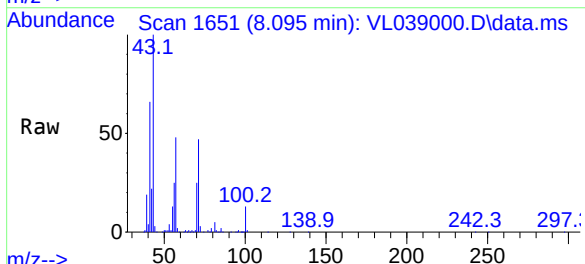



#13
Ethanol
Concen: 688.667 ppbv
RT: 3.584 min Scan# 248
Delta R.T. -0.026 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42



Instrument :
MSVOA_L
ClientSampleId :
SV2DL





Tgt Ion: 45 Resp: 3375798
Ion Ratio Lower Upper
45 100
46 37.9 18.0 72.2

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

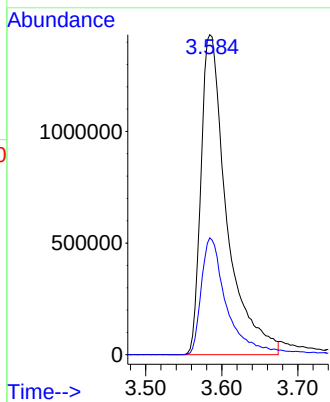


#15
Acetone
Concen: 5.833 ppbv
RT: 3.835 min Scan# 326
Delta R.T. -0.013 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

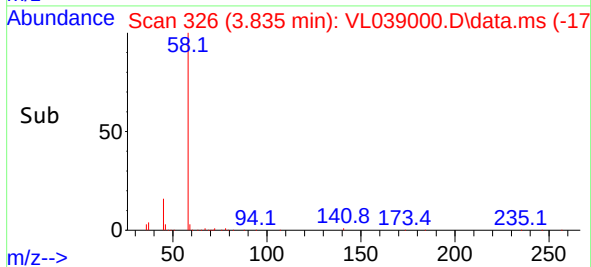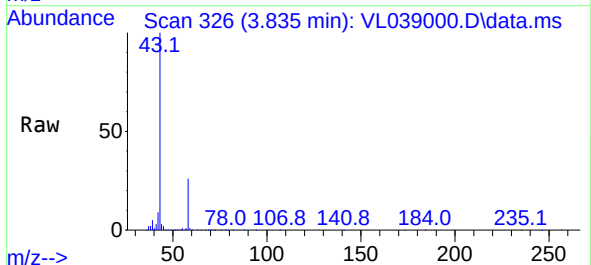


Tgt Ion: 43 Resp: 703366
Ion Ratio Lower Upper
43 100
58 45.2 21.3 31.9

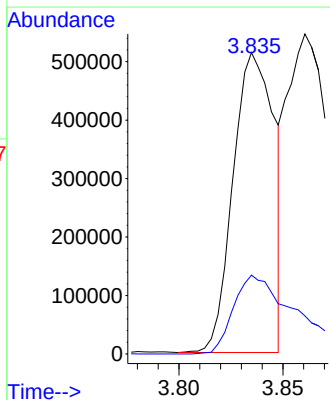



#17
tert-Butyl alcohol
Concen: 0.814 ppbv
RT: 4.282 min Scan# 409
Delta R.T. -0.000 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL




Tgt Ion: 59 Resp: 7546
Ion Ratio Lower Upper
59 100
57 0.0 9.2 13.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

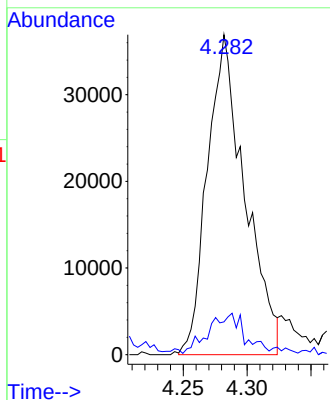


#20
Methylene Chloride
Concen: 1.803 ppbv
RT: 4.333 min Scan# 481
Delta R.T. -0.010 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Tgt Ion: 84 Resp: 81946
Ion Ratio Lower Upper
84 100
49 144.7 119.9 179.9
51 42.7 35.7 53.5
86 58.8 53.8 80.6

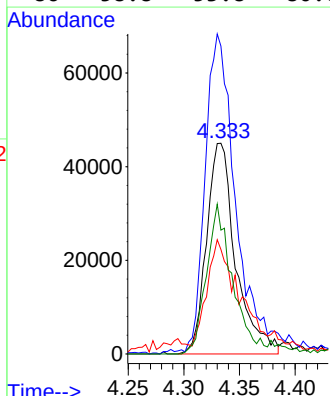



#26
Hexane
Concen: 6.896 ppbv
RT: 5.671 min Scan# 897
Delta R.T. -0.013 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL




Tgt Ion: 57 Resp: 884288
Ion Ratio Lower Upper
57 100
41 90.7 75.2 112.8
43 75.6 190.8 286.2
56 52.2 43.0 64.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

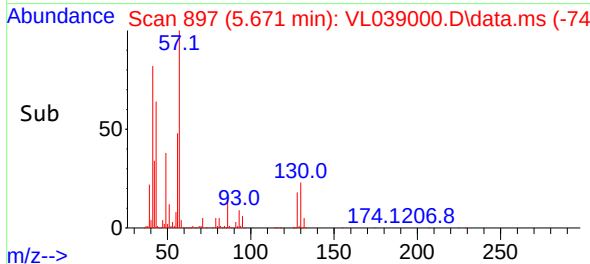


#27
Carbon Disulfide
Concen: 0.365 ppbv
RT: 4.539 min Scan# 545
Delta R.T. -0.013 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Tgt Ion: 76 Resp: 44518
Ion Ratio Lower Upper
76 100
44 25.5 15.3 22.9#
78 12.8 8.2 12.2#

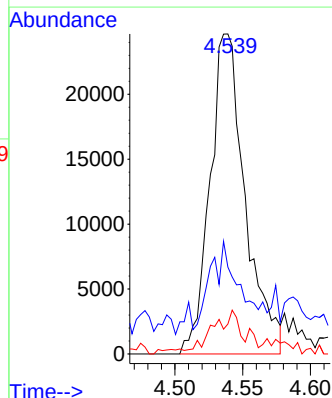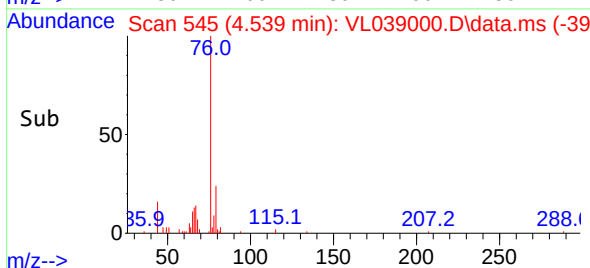



#30
Cyclohexane
Concen: 1.704 ppbv
RT: 7.108 min Scan# 1344
Delta R.T. -0.019 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL




Tgt Ion: 84 Resp: 18299
Ion Ratio Lower Upper
84 100
56 177.2 115.3 172.9
41 89.0 72.0 108.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

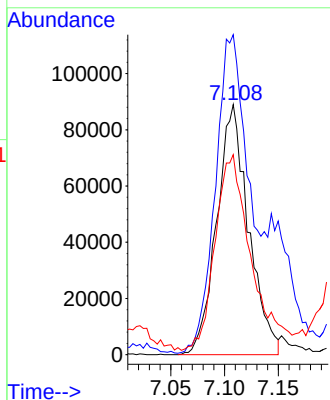


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.150 min Scan# 1357
Delta R.T. -0.023 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Tgt Ion:114 Resp: 3437787
Ion Ratio Lower Upper
114 100
63 24.3 22.6 33.8
88 17.6 15.4 23.0

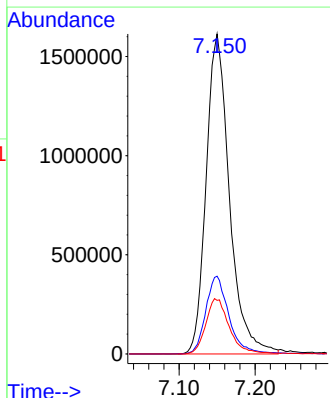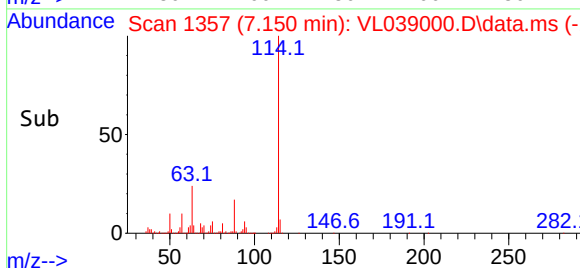



#34
2-Butanone
Concen: 5.361 ppbv
RT: 5.221 min Scan# 71
Delta R.T. -0.019 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL



Tgt Ion: 43 Resp: 940309
Ion Ratio Lower Upper
43 100
72 22.4 17.8 26.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022



#35
Carbon Tetrachloride
Concen: 0.030 ppbv m
RT: 7.002 min Scan# 1311
Delta R.T. -0.013 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

Tgt Ion:117 Resp: 6827
Ion Ratio Lower Upper
117 100
119 108.8 75.2 112.8
121 17.9 24.6 37.0#

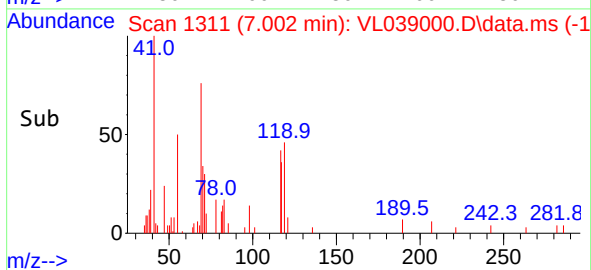







#36
Benzene
Concen: 1.511 ppbv
RT: 6.864 min Scan# 11
Delta R.T. -0.023 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

Instrument :
MSVOA_L
ClientSampleId :
SV2DL

Tgt Ion: 78 Resp: 444662
Ion Ratio Lower Upper
78 100
77 24.0 18.6 28.0
50 17.2 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022



#41
Tetrahydrofuran
Concen: 1.044 ppbv
RT: 6.034 min Scan# 1010
Delta R.T. -0.006 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

Tgt Ion: 42 Resp: 123066
Ion Ratio Lower Upper
42 100
72 45.2 31.8 47.6
71 42.0 30.6 45.8

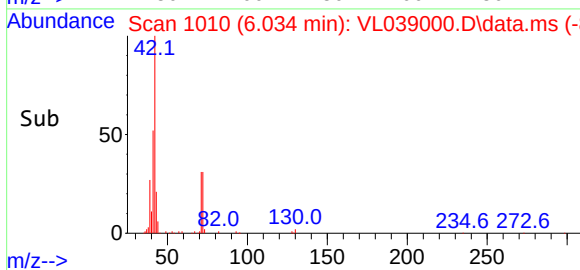







#44
2,2,4-Trimethylpentane
Concen: 4.835 ppbv
RT: 7.841 min Scan# 11
Delta R.T. -0.023 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

Instrument :
MSVOA_L
ClientSampleId :
SV2DL

Tgt Ion: 57 Resp: 249610
Ion Ratio Lower Upper
57 100
41 34.8 26.3 39.5
56 37.0 24.6 37.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022



#50
4-Methyl-2-Pentanone
Concen: 0.407 ppbv
RT: 8.725 min Scan# 1847
Delta R.T. -0.006 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42


Tgt Ion: 43 Resp: 125164
Ion Ratio Lower Upper
43 100
58 38.4 28.4 42.6

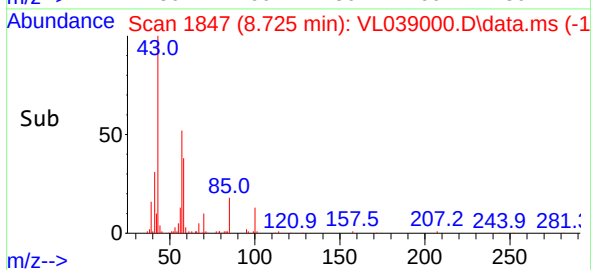



#51
2-Hexanone
Concen: 1.740 ppbv m
RT: 10.105 min Scan# 21
Delta R.T. -0.016 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL




Tgt Ion: 43 Resp: 390632
Ion Ratio Lower Upper
43 100
58 0.0 39.3 58.9
98 0.7 0.2 0.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022




#52
Tetrachloroethene
Concen: 8.664 ppbv
RT: 11.188 min Scan# 2613
Delta R.T. -0.023 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42



Tgt Ion:164 Resp: 910829
Ion Ratio Lower Upper
164 100
166 123.7 102.5 153.7
129 103.0 90.1 135.1
131 100.2 84.8 127.2

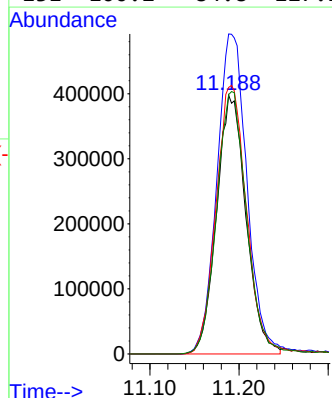

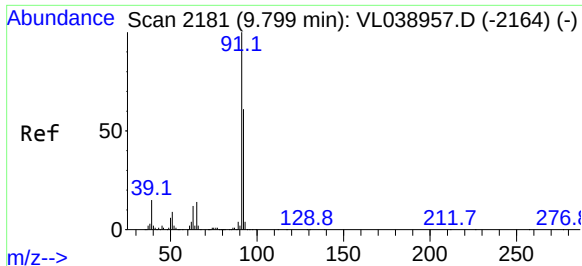





#53
Toluene
Concen: 9.778 ppbv
RT: 9.774 min Scan# 2181
Delta R.T. -0.026 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

Instrument :
MSVOA_L
ClientSampleId :
SV2DL

Tgt Ion: 91 Resp: 322417
Ion Ratio Lower Upper
91 100
92 61.3 48.2 72.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

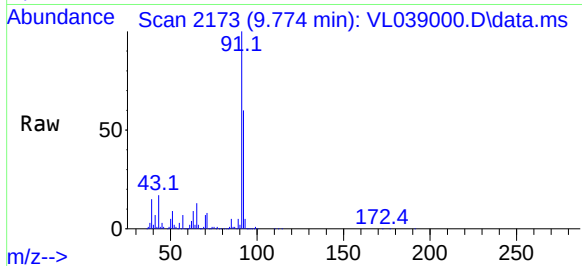

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.053 min Scan# 2882
Delta R.T. -0.023 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42


Tgt Ion:117 Resp: 2948964
Ion Ratio Lower Upper
117 100
82 63.6 57.0 85.6
119 33.8 27.2 40.8

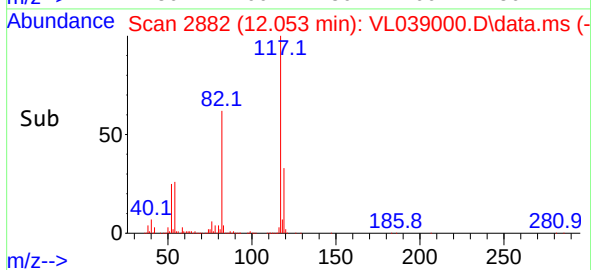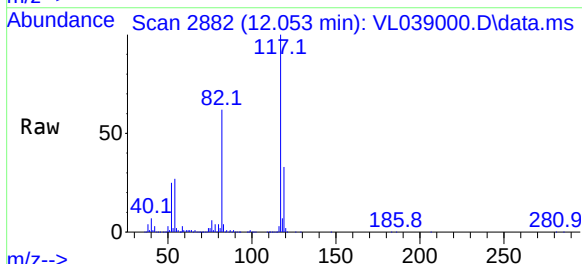



#58
Ethyl Benzene
Concen: 2.421 ppbv
RT: 12.677 min Scan# 3083
Delta R.T. -0.023 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL




Tgt Ion: 91 Resp: 1027464
Ion Ratio Lower Upper
91 100
106 28.6 24.2 36.4

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

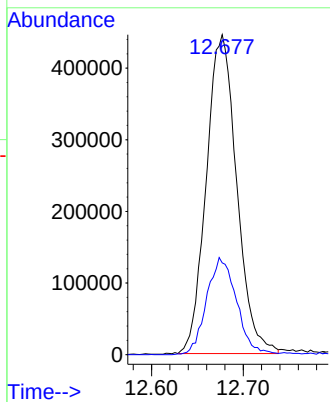


#59
m/p-Xylene
Concen: 7.484 ppbv
RT: 12.934 min Scan# 3156
Delta R.T. -0.052 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

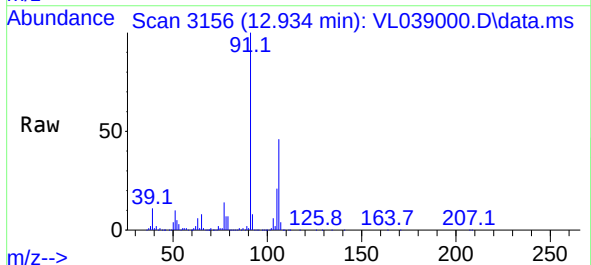

Tgt Ion: 91 Resp: 2711580
Ion Ratio Lower Upper
91 100
106 47.6 34.6 52.0

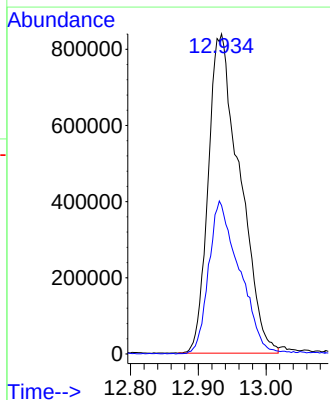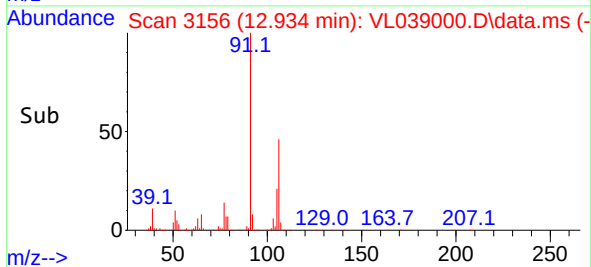







#60
o-Xylene
Concen: 2.951 ppbv
RT: 13.658 min Scan# 31
Delta R.T. -0.023 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

Instrument :
MSVOA_L
ClientSampleId :
SV2DL

Tgt Ion: 91 Resp: 1006210
Ion Ratio Lower Upper
91 100
106 44.8 22.2 66.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022



#62
Isopropylbenzene
Concen: 0.186 ppbv
RT: 14.629 min Scan# 3683
Delta R.T. -0.025 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42


Tgt Ion:105 Resp: 92751
Ion Ratio Lower Upper
105 100
120 26.9 20.5 30.7

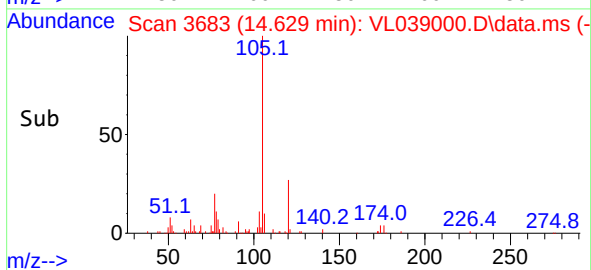



#64
n-propylbenzene
Concen: 0.527 ppbv
RT: 15.529 min Scan# 3963
Delta R.T. -0.019 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42




Instrument :
MSVOA_L
ClientSampleId :
SV2DL




Tgt Ion: 120 Resp: 6349
Ion Ratio Lower Upper
120 100
91 517.0 400.6 601.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

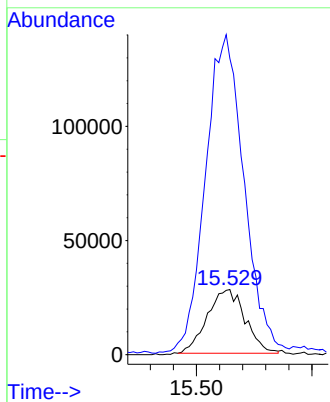


#68
1-Bromo-4-Fluorobenzene
Concen: 9.611 ppbv
RT: 14.378 min Scan# 3605
Delta R.T. -0.026 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

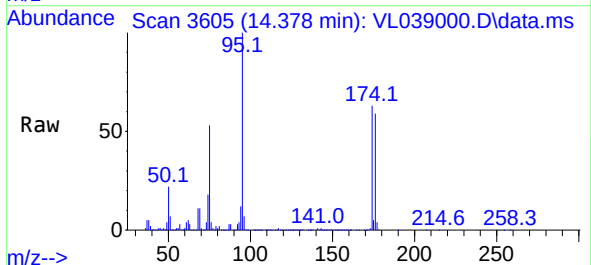

Tgt Ion: 95 Resp: 2244696
Ion Ratio Lower Upper
95 100
174 66.6 50.8 76.2
175 4.8 3.8 5.6

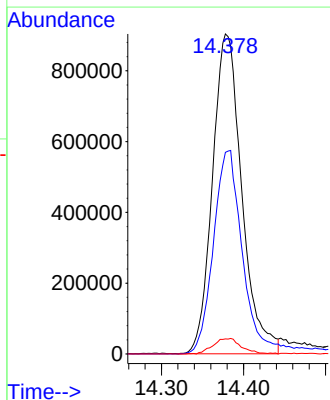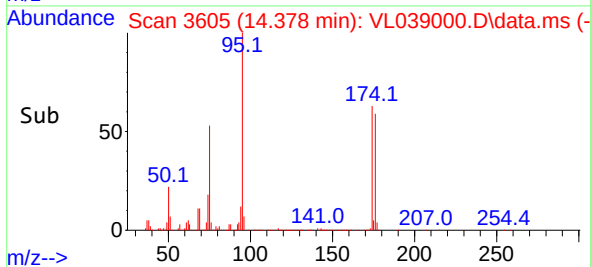



#70

n-Butylbenzene

Concen: 0.137 ppbv m

RT: 18.526 min Scan# 4898

Delta R.T. -0.010 min

Lab File: VL039000.D

Acq: 9 May 2022 23:42

Instrument :

MSVOA_L

ClientSampleId :

SV2DL





Tgt Ion: 91 Resp: 7328

Ion	Ratio	Lower	Upper
91	100		
92	38.1	43.1	64.7
134	80.7	17.0	25.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

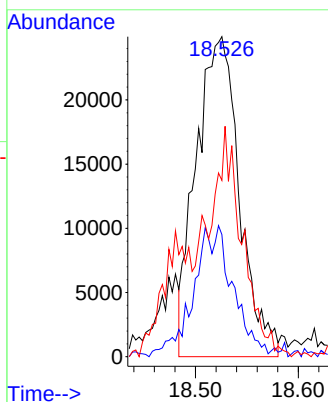

#72

4-Ethyltoluene

Concen: 0.945 ppbv

RT: 15.802 min Scan# 4048




Delta R.T. -0.026 min


Lab File: VL039000.D

Acq: 9 May 2022 23:42

Tgt Ion:105 Resp: 367277

Ion	Ratio	Lower	Upper
105	100		
120	29.6	23.4	35.0
91	13.1	10.6	16.0
77	12.1	12.5	18.7

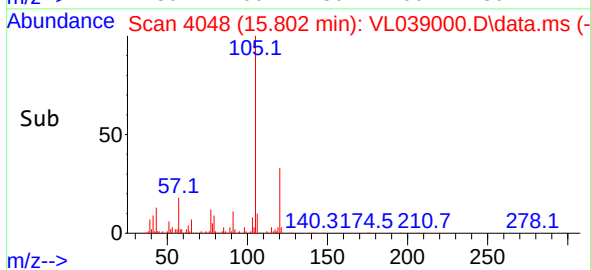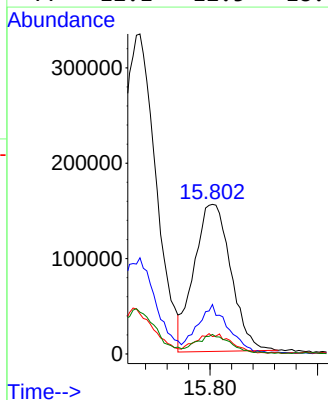







#73
 1,3,5-Trimethylbenzene
 Concen: 0.786 ppbv
 RT: 15.963 min Scan# 4098
 Delta R.T. -0.023 min
 Lab File: VL039000.D
 Acq: 9 May 2022 23:42

Instrument :
 MSVOA_L
 ClientSampleId :
 SV2DL

Tgt Ion:105 Resp: 275029
 Ion Ratio Lower Upper
 105 100
 120 45.1 34.4 51.6




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/11/2022

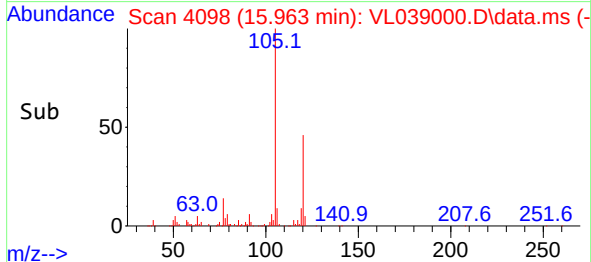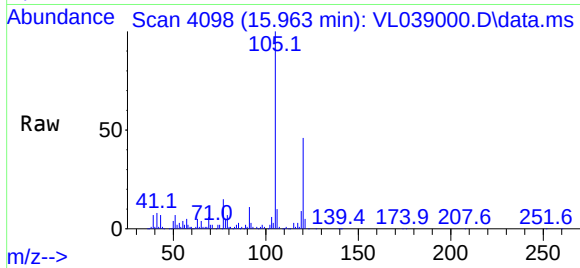

#74
 1,2,4-Trimethylbenzene
 Concen: 2.677 ppbv
 RT: 16.722 min Scan# 4334
 Delta R.T. -0.026 min
 Lab File: VL039000.D
 Acq: 9 May 2022 23:42

Tgt Ion:105 Resp: 1025187
 Ion Ratio Lower Upper
 105 100
 120 42.6 36.9 55.3
 91 11.0 45.0 67.4#
 77 13.3 19.2 28.8#

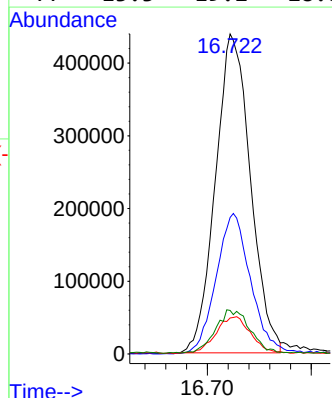



#79
Naphthalene
Concen: 0.164 ppbv m
RT: 22.159 min Scan# 6025
Delta R.T. -0.013 min
Lab File: VL039000.D
Acq: 9 May 2022 23:42

Instrument :
MSVOA_L
ClientSampleId :
SV2DL

Tgt Ion:	128	Resp:	5107
Ion	Ratio	Lower	Upper
128	100		
127	10.4	10.2	15.2
129	9.5	8.9	13.3

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/11/2022

