


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050922\
 Data File : VL038987.D
 Acq On : 9 May 2022 13:39
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
 Last Update : Thu May 05 10:12:15 2022

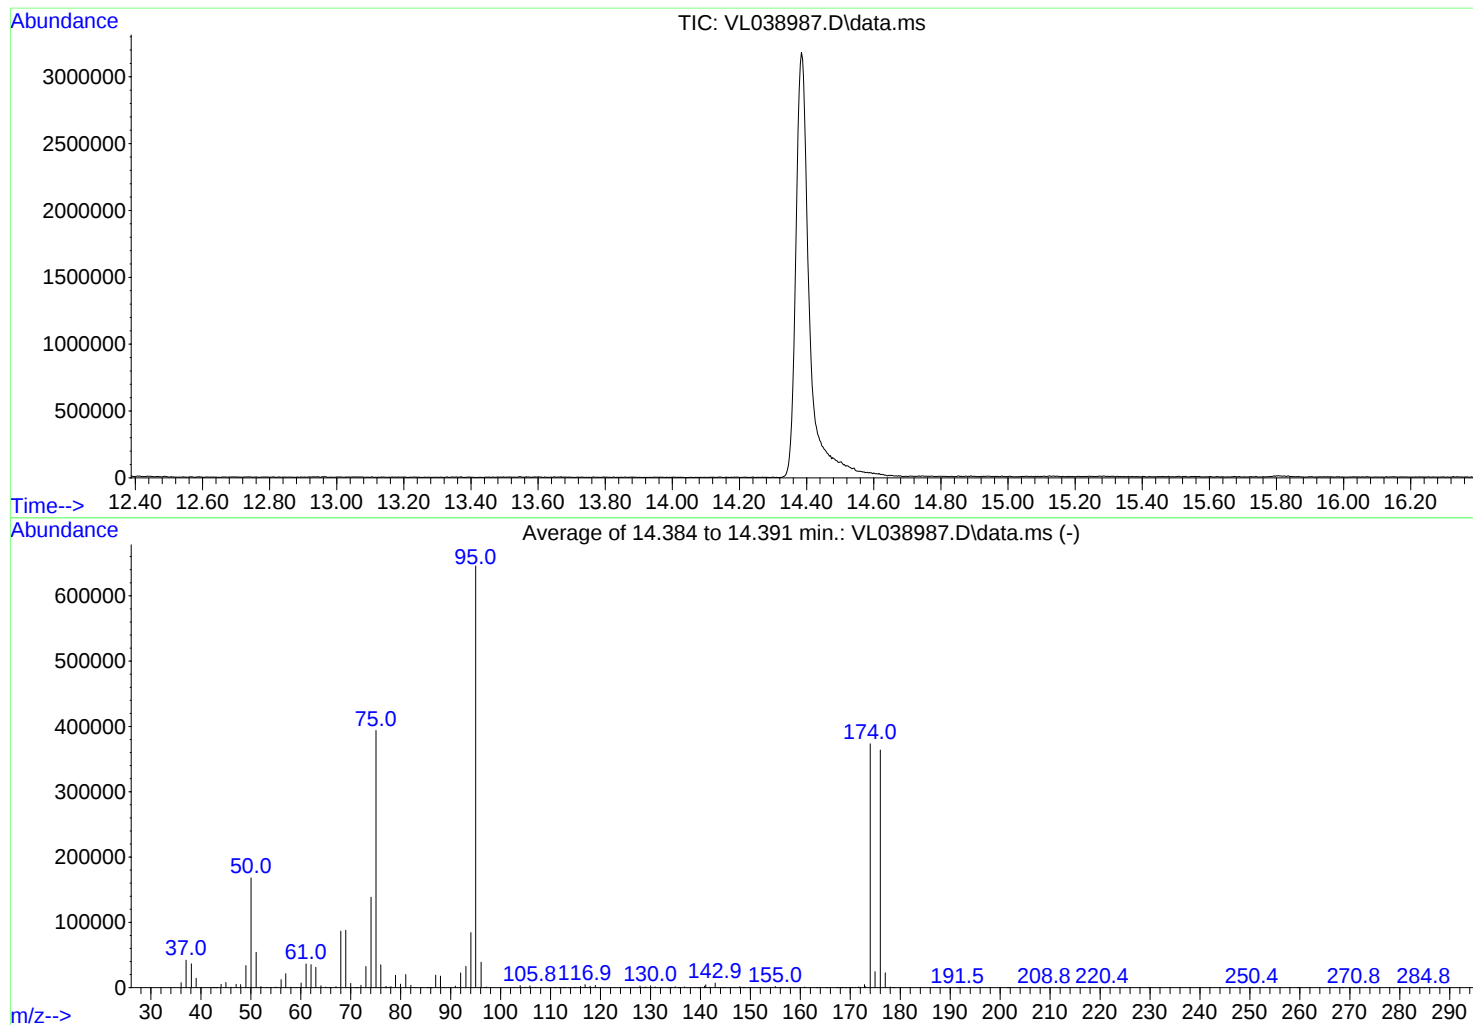

AutoFind: Scans 3607, 3608, 3609; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.0	168171	PASS
75	95	30	66	61.0	393792	PASS
95	95	100	100	100.0	645952	PASS
96	95	5	9	6.0	39056	PASS
173	174	0.00	2	1.3	4765	PASS
174	95	50	120	57.8	373483	PASS
175	174	4	9	6.6	24579	PASS
176	174	93	101	97.4	363861	PASS
177	176	5	9	6.3	22909	PASS

Average of 14.384 to 14.391 min.: VL038987.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7616	46.05	831	55.10	817	65.80	81
37.05	42176	47.05	5132	56.05	12224	66.10	28
38.10	36619	47.95	4761	57.00	21424	67.05	183
39.05	14512	49.00	33855	58.00	858	68.00	8640
40.00	428	50.05	168171	59.10	263	69.00	87947
42.30	168	51.05	54272	60.05	7089	70.00	6718
42.50	82	52.00	1535	61.05	36205	71.10	59
42.90	192	52.20	699	62.05	35219	72.05	3659
43.10	52	53.10	179	63.00	31235	73.05	32291
44.05	5169	53.90	76	64.05	3069	74.05	138347
45.00	7972	54.85	851	65.00	933	75.05	393792

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 14.384 to 14.391 min.: VL038987.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	34974	84.10	104	95.00	645952	110.80	150
76.90	1216	85.30	57	96.10	39056	111.10	622
77.15	1610	85.80	125	96.90	504	111.70	134
77.80	677	86.10	110	97.15	896	112.05	533
78.05	1395	87.00	19075	102.70	392	112.60	67
78.95	18792	87.95	17759	103.90	3325	112.95	525
79.95	5285	88.70	606	104.90	851	113.70	92
81.00	20056	90.95	2431	105.85	2638	114.85	573
82.05	3697	92.00	22496	107.00	441	115.10	350
82.75	300	93.05	32715	109.80	167	116.00	1864
83.10	377	94.05	84440	110.05	581	116.90	4583

Average of 14.384 to 14.391 min.: VL038987.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.90	2164	129.05	1012	138.95	371	145.80	526
118.95	3374	130.00	2750	139.60	92	146.10	452
120.00	307	130.95	1332	140.05	850	146.90	169
121.80	53	131.90	105	140.80	2259	147.90	1423
122.90	201	132.15	251	141.05	4383	148.60	72
123.90	558	133.60	66	141.90	695	149.05	243
124.75	299	134.10	107	142.95	7239	149.60	284
125.95	263	134.95	1536	143.70	193	150.00	472
126.75	188	135.60	60	144.00	580	151.80	237
127.90	2358	135.95	234	144.50	80	152.00	72
128.80	378	136.85	1309	145.00	598	153.00	288

Average of 14.384 to 14.391 min.: VL038987.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.00	201	167.20	228	172.85	4765	208.85	153
155.00	1695	167.50	107	173.10	1418	211.90	52
156.10	80	168.20	68	174.00	373483	220.45	130
156.70	239	168.65	277	174.95	24579	229.70	66
156.95	614	169.05	32	176.00	363861	250.40	141
157.60	81	169.60	221	177.00	22909	259.50	52
158.70	193	170.10	220	178.00	1089	268.50	74
158.95	450	170.45	608	178.70	55	270.80	113
160.85	928	171.00	567	191.50	125	278.70	61
163.30	153	171.65	985	201.50	64	284.80	58
165.20	99	171.95	696	205.90	54		