


Data Path : W:\HPCHEM1\MSVOA L\Data\VL051618\
Data File : VL032003.D
Acq On : 16 May 2018 12:53
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL050318AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu May 03 15:52:13 2018
Last Update : Thu May 03 15:52:13 2018

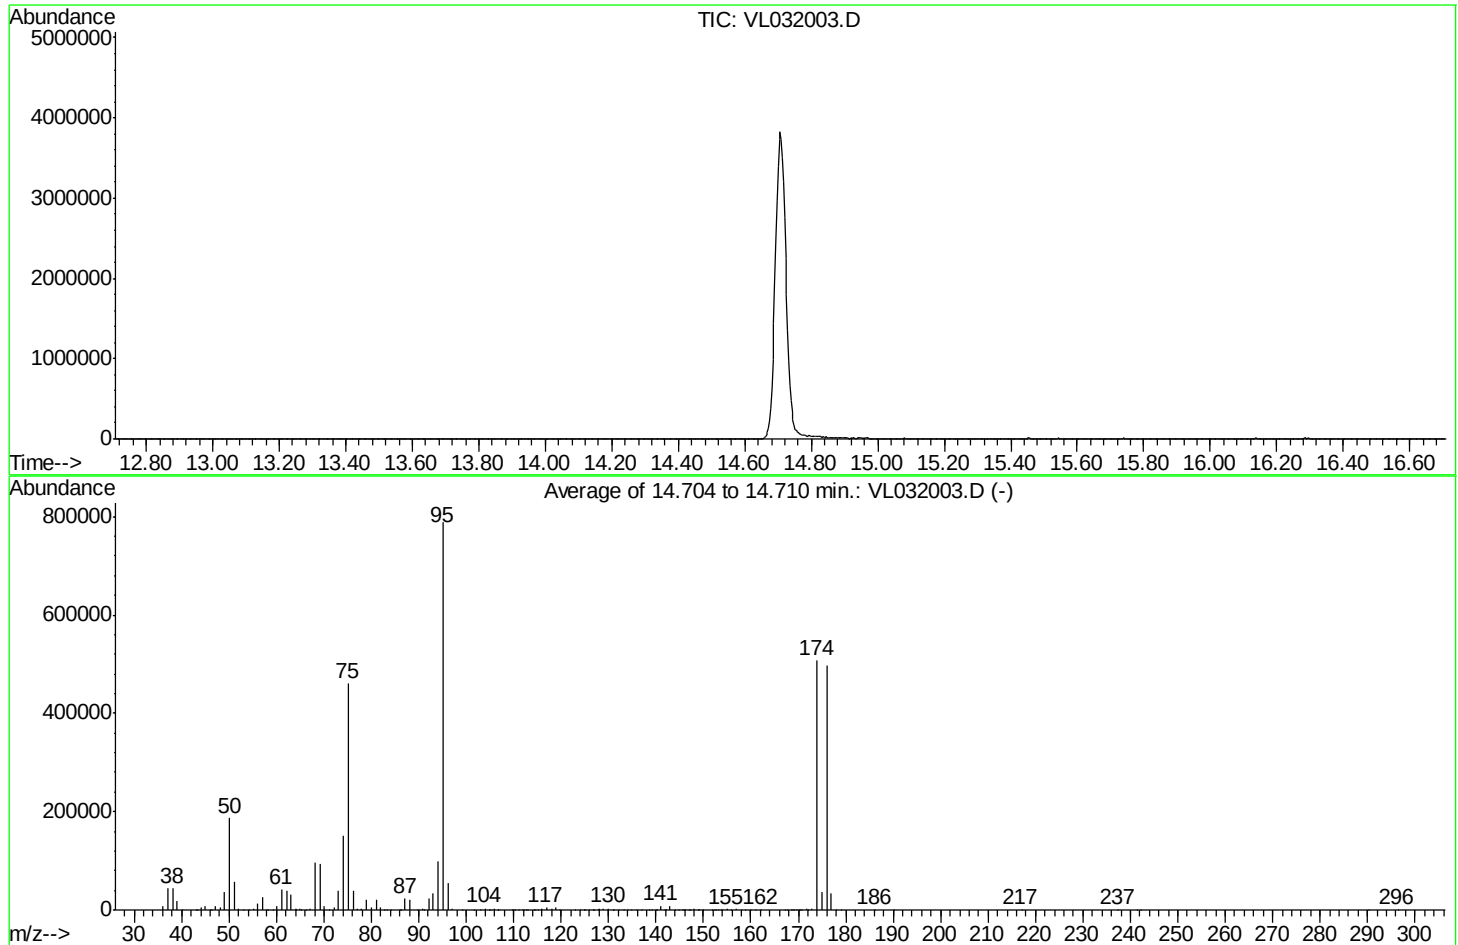

AutoFind: Scans 4235, 4236, 4237; Background Corrected with Scan 4212

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	187264	PASS
75	95	30	66	58.3	459648	PASS
95	95	100	100	100.0	788309	PASS
96	95	5	9	7.1	55949	PASS
173	174	0.00	2	0.8	3981	PASS
174	95	50	120	64.2	506453	PASS
175	174	4	9	7.1	35936	PASS
176	174	93	101	98.1	496704	PASS
177	176	5	9	7.0	34829	PASS