


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051722\
 Data File : VL039066.D
 Acq On : 17 May 2022 10:14
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
 Last Update : Thu May 05 10:12:15 2022

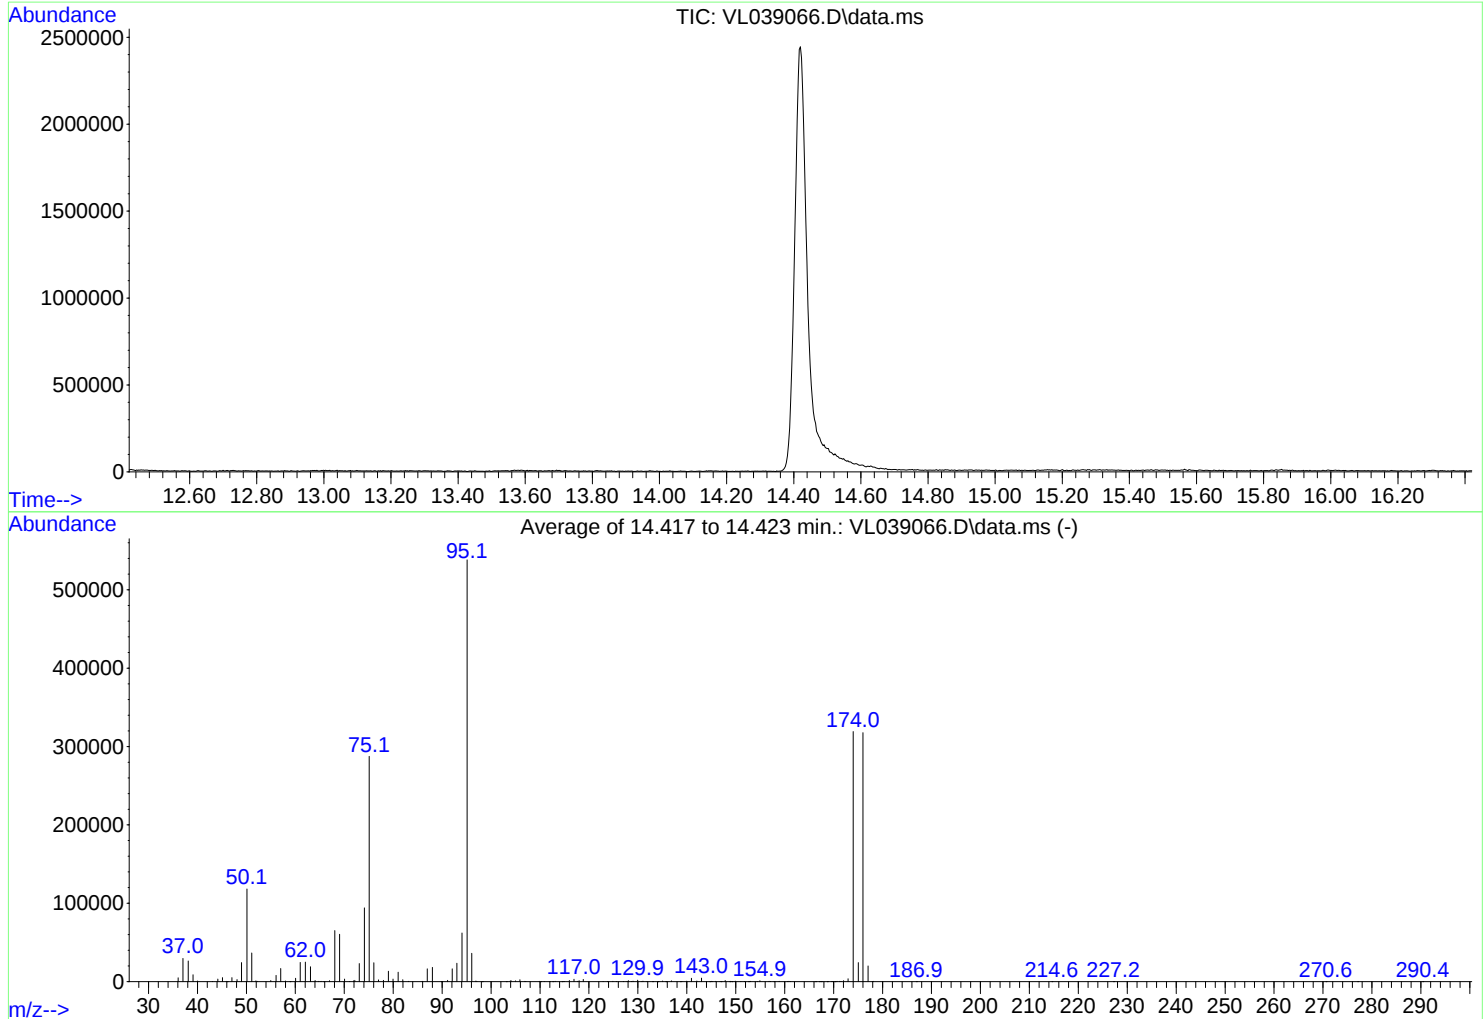

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	118261	PASS
75	95	30	66	53.4	287424	PASS
95	95	100	100	100.0	538241	PASS
96	95	5	9	6.7	36069	PASS
173	174	0.00	2	1.1	3591	PASS
174	95	50	120	59.3	319147	PASS
175	174	4	9	7.6	24291	PASS
176	174	93	101	99.5	317611	PASS
177	176	5	9	6.3	20120	PASS

Average of 14.417 to 14.423 min.: VL039066.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	5006	48.10	2758	60.05	4252	70.05	3354
37.05	29653	49.00	24248	61.00	24616	71.10	1907
38.10	26360	50.10	118261	62.05	24843	71.90	1071
39.10	8861	51.10	36531	63.10	18944	72.15	1671
40.00	744	51.95	1007	64.05	1549	73.05	23032
43.05	151	52.20	521	64.80	457	74.10	94093
44.15	3252	55.00	1491	65.25	365	75.10	287424
45.10	5212	56.05	8080	65.80	52	76.05	24037
45.85	374	57.00	16800	67.00	1248	77.00	2305
46.10	53	58.00	898	68.05	65115	78.00	1740
47.05	5061	58.90	57	69.05	60357	79.00	13386

Average of 14.417 to 14.423 min.: VL039066.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	3310	93.00	23421	105.90	2433	114.75	215
81.00	12136	94.05	62200	106.90	362	115.00	134
81.95	2416	95.10	538241	107.10	209	116.00	1351
83.15	323	96.05	36069	109.85	357	116.95	3042
85.90	347	96.90	797	110.10	52	117.70	367
86.95	16419	97.10	263	110.85	211	118.00	1328
88.00	18302	98.20	62	111.90	281	118.85	2881
89.80	88	103.10	52	112.10	230	122.90	169
90.10	186	103.90	640	112.60	71	123.80	141
91.10	1682	104.05	1457	113.10	345	123.95	313
92.05	16289	105.00	940	114.50	64	124.90	432

Average of 14.417 to 14.423 min.: VL039066.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.60	185	134.10	53	144.00	205	149.90	674
127.05	230	135.05	883	144.70	120	151.05	160
127.80	443	135.70	105	145.05	338	151.75	172
128.05	1279	135.90	187	145.30	162	152.60	74
128.70	247	136.85	986	145.90	373	153.00	494
129.00	703	138.70	123	146.80	302	154.40	144
129.95	1911	139.00	216	147.00	65	154.95	1160
130.80	242	140.00	553	147.85	1522	156.80	374
131.05	707	140.95	4393	148.80	115	157.10	254
131.85	174	142.05	797	149.00	335	157.80	55
133.00	50	143.00	4443	149.20	120	158.85	353

Average of 14.417 to 14.423 min.: VL039066.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.60	235	170.30	106	178.10	355		
160.85	341	170.70	492	186.90	86		
161.10	288	171.25	367	214.60	52		
166.30	85	171.50	200	227.20	58		
167.10	58	172.05	1194	270.60	76		
167.50	85	172.95	3591	277.10	54		
168.70	55	174.00	319147	290.40	62		
168.85	268	175.05	24291				
169.60	163	176.00	317611				
169.80	143	177.05	20120				
170.05	242	177.90	208				