


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL051921\
 Data File : VL036984.D
 Acq On : 19 May 2021 8:50
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL051821AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue May 18 12:00:15 2021
 Last Update : Tue May 18 12:00:15 2021

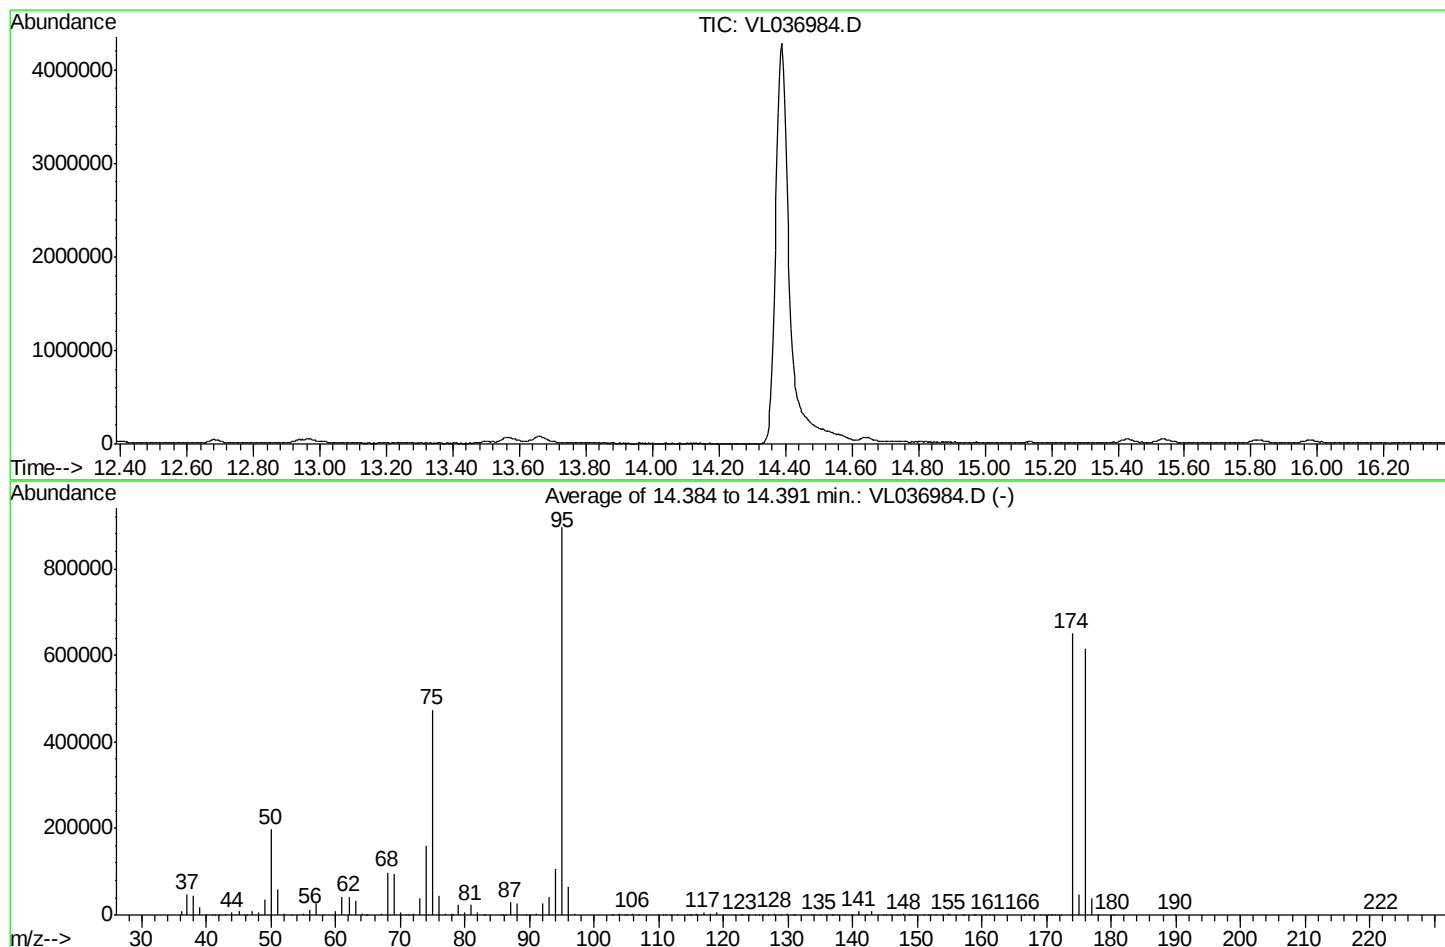

AutoFind: Scans 3607, 3608, 3609; Background Corrected with Scan 3579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	196949	PASS
75	95	30	66	52.9	473578	PASS
95	95	100	100	100.0	895680	PASS
96	95	5	9	7.1	63800	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.6	650112	PASS
175	174	4	9	7.5	48538	PASS
176	174	93	101	94.6	614933	PASS
177	176	5	9	6.5	39880	PASS