

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052124\
 Data File : VL041262.D
 Acq On : 21 May 2024 12:53
 Operator : SY/MD
 Sample : QC051524 CAN 10331
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC051524 CAN 10331

Quant Time: May 22 05:43:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed May 22 05:39:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.198	49	918196	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.655	114	2476753	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.462	117	2274490	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.774	95	1713031	9.976	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.800%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052124\
Data File : VL041262.D
Acq On : 21 May 2024 12:53
Operator : SY/MD
Sample : QC051524 CAN 10331
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC051524 CAN 10331

Quant Time: May 22 05:43:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Wed May 22 05:39:49 2024
Response via : Initial Calibration




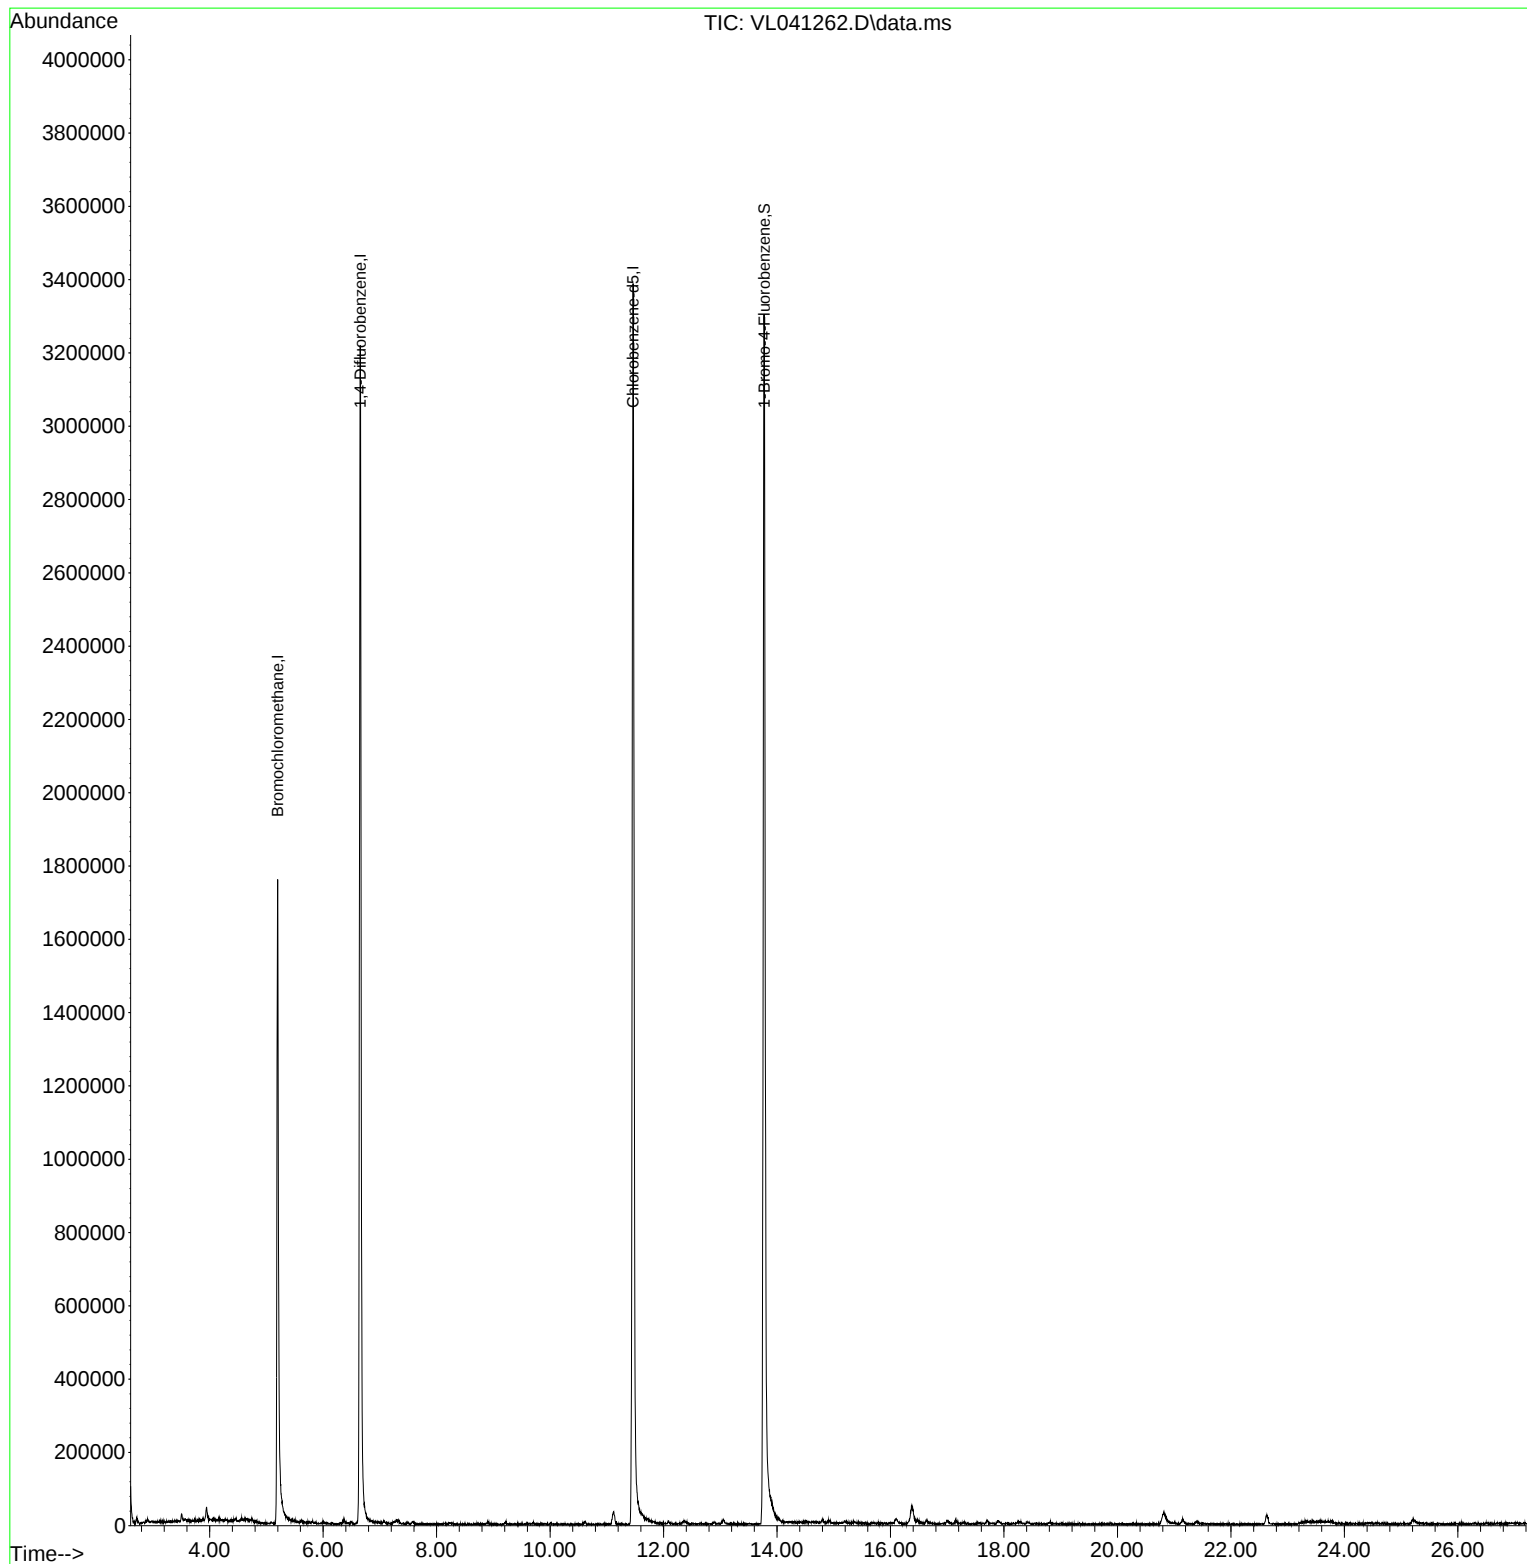


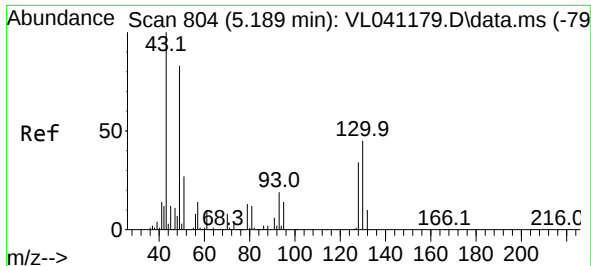

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.198 min Scan# 804
Delta R.T. -0.003 min
Lab File: VL041262.D
Acq: 21 May 2024 12:53




Instrument :
MSVOA_L
ClientSampleId :
QC051524 CAN 10331


Tgt Ion: 49 Resp: 918196
Ion Ratio Lower Upper
49 100
128 47.0 21.5 64.5
130 60.0 27.2 81.6

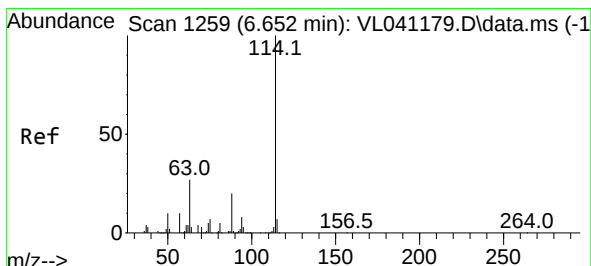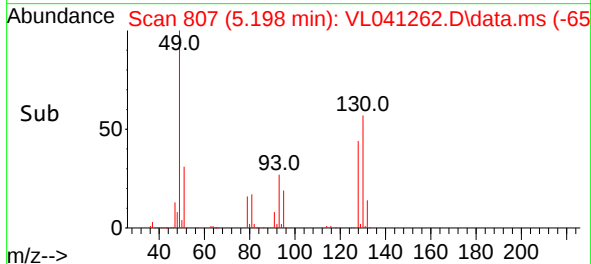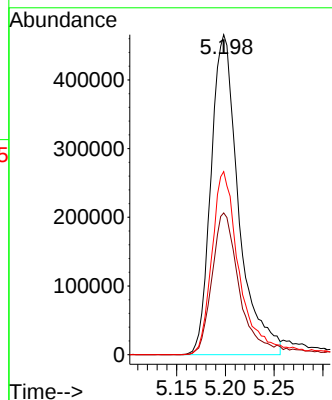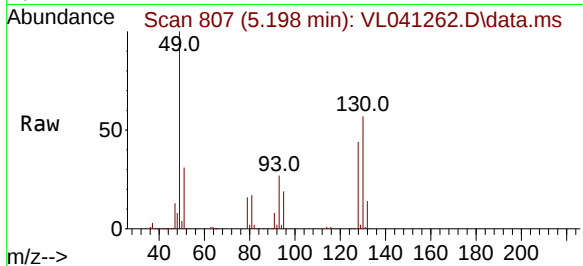

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.655 min Scan# 1260
Delta R.T. -0.003 min
Lab File: VL041262.D
Acq: 21 May 2024 12:53

Tgt Ion: 114 Resp: 2476753
Ion Ratio Lower Upper
114 100
63 25.6 21.8 32.6
88 18.1 15.2 22.8


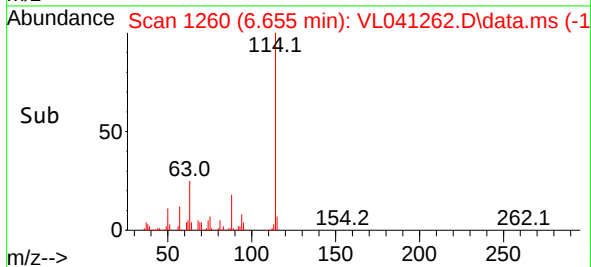
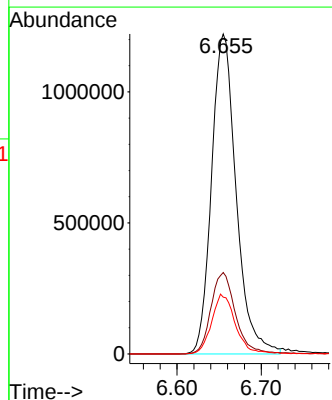
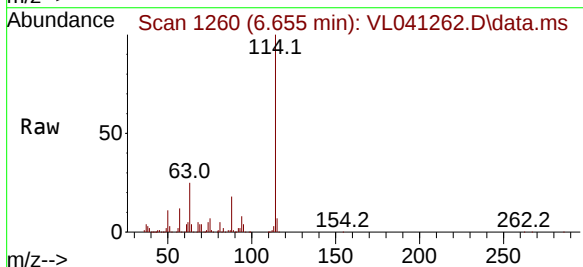


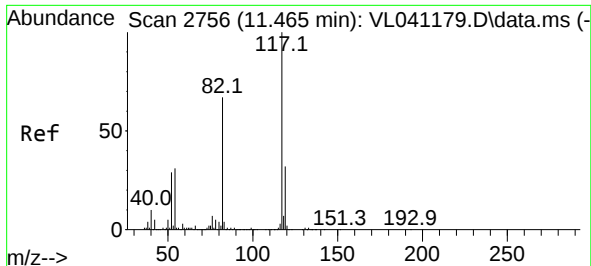

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.462 min Scan# 21
Delta R.T. -0.003 min
Lab File: VL041262.D
Acq: 21 May 2024 12:53

Instrument :
MSVOA_L
ClientSampleId :
QC051524 CAN 10331

Tgt Ion:117 Resp: 2274490
Ion Ratio Lower Upper
117 100
82 66.2 53.6 80.4
119 33.2 27.2 40.8

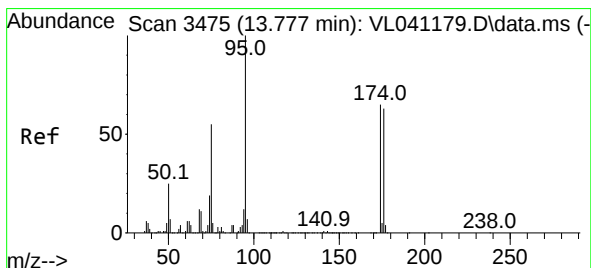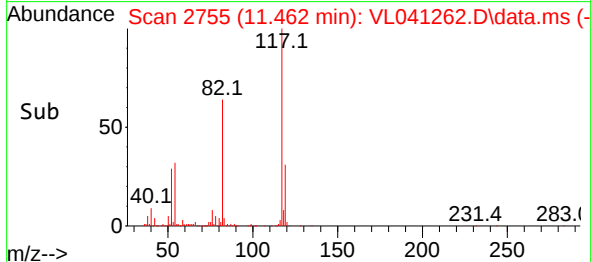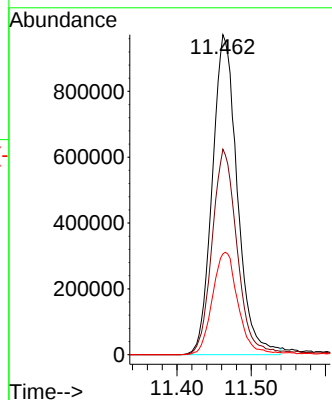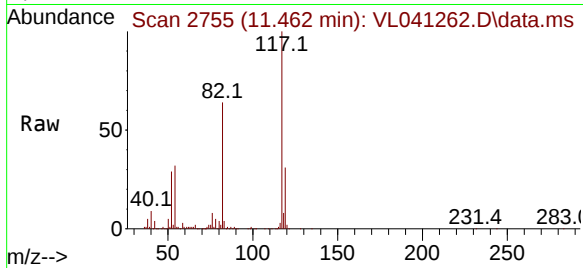

#68
1-Bromo-4-Fluorobenzene
Concen: 9.976 ppbv
RT: 13.774 min Scan# 3474
Delta R.T. 0.000 min
Lab File: VL041262.D
Acq: 21 May 2024 12:53

Tgt Ion: 95 Resp: 1713031
Ion Ratio Lower Upper
95 100
174 66.6 53.6 80.4
175 4.8 4.2 6.4

