
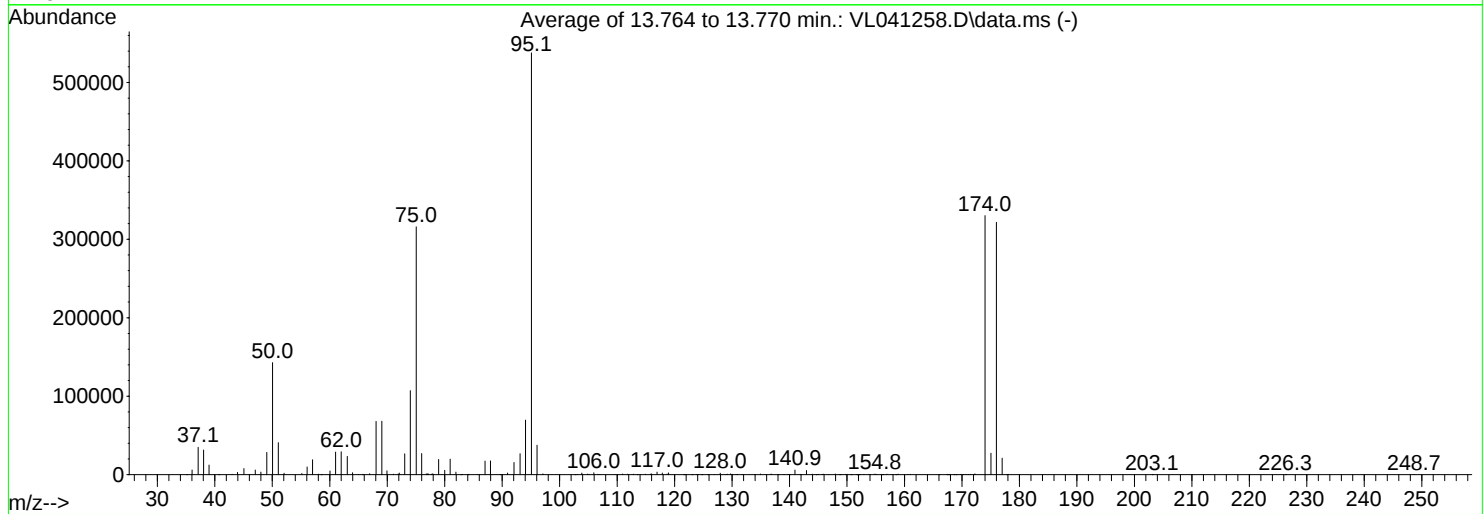


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052124\
Data File : VL041258.D
Acq On : 21 May 2024 9:10
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed May 22 05:39:49 2024

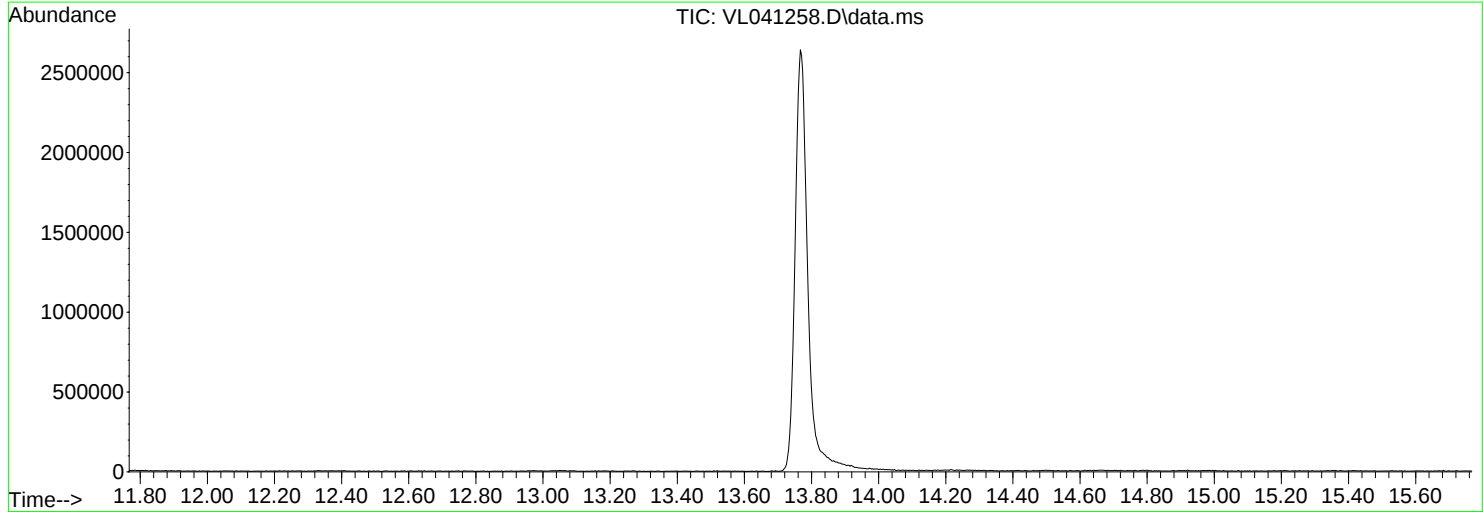

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3444

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	26.6	142869	PASS
75	95	30	66	58.7	315883	PASS
95	95	100	100	100.0	537728	PASS
96	95	5	9	7.0	37445	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	61.4	330197	PASS
175	174	4	9	8.3	27291	PASS
176	174	93	101	97.4	321728	PASS
177	176	5	9	6.6	21096	PASS

Average of 13.764 to 13.770 min.: VL041258.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	99	47.05	5969	60.05	4777	71.05	581
36.05	5989	48.00	3364	61.00	28875	71.90	901
37.10	34875	49.05	28397	62.00	29115	72.10	206
38.05	31544	50.05	142869	63.05	23181	73.05	2644
39.00	12207	51.05	40789	63.95	2510	74.00	107133
39.95	200	52.05	1777	65.00	262	75.05	315883
40.70	68	55.15	1552	65.70	72	76.00	26936
43.00	436	56.05	9773	66.95	1332	76.80	1047
43.95	2915	57.00	18949	68.05	67973	77.00	974
45.05	7696	58.05	578	69.05	68077	77.20	858
46.00	355	58.50	119	69.95	4997	77.70	502

Average of 13.764 to 13.770 min.: VL041258.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.80	917	87.00	17427	103.10	137	112.85	633
77.95	1042	87.95	17597	103.85	2169	113.50	76
78.95	19355	89.70	79	104.90	917	114.95	677
80.00	5540	90.95	2171	105.10	258	115.80	577
80.95	19835	92.05	15427	105.95	2412	116.00	1031
81.95	3230	93.10	26659	106.65	473	116.95	3299
82.80	80	94.05	69651	107.00	276	117.85	2141
83.05	498	95.10	537728	109.60	180	118.70	853
84.05	104	96.05	37445	110.10	263	118.95	2201
85.80	231	97.10	1132	110.95	877	121.60	96
86.10	207	102.70	54	111.85	636	121.90	108

Average of 13.764 to 13.770 min.: VL041258.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.05	38	130.70	247	140.95	5859	148.70	67
123.80	252	130.95	371	141.85	527	149.10	308
124.10	197	131.85	144	142.10	289	149.70	531
124.75	110	133.90	108	142.95	5377	150.00	443
125.80	84	134.95	799	143.95	557	150.70	57
126.95	159	135.90	192	144.60	103	151.70	53
127.95	1795	136.80	922	145.00	419	151.90	164
128.90	315	138.00	66	145.70	382	152.10	113
129.15	685	139.05	161	145.95	545	152.95	377
129.75	1123	139.70	157	146.85	300	153.80	473
130.00	471	140.10	175	147.95	773	154.10	145

Average of 13.764 to 13.770 min.: VL041258.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.85	807	167.40	92	175.05	27291		
155.10	211	167.70	88	176.00	321728		
155.95	157	168.60	66	177.00	21096		
156.20	72	169.00	74	177.80	100		
156.95	636	169.70	330	178.05	431		
157.90	203	170.25	303	203.10	55		
158.50	59	170.70	148	226.30	57		
158.90	566	171.10	164	248.70	168		
160.60	187	171.45	388				
161.00	419	172.25	958				
166.00	120	174.00	330197				