
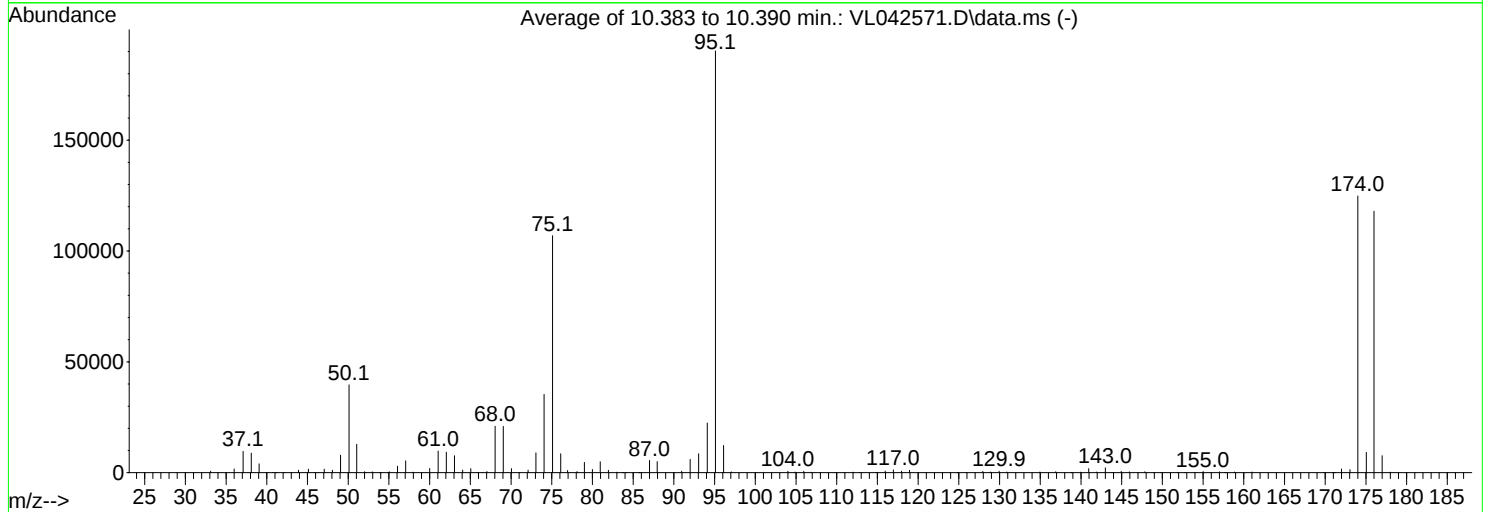


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052225\
Data File : VL042571.D
Acq On : 22 May 2025 07:51
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052025AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed May 21 00:21:29 2025

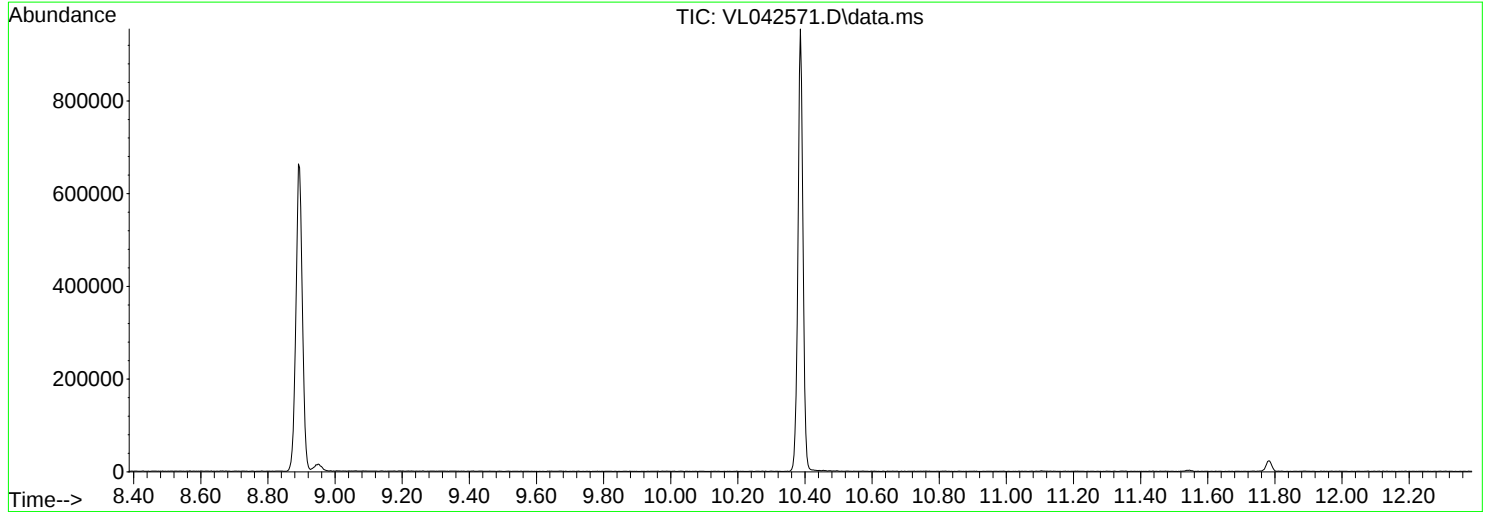

AutoFind: Scans 3181, 3182, 3183; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	20.8	39629	PASS
75	95	30	66	56.2	106936	PASS
95	95	100	100	100.0	190336	PASS
96	95	5	9	6.5	12283	PASS
173	174	0.00	2	1.1	1358	PASS
174	95	50	120	65.6	124811	PASS
175	174	4	9	7.4	9196	PASS
176	174	93	101	94.5	118003	PASS
177	176	5	9	6.5	7644	PASS

Average of 10.383 to 10.390 min.: VL042571.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	625	43.90	1114	52.95	339	63.05	769
33.95	51	45.10	1594	53.90	34	64.05	116
36.00	1634	45.90	55	54.15	68	65.05	178
37.10	9617	46.30	126	54.90	186	65.90	8
38.10	8831	47.05	1594	55.10	344	66.45	97
39.05	3948	48.05	1121	56.05	2924	67.05	533
40.00	86	49.05	7841	57.05	5333	68.05	20971
40.70	66	50.10	39629	57.95	247	69.05	20877
41.10	35	51.05	12814	60.00	1871	70.05	1807
42.15	46	52.00	415	61.05	9728	71.05	42
43.00	120	52.20	177	62.05	9261	72.10	1149

Average of 10.383 to 10.390 min.: VL042571.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	8973	83.70	19	96.10	12283	113.10	62
74.05	35333	84.20	53	97.05	359	114.80	103
75.10	106936	85.70	36	104.00	648	115.00	78
76.10	8518	85.90	80	104.90	287	115.95	756
76.95	980	87.00	5524	105.95	581	116.95	1202
78.10	480	87.95	4956	106.85	195	117.95	649
79.00	4604	90.95	635	108.00	83	118.95	1124
80.00	1457	92.00	5975	109.75	43	123.95	70
80.95	4907	93.05	8528	110.95	174	124.80	38
81.95	1059	94.10	22355	112.00	238	125.90	76
83.00	202	95.10	190336	112.80	110	127.95	579

Average of 10.383 to 10.390 min.: VL042571.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.90	285	144.05	99	154.00	128	173.05	1358
129.95	631	144.95	604	155.00	494	174.00	124811
130.90	298	145.95	358	155.95	78	175.05	9196
134.95	308	147.00	143	157.00	330	176.00	118003
136.90	437	147.85	404	157.70	24	177.00	7644
138.80	19	148.95	115	158.85	316	178.00	213
139.95	200	149.80	56	161.00	304		
140.95	1789	150.05	74	169.85	53		
141.90	288	151.85	117	170.90	118		
143.00	2205	152.70	49	171.10	21		
143.80	41	152.90	55	172.00	1650		