


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL052319\
Data File : VL033768.D
Acq On : 23 May 2019 9:47
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL051719AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri May 17 08:15:41 2019
Last Update : Fri May 17 08:15:41 2019

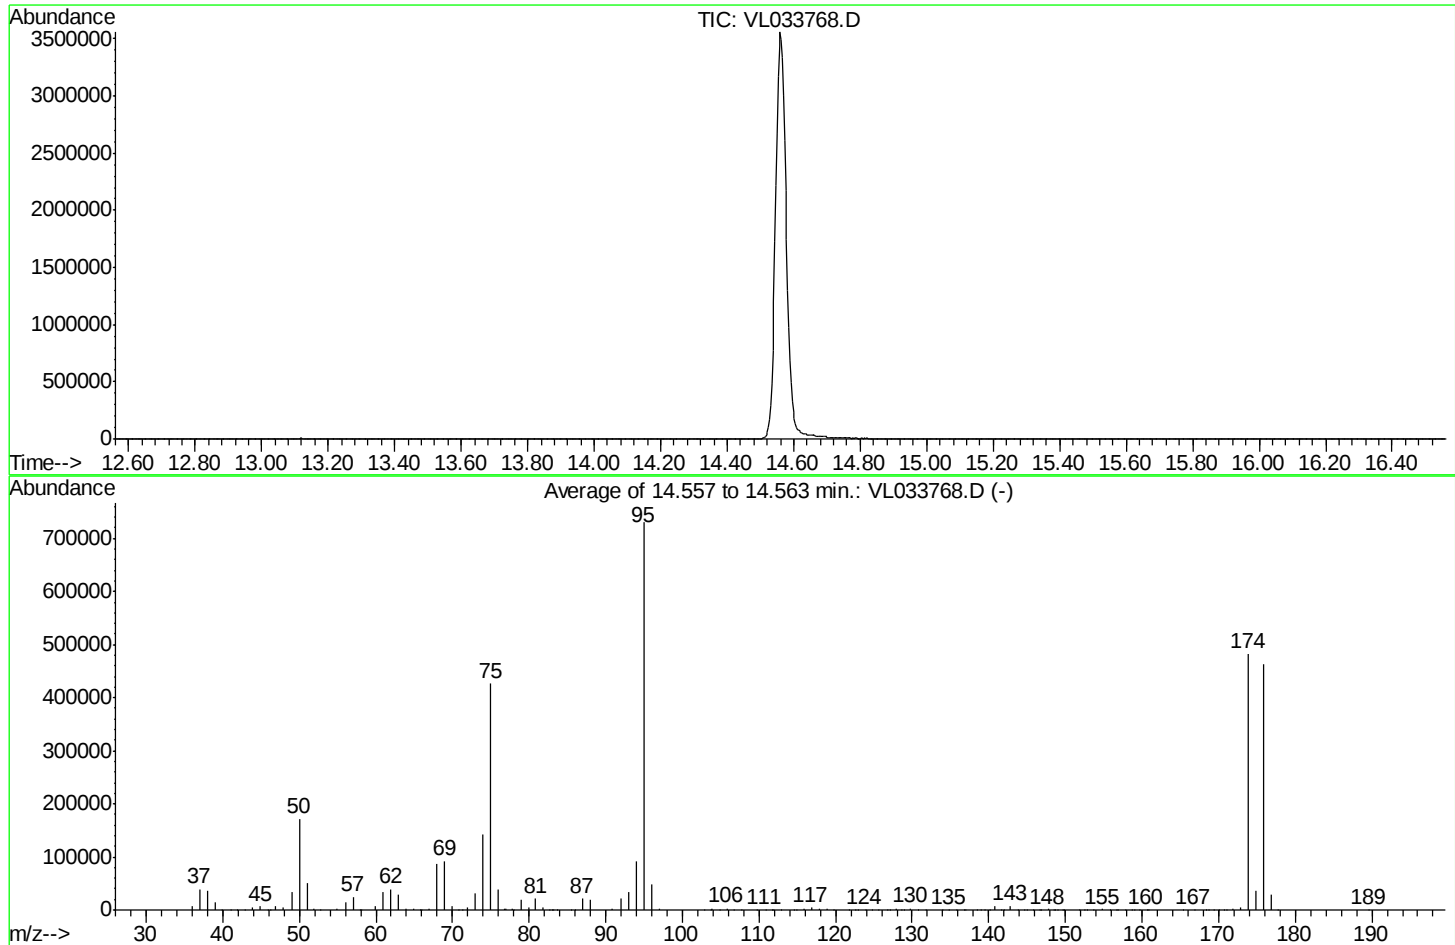

AutoFind: Scans 3614, 3615, 3616; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.5	171712	PASS
75	95	30	66	58.4	426410	PASS
95	95	100	100	100.0	730389	PASS
96	95	5	9	6.7	48672	PASS
173	174	0.00	2	0.9	4199	PASS
174	95	50	120	66.2	483370	PASS
175	174	4	9	7.5	36344	PASS
176	174	93	101	95.8	462997	PASS
177	176	5	9	6.3	29293	PASS