

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052322\
 Data File : VL039101.D
 Acq On : 24 May 2022 2:23
 Operator : SY/AP
 Sample : N2957-01DL 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VP-1DL

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/25/2022
 Supervised By : Mahesh Dadoda 05/26/2022

Quant Time: May 24 06:05:46 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 26 13:04:34 2022

QLast Update : Thu May 05 10:12:15 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.652	49	1290590	10.000	ppbv	-0.01
33) 1,4-Difluorobenzene	7.153	114	3488254	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.056	117	3072370	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.384	95	2304056	9.469	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	94.700%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	3.044	85	80219	0.397	ppbv	93
3) Chlorodifluoromethane	2.976	51	19976m	0.125	ppbv	
4) Chloromethane	3.137	50	10157m	0.127	ppbv	
9) Propene	3.005	41	108281	1.548	ppbv	87
10) Heptane	8.098	43	66601m	0.388	ppbv	
13) Ethanol	3.587	45	58099m	11.739	ppbv	
15) Acetone	3.838	43	1109413	9.113	ppbv	95
17) tert-Butyl alcohol	4.288	59	16044m	0.171	ppbv	
19) Isopropyl Alcohol	3.963	45	22139	0.382	ppbv #	95
20) Methylene Chloride	4.333	84	161133	3.512	ppbv	94
26) Hexane	5.674	57	217522	1.680	ppbv #	38
27) Carbon Disulfide	4.539	76	39757	0.323	ppbv #	89
29) Chloroform	5.735	83	189420	0.904	ppbv	94
30) Cyclohexane	7.105	84	25785m	0.238	ppbv	
34) 2-Butanone	5.230	43	237450m	1.334	ppbv	
36) Benzene	6.870	78	117292	0.393	ppbv #	91
38) Trichloroethene	7.815	130	21980m	0.166	ppbv	
41) Tetrahydrofuran	6.044	42	23946m	0.200	ppbv	
44) 2,2,4-Trimethylpentane	7.854	57	91964m	0.176	ppbv	
50) 4-Methyl-2-Pentanone	8.735	43	56247m	0.180	ppbv	
52) Tetrachloroethene	11.201	164	222985	2.090	ppbv	93
53) Toluene	9.780	91	583186	1.743	ppbv	99
57) Chlorobenzene	12.121	112	58550	0.254	ppbv #	86
58) Ethyl Benzene	12.687	91	164137m	0.371	ppbv	
59) m/p-Xylene	12.937	91	476331	1.262	ppbv	92
60) o-Xylene	13.661	91	205666	0.579	ppbv	99
72) 4-Ethyltoluene	15.809	105	87243	0.216	ppbv #	97
73) 1,3,5-Trimethylbenzene	15.966	105	93854m	0.258	ppbv	
74) 1,2,4-Trimethylbenzene	16.731	105	316702	0.794	ppbv #	67
79) Naphthalene	22.159	128	35676m	0.110	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

Abundance

TIC: VL039101.D\data.ms

Time-->

Chlorobenzene-d5, I

Chlorobenzene, I

1,4-Difluorobenzene, I

Bromo-4-Fluorobenzene, S

1,2,4-Trimethylbenzene, T

4-Ethyltoluene, T

1,3,5-Trimethylbenzene, T

1,2,4-Trimethylbenzene, T

Naphthalene, T

o-Xylene, T

m,p-Xylene, T

Ethyl Benzene, T

Tetrachloroethene, T

Toluene, T

4-Methyl-2-Pentanone, T

Heptane, T

1,2-Dichloroethane, T

1,3-Dichlorobenzene, T

Cyclohexane, I

Benzene, T

Tetrahydrofuran, T

2-Butanone, T

Hexane, T

Bromochloromethane, I

Carbon Disulfide, I

Methylene Chloride, T


tert-Butyl alcohol

Isopropyl Alcohol, T

Ethanol


Acetone, T

1,1,1-Trichloroethane, T

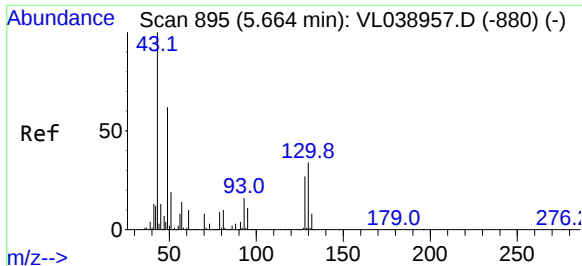

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.652 min Scan# 891
Delta R.T. -0.013 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL

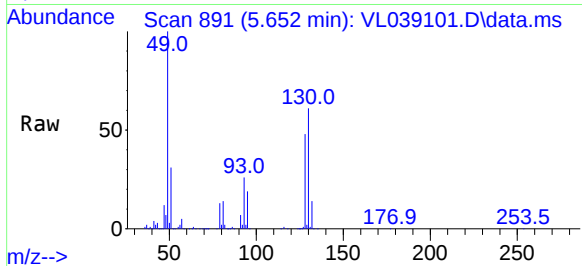


Tgt Ion: 49 Resp: 1290590
Ion Ratio Lower Upper
49 100
128 49.1 23.3 69.8
130 64.3 29.8 89.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

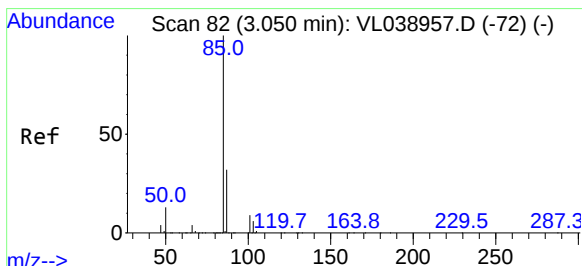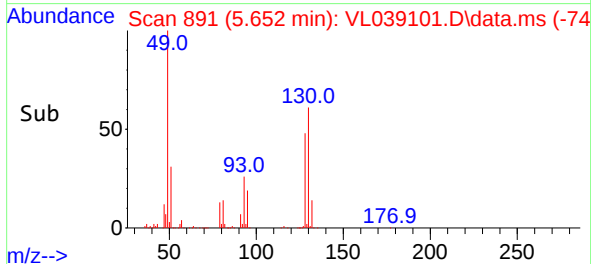


#2
Dichlorodifluoromethane
Concen: 0.397 ppbv
RT: 3.044 min Scan# 80
Delta R.T. -0.006 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

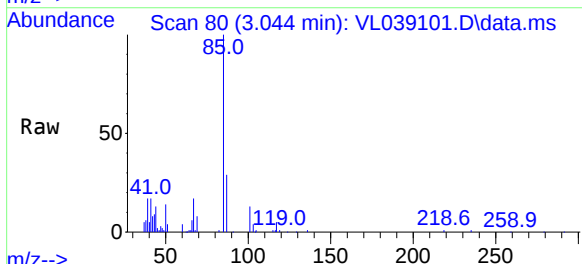

Tgt Ion: 85 Resp: 80219
Ion Ratio Lower Upper
85 100
87 27.9 25.7 38.5

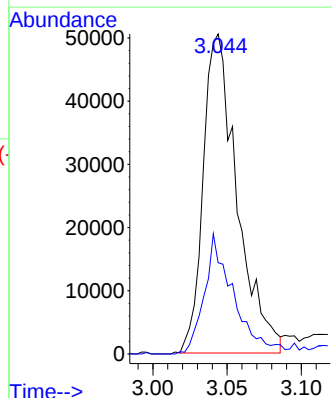

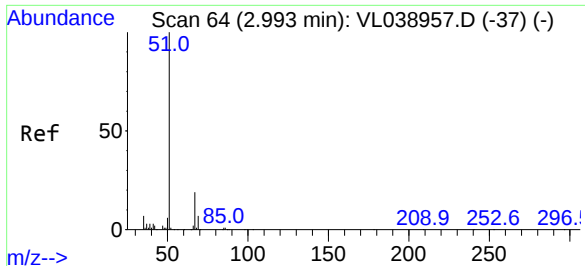





#3
Chlorodifluoromethane
Concen: 0.125 ppbv m
RT: 2.976 min Scan# 51
Delta R.T. -0.016 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

Instrument :
MSVOA_L
ClientSampleId :
VP-1DL

Tgt Ion: 51 Resp: 19970
Ion Ratio Lower Upper
51 100
67 16.7 15.8 23.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

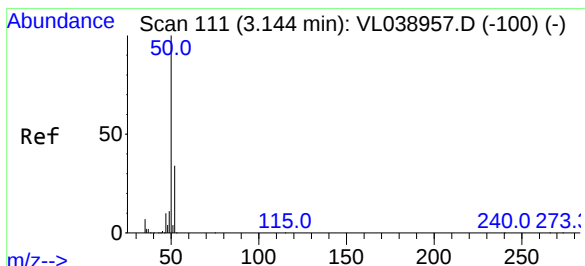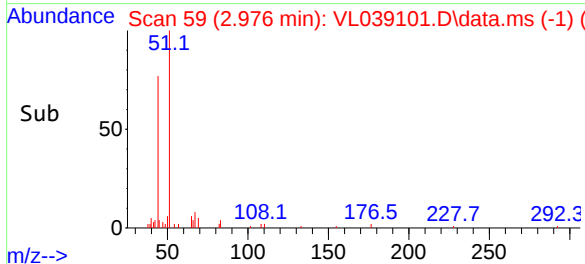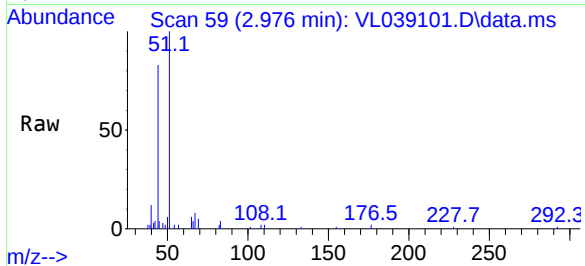

#4
Chloromethane
Concen: 0.127 ppbv m
RT: 3.137 min Scan# 109
Delta R.T. -0.006 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23


Tgt Ion: 50 Resp: 10157
Ion Ratio Lower Upper
50 100
52 20.3 27.3 40.9#

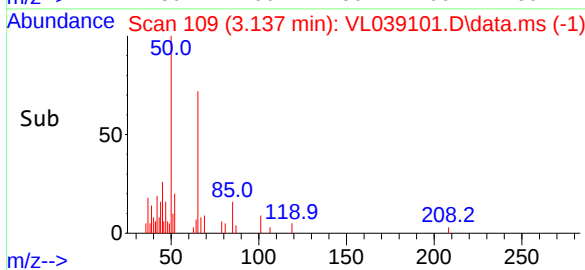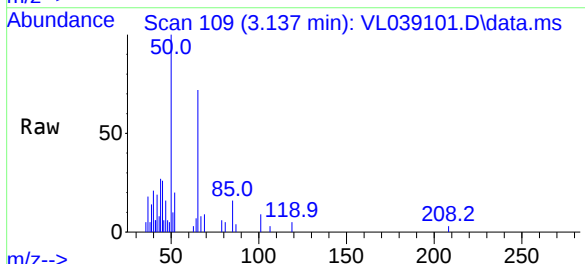



#9
Propene
Concen: 1.548 ppbv
RT: 3.005 min Scan# 61
Delta R.T. -0.006 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL

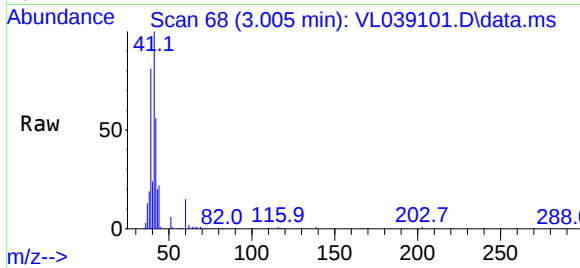

Tgt Ion: 41 Resp: 10828
Ion Ratio Lower Upper
41 100
42 62.4 58.3 87.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

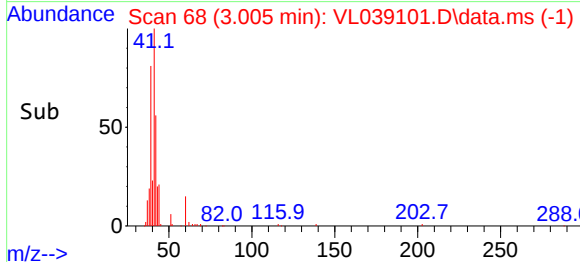

#10
Heptane
Concen: 0.388 ppbv m
RT: 8.098 min Scan# 1652
Delta R.T. -0.016 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23


Tgt Ion: 43 Resp: 66601
Ion Ratio Lower Upper
43 100
57 54.8 40.5 60.7

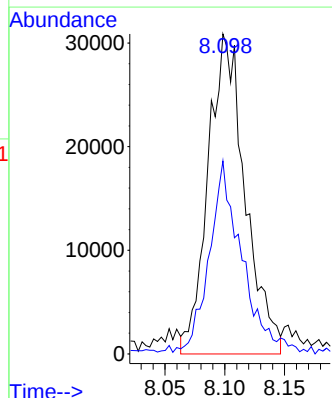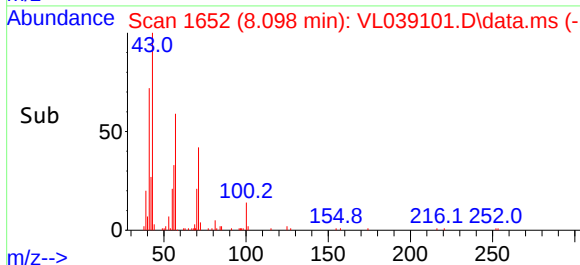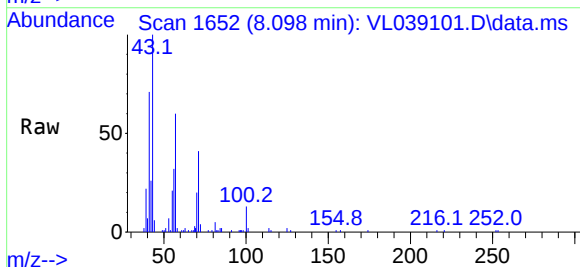



#13
Ethanol
Concen: 11.739 ppbv m
RT: 3.587 min Scan# 249
Delta R.T. -0.023 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL




Tgt Ion: 45 Resp: 5809
Ion Ratio Lower Upper
45 100
46 37.4 18.0 72.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

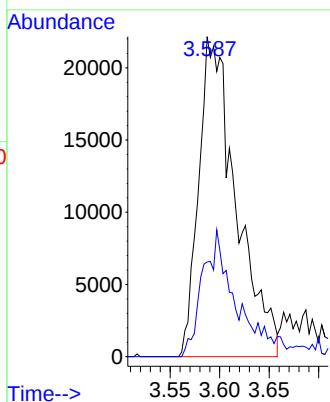


#15
Acetone
Concen: 9.113 ppbv
RT: 3.838 min Scan# 327
Delta R.T. -0.010 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Tgt Ion: 43 Resp: 1109413
Ion Ratio Lower Upper
43 100
58 29.3 21.3 31.9

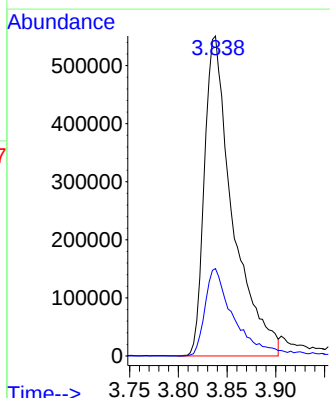



#17
tert-Butyl alcohol
Concen: 0.171 ppbv m
RT: 4.288 min Scan# 4
Delta R.T. 0.006 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL




Tgt Ion: 59 Resp: 1604
Ion Ratio Lower Upper
59 100
57 0.0 9.2 13.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

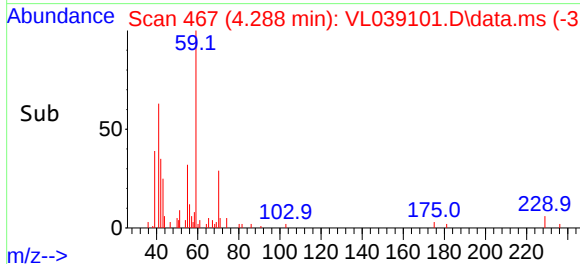


#19
Isopropyl Alcohol
Concen: 0.382 ppbv
RT: 3.963 min Scan# 366
Delta R.T. 0.006 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

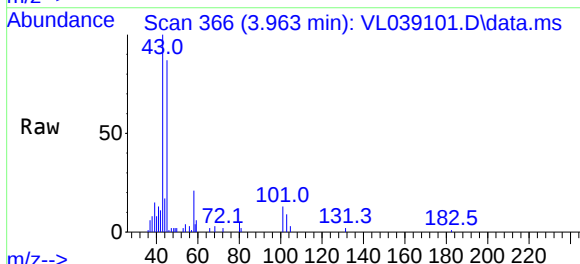


Tgt Ion: 45 Resp: 22139
Ion Ratio Lower Upper
45 100
58 0.0 1.4 2.2#

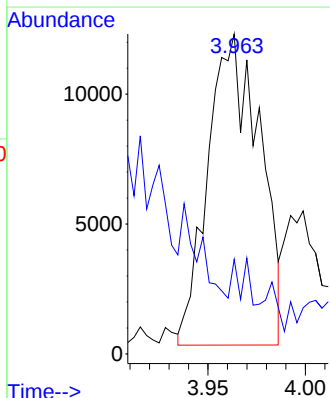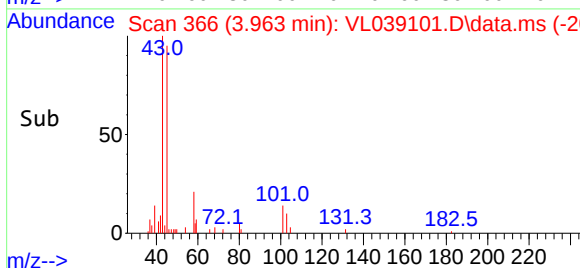

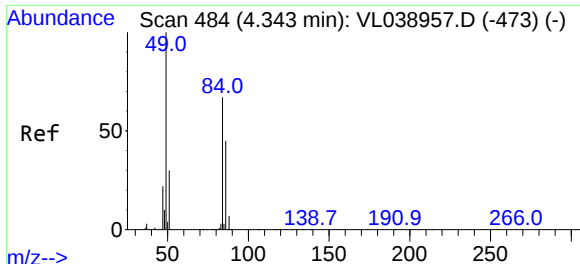

#20
Methylene Chloride
Concen: 3.512 ppbv
RT: 4.333 min Scan# 41
Delta R.T. -0.010 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL




Tgt Ion: 84 Resp: 16113
Ion Ratio Lower Upper
84 100
49 157.4 119.9 179.9
51 49.1 35.7 53.5
86 62.1 53.8 80.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022




#26
Hexane
Concen: 1.680 ppbv
RT: 5.674 min Scan# 898
Delta R.T. -0.010 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

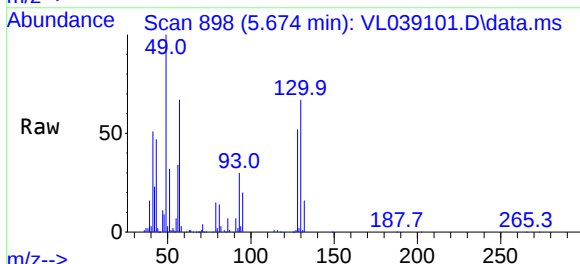


Tgt Ion: 57 Resp: 217522
Ion Ratio Lower Upper
57 100
41 87.3 75.2 112.8
43 73.9 190.8 286.2#
56 52.3 43.0 64.6

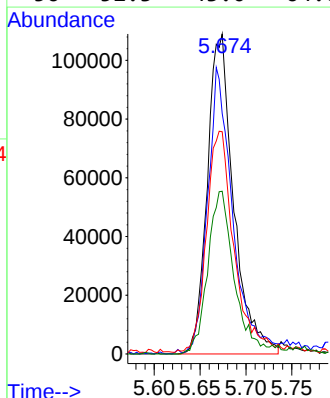

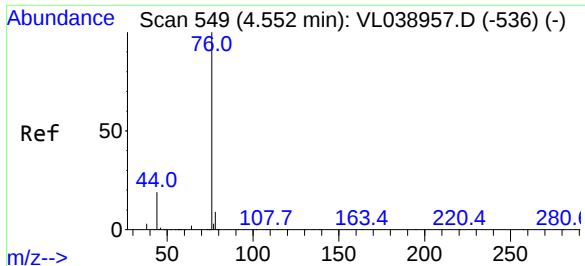

#27
Carbon Disulfide
Concen: 0.323 ppbv
RT: 4.539 min Scan# 549
Delta R.T. -0.013 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL

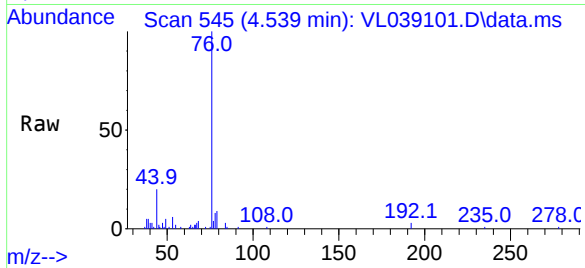


Tgt Ion: 76 Resp: 3975
Ion Ratio Lower Upper
76 100
44 26.1 15.3 22.9
78 10.9 8.2 12.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

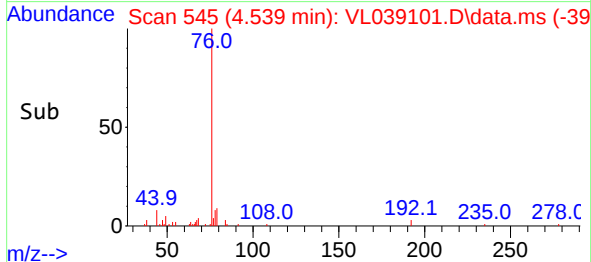


#29
Chloroform
Concen: 0.904 ppbv
RT: 5.735 min Scan# 917
Delta R.T. -0.016 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

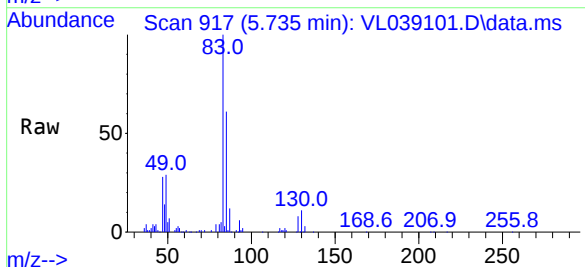

Tgt Ion: 83 Resp: 189420
Ion Ratio Lower Upper
83 100
85 59.6 51.8 77.6

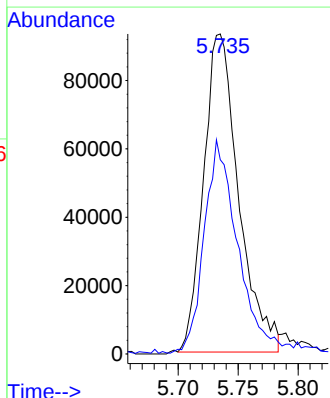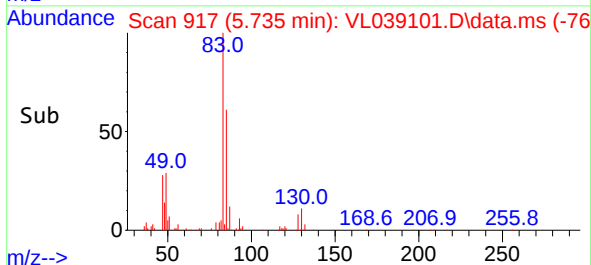







#30
Cyclohexane
Concen: 0.238 ppbv m
RT: 7.105 min Scan# 1350
Delta R.T. -0.023 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

Instrument :
MSVOA_L
ClientSampleId :
VP-1DL

Tgt Ion: 84 Resp: 2578
Ion Ratio Lower Upper
84 100
56 0.0 115.3 172.9
41 75.9 72.0 108.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

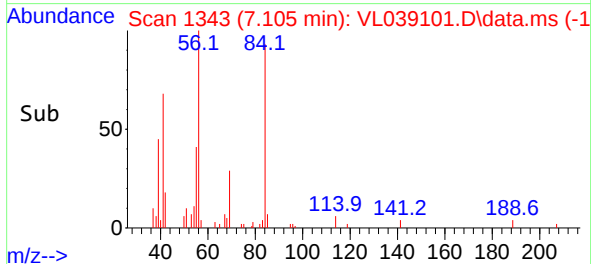

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.153 min Scan# 1358
Delta R.T. -0.019 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23


Tgt Ion:114 Resp: 3488254
Ion Ratio Lower Upper
114 100
63 24.4 22.6 33.8
88 17.9 15.4 23.0

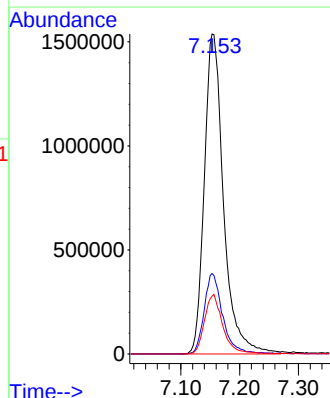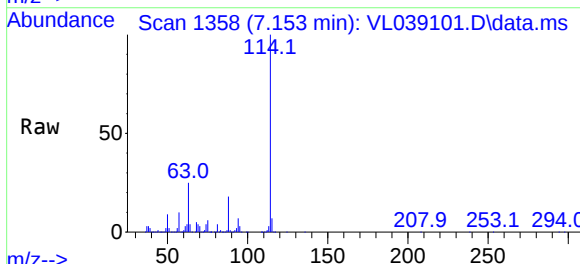

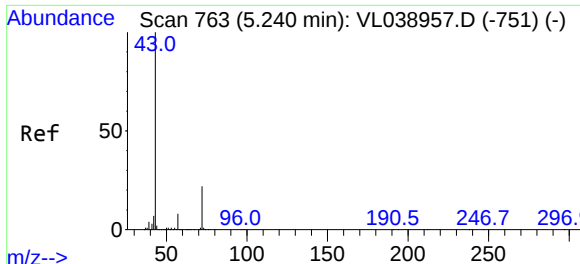

#34
2-Butanone
Concen: 1.334 ppbv m
RT: 5.230 min Scan# 7
Delta R.T. -0.010 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL



Tgt Ion: 43 Resp: 237450
Ion Ratio Lower Upper
43 100
72 23.6 17.8 26.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022



#36
Benzene
Concen: 0.393 ppbv
RT: 6.870 min Scan# 1270
Delta R.T. -0.016 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

Tgt Ion: 78 Resp: 117292
Ion Ratio Lower Upper
78 100
77 19.7 18.6 28.0
50 14.8 15.6 23.4

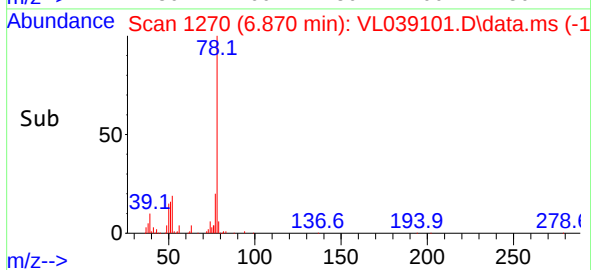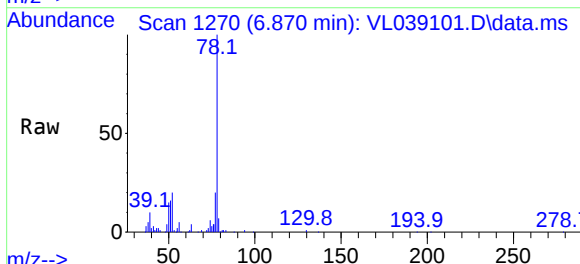







#38
Trichloroethene
Concen: 0.166 ppbv m
RT: 7.815 min Scan# 1
Delta R.T. -0.013 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

Instrument :
MSVOA_L
ClientSampleId :
VP-1DL

Tgt Ion:	130	Resp:	21980
Ion Ratio	Lower	Upper	
130	100		
95	112.0	94.8	142.2
132	103.5	75.8	113.8
97	64.3	63.6	95.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

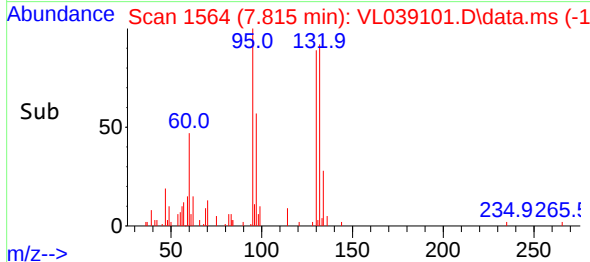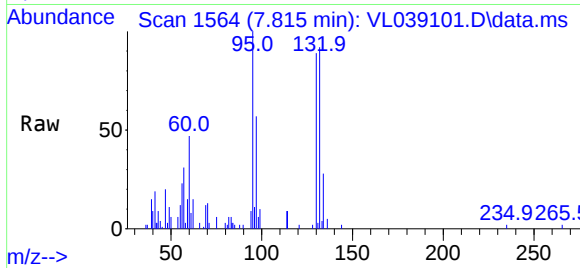

#41
Tetrahydrofuran
Concen: 0.200 ppbv m
RT: 6.044 min Scan# 1013
Delta R.T. 0.003 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23


Tgt Ion:	42	Resp:	23946
Ion Ratio	Lower	Upper	
42	100		
72	40.4	31.8	47.6
71	40.5	30.6	45.8

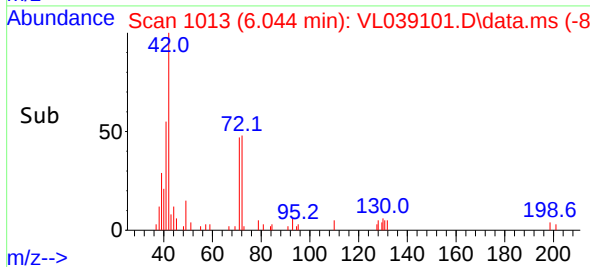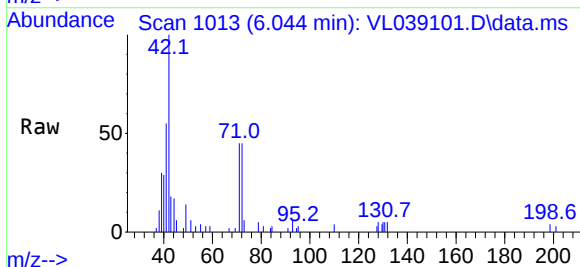



#44
2,2,4-Trimethylpentane
Concen: 0.176 ppbv m
RT: 7.854 min Scan# 11
Delta R.T. -0.010 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL



Tgt Ion: 57 Resp: 91964
Ion Ratio Lower Upper
57 100
41 0.0 26.3 39.5
56 46.5 24.6 37.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

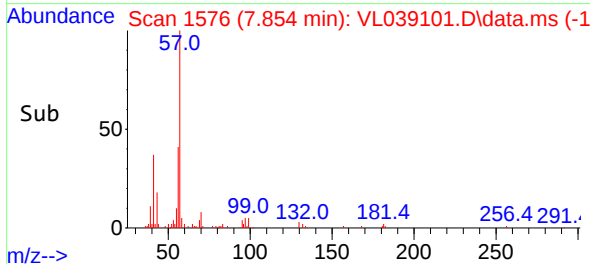

#50
4-Methyl-2-Pentanone
Concen: 0.180 ppbv m
RT: 8.735 min Scan# 1850
Delta R.T. 0.003 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23


Tgt Ion: 43 Resp: 56247
Ion Ratio Lower Upper
43 100
58 38.7 28.4 42.6

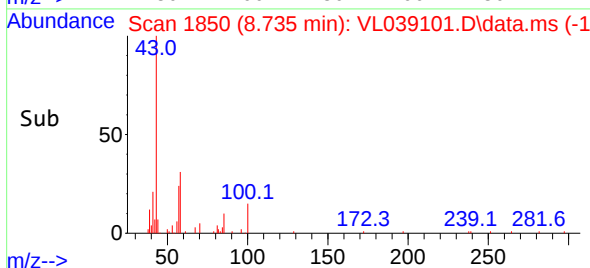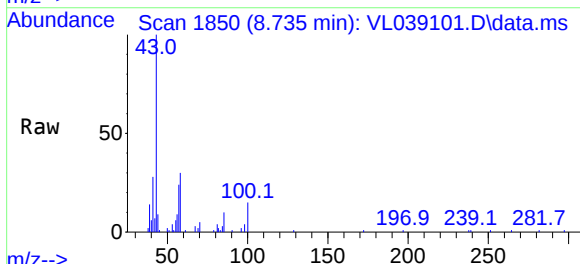



#52
Tetrachloroethene
Concen: 2.090 ppbv
RT: 11.201 min Scan# 2175
Delta R.T. -0.010 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL




Tgt Ion:164 Resp: 222985
Ion Ratio Lower Upper
164 100
166 121.1 102.5 153.7
129 101.7 90.1 135.1
131 100.9 84.8 127.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

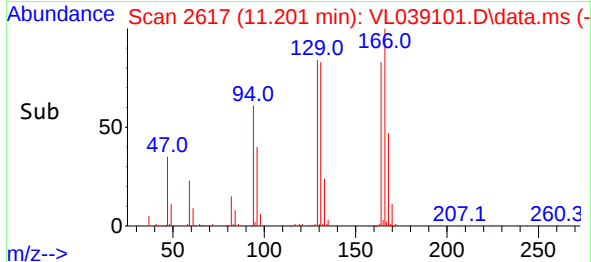


#53
Toluene
Concen: 1.743 ppbv
RT: 9.780 min Scan# 2175
Delta R.T. -0.019 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

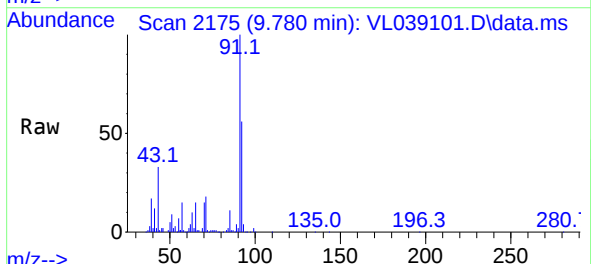

Tgt Ion: 91 Resp: 583186
Ion Ratio Lower Upper
91 100
92 61.1 48.2 72.2

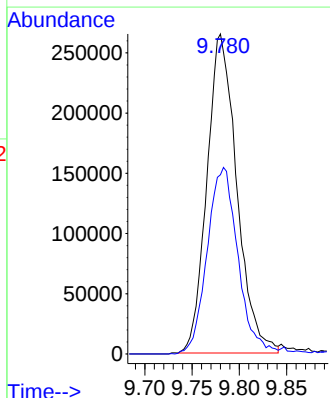



#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.056 min Scan# 2883

Delta R.T. -0.019 min

Lab File: VL039101.D

Acq: 24 May 2022 2:23

Instrument :

MSVOA_L

ClientSampleId :

VP-1DL

Tgt Ion:117 Resp: 3072370

Ion Ratio Lower Upper

117 100

82 66.3 57.0 85.6





119 33.8 27.2 40.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/25/2022

Supervised By :Mahesh Dadoda 05/26/2022

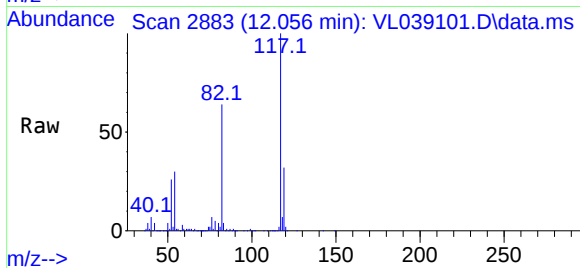

#57

Chlorobenzene

Concen: 0.254 ppbv

RT: 12.121 min Scan# 2903

Delta R.T. -0.016 min

Lab File: VL039101.D

Acq: 24 May 2022 2:23




Tgt Ion:112 Resp: 58550


Ion Ratio Lower Upper

112 100

77 55.2 57.7 86.5


114 32.8 30.1 36.7

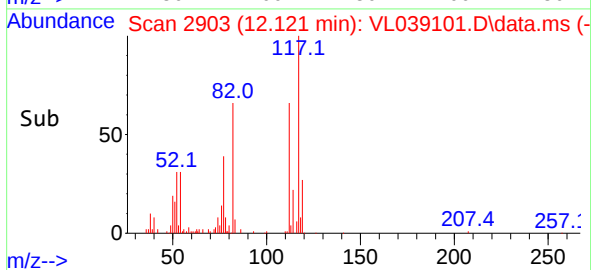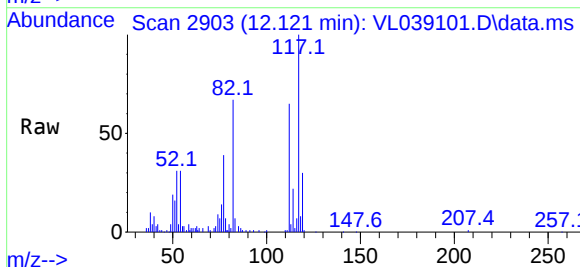



#58
Ethyl Benzene
Concen: 0.371 ppbv m
RT: 12.687 min Scan# 3083
Delta R.T. -0.013 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL




Tgt Ion: 91 Resp: 16413
Ion Ratio Lower Upper
91 100
106 22.9 24.2 36.4

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

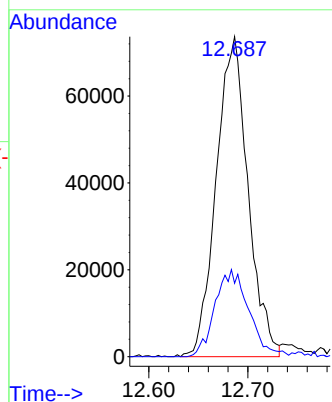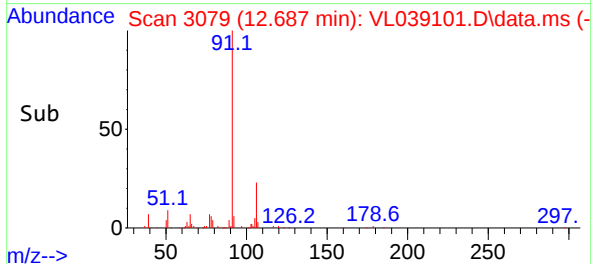


#59
m/p-Xylene
Concen: 1.262 ppbv
RT: 12.937 min Scan# 3157
Delta R.T. -0.048 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

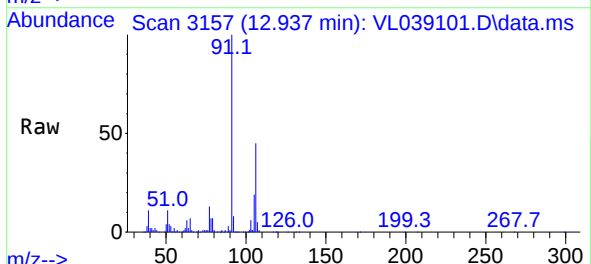

Tgt Ion: 91 Resp: 476331
Ion Ratio Lower Upper
91 100
106 48.1 34.6 52.0









#60
o-Xylene
Concen: 0.579 ppbv
RT: 13.661 min Scan# 310
Delta R.T. -0.019 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

Instrument :
MSVOA_L
ClientSampleId :
VP-1DL

Tgt Ion: 91 Resp: 205660
Ion Ratio Lower Upper
91 100
106 43.4 22.2 66.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

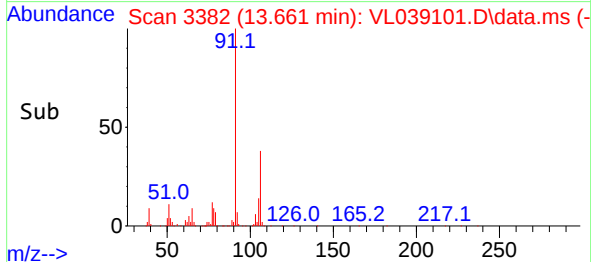

#68
1-Bromo-4-Fluorobenzene
Concen: 9.469 ppbv
RT: 14.384 min Scan# 3607
Delta R.T. -0.019 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

Tgt Ion: 95 Resp: 2304056
Ion Ratio Lower Upper
95 100
174 67.8 50.8 76.2
175 5.1 3.8 5.6

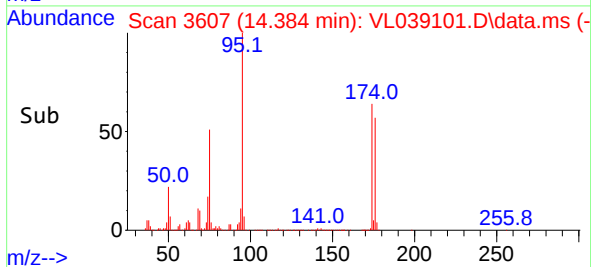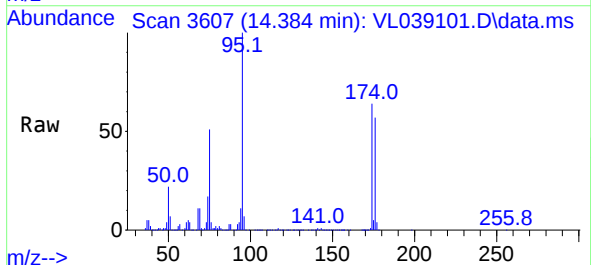







#72
4-Ethyltoluene
Concen: 0.216 ppbv
RT: 15.809 min Scan# 4050
Delta R.T. -0.019 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

Instrument :
MSVOA_L
ClientSampleId :
VP-1DL

Tgt Ion:	105	Resp:	8724
Ion Ratio	Lower	Upper	
105	100		
120	30.0	23.4	35.0
91	16.0	10.6	16.0
77	17.3	12.5	18.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

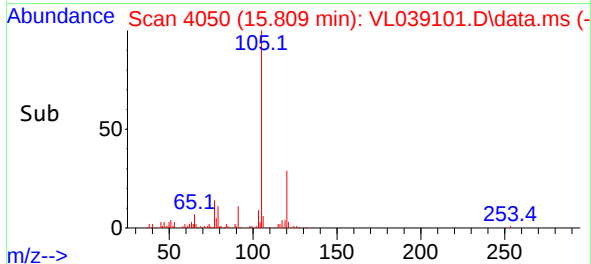

#73
1,3,5-Trimethylbenzene
Concen: 0.258 ppbv m
RT: 15.966 min Scan# 4099
Delta R.T. -0.019 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23


Tgt Ion:	105	Resp:	93854
Ion Ratio	Lower	Upper	
105	100		
120	43.9	34.4	51.6

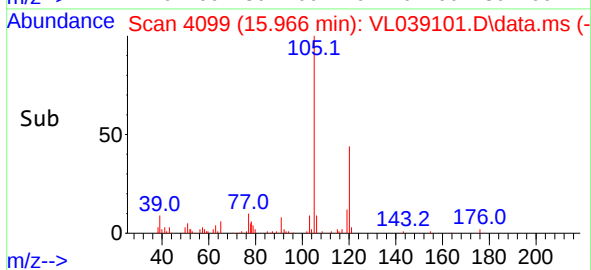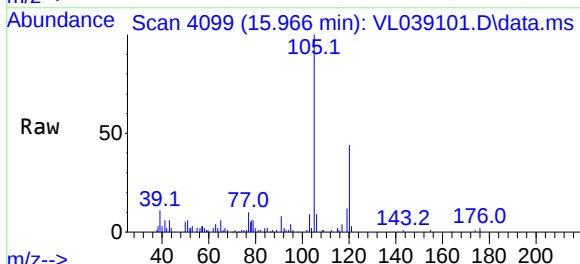



#74
1,2,4-Trimethylbenzene
Concen: 0.794 ppbv
RT: 16.731 min Scan# 41
Delta R.T. -0.016 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23




Instrument :
MSVOA_L
ClientSampleId :
VP-1DL




Tgt Ion:105 Resp: 31670
Ion Ratio Lower Upper
105 100
120 43.4 36.9 55.3
91 11.9 45.0 67.4
77 12.5 19.2 28.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/25/2022
Supervised By :Mahesh Dadoda 05/26/2022

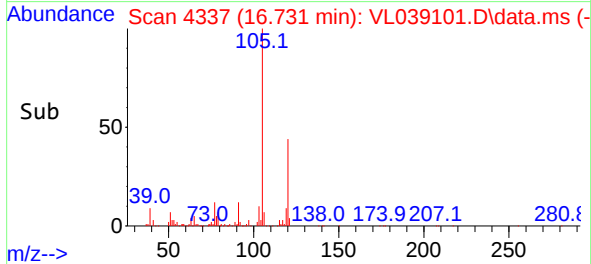

#79
Naphthalene
Concen: 0.110 ppbv m
RT: 22.159 min Scan# 6025
Delta R.T. -0.013 min
Lab File: VL039101.D
Acq: 24 May 2022 2:23

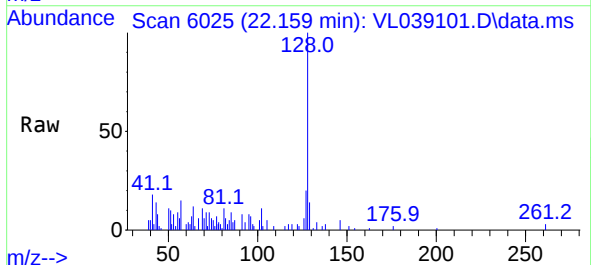

Tgt Ion:128 Resp: 35676
Ion Ratio Lower Upper
128 100
127 20.0 10.2 15.2#
129 14.4 8.9 13.3#

