


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052322\
 Data File : VL039082.D
 Acq On : 23 May 2022 11:09
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
 Last Update : Thu May 05 10:12:15 2022

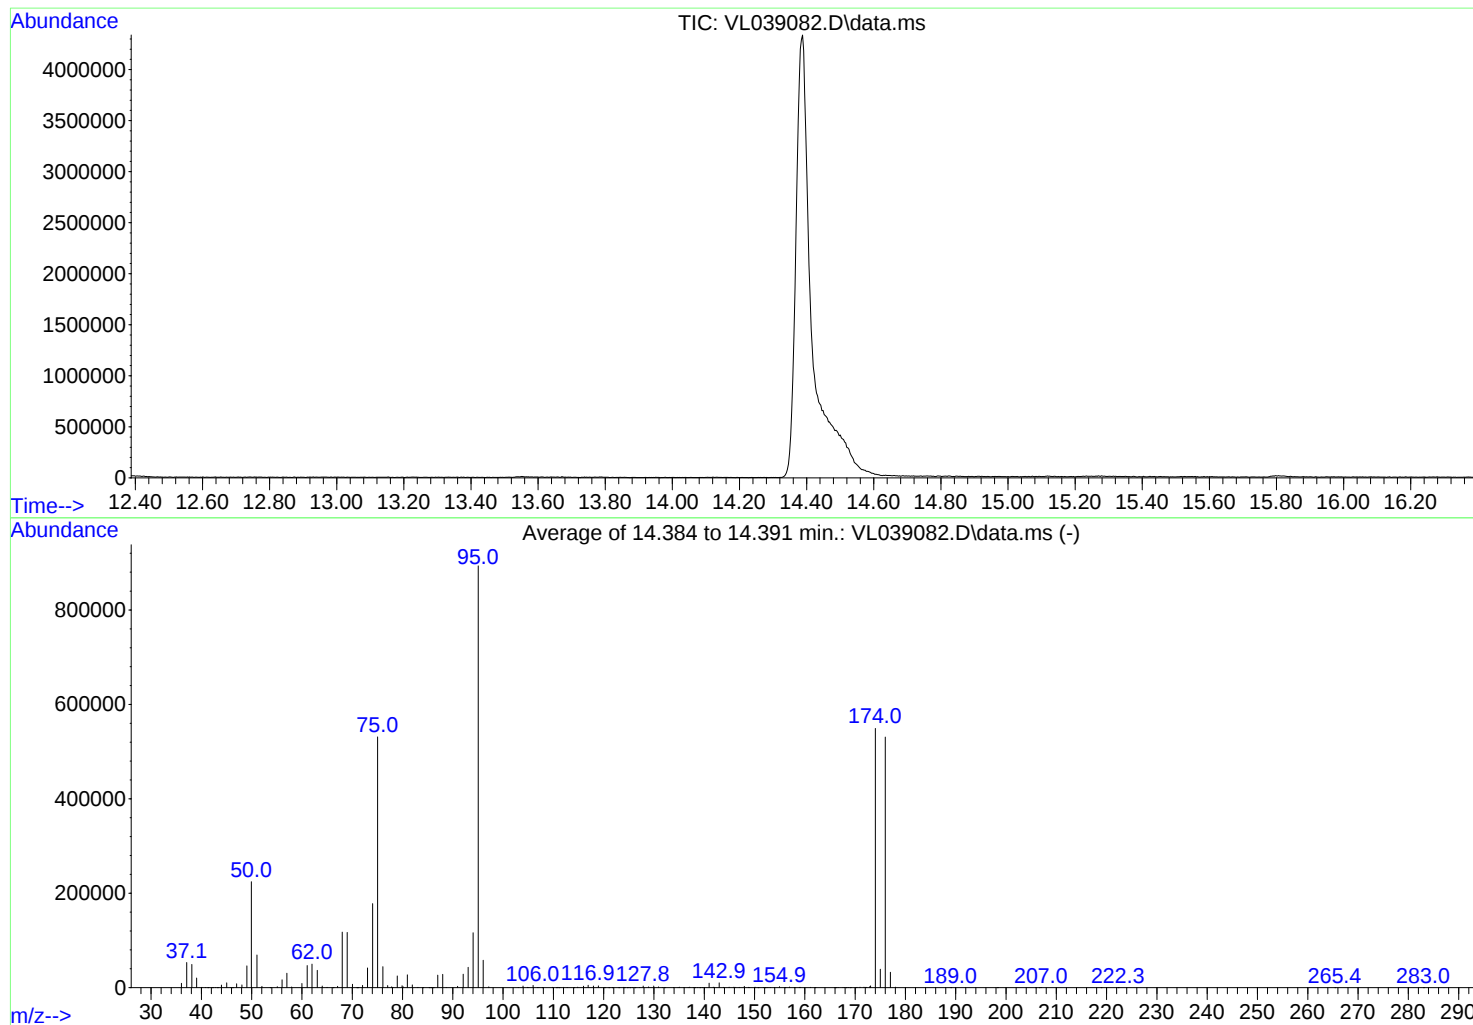

AutoFind: Scans 3607, 3608, 3609; Background Corrected with Scan 3579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.1	224390	PASS
75	95	30	66	59.5	531221	PASS
95	95	100	100	100.0	893461	PASS
96	95	5	9	6.5	57960	PASS
173	174	0.00	2	0.7	3811	PASS
174	95	50	120	61.5	549163	PASS
175	174	4	9	7.1	39005	PASS
176	174	93	101	96.7	530901	PASS
177	176	5	9	6.1	32443	PASS

Average of 14.384 to 14.391 min.: VL039082.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9179	45.05	10055	56.05	16749	68.00	11755
37.10	53233	45.85	535	57.00	30605	69.00	11678
38.10	49168	46.20	70	57.95	1445	70.05	732
39.05	20249	47.00	8027	60.00	8852	70.90	11
40.10	803	48.05	5897	61.05	46683	71.10	122
40.85	211	49.05	46128	62.00	49832	72.05	4843
41.30	75	49.95	224390	63.05	36696	73.05	41787
42.20	58	51.05	69120	64.05	3304	74.05	178027
42.85	512	52.05	2694	65.00	675	75.05	531221
43.20	105	53.70	88	66.20	104	76.10	44589
44.00	5336	55.10	2226	67.10	2697	77.05	4425

Average of 14.384 to 14.391 min.: VL039082.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.85	1698	85.90	270	97.15	1772	110.90	780
78.10	692	86.10	74	103.00	318	111.10	179
78.95	24627	87.00	26491	103.95	3315	112.05	736
79.90	4103	88.00	28200	104.85	693	112.75	506
80.10	2095	88.70	259	105.10	513	114.00	80
80.95	27083	90.95	2828	105.95	4620	114.85	1072
81.95	5869	92.05	28501	106.85	431	116.00	2960
83.05	698	93.05	43072	107.10	331	116.90	4988
84.00	94	94.05	116299	107.80	71	117.95	3267
85.30	67	95.05	893461	109.85	617	118.95	3674
85.60	140	96.05	57960	110.60	145	120.15	180

Average of 14.384 to 14.391 min.: VL039082.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.00	53	128.95	1646	137.80	201	144.95	888
121.70	57	129.95	3355	138.05	173	145.90	923
123.00	59	130.90	1645	138.70	369	146.10	671
123.90	637	131.75	205	139.10	154	146.95	729
124.10	105	132.10	94	139.70	312	147.95	2604
124.70	55	133.90	303	140.00	268	148.80	604
125.20	116	134.80	466	140.95	9667	149.00	296
125.75	365	135.05	1071	141.80	1024	150.10	989
126.20	62	135.95	257	142.00	792	150.70	53
127.15	359	136.80	469	142.95	10182	151.75	235
127.85	3360	137.10	1051	143.85	691	152.10	173

Average of 14.384 to 14.391 min.: VL039082.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.65	375	165.90	76	170.95	1084	189.00	133
153.10	474	166.10	157	171.75	1094	198.30	64
153.95	357	166.60	229	172.10	848	205.90	87
154.95	2228	167.60	355	172.30	722	206.60	56
156.00	71	167.90	193	172.90	2134	207.00	311
156.95	1262	168.20	68	173.05	3811	218.90	59
157.90	88	168.70	301	174.00	549163	222.30	61
158.90	612	169.00	146	175.00	39005	265.40	60
159.05	599	169.20	435	176.00	530901	283.00	81
161.10	777	170.20	241	177.00	32443		
162.00	53	170.35	666	178.05	959		