


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL053118\
Data File : VL032015.D
Acq On : 31 May 2018 15:26
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL053118AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jun 01 02:31:35 2018
Last Update : Fri Jun 01 02:31:35 2018

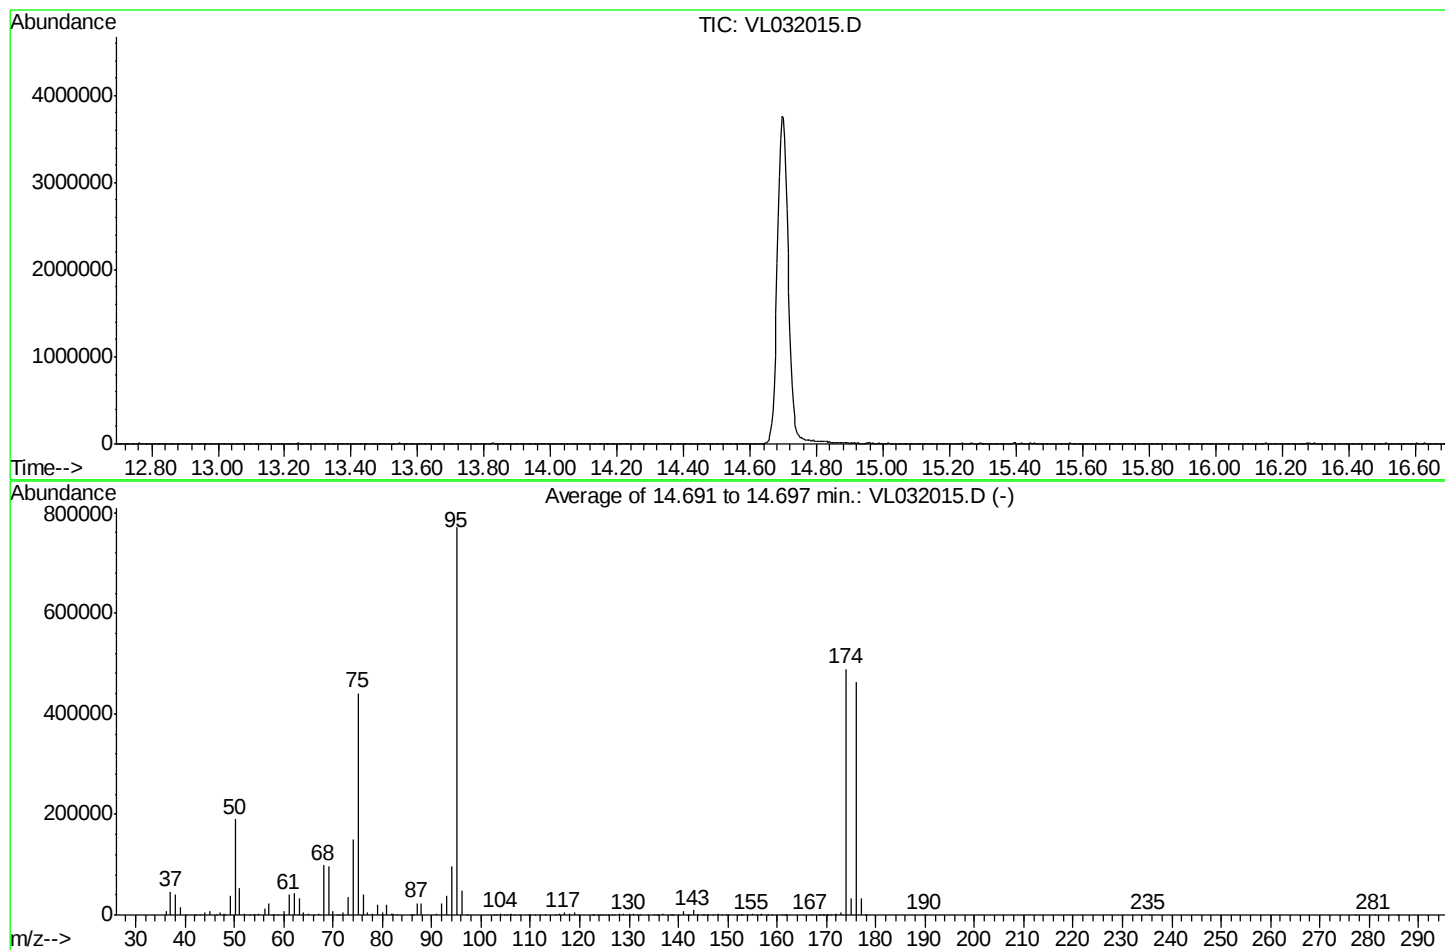

AutoFind: Scans 4231, 4232, 4233; Background Corrected with Scan 4209

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.7	190037	PASS
75	95	30	66	57.2	441194	PASS
95	95	100	100	100.0	770794	PASS
96	95	5	9	6.3	48392	PASS
173	174	0.00	2	1.1	5528	PASS
174	95	50	120	63.5	489194	PASS
175	174	4	9	6.7	32882	PASS
176	174	93	101	94.4	462016	PASS
177	176	5	9	7.3	33810	PASS