


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL060121\
 Data File : VL037063.D
 Acq On : 1 Jun 2021 9:01
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL051821AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue May 18 12:00:15 2021
 Last Update : Tue May 18 12:00:15 2021

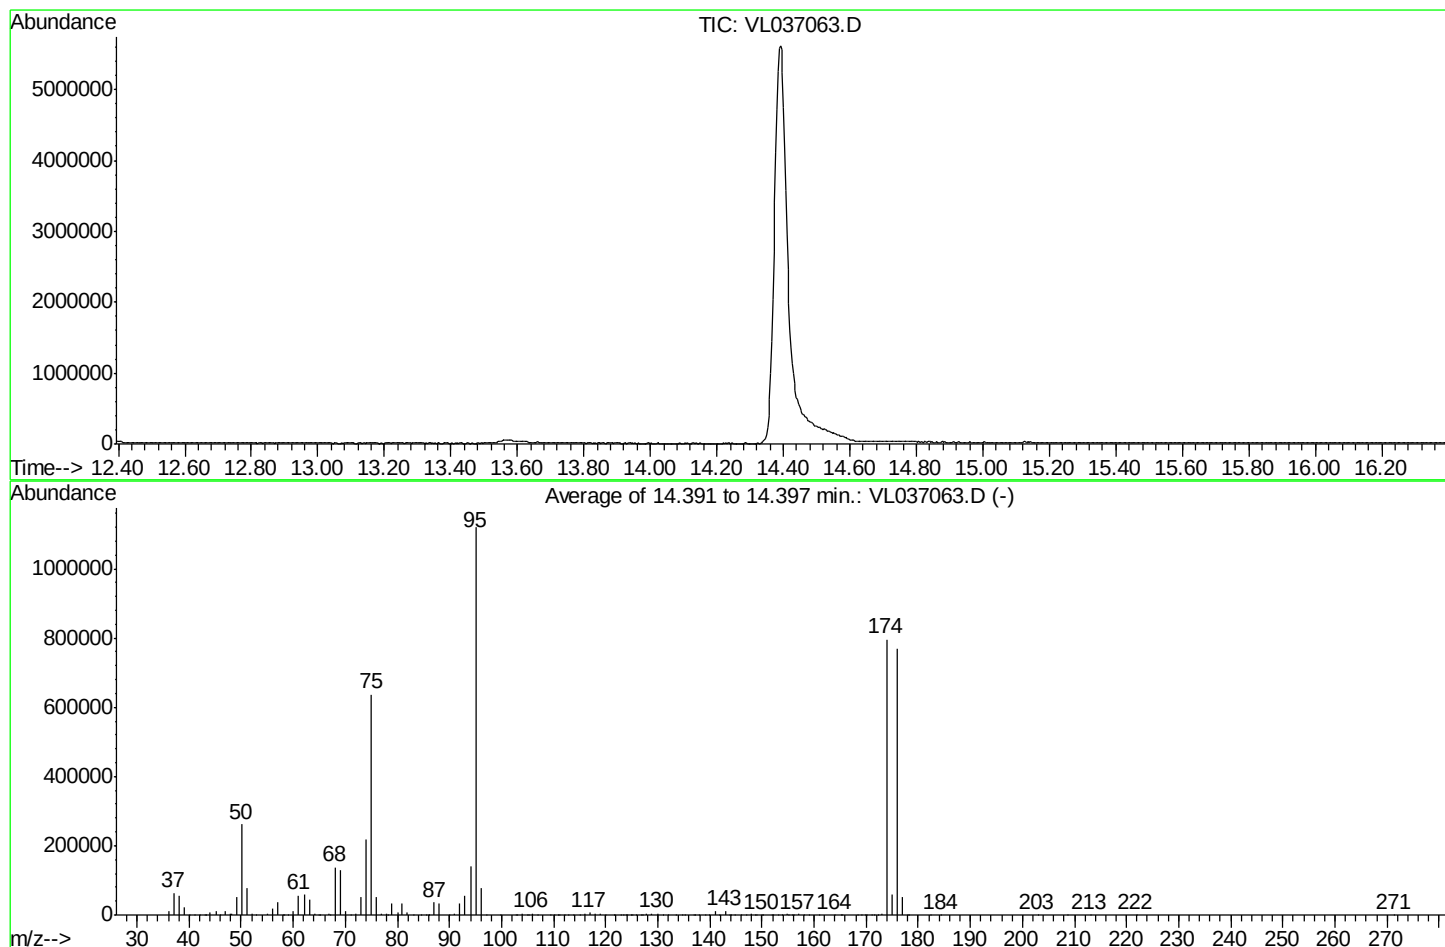

AutoFind: Scans 3609, 3610, 3611; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	261610	PASS
75	95	30	66	56.8	636458	PASS
95	95	100	100	100.0	1119590	PASS
96	95	5	9	7.1	79456	PASS
173	174	0.00	2	0.4	3080	PASS
174	95	50	120	71.1	795690	PASS
175	174	4	9	7.5	59813	PASS
176	174	93	101	96.8	770602	PASS
177	176	5	9	6.9	53266	PASS