
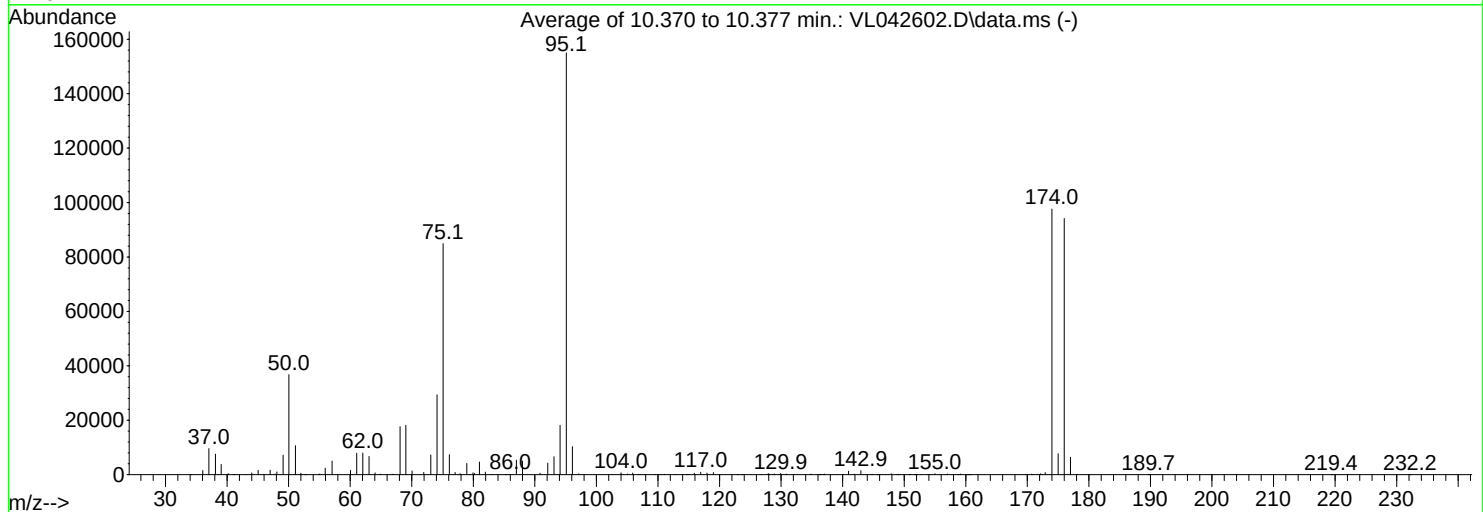


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060325\
Data File : VL042602.D
Acq On : 03 Jun 2025 09:12
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052925AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 30 02:01:56 2025

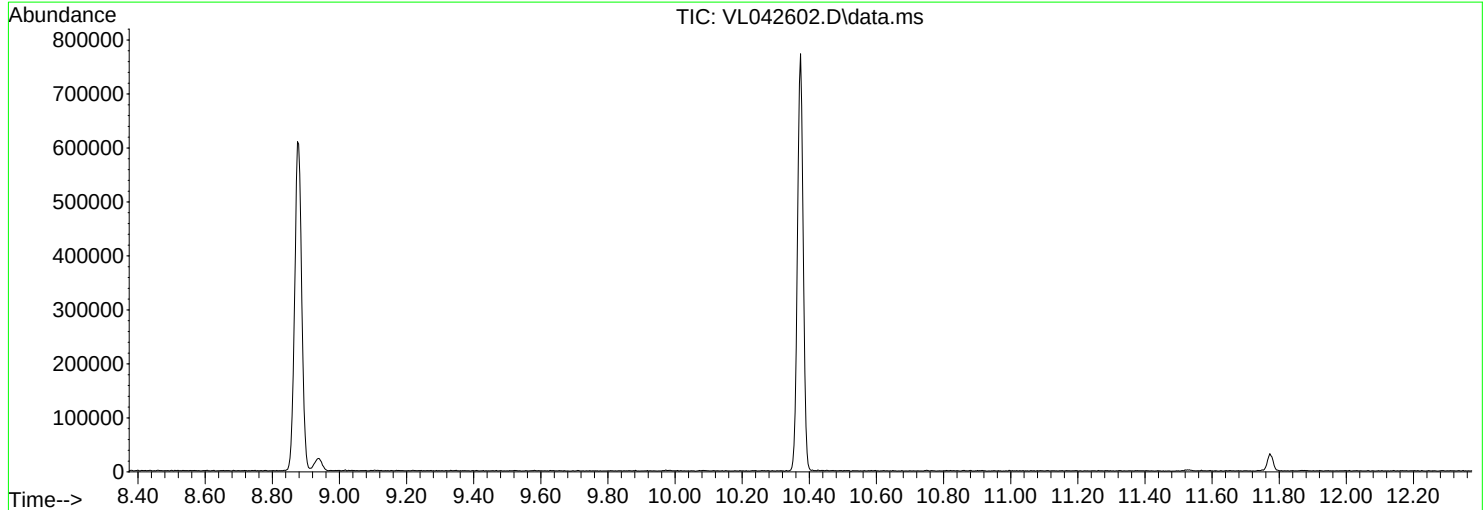

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3162

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.7	36789	PASS
75	95	30	66	54.8	84909	PASS
95	95	100	100	100.0	155029	PASS
96	95	5	9	6.6	10288	PASS
173	174	0.00	2	0.8	784	PASS
174	95	50	120	63.0	97645	PASS
175	174	4	9	7.9	7719	PASS
176	174	93	101	96.4	94149	PASS
177	176	5	9	6.8	6410	PASS

Average of 10.370 to 10.377 min.: VL042602.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
34.10	29	45.95	96	55.95	2433	67.10	90
36.05	1530	47.00	1650	57.05	4987	68.10	1764
37.05	9614	47.80	242	57.95	66	69.05	1811
38.10	7541	48.10	1015	60.05	1613	70.05	135
39.05	3774	49.10	7183	61.05	7908	71.95	818
40.20	360	50.05	36789	62.05	7925	73.10	7233
41.10	18	51.10	10679	63.05	6708	74.10	29355
41.95	123	52.00	564	64.05	665	75.10	84909
43.05	59	52.70	23	64.90	195	76.10	7345
44.00	648	54.90	103	66.00	66	77.05	823
45.05	1584	55.05	224	66.80	194	77.85	352

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 10.370 to 10.377 min.: VL042602.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	4127	90.85	535	106.80	134	115.10	74
79.95	717	92.10	4215	107.10	46	115.90	525
80.20	394	93.10	6593	107.80	26	116.95	902
81.00	4631	94.10	18128	109.60	38	117.95	581
81.95	940	95.10	155029	110.15	86	119.00	747
83.00	109	96.10	10288	110.60	39	122.90	20
85.20	18	97.15	284	111.10	126	123.60	19
85.80	47	102.65	51	111.75	88	124.10	37
86.05	141	104.00	705	112.85	119	125.10	35
87.00	5340	105.05	227	114.60	25	125.95	117
88.00	4987	105.90	612	114.90	63	126.85	46

Average of 10.370 to 10.377 min.: VL042602.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.90	394	137.05	233	146.95	60	155.00	342
128.10	168	139.10	40	147.90	374	155.80	131
128.70	69	140.05	124	148.75	41	156.80	65
128.95	264	140.95	1293	149.00	18	157.05	216
129.95	424	141.90	190	150.00	128	158.70	24
130.85	258	142.95	1490	150.80	23	159.15	223
132.15	66	143.80	33	151.70	21	160.30	21
134.85	214	144.70	41	152.10	57	160.60	22
136.20	21	144.85	124	152.75	66	160.95	93
136.50	36	145.60	21	153.80	40	169.70	75
136.90	45	146.05	94	154.10	40	170.70	159

Average of 10.370 to 10.377 min.: VL042602.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.90	69	219.40	29				
171.60	135	232.20	18				
172.15	281						
172.40	150						
172.90	784						
174.00	97645						
175.00	7719						
176.00	94149						
177.00	6410						
178.05	192						
189.70	20						