


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060523\
 Data File : VL040454.D
 Acq On : 5 Jun 2023 13:29
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Jun 06 06:22:12 2023

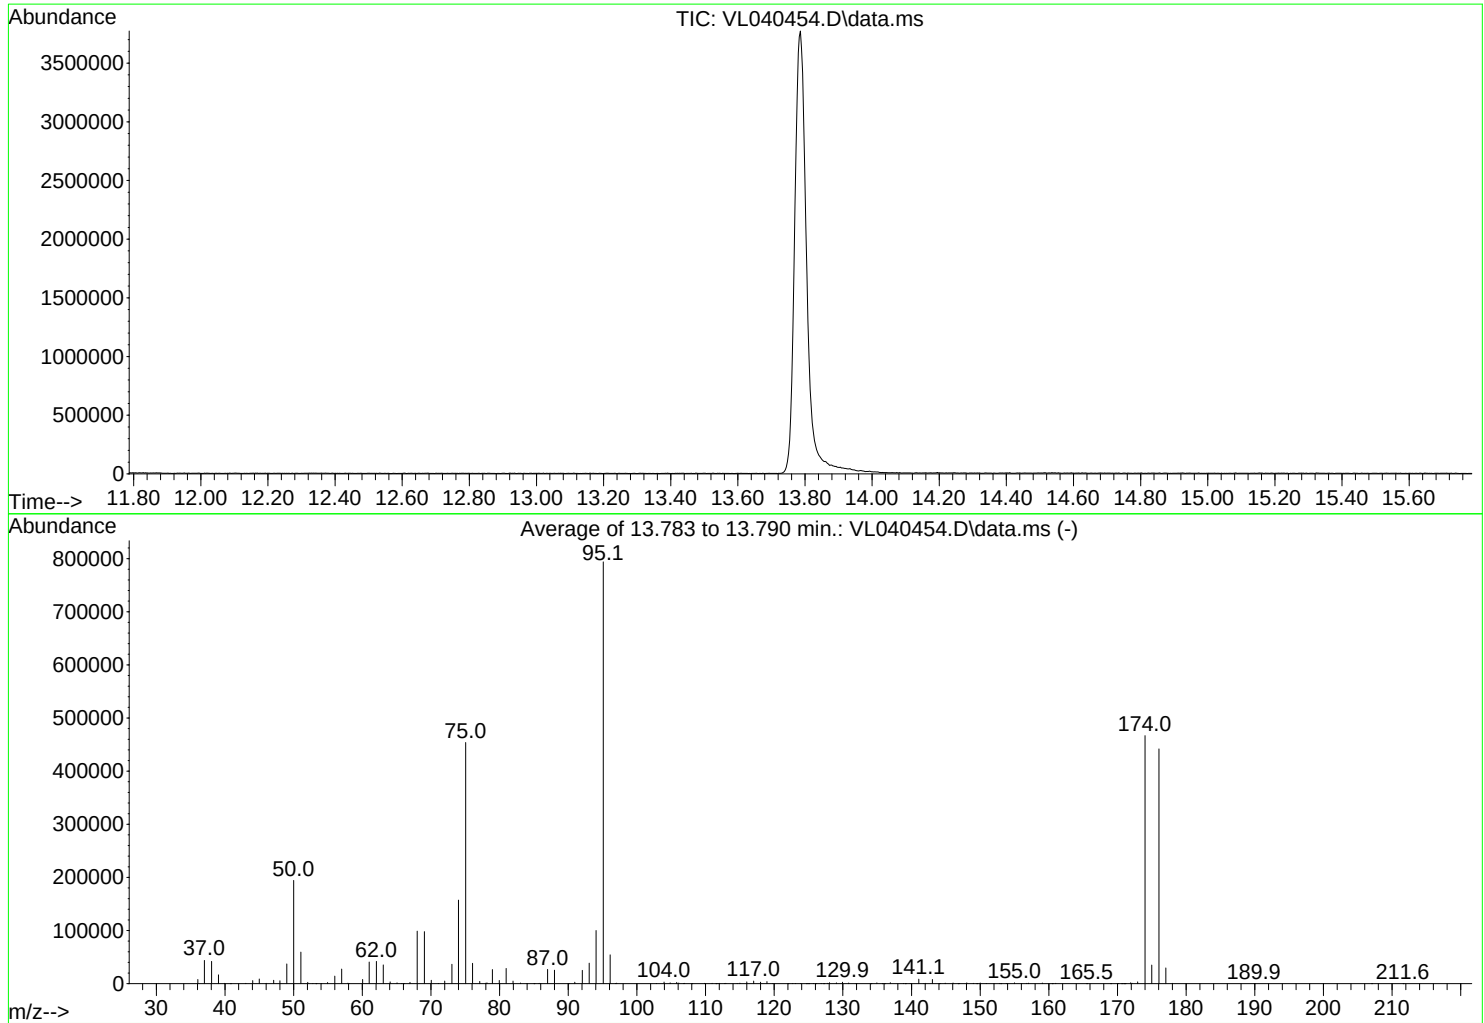

AutoFind: Scans 3477, 3478, 3479; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.5	194219	PASS
75	95	30	66	57.2	453995	PASS
95	95	100	100	100.0	793984	PASS
96	95	5	9	6.8	54091	PASS
173	174	0.00	2	0.7	3470	PASS
174	95	50	120	58.8	466816	PASS
175	174	4	9	7.5	34888	PASS
176	174	93	101	94.7	441984	PASS
177	176	5	9	6.7	29408	PASS

Average of 13.783 to 13.790 min.: VL040454.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7879	48.00	5414	57.90	913	68.00	9887
37.00	43789	49.00	36928	58.10	361	69.05	9799
38.05	41755	50.00	194219	60.05	7920	70.05	624
39.05	16681	51.05	59509	61.00	40664	71.10	30
39.95	547	52.05	2328	62.05	41875	72.00	4825
40.80	89	52.80	315	63.05	35251	73.05	36525
43.05	647	53.25	103	64.05	3346	74.00	157205
44.05	5823	54.05	335	65.05	1626	75.05	453995
45.00	8853	54.95	2239	65.75	377	76.05	38395
46.00	646	56.00	14304	66.00	123	77.10	4307
47.10	6489	57.00	27568	66.95	2487	78.00	955

Average of 13.783 to 13.790 min.: VL040454.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.15	1450	88.00	25315	103.95	2903	112.05	594
78.95	26547	90.00	56	104.85	1407	112.80	223
79.95	6176	90.95	2823	105.80	2333	112.95	680
80.95	28576	92.05	25133	106.10	1375	114.60	211
81.95	4982	93.05	38531	106.80	228	115.00	950
83.05	1135	94.05	99936	106.95	492	116.00	3425
84.00	197	95.10	793984	108.00	106	117.00	4791
85.00	50	96.10	54091	109.85	615	118.00	2602
85.75	513	96.90	456	110.95	674	118.95	3874
86.00	364	97.05	925	111.50	79	119.80	212
87.00	26771	102.85	349	111.80	239	122.00	126

Average of 13.783 to 13.790 min.: VL040454.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.70	239	129.05	1577	139.80	417	148.05	1646
123.10	200	129.95	2809	141.05	8332	149.00	765
123.85	412	130.85	1214	141.80	275	149.50	89
124.70	174	131.90	92	142.05	727	150.00	1148
125.00	171	134.10	65	143.05	7963	150.90	195
125.75	217	134.95	1555	144.00	164	152.00	449
126.00	79	135.75	180	144.15	384	152.80	314
126.85	233	136.05	179	144.90	913	153.00	64
127.20	101	136.90	1768	146.05	1143	153.80	227
127.80	707	138.85	302	146.80	187	154.00	445
128.05	1763	139.10	59	147.00	457	155.00	1597

Average of 13.783 to 13.790 min.: VL040454.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.05	252	171.10	65	211.60	80		
156.80	497	171.90	1509				
157.05	948	172.10	1004				
159.05	1265	172.95	3470				
160.50	164	174.00	466816				
161.00	510	175.00	34888				
165.50	66	176.05	441984				
169.00	156	177.05	29408				
170.15	204	178.00	554				
170.60	62	189.90	73				
170.90	189	207.00	67				