

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060622\
 Data File : VL039183.D
 Acq On : 6 Jun 2022 12:55
 Operator : SY/AP
 Sample : N3110-05 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-10

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2022
 Supervised By :Mahesh Dadoda 06/07/2022

Quant Time: Jun 06 13:49:14 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 06 13:49:14 2022

QLast Update : Wed Jun 01 01:22:18 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.664	49	1298440	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	7.169	114	3532948	10.000	ppbv	-0.01
55) Chlorobenzene-d5	12.076	117	3252611	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.404	95	2495369	9.280	ppbv	-0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	92.800%
Target Compounds						
					Qvalue	
3) Chlorodifluoromethane	2.986	51	16814	0.102	ppbv	99
4) Chloromethane	3.144	50	14963	0.176	ppbv	90
9) Propene	3.018	41	43169	0.599	ppbv	98
10) Heptane	8.114	43	48550m	0.289	ppbv	
11) Trichlorofluoromethane	3.954	101	677879	3.284	ppbv	100
13) Ethanol	3.603	45	114493	29.143	ppbv #	100
15) Acetone	3.845	43	3636205	26.884	ppbv	96
17) tert-Butyl alcohol	4.288	59	147708	1.408	ppbv #	93
19) Isopropyl Alcohol	3.967	45	71371	1.125	ppbv #	93
20) Methylene Chloride	4.343	84	134651	2.362	ppbv	94
26) Hexane	5.684	57	340804	2.544	ppbv #	40
27) Carbon Disulfide	4.549	76	30309	0.218	ppbv #	36
29) Chloroform	5.754	83	29278m	0.130	ppbv	
30) Cyclohexane	7.121	84	12087m	0.107	ppbv	
34) 2-Butanone	5.240	43	393671	2.051	ppbv	96
36) Benzene	6.880	78	38470m	0.134	ppbv	
38) Trichloroethene	7.822	130	22352m	0.170	ppbv	
44) 2,2,4-Trimethylpentane	7.857	57	48081m	0.096	ppbv	
51) 2-Hexanone	10.137	43	118851m	0.532	ppbv	
52) Tetrachloroethene	11.214	164	214915	1.919	ppbv	93
53) Toluene	9.796	91	405686	1.228	ppbv	99
58) Ethyl Benzene	12.700	91	247709	0.553	ppbv	92
59) m/p-Xylene	12.957	91	888381	2.252	ppbv	94
60) o-Xylene	13.680	91	366480	0.989	ppbv	99
61) Styrene	13.513	104	25530m	0.129	ppbv	
64) n-propylbenzene	15.551	120	29327m	0.217	ppbv	
65) tert-Butylbenzene	16.744	119	65564	0.130	ppbv #	67
70) n-Butylbenzene	18.542	91	74599m	0.125	ppbv	
72) 4-Ethyltoluene	15.828	105	177204	0.408	ppbv	94
73) 1,3,5-Trimethylbenzene	15.986	105	160166m	0.409	ppbv	
74) 1,2,4-Trimethylbenzene	16.748	105	602662	1.378	ppbv #	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060622\
Data File : VL039183.D
Acq On : 6 Jun 2022 12:55
Operator : SY/AP
Sample : N3110-05 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SG-10

Quant Time: Jun 06 13:49:14 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun
QLast Update : Wed Jun 01 01:22:18 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

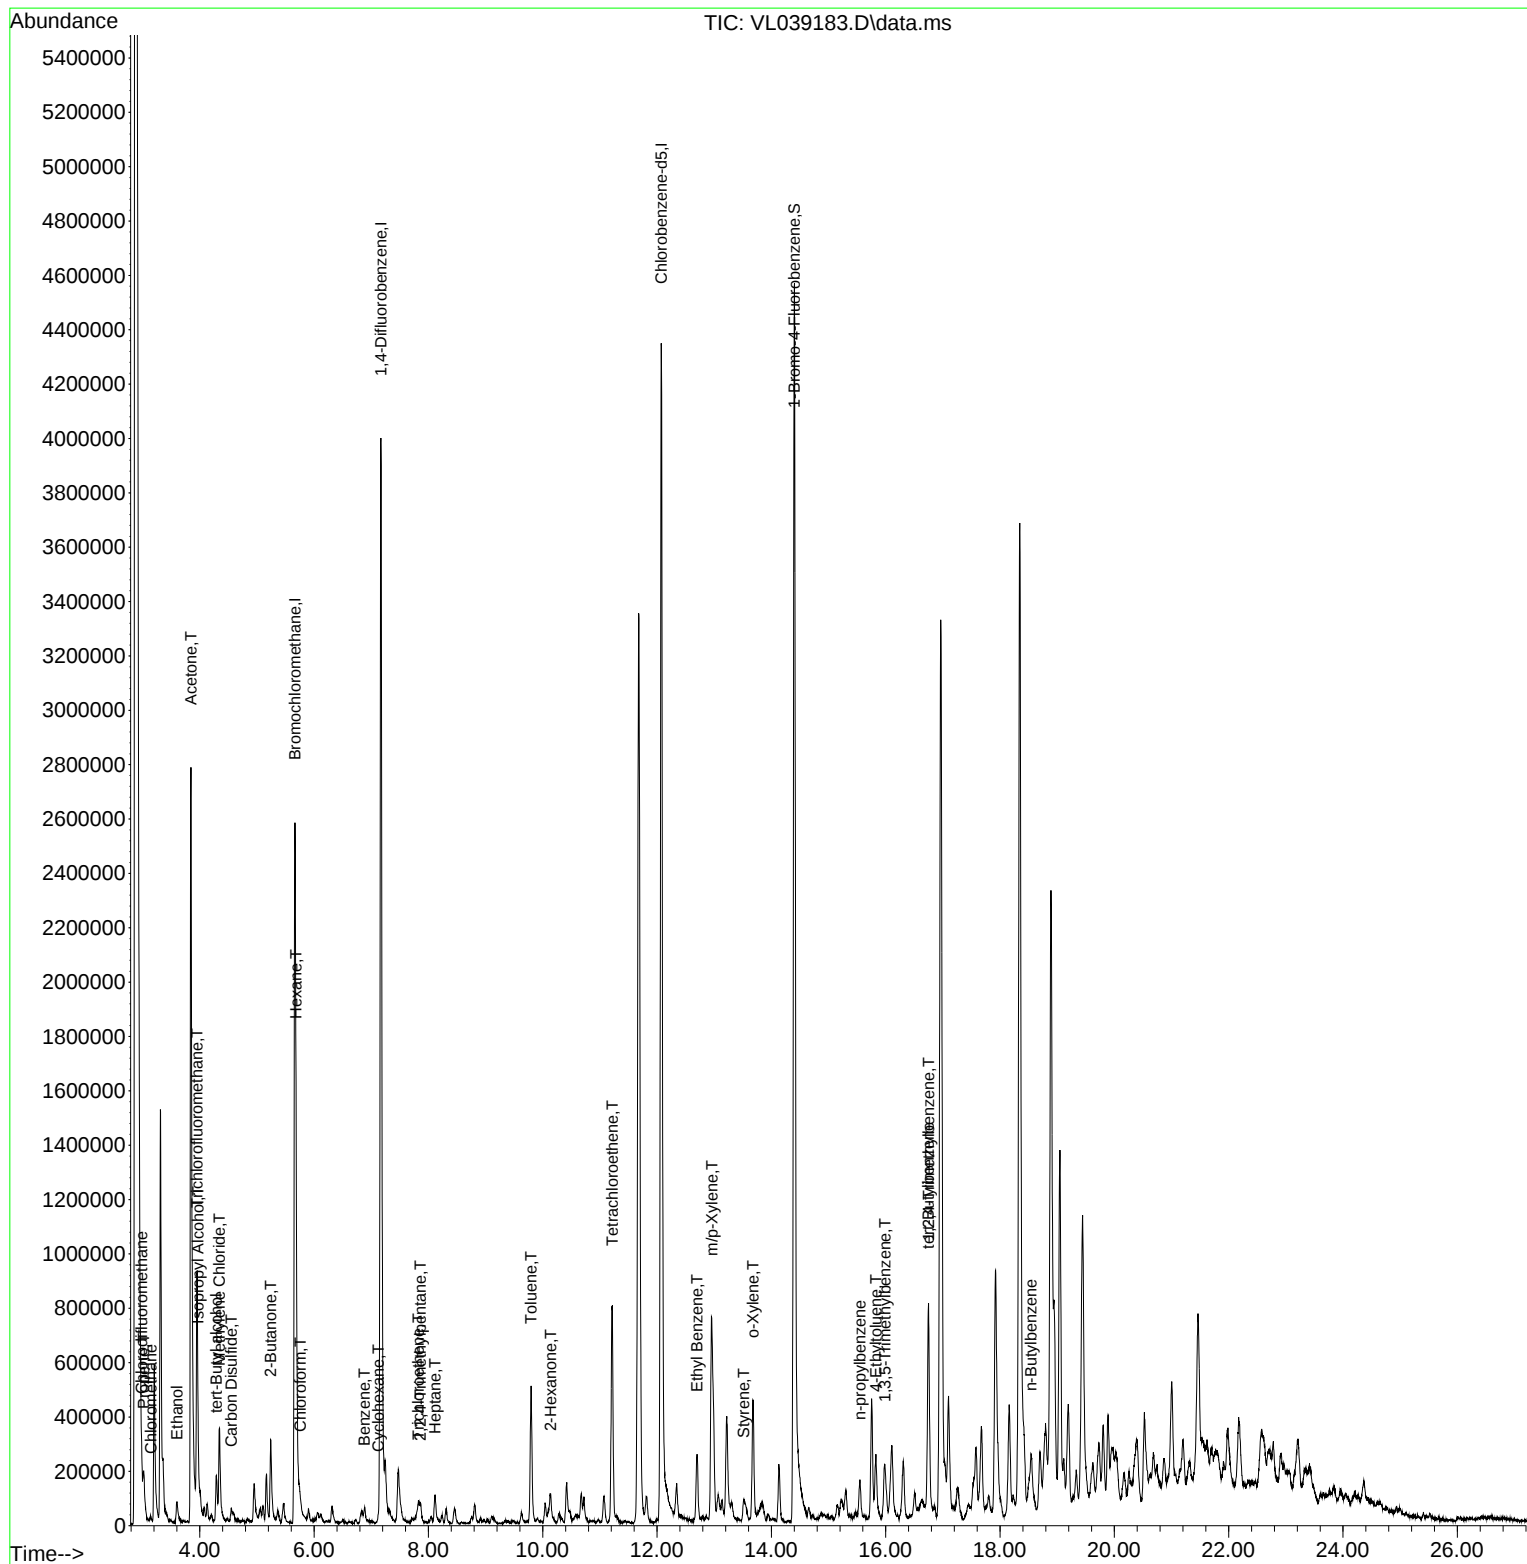



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.664 min Scan# 89
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10




Tgt Ion: 49 Resp: 1298440
Ion Ratio Lower Upper
49 100
128 52.6 24.7 74.1
130 67.0 31.4 94.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

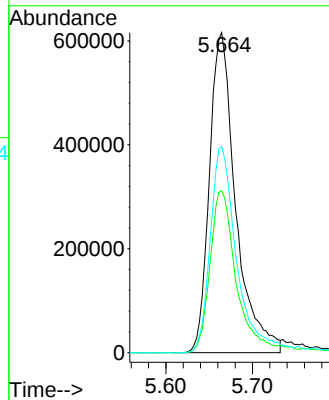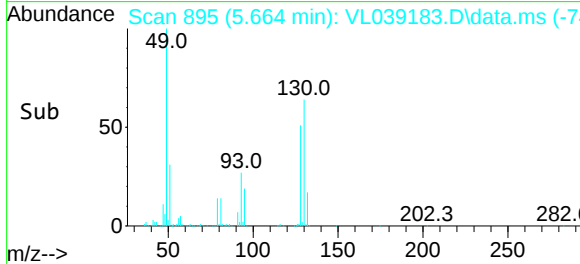


#3
Chlorodifluoromethane
Concen: 0.102 ppbv
RT: 2.986 min Scan# 62
Delta R.T. -0.013 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

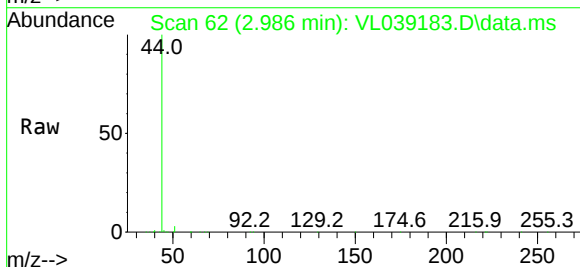

Tgt Ion: 51 Resp: 16814
Ion Ratio Lower Upper
51 100
67 19.8 16.2 24.4

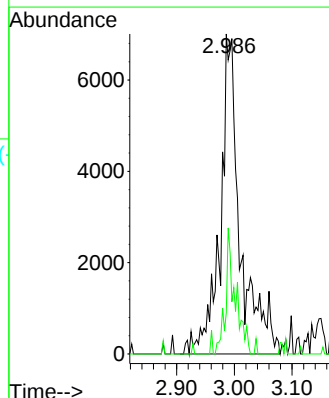







#4
Chloromethane
Concen: 0.176 ppbv
RT: 3.144 min Scan# 113
Delta R.T. -0.006 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

Instrument :
MSVOA_L
ClientSampleId :
SG-10

Tgt Ion: 50 Resp: 1496
Ion Ratio Lower Upper
50 100
52 26.8 25.9 38.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

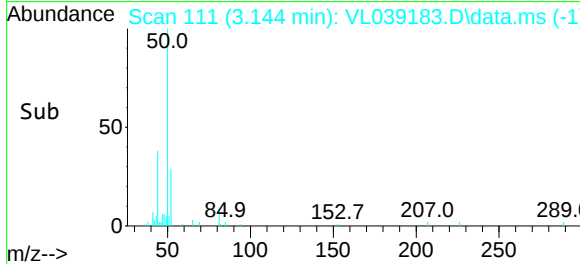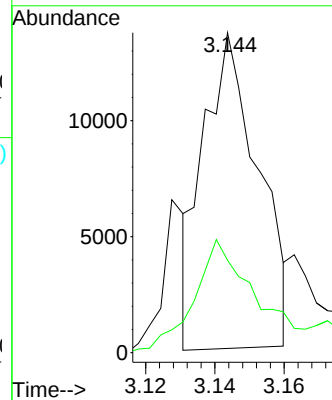

#9
Propene
Concen: 0.599 ppbv
RT: 3.018 min Scan# 72
Delta R.T. -0.000 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

Tgt Ion: 41 Resp: 43169
Ion Ratio Lower Upper
41 100
42 71.3 55.4 83.2

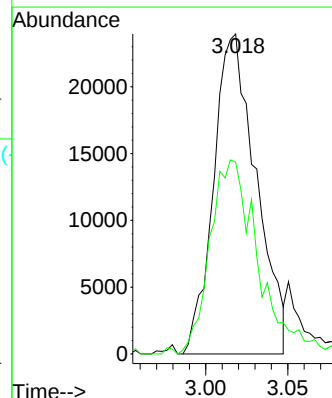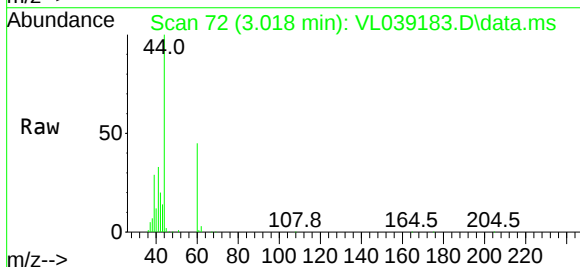



#10

Heptane

Concen: 0.289 ppbv

RT: 8.114 min Scan# 1

Delta R.T. -0.013 min

Lab File: VL039183.D

Acq: 6 Jun 2022 12:55

Instrument :

MSVOA_L

ClientSampleId :

SG-10

Tgt Ion: 43 Resp: 48550

Ion Ratio Lower Upper

43 100





57 59.4 41.4 62.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2022

Supervised By :Mahesh Dadoda 06/07/2022

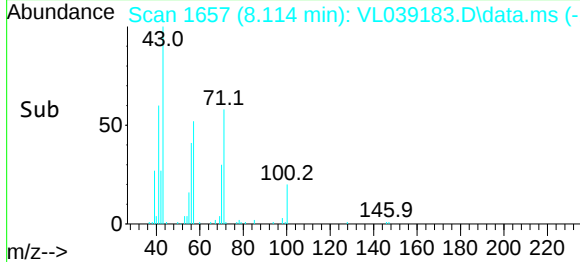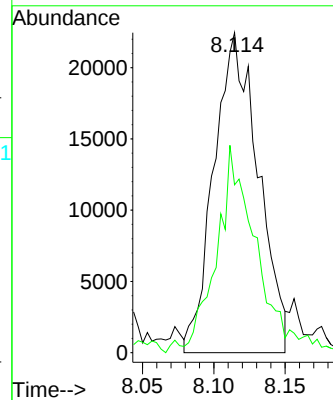

#11

Trichlorofluoromethane

Concen: 3.284 ppbv

RT: 3.954 min Scan# 363

Delta R.T. -0.006 min

Lab File: VL039183.D




Acq: 6 Jun 2022 12:55


Tgt Ion:101 Resp: 677879

Ion Ratio Lower Upper

101 100


103 64.4 51.7 77.5

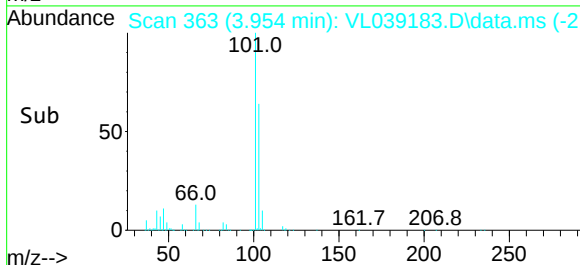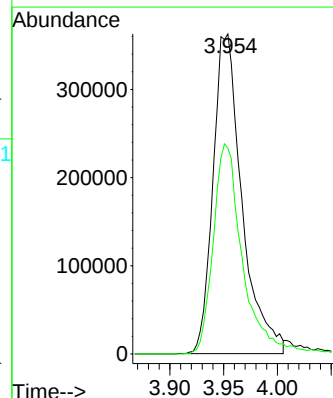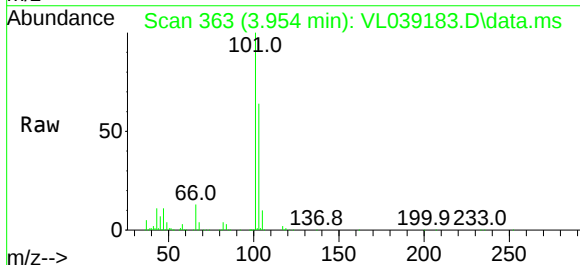



#13
Ethanol
Concen: 29.143 ppbv
RT: 3.603 min Scan# 21
Delta R.T. -0.006 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10



Tgt Ion: 45 Resp: 11449
Ion Ratio Lower Upper
45 100
46 33.5 0.0 0.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

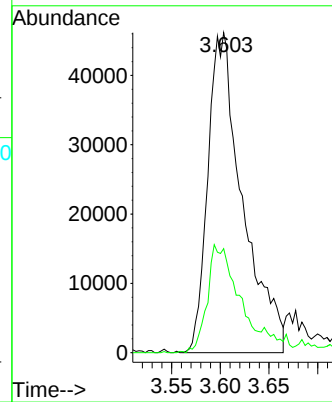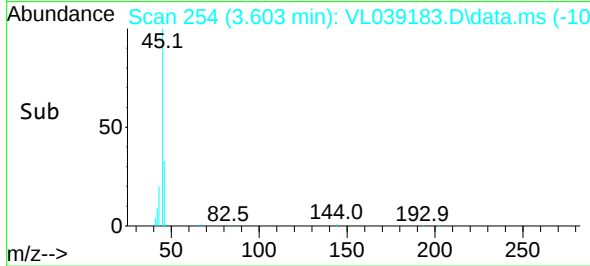

#15
Acetone
Concen: 26.884 ppbv
RT: 3.845 min Scan# 329
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55


Tgt Ion: 43 Resp: 3636205
Ion Ratio Lower Upper
43 100
58 30.4 22.5 33.7

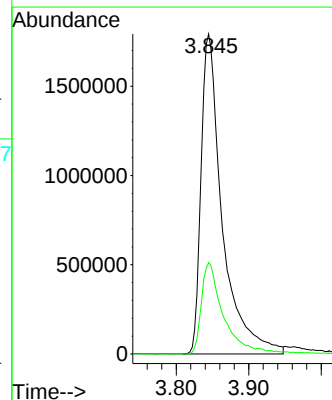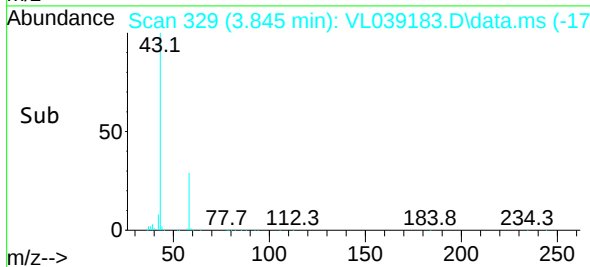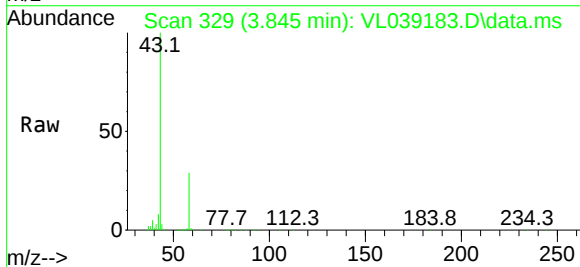

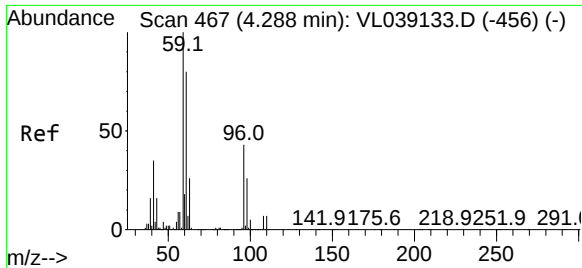

#17
tert-Butyl alcohol
Concen: 1.408 ppbv
RT: 4.288 min Scan# 467
Delta R.T. -0.000 min
Lab File: VL039133.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10

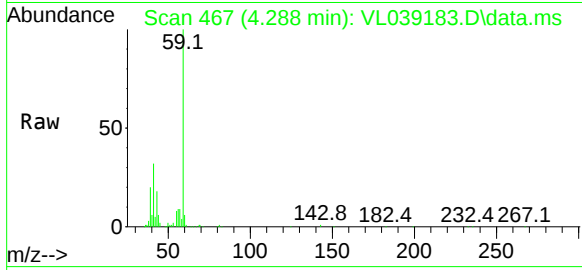


Tgt Ion: 59 Resp: 147708
Ion Ratio Lower Upper
59 100
57 14.3 9.1 13.7

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

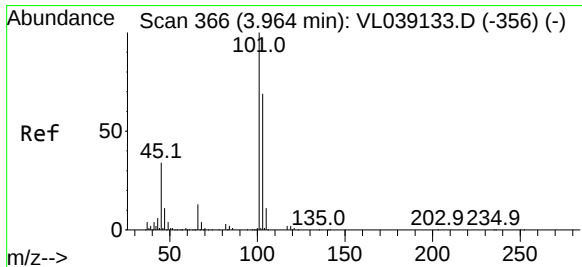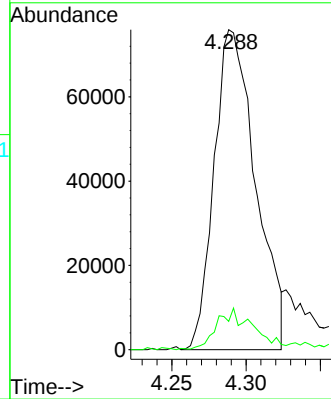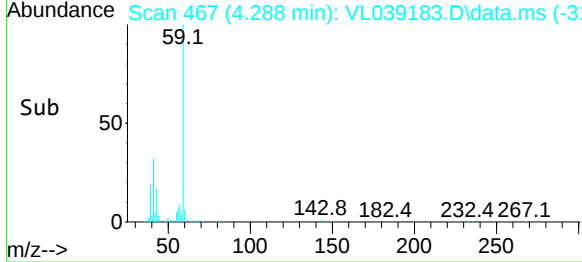


#19
Isopropyl Alcohol
Concen: 1.125 ppbv
RT: 3.967 min Scan# 367
Delta R.T. 0.003 min
Lab File: VL039133.D
Acq: 6 Jun 2022 12:55

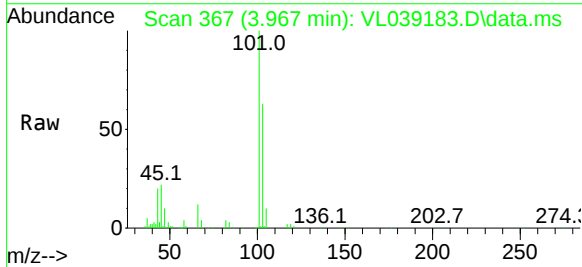


Tgt Ion: 45 Resp: 71371
Ion Ratio Lower Upper
45 100
58 0.0 1.8 2.8

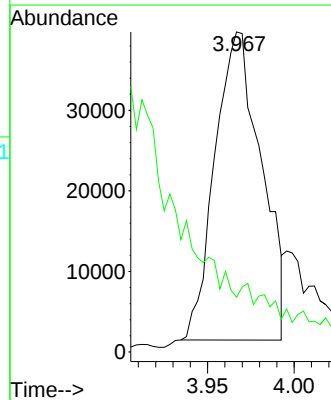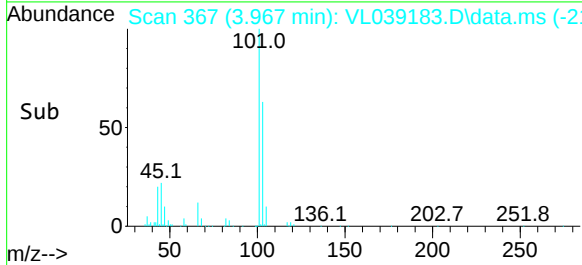



#20
Methylene Chloride
Concen: 2.362 ppbv
RT: 4.343 min Scan# 41
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10




Tgt Ion: 84 Resp: 13465
Ion Ratio Lower Upper
84 100
49 151.2 111.1 166.7
51 45.3 35.3 52.9
86 63.8 51.9 77.9

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

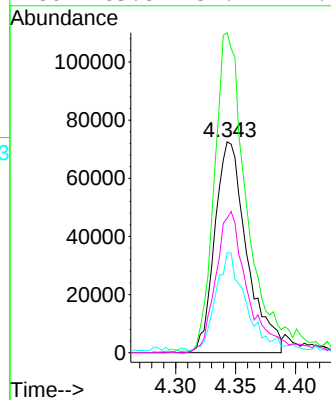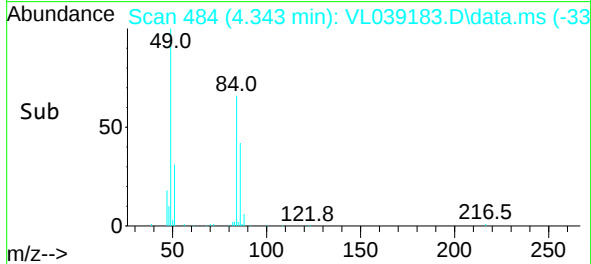


#26
Hexane
Concen: 2.544 ppbv
RT: 5.684 min Scan# 901
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

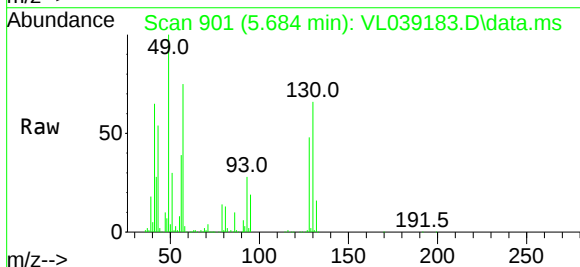


Tgt Ion: 57 Resp: 340804
Ion Ratio Lower Upper
57 100
41 90.9 72.4 108.6
43 73.8 187.0 280.6#
56 55.6 41.8 62.6

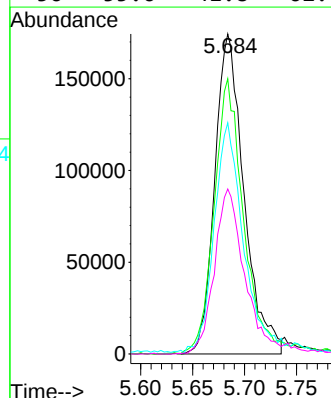



#27
Carbon Disulfide
Concen: 0.218 ppbv
RT: 4.549 min Scan# 549
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10



Tgt Ion: 76 Resp: 30309
Ion Ratio Lower Upper
76 100
44 54.3 14.4 21.6
78 20.9 7.7 11.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

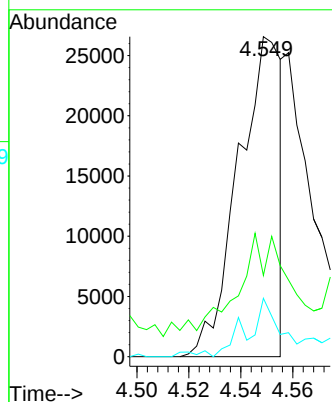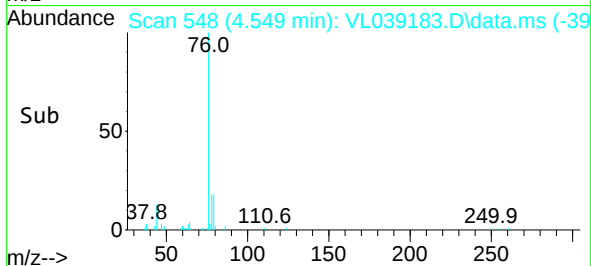

#29
Chloroform
Concen: 0.130 ppbv m
RT: 5.754 min Scan# 923
Delta R.T. -0.006 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55


Tgt Ion: 83 Resp: 29278
Ion Ratio Lower Upper
83 100
85 66.2 52.4 78.6

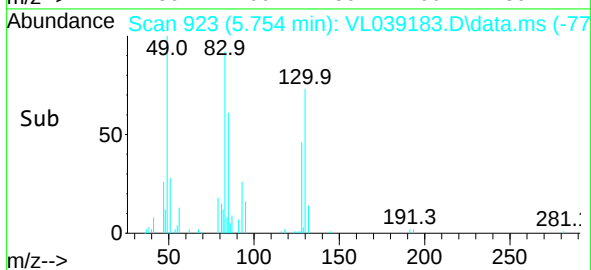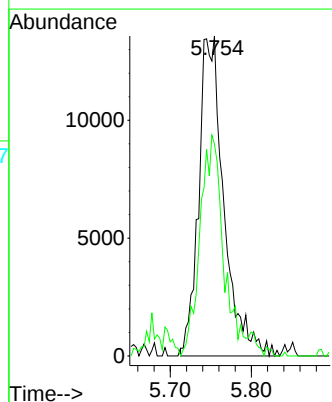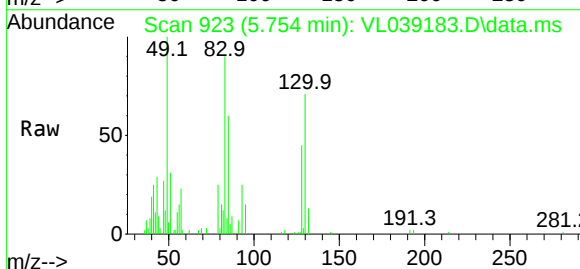

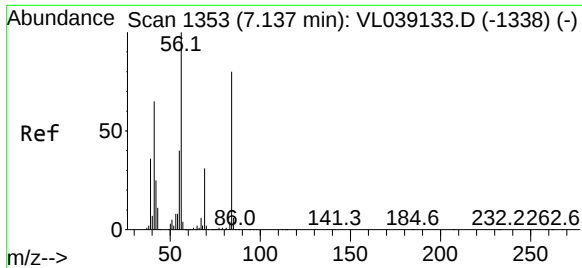

#30
Cyclohexane
Concen: 0.107 ppbv m
RT: 7.121 min Scan# 1348
Delta R.T. -0.016 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10

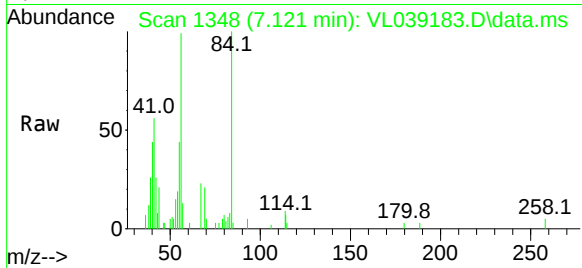


Tgt Ion: 84 Resp: 12085
Ion Ratio Lower Upper
84 100
56 0.0 110.6 165.8
41 99.2 68.9 103.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

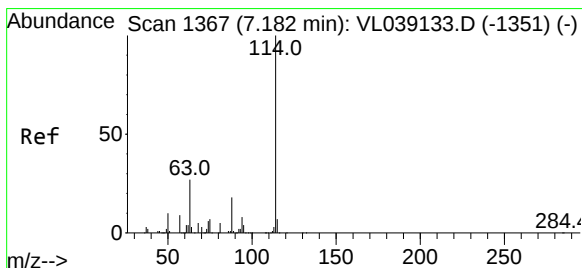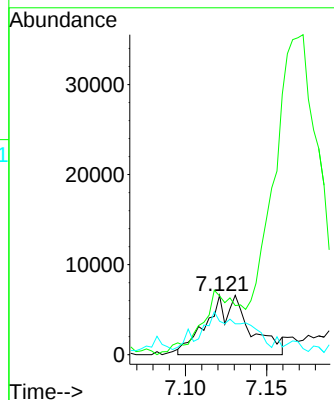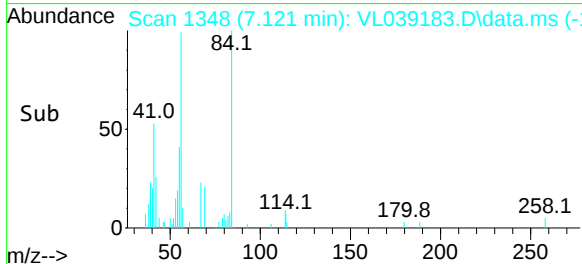


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.169 min Scan# 1363
Delta R.T. -0.013 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

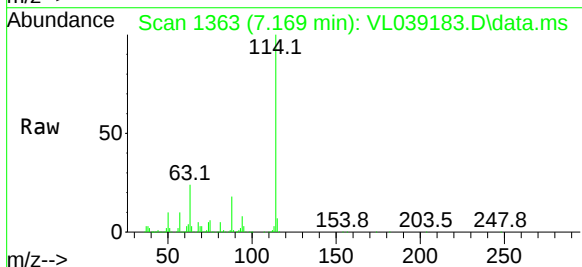


Tgt Ion:114 Resp: 3532948
Ion Ratio Lower Upper
114 100
63 24.3 21.7 32.5
88 17.7 14.8 22.2

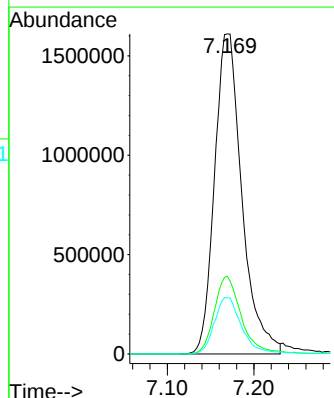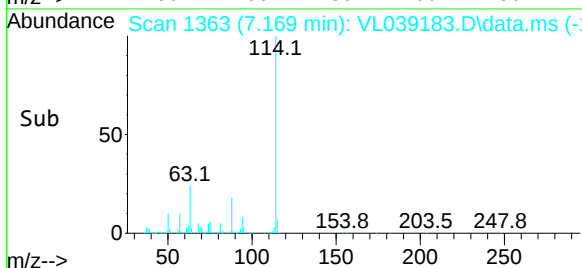

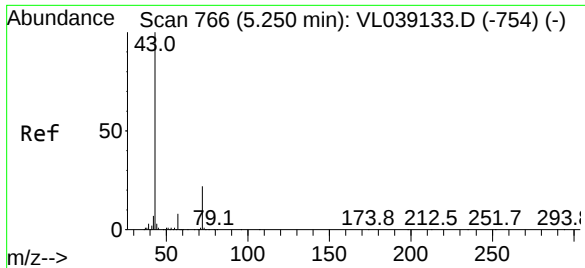

#34
2-Butanone
Concen: 2.051 ppbv
RT: 5.240 min Scan# 71
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10

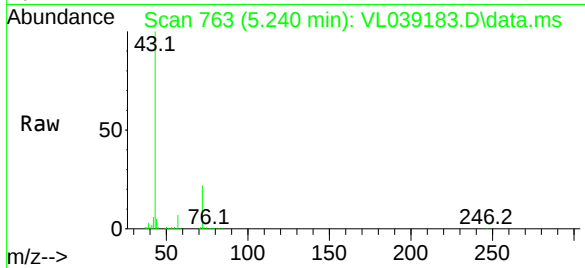


Tgt Ion: 43 Resp: 39367
Ion Ratio Lower Upper
43 100
72 24.5 18.2 27.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

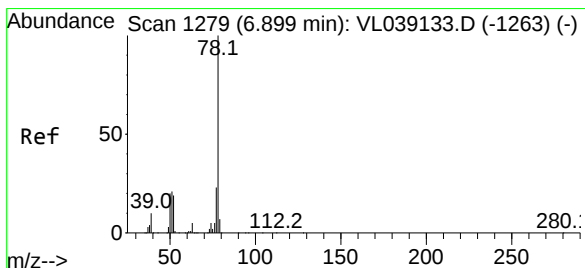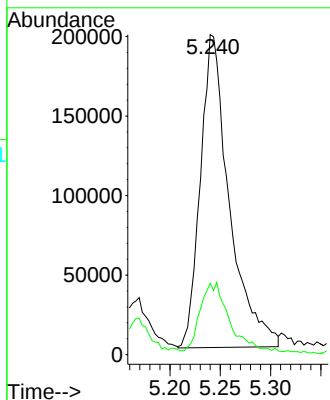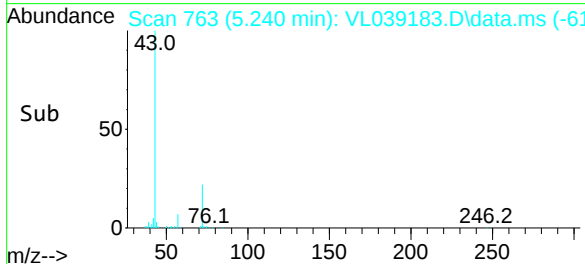


#36
Benzene
Concen: 0.134 ppbv m
RT: 6.880 min Scan# 1273
Delta R.T. -0.019 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

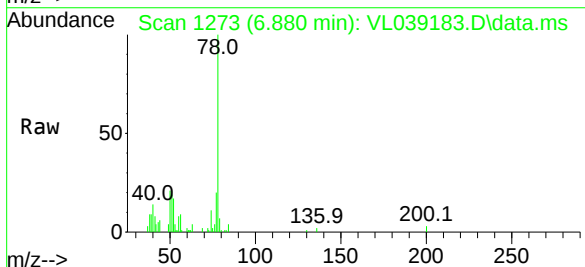


Tgt Ion: 78 Resp: 38470
Ion Ratio Lower Upper
78 100
77 20.1 18.6 27.8
50 21.0 15.8 23.8

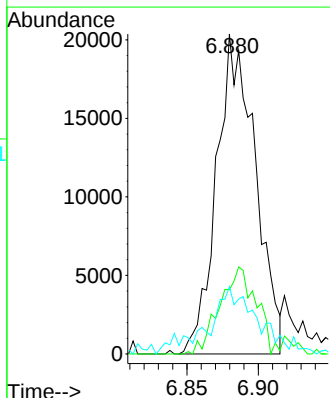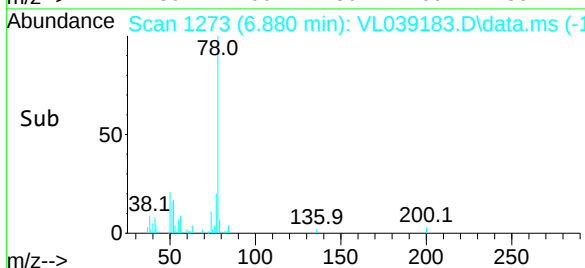



#38
Trichloroethene
Concen: 0.170 ppbv m
RT: 7.822 min Scan# 1566
Delta R.T. -0.023 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10




Tgt Ion:130 Resp: 22352
Ion Ratio Lower Upper
130 100
95 90.1 93.3 139.9
132 89.5 79.0 118.4
97 55.5 59.4 89.2#

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

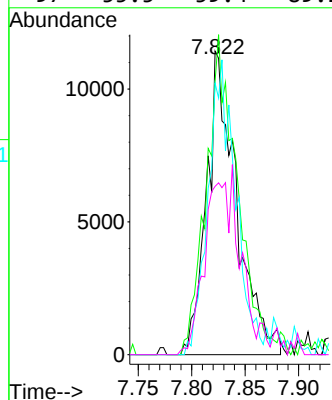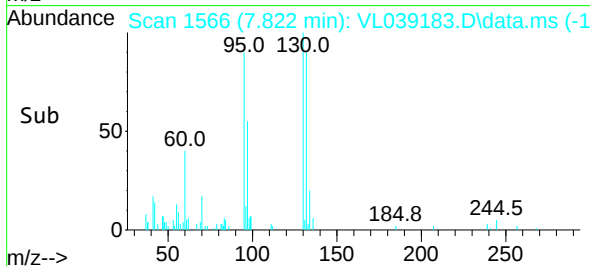


#44
2,2,4-Trimethylpentane
Concen: 0.096 ppbv m
RT: 7.857 min Scan# 1577
Delta R.T. -0.019 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

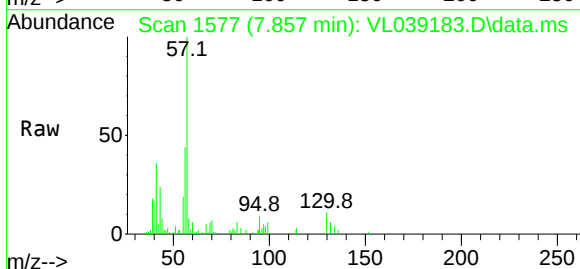


Tgt Ion: 57 Resp: 48081
Ion Ratio Lower Upper
57 100
41 37.8 26.2 39.4
56 48.3 24.7 37.1#

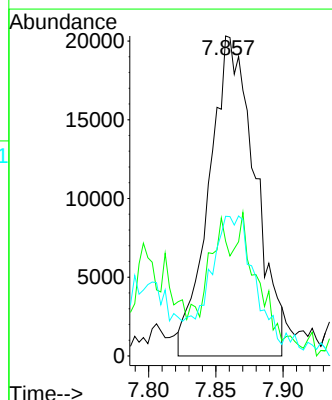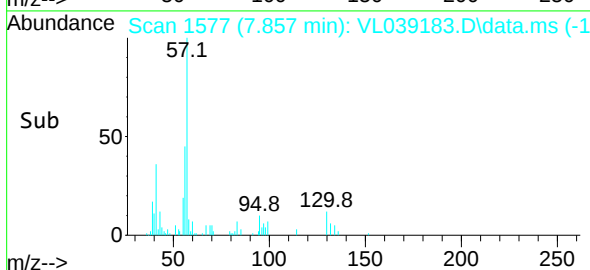

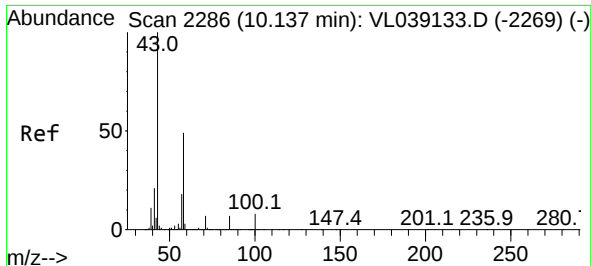

#51
2-Hexanone
Concen: 0.532 ppbv m
RT: 10.137 min Scan# 2185
Delta R.T. -0.000 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10

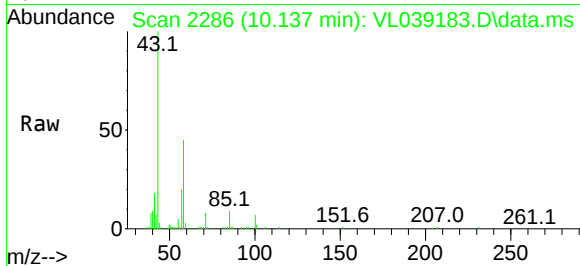


Tgt Ion: 43 Resp: 11885
Ion Ratio Lower Upper
43 100
58 0.0 40.0 60.0
98 0.0 0.1 0.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

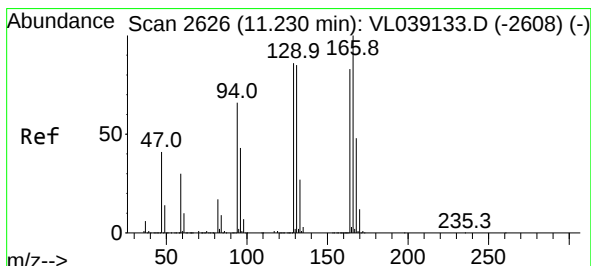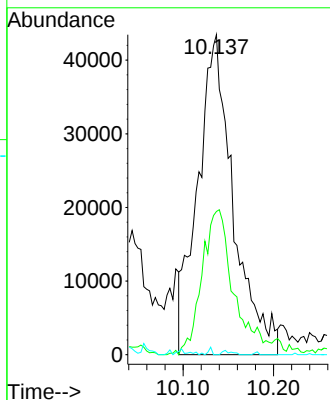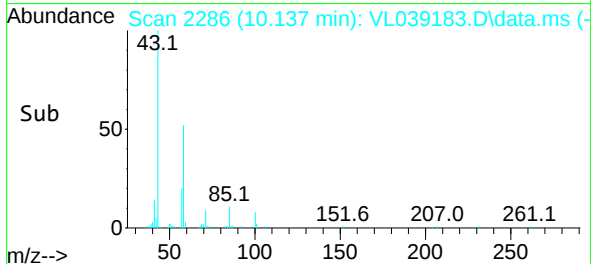


#52
Tetrachloroethene
Concen: 1.919 ppbv
RT: 11.214 min Scan# 2621
Delta R.T. -0.016 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

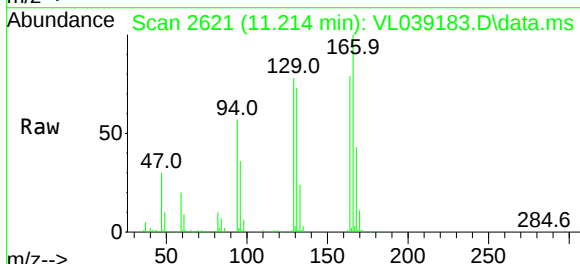


Tgt Ion:164 Resp: 214915
Ion Ratio Lower Upper
164 100
166 126.7 96.3 144.5
129 98.7 82.5 123.7
131 92.6 82.1 123.1

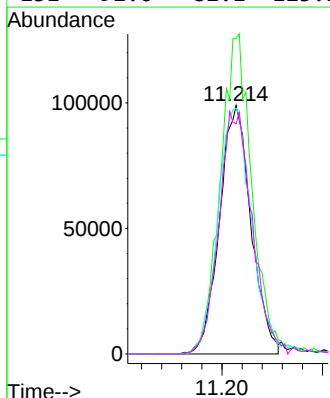

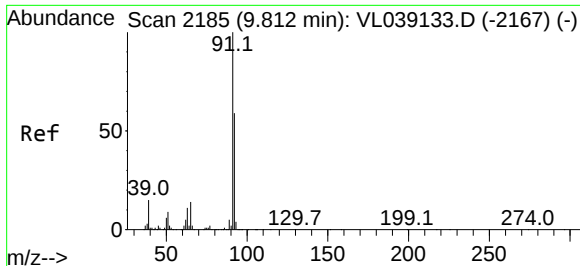

#53
Toluene
Concen: 1.228 ppbv
RT: 9.796 min Scan# 2185
Delta R.T. -0.016 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10




Tgt Ion: 91 Resp: 405680
Ion Ratio Lower Upper
91 100
92 61.2 48.1 72.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

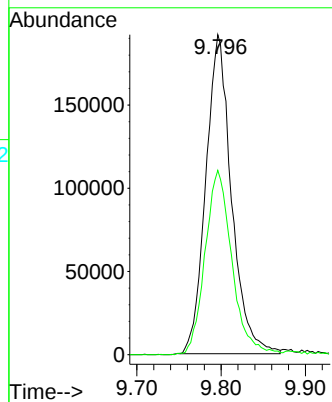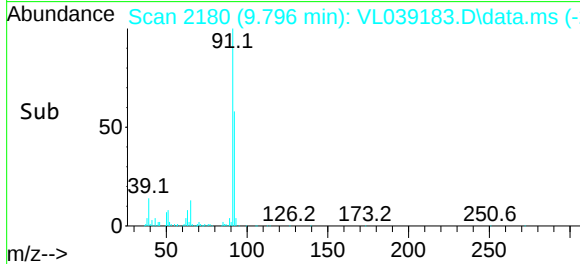


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.076 min Scan# 2889
Delta R.T. -0.016 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

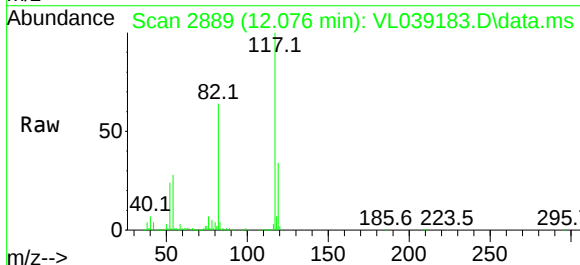

Tgt Ion:117 Resp: 3252611
Ion Ratio Lower Upper
117 100
82 66.1 55.1 82.7
119 33.3 24.7 37.1

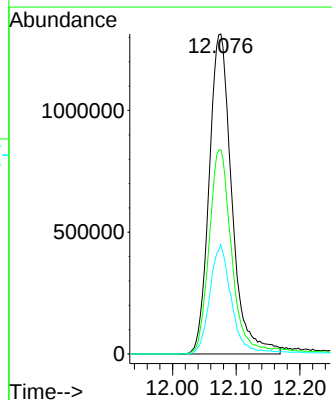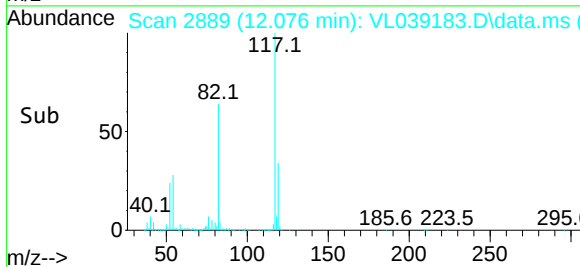

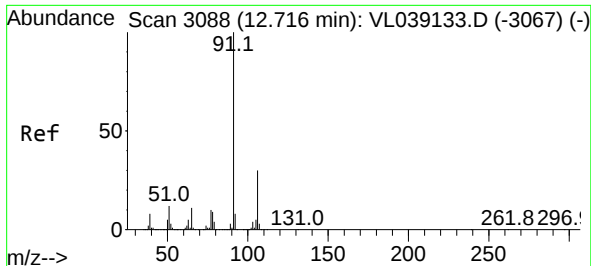





#58
Ethyl Benzene
Concen: 0.553 ppbv
RT: 12.700 min Scan# 3088
Delta R.T. -0.016 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

Instrument :
MSVOA_L
ClientSampleId :
SG-10

Tgt Ion: 91 Resp: 247709
Ion Ratio Lower Upper
91 100
106 25.8 24.2 36.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

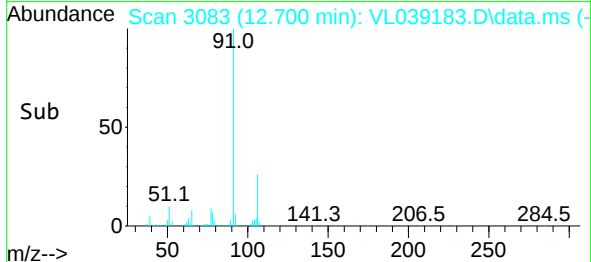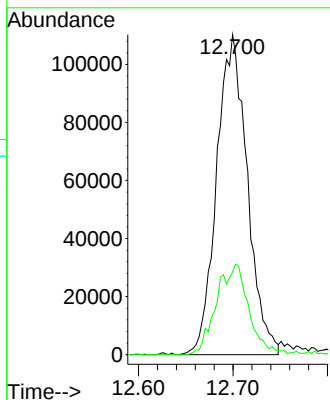

#59
m/p-Xylene
Concen: 2.252 ppbv
RT: 12.957 min Scan# 3163
Delta R.T. -0.042 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

Tgt Ion: 91 Resp: 888381
Ion Ratio Lower Upper
91 100
106 46.7 34.3 51.5

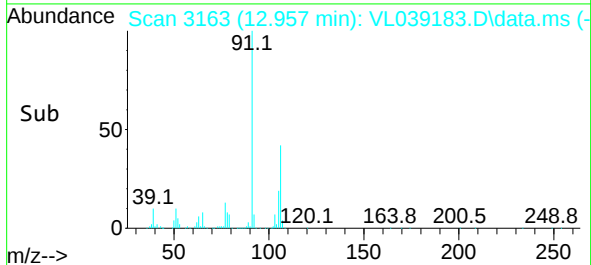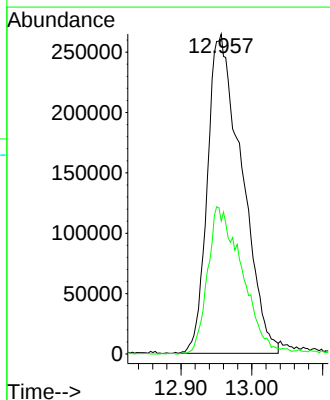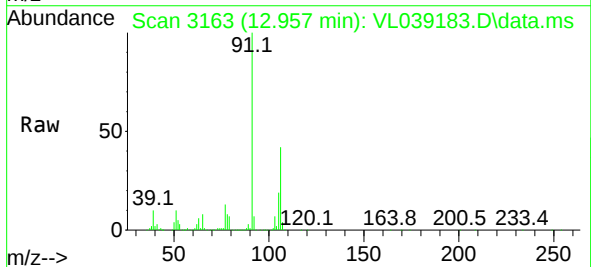



#60

o-Xylene

Concen: 0.989 ppbv

RT: 13.680 min Scan# 31

Delta R.T. -0.016 min

Lab File: VL039183.D

Acq: 6 Jun 2022 12:55

Instrument :

MSVOA_L

ClientSampleId :

SG-10

Tgt Ion: 91 Resp: 366480

Ion Ratio Lower Upper

91 100





106 45.5 22.3 66.9

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2022

Supervised By :Mahesh Dadoda 06/07/2022

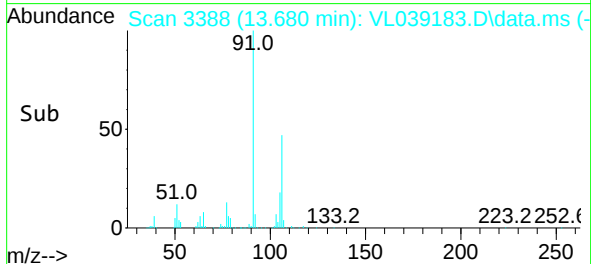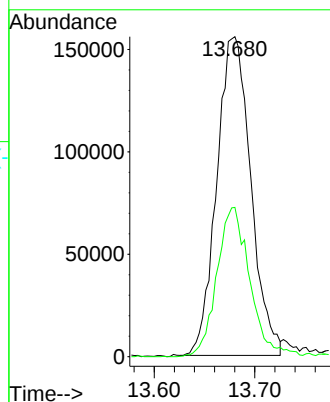

#61

Styrene

Concen: 0.129 ppbv m

RT: 13.513 min Scan# 3336

Delta R.T. -0.019 min

Lab File: VL039183.D

Acq: 6 Jun 2022 12:55




Tgt Ion:104 Resp: 25530


Ion Ratio Lower Upper

104 100

78 0.0 45.7 68.5#


103 54.1 39.6 59.4

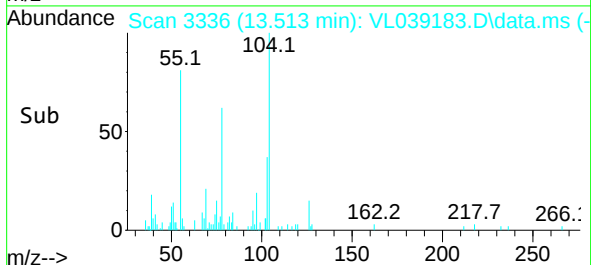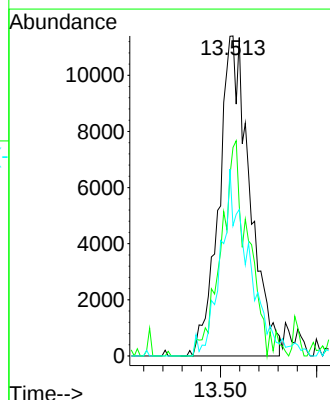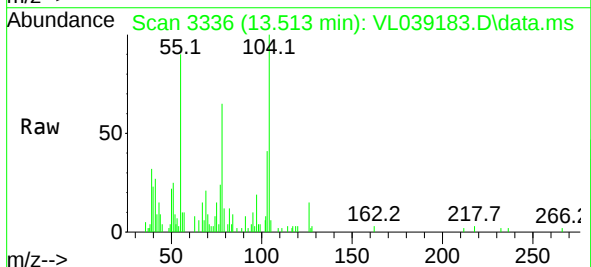



#64
n-propylbenzene
Concen: 0.217 ppbv
RT: 15.551 min Scan# 3973
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10

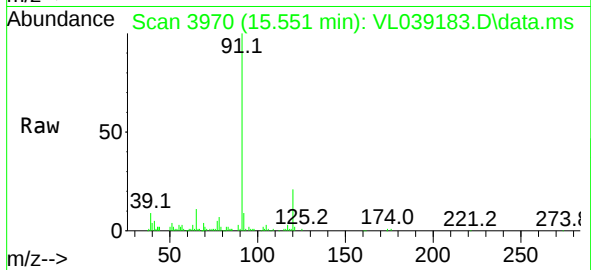


Tgt Ion:120 Resp: 2932
Ion Ratio Lower Upper
120 100
91 0.0 388.4 582.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

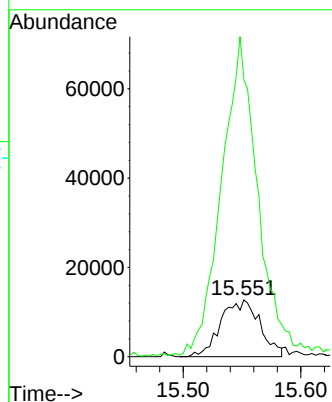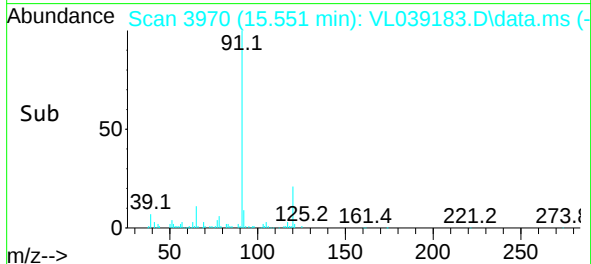


#65
tert-Butylbenzene
Concen: 0.130 ppbv
RT: 16.744 min Scan# 4341
Delta R.T. -0.003 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

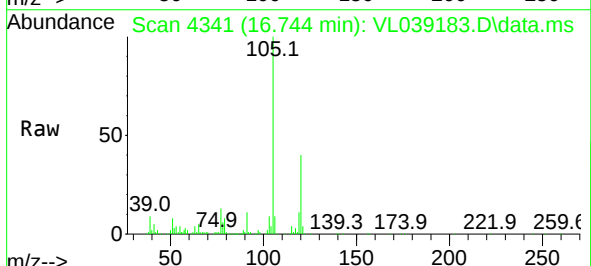


Tgt Ion:119 Resp: 65564
Ion Ratio Lower Upper
119 100
91 111.2 67.1 100.7#
134 0.0 15.8 23.8#

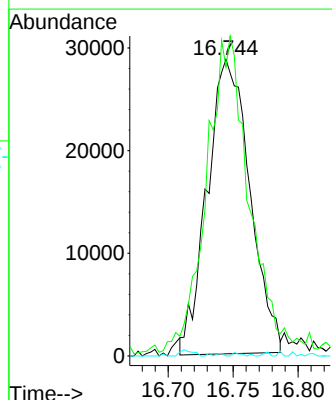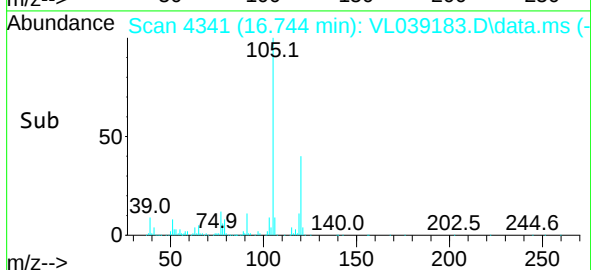

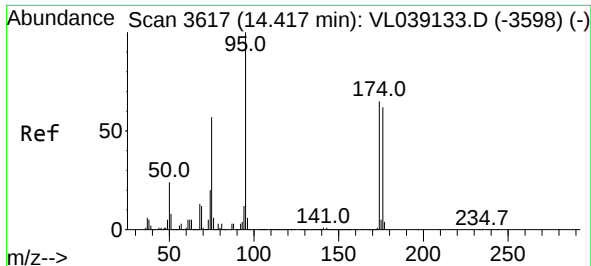

#68
1-Bromo-4-Fluorobenzene
Concen: 9.280 ppbv
RT: 14.404 min Scan# 3613
Delta R.T. -0.013 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10




Tgt Ion: 95 Resp: 249536
Ion Ratio Lower Upper
95 100
174 70.9 53.8 80.8
175 5.2 4.1 6.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

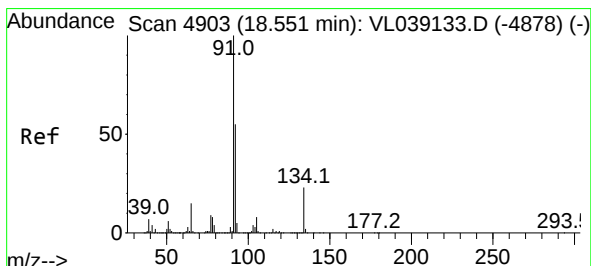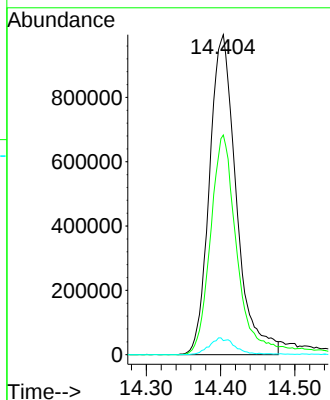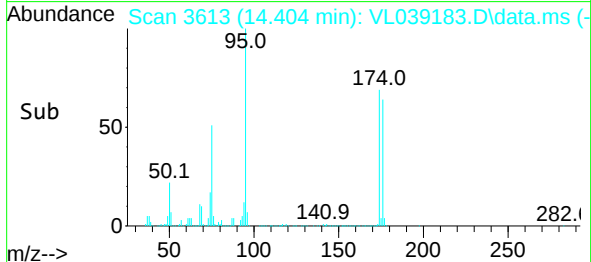


#70
n-Butylbenzene
Concen: 0.125 ppbv m
RT: 18.542 min Scan# 4900
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55

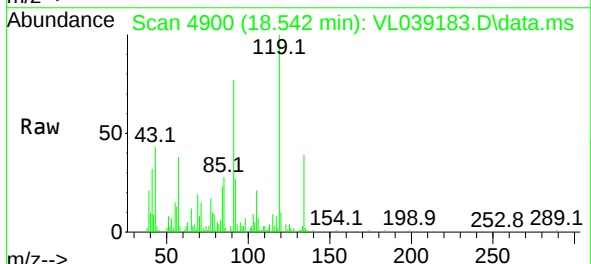


Tgt Ion: 91 Resp: 74599
Ion Ratio Lower Upper
91 100
92 37.4 43.6 65.4#
134 68.0 17.7 26.5#

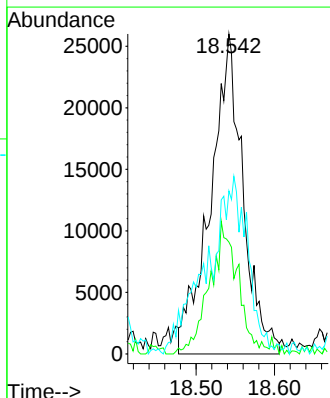



#72
4-Ethyltoluene
Concen: 0.408 ppbv
RT: 15.828 min Scan# 4056
Delta R.T. -0.013 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55




Instrument :
MSVOA_L
ClientSampleId :
SG-10



Tgt Ion:105 Resp: 177204
Ion Ratio Lower Upper
105 100
120 34.9 23.9 35.9
91 14.4 10.6 16.0
77 13.8 11.7 17.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

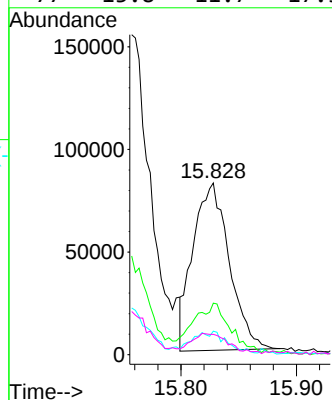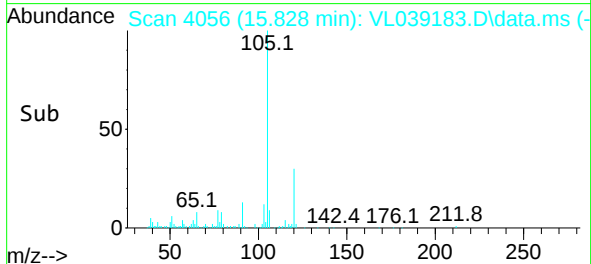

#73
1,3,5-Trimethylbenzene
Concen: 0.409 ppbv m
RT: 15.986 min Scan# 4105
Delta R.T. -0.010 min
Lab File: VL039183.D
Acq: 6 Jun 2022 12:55


Tgt Ion:105 Resp: 160166
Ion Ratio Lower Upper
105 100
120 47.0 36.7 55.1

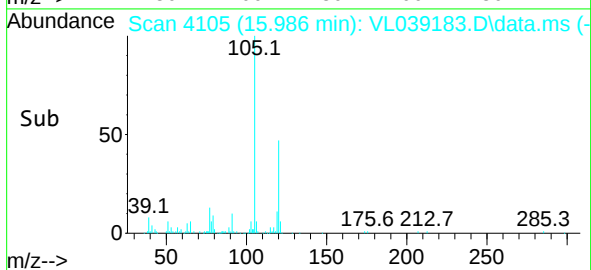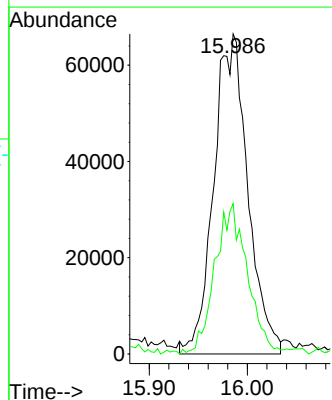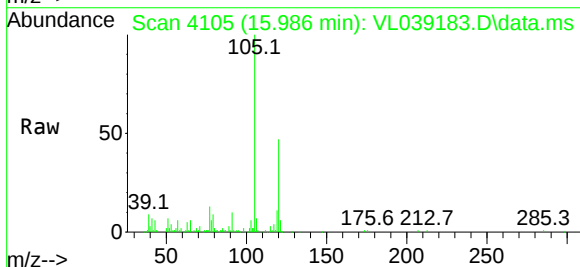

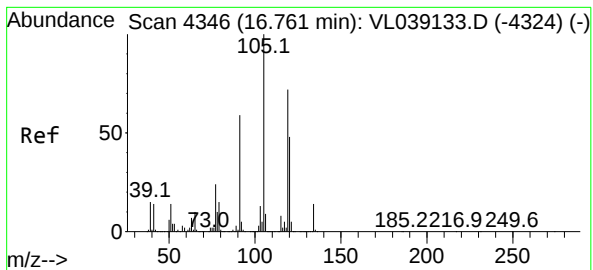

#74
 1,2,4-Trimethylbenzene
 Concen: 1.378 ppbv
 RT: 16.748 min Scan# 41
 Delta R.T. -0.013 min
 Lab File: VL039183.D
 Acq: 6 Jun 2022 12:55

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-10



Tgt Ion:	105	Resp:	602662
Ion	Ratio	Lower	Upper
105	100		
120	38.5	38.1	57.1
91	11.3	47.4	71.0
77	13.0	19.5	29.3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2022
 Supervised By :Mahesh Dadoda 06/07/2022

