

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060622\
 Data File : VL039198.D
 Acq On : 7 Jun 2022 00:01
 Operator : SY/AP
 Sample : N3110-09 2X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-5

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 06/07/2022
 Supervised By : Mahesh Dadoda 06/07/2022

Quant Time: Jun 07 03:21:24 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jun 07 03:21:24 2022

QLast Update : Wed Jun 01 01:22:18 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.661	49	1234485	10.000	ppbv	-0.01
33) 1,4-Difluorobenzene	7.169	114	3358670	10.000	ppbv	-0.01
55) Chlorobenzene-d5	12.073	117	2998462	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.404	95	2338697	9.434	ppbv	-0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	94.300%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	3.047	85	36081m	0.166	ppbv	
3) Chlorodifluoromethane	2.989	51	25137m	0.160	ppbv	
4) Chloromethane	3.140	50	13491	0.167	ppbv #	84
9) Propene	3.018	41	18040m	0.263	ppbv	
10) Heptane	8.111	43	47142	0.295	ppbv	86
11) Trichlorofluoromethane	3.951	101	25233	0.129	ppbv	93
13) Ethanol	3.600	45	243090	65.082	ppbv #	100
15) Acetone	3.845	43	1081971	8.414	ppbv	92
17) tert-Butyl alcohol	4.292	59	53663	0.538	ppbv #	92
19) Isopropyl Alcohol	3.964	45	28440m	0.472	ppbv	
20) Methylene Chloride	4.340	84	852319	15.728	ppbv	94
26) Hexane	5.681	57	1706079	13.395	ppbv #	38
29) Chloroform	5.748	83	41667m	0.194	ppbv	
30) Cyclohexane	7.124	84	15269m	0.143	ppbv	
34) 2-Butanone	5.237	43	303846	1.665	ppbv	94
36) Benzene	6.883	78	33989m	0.125	ppbv	
44) 2,2,4-Trimethylpentane	7.857	57	51706m	0.108	ppbv	
51) 2-Hexanone	10.137	43	116888m	0.550	ppbv	
52) Tetrachloroethene	11.211	164	193724	1.820	ppbv	94
53) Toluene	9.796	91	371253	1.182	ppbv	97
58) Ethyl Benzene	12.696	91	262821	0.636	ppbv	100
59) m/p-Xylene	12.957	91	932987	2.565	ppbv	91
60) o-Xylene	13.677	91	436812	1.278	ppbv	98
61) Styrene	13.516	104	36833m	0.201	ppbv	
64) n-propylbenzene	15.539	120	39379m	0.315	ppbv	
70) n-Butylbenzene	18.535	91	118944m	0.217	ppbv	
72) 4-Ethyltoluene	15.822	105	254692	0.636	ppbv	98
73) 1,3,5-Trimethylbenzene	15.982	105	247501m	0.685	ppbv	
74) 1,2,4-Trimethylbenzene	16.748	105	962317	2.387	ppbv #	64
79) Naphthalene	22.181	128	82037m	0.264	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060622\
Data File : VL039198.D
Acq On : 7 Jun 2022 00:01
Operator : SY/AP
Sample : N3110-09 2X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SG-5

Quant Time: Jun 07 03:21:24 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun
QLast Update : Wed Jun 01 01:22:18 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

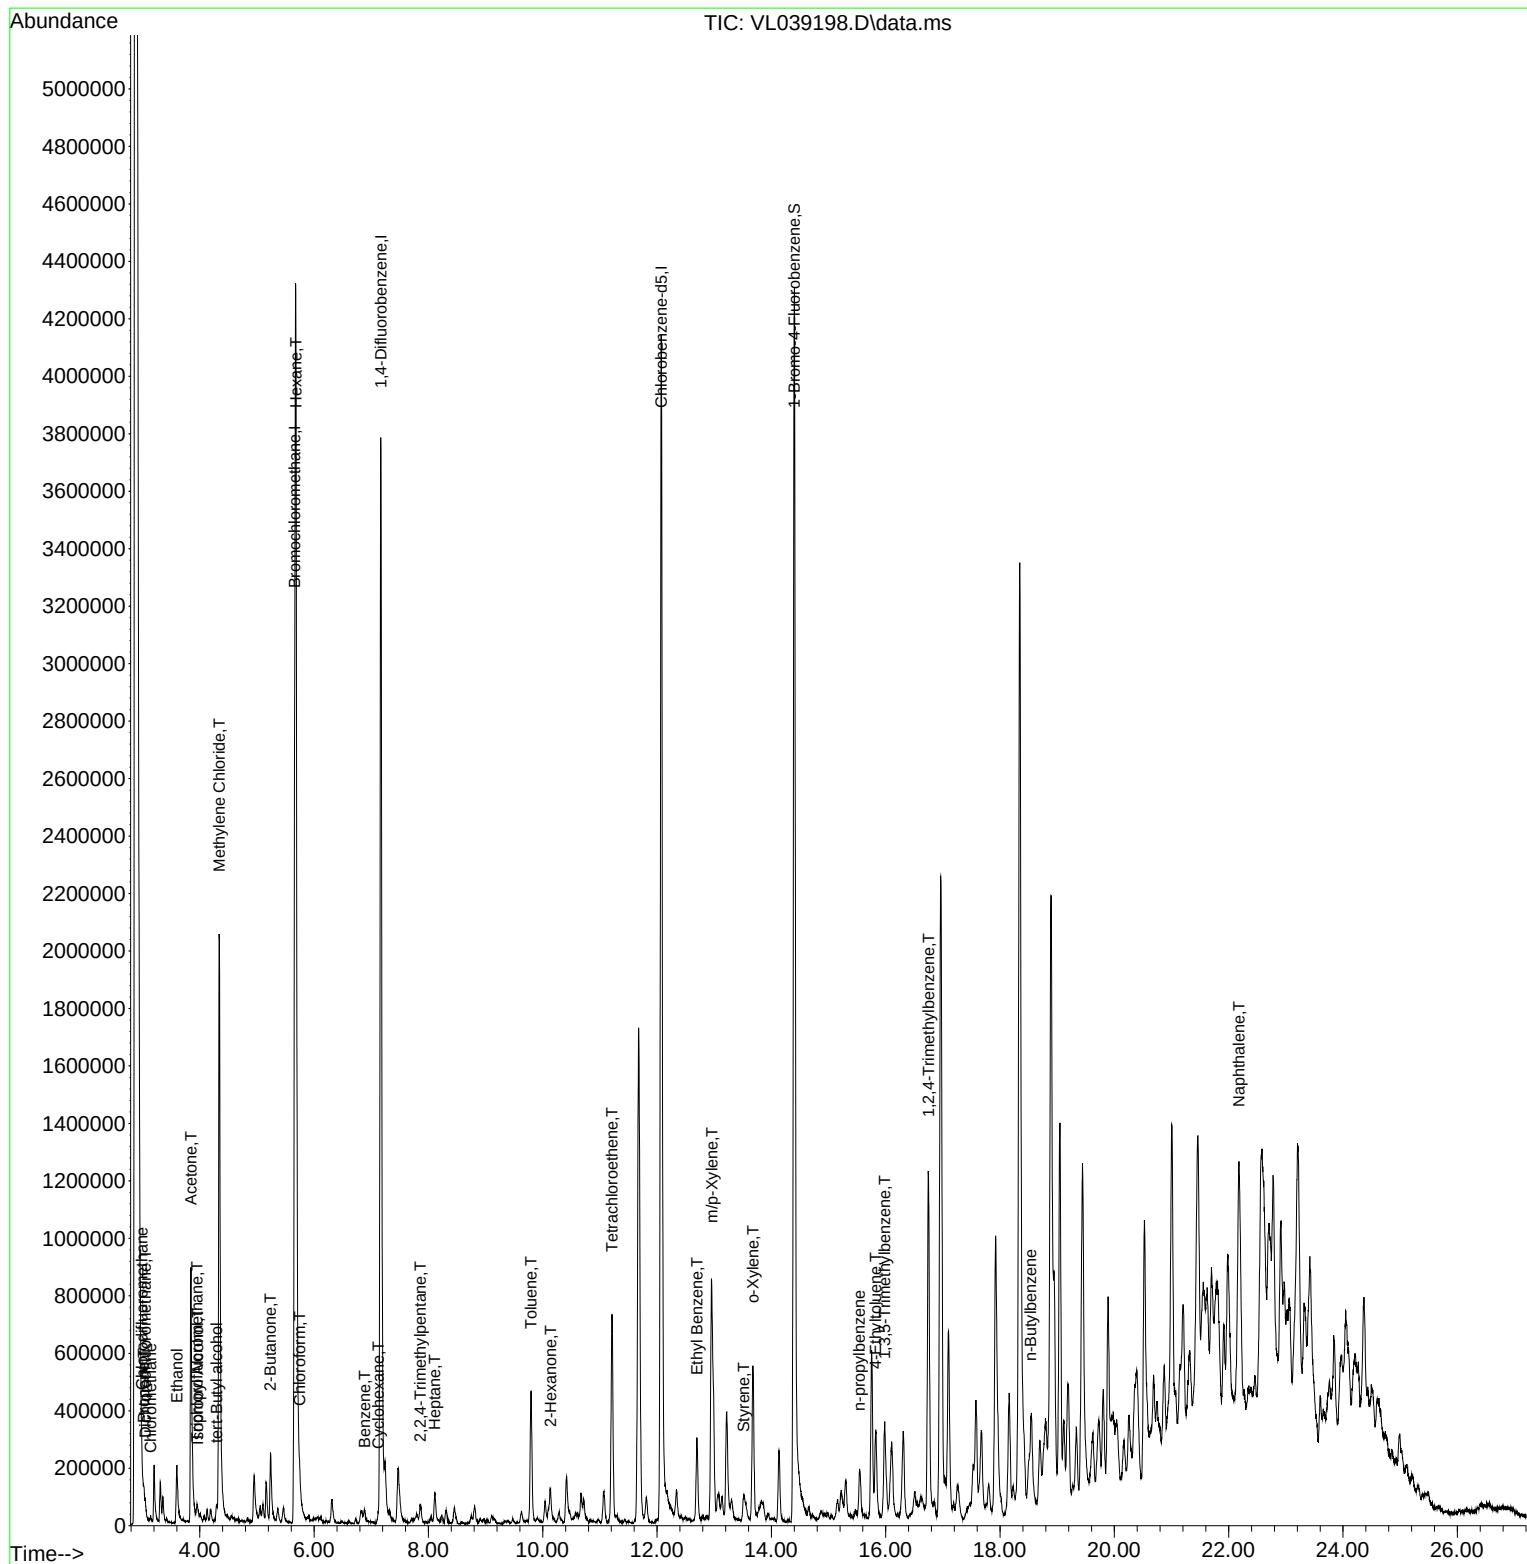



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.661 min Scan# 89
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5



Tgt Ion: 49 Resp: 123448
Ion Ratio Lower Upper
49 100
128 52.0 24.7 74.1
130 64.9 31.4 94.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

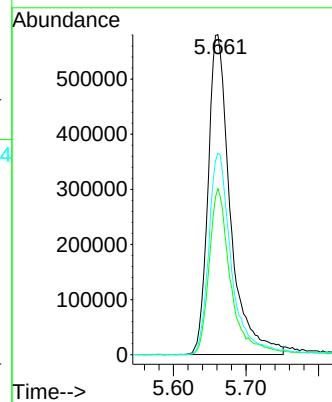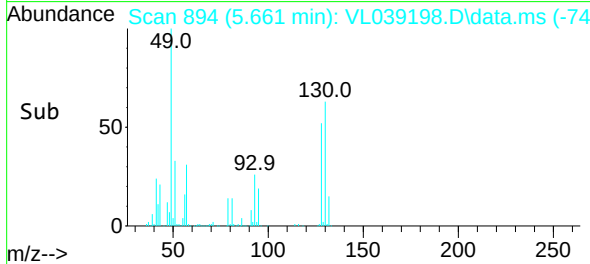

#2
Dichlorodifluoromethane
Concen: 0.166 ppbv m
RT: 3.047 min Scan# 81
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01


Tgt Ion: 85 Resp: 36081
Ion Ratio Lower Upper
85 100
87 29.4 26.9 40.3

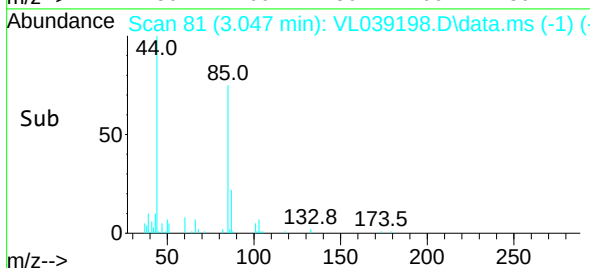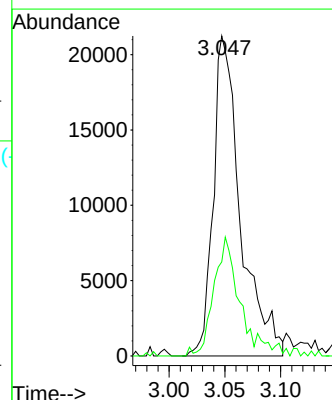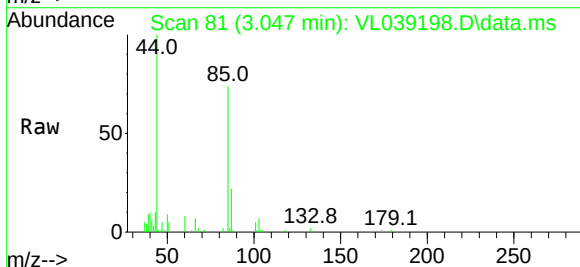



#3
Chlorodifluoromethane
Concen: 0.160 ppbv m
RT: 2.989 min Scan# 61
Delta R.T. -0.010 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5



Tgt Ion: 51 Resp: 2513
Ion Ratio Lower Upper
51 100
67 17.3 16.2 24.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

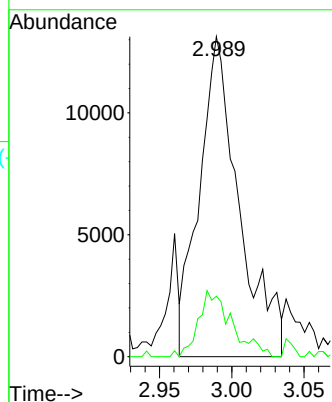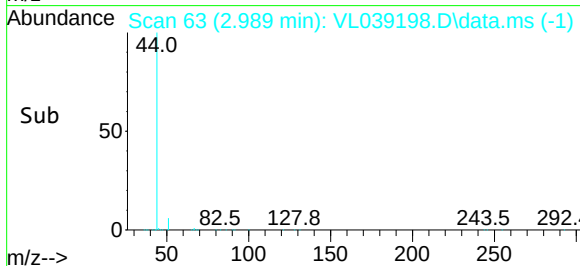

#4
Chloromethane
Concen: 0.167 ppbv
RT: 3.140 min Scan# 110
Delta R.T. -0.010 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01


Tgt Ion: 50 Resp: 13491
Ion Ratio Lower Upper
50 100
52 23.5 25.9 38.9#

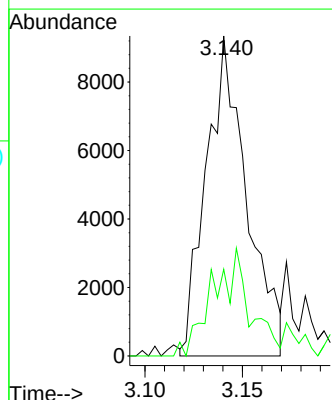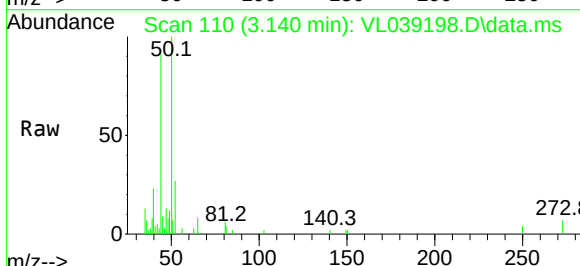



#9
 Propene
 Concen: 0.263 ppbv m
 RT: 3.018 min Scan# 72
 Delta R.T. -0.000 min
 Lab File: VL039198.D
 Acq: 7 Jun 2022 00:01




Instrument :
 MSVOA_L
 ClientSampleId :
 SG-5



Tgt Ion: 41 Resp: 18040
 Ion Ratio Lower Upper
 41 100
 42 61.1 55.4 83.2




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
 Supervised By :Mahesh Dadoda 06/07/2022

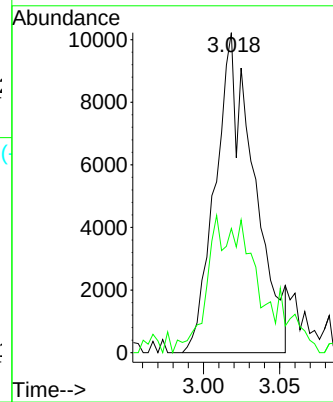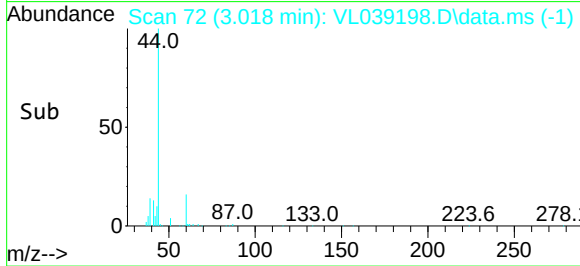

#10
 Heptane
 Concen: 0.295 ppbv
 RT: 8.111 min Scan# 1656
 Delta R.T. -0.016 min
 Lab File: VL039198.D
 Acq: 7 Jun 2022 00:01


Tgt Ion: 43 Resp: 47142
 Ion Ratio Lower Upper
 43 100
 57 61.7 41.4 62.2

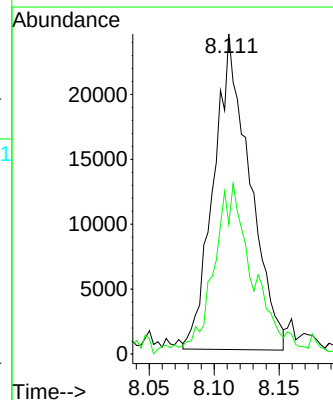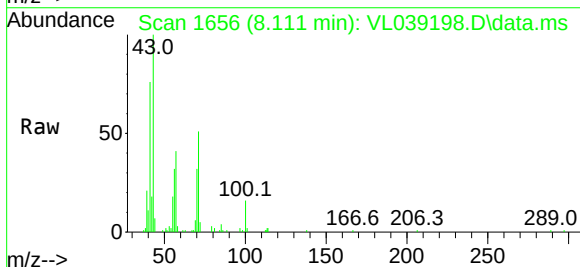



#11
Trichlorofluoromethane
Concen: 0.129 ppbv
RT: 3.951 min Scan# 30
Delta R.T. -0.010 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5



Tgt Ion:101 Resp: 2523
Ion Ratio Lower Upper
101 100
103 59.2 51.7 77.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

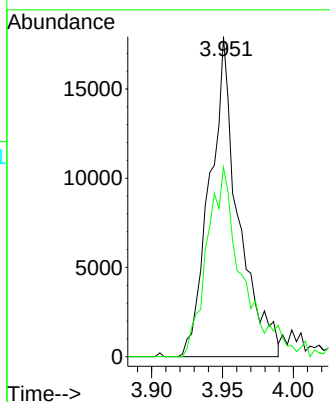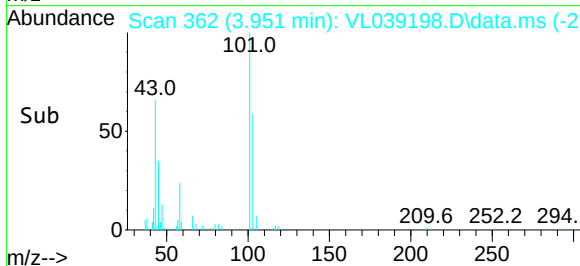

#13
Ethanol
Concen: 65.082 ppbv
RT: 3.600 min Scan# 253
Delta R.T. -0.010 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01


Tgt Ion: 45 Resp: 243090
Ion Ratio Lower Upper
45 100
46 40.0 0.0 0.0#

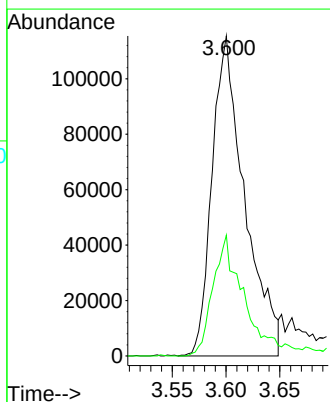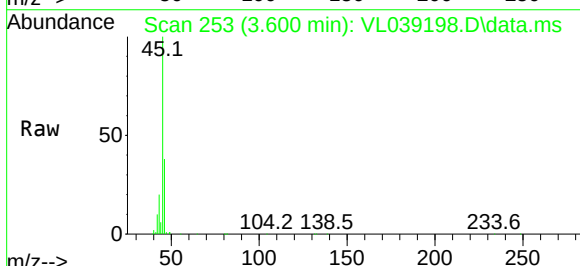

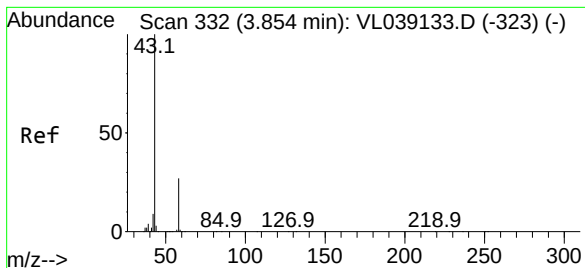

#15
Acetone
Concen: 8.414 ppbv
RT: 3.845 min Scan# 31
Delta R.T. -0.010 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5

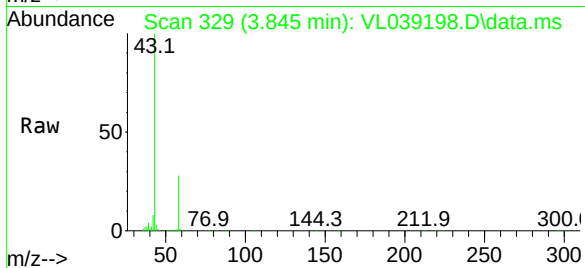

Tgt Ion: 43 Resp: 108197
Ion Ratio Lower Upper
43 100
58 32.2 22.5 33.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

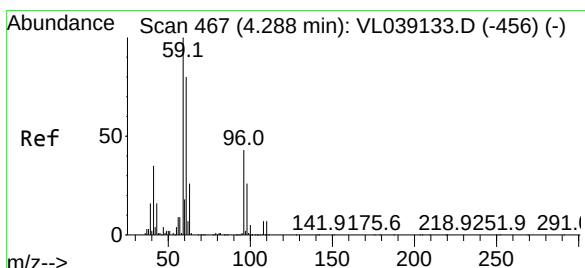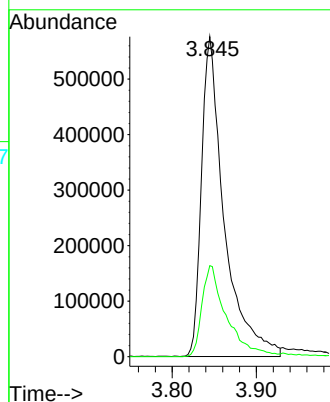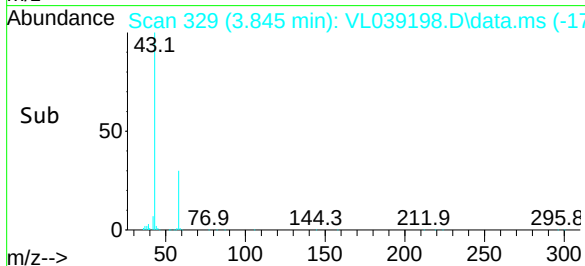

#17
tert-Butyl alcohol
Concen: 0.538 ppbv
RT: 4.292 min Scan# 468
Delta R.T. 0.003 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01


Tgt Ion: 59 Resp: 53663
Ion Ratio Lower Upper
59 100
57 14.6 9.1 13.7#

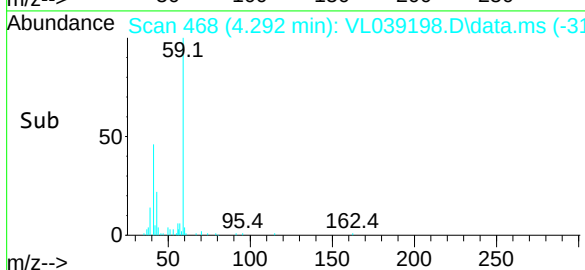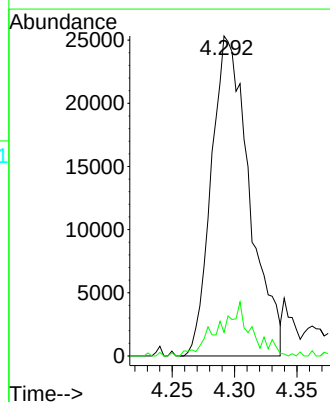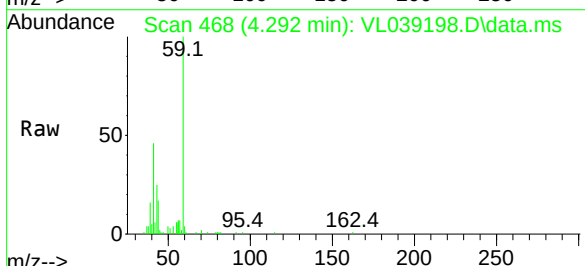



#19
Isopropyl Alcohol
Concen: 0.472 ppbv m
RT: 3.964 min Scan# 30
Delta R.T. -0.000 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5




Tgt Ion: 45 Resp: 28440
Ion Ratio Lower Upper
45 100
58 1213.5 1.8 2.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

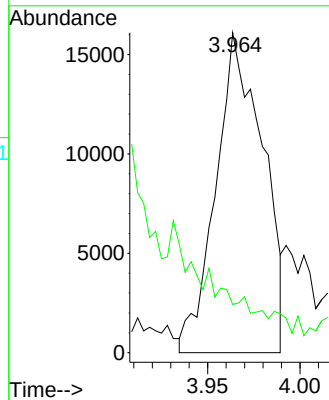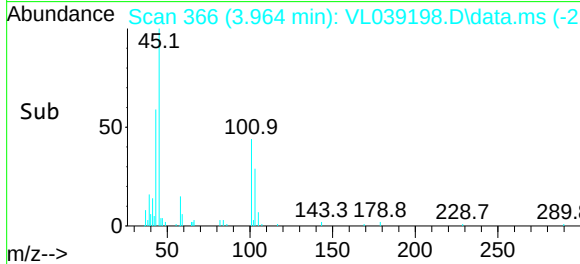


#20
Methylene Chloride
Concen: 15.728 ppbv
RT: 4.340 min Scan# 483
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01

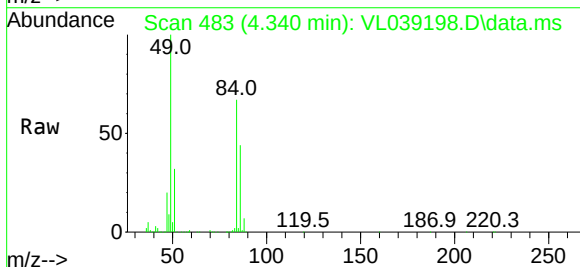


Tgt Ion: 84 Resp: 852319
Ion Ratio Lower Upper
84 100
49 149.7 111.1 166.7
51 47.2 35.3 52.9
86 65.5 51.9 77.9

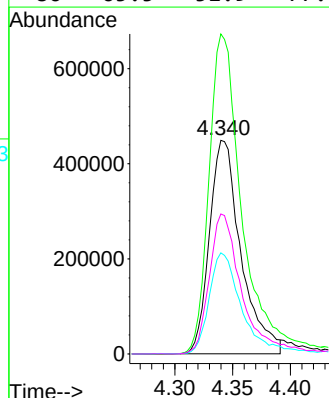



#26
Hexane
Concen: 13.395 ppbv
RT: 5.681 min Scan# 904
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5



Tgt Ion: 57 Resp: 1706079
Ion Ratio Lower Upper
57 100
41 84.1 72.4 108.6
43 70.7 187.0 280.6
56 51.8 41.8 62.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

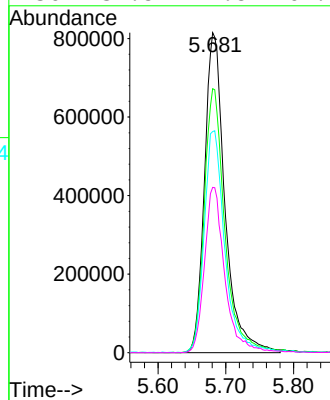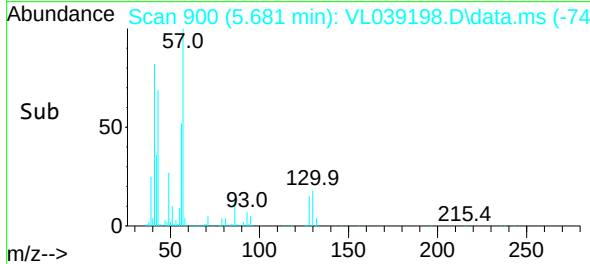

#29
Chloroform
Concen: 0.194 ppbv m
RT: 5.748 min Scan# 921
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01


Tgt Ion: 83 Resp: 41667
Ion Ratio Lower Upper
83 100
85 59.3 52.4 78.6

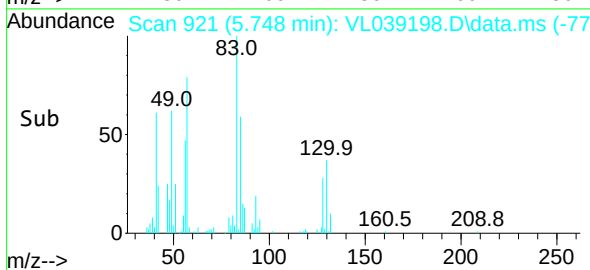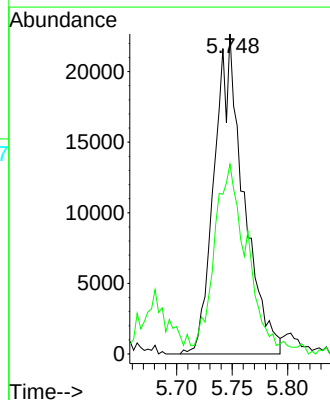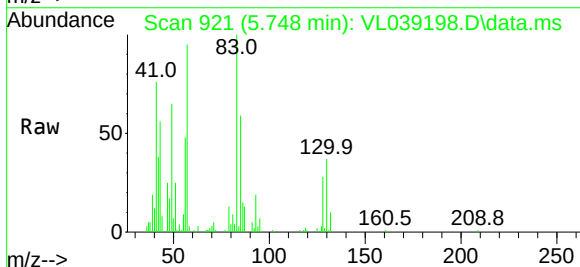

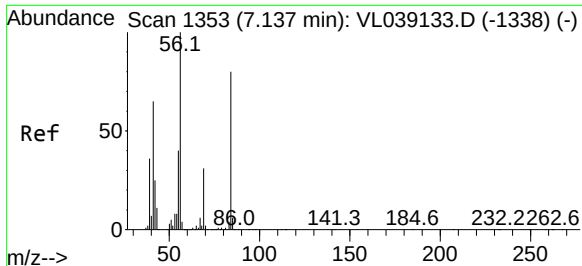

#30
Cyclohexane
Concen: 0.143 ppbv m
RT: 7.124 min Scan# 1349
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5

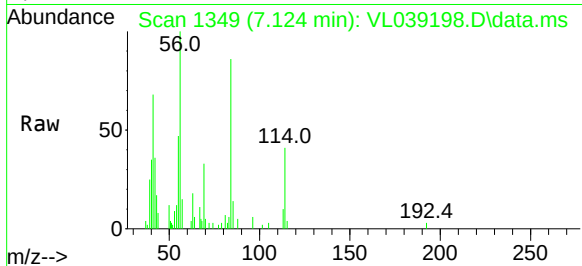


Tgt Ion: 84 Resp: 15269
Ion Ratio Lower Upper
84 100
56 0.0 110.6 165.8
41 69.4 68.9 103.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

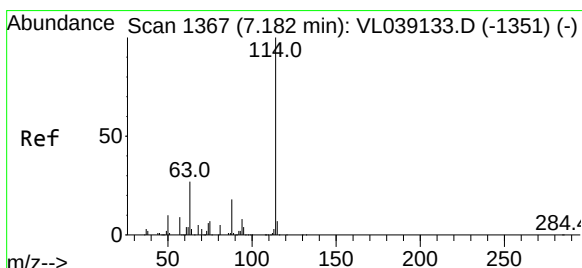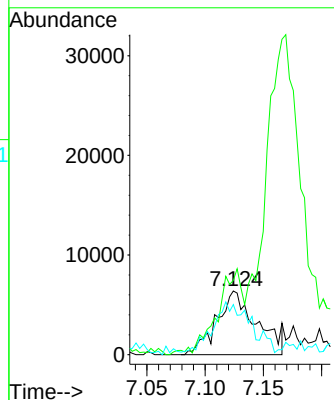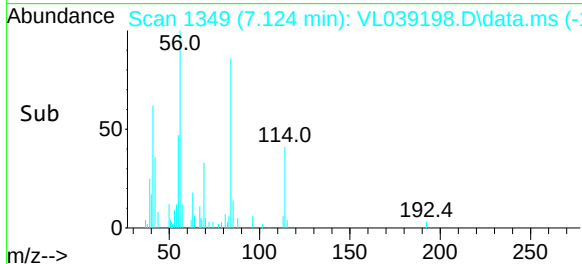


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.169 min Scan# 1363
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01

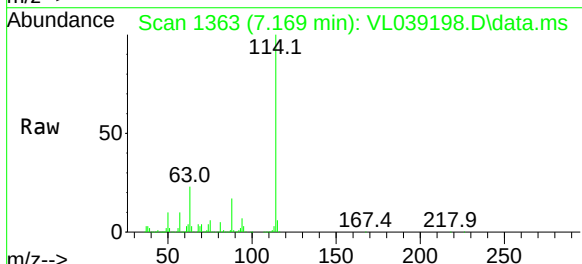


Tgt Ion:114 Resp: 3358670
Ion Ratio Lower Upper
114 100
63 23.8 21.7 32.5
88 17.7 14.8 22.2

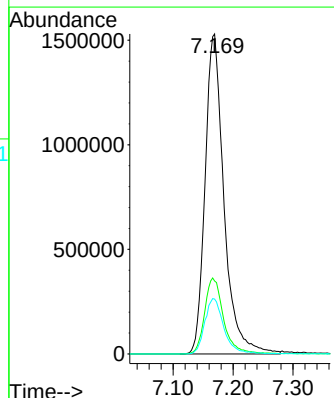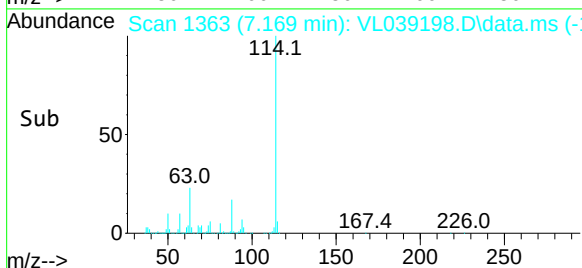

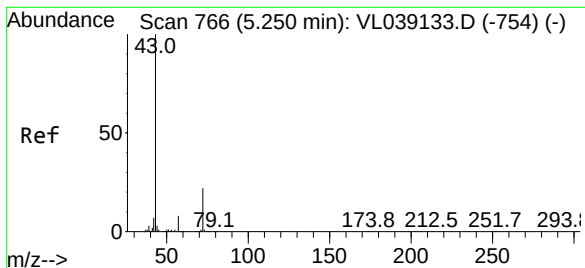

#34
2-Butanone
Concen: 1.665 ppbv
RT: 5.237 min Scan# 762
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5

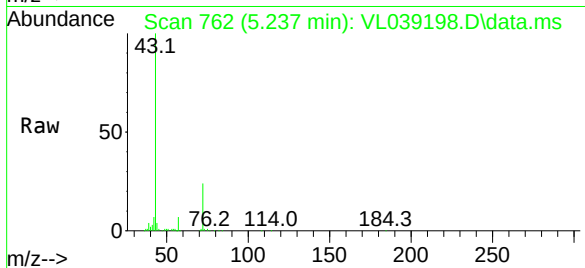

Tgt Ion: 43 Resp: 303840
Ion Ratio Lower Upper
43 100
72 25.7 18.2 27.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

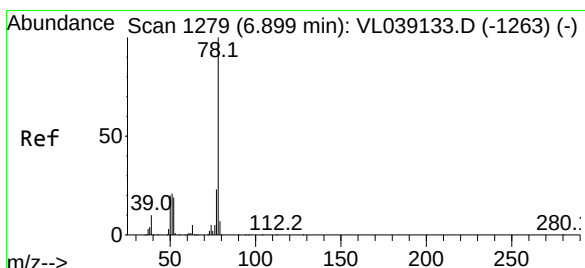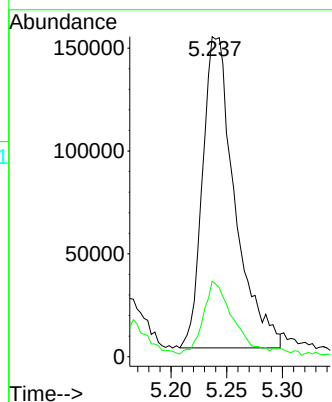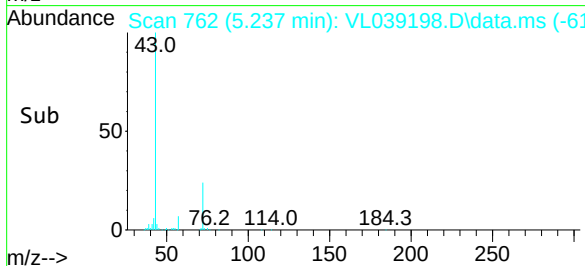

#36
Benzene
Concen: 0.125 ppbv m
RT: 6.883 min Scan# 1274
Delta R.T. -0.016 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01


Tgt Ion: 78 Resp: 33989
Ion Ratio Lower Upper
78 100
77 24.7 18.6 27.8
50 12.6 15.8 23.8#

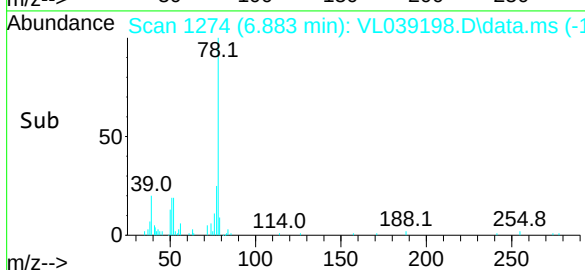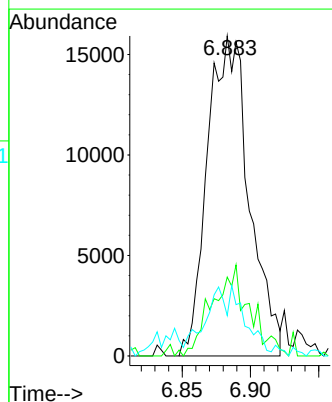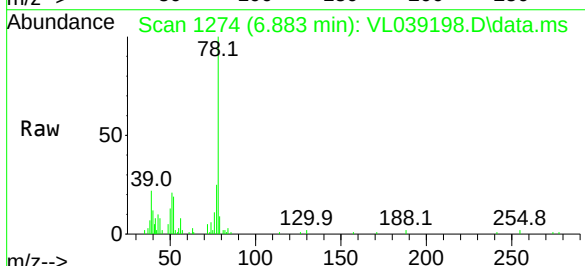



#44
2,2,4-Trimethylpentane
Concen: 0.108 ppbv m
RT: 7.857 min Scan# 1577
Delta R.T. -0.019 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument : MSVOA_L
ClientSampleId : SG-5




Tgt Ion: 57 Resp: 51700
Ion Ratio Lower Upper
57 100
41 37.7 26.2 39.4
56 44.5 24.7 37.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

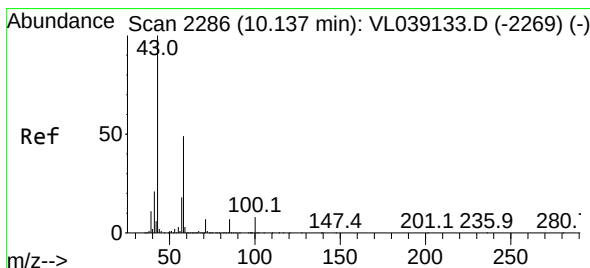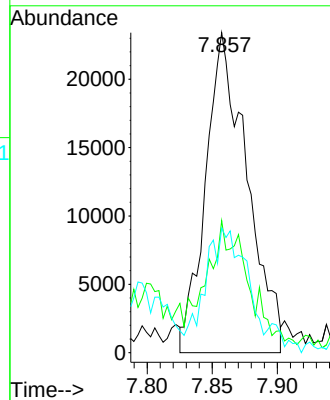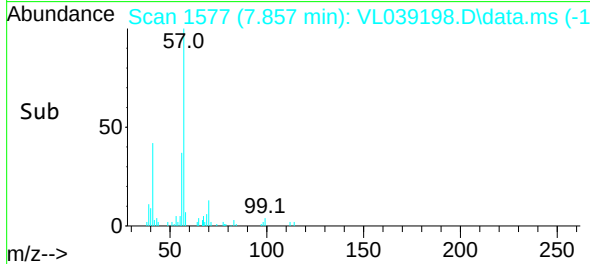


#51
2-Hexanone
Concen: 0.550 ppbv m
RT: 10.137 min Scan# 2286
Delta R.T. -0.000 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01

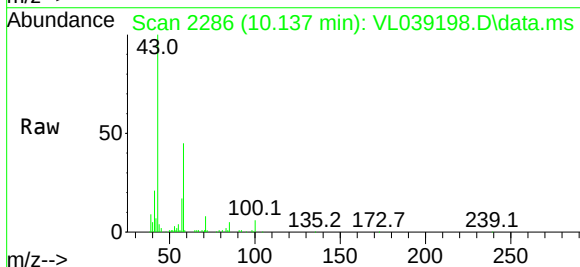


Tgt Ion: 43 Resp: 116888
Ion Ratio Lower Upper
43 100
58 47.9 40.0 60.0
98 0.0 0.1 0.1

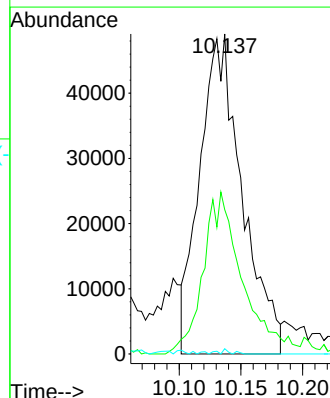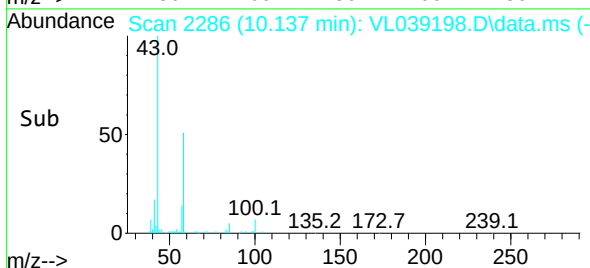



#52
Tetrachloroethene
Concen: 1.820 ppbv
RT: 11.211 min Scan# 2180
Delta R.T. -0.019 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5




Tgt Ion:164 Resp: 193724
Ion Ratio Lower Upper
164 100
166 126.5 96.3 144.5
129 109.3 82.5 123.7
131 96.5 82.1 123.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

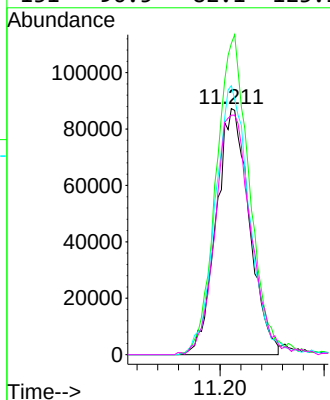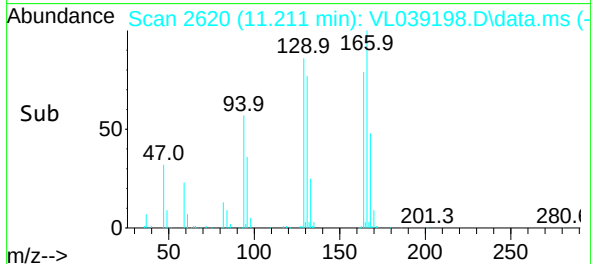


#53
Toluene
Concen: 1.182 ppbv
RT: 9.796 min Scan# 2180
Delta R.T. -0.016 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01

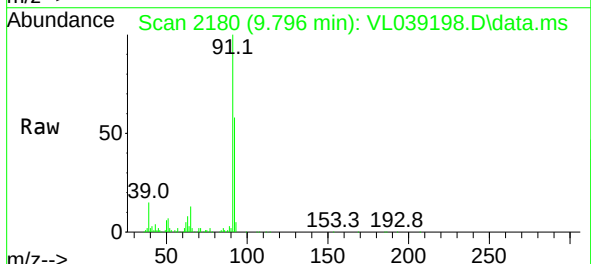


Tgt Ion: 91 Resp: 371253
Ion Ratio Lower Upper
91 100
92 62.3 48.1 72.1

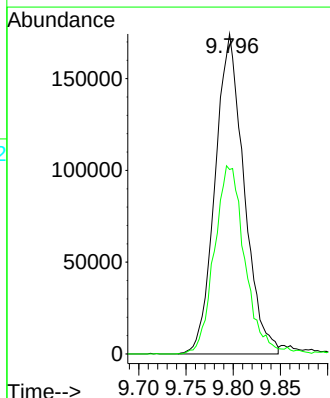



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.073 min Scan# 21
Delta R.T. -0.019 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5




Tgt Ion: 117 Resp: 2998462
Ion Ratio Lower Upper
117 100
82 66.6 55.1 82.7
119 34.0 24.7 37.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

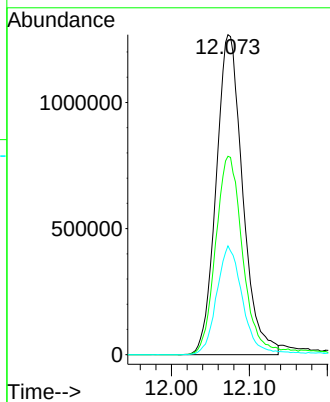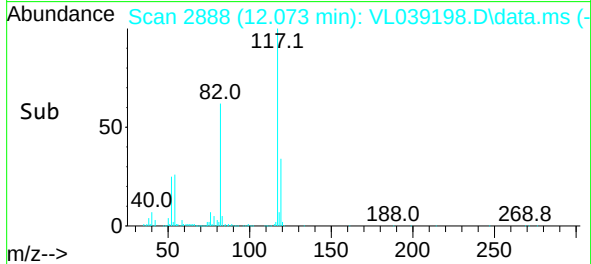


#58
Ethyl Benzene
Concen: 0.636 ppbv
RT: 12.696 min Scan# 3082
Delta R.T. -0.019 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01

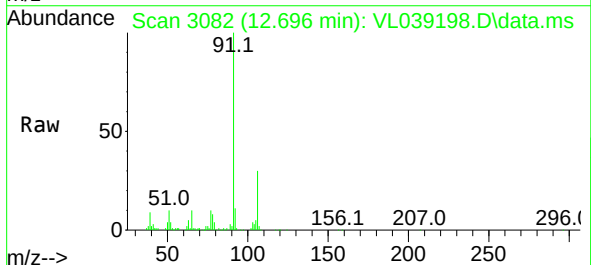

Tgt Ion: 91 Resp: 262821
Ion Ratio Lower Upper
91 100
106 30.4 24.2 36.4

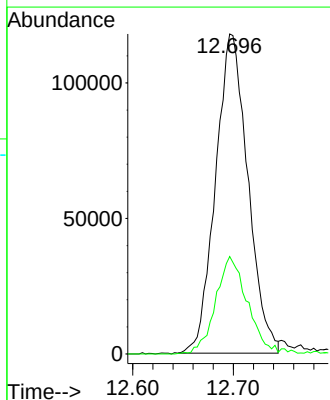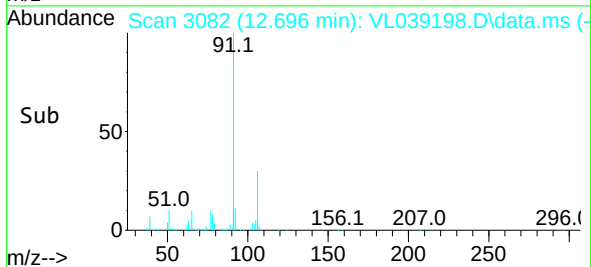



#59

m/p-Xylene

Concen: 2.565 ppbv

RT: 12.957 min Scan# 3176

Delta R.T. -0.042 min

Lab File: VL039198.D

Acq: 7 Jun 2022 00:01

Instrument :

MSVOA_L

ClientSampleId :

SG-5

Tgt Ion: 91 Resp: 93298

Ion Ratio Lower Upper

91 100





106 49.0 34.3 51.5

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2022

Supervised By :Mahesh Dadoda 06/07/2022

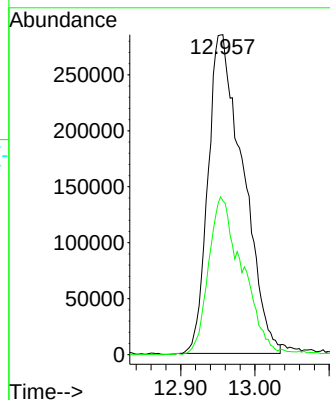

#60

o-Xylene

Concen: 1.278 ppbv

RT: 13.677 min Scan# 3387

Delta R.T. -0.019 min

Lab File: VL039198.D




Acq: 7 Jun 2022 00:01


Tgt Ion: 91 Resp: 436812

Ion Ratio Lower Upper

91 100

106 45.7 22.3 66.9

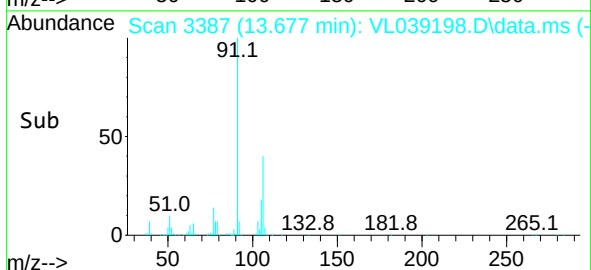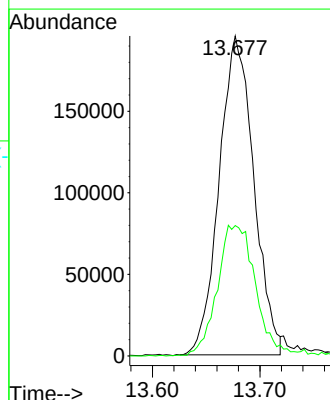



#61

Styrene

Concen: 0.201 ppbv m

RT: 13.516 min Scan# 31

Delta R.T. -0.016 min

Lab File: VL039198.D

Acq: 7 Jun 2022 00:01

Instrument :

MSVOA_L

ClientSampleId :





SG-5

Tgt Ion:104 Resp: 3683
 Ion Ratio Lower Upper
 104 100
 78 0.0 45.7 68.5
 103 0.0 39.6 59.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2022
 Supervised By :Mahesh Dadoda 06/07/2022

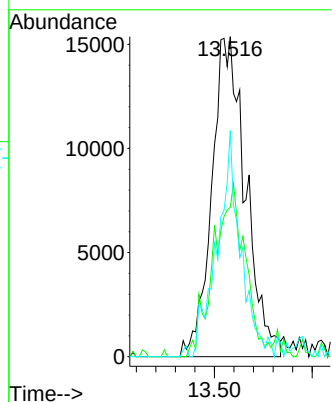

#64

n-propylbenzene

Concen: 0.315 ppbv m




RT: 15.539 min Scan# 3966


Delta R.T. -0.023 min

Lab File: VL039198.D

Acq: 7 Jun 2022 00:01


Tgt Ion:120 Resp: 39379
 Ion Ratio Lower Upper
 120 100
 91 488.4 388.4 582.6

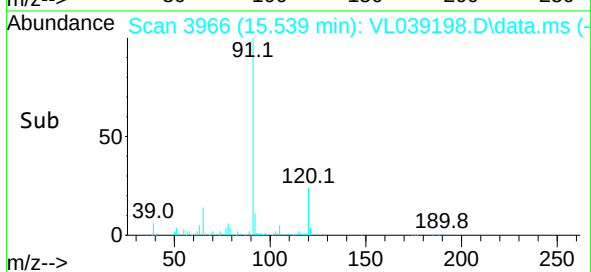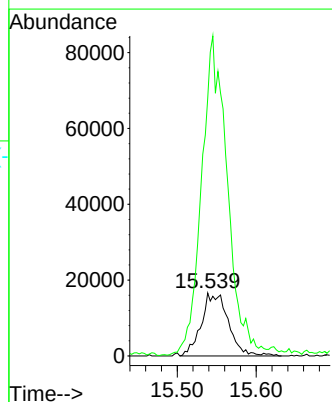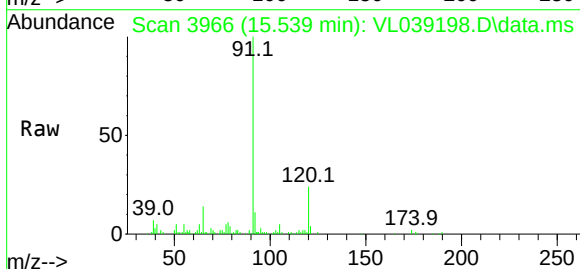



#68
1-Bromo-4-Fluorobenzene
Concen: 9.434 ppbv
RT: 14.404 min Scan# 30
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5




Tgt Ion: 95 Resp: 233869
Ion Ratio Lower Upper
95 100
174 70.4 53.8 80.8
175 5.0 4.1 6.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

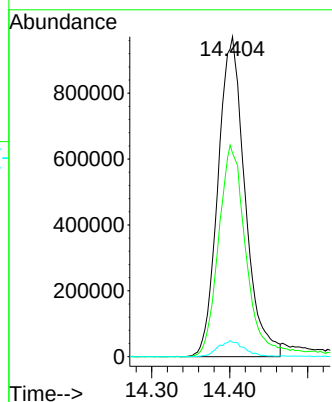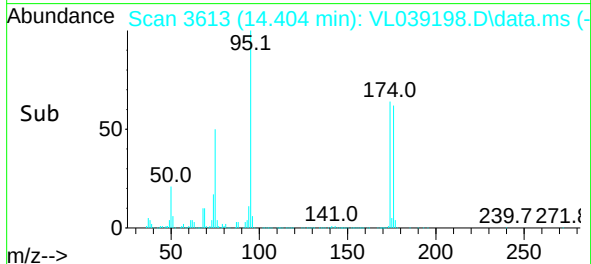


#70
n-Butylbenzene
Concen: 0.217 ppbv m
RT: 18.535 min Scan# 4898
Delta R.T. -0.016 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Tgt Ion: 91 Resp: 118944
Ion Ratio Lower Upper
91 100
92 37.3 43.6 65.4#
134 0.0 17.7 26.5#

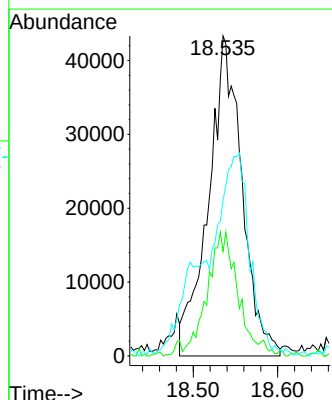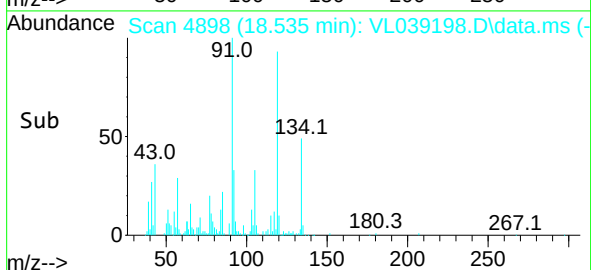



#72
4-Ethyltoluene
Concen: 0.636 ppbv
RT: 15.822 min Scan# 4060
Delta R.T. -0.019 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5



Tgt Ion:105 Resp: 254692
Ion Ratio Lower Upper
105 100
120 30.6 23.9 35.9
91 12.5 10.6 16.0
77 12.9 11.7 17.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

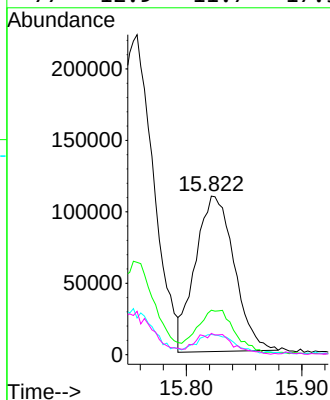

#73
1,3,5-Trimethylbenzene
Concen: 0.685 ppbv m
RT: 15.982 min Scan# 4104
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01


Tgt Ion:105 Resp: 247501
Ion Ratio Lower Upper
105 100
120 42.7 36.7 55.1

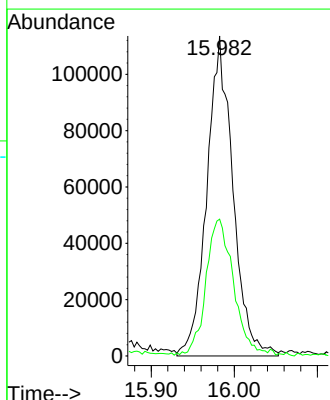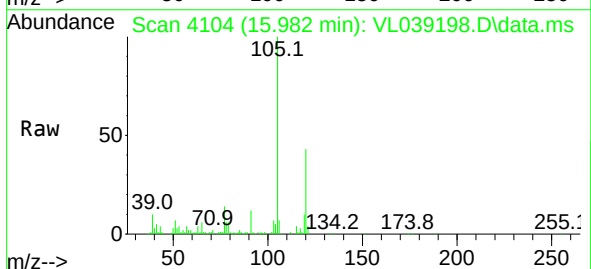



#74
1,2,4-Trimethylbenzene
Concen: 2.387 ppbv
RT: 16.748 min Scan# 41
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01




Instrument :
MSVOA_L
ClientSampleId :
SG-5



Tgt Ion:105 Resp: 96231
Ion Ratio Lower Upper
105 100
120 41.9 38.1 57.1
91 10.4 47.4 71.0
77 13.7 19.5 29.3#

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2022
Supervised By :Mahesh Dadoda 06/07/2022

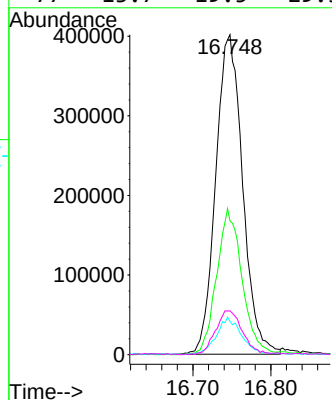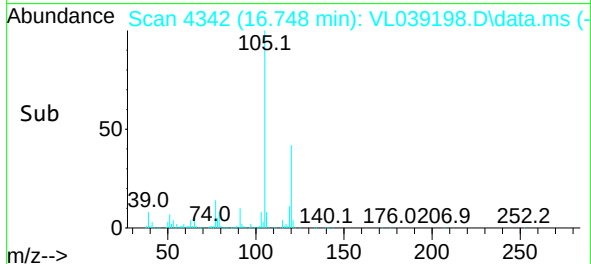

#79
Naphthalene
Concen: 0.264 ppbv m
RT: 22.181 min Scan# 6032
Delta R.T. -0.013 min
Lab File: VL039198.D
Acq: 7 Jun 2022 00:01

Tgt Ion:128 Resp: 82037
Ion Ratio Lower Upper
128 100
127 13.8 10.4 15.6
129 13.7 9.0 13.6#

