
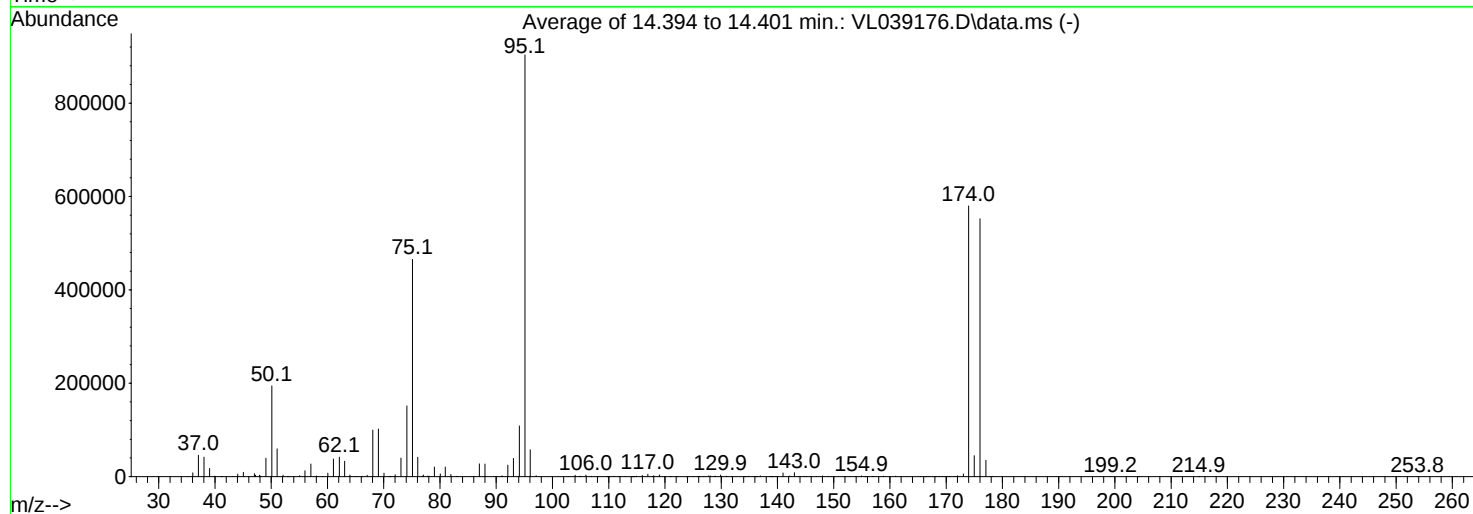


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060622\
Data File : VL039176.D
Acq On : 6 Jun 2022 7:58
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
Last Update : Wed Jun 01 01:22:18 2022

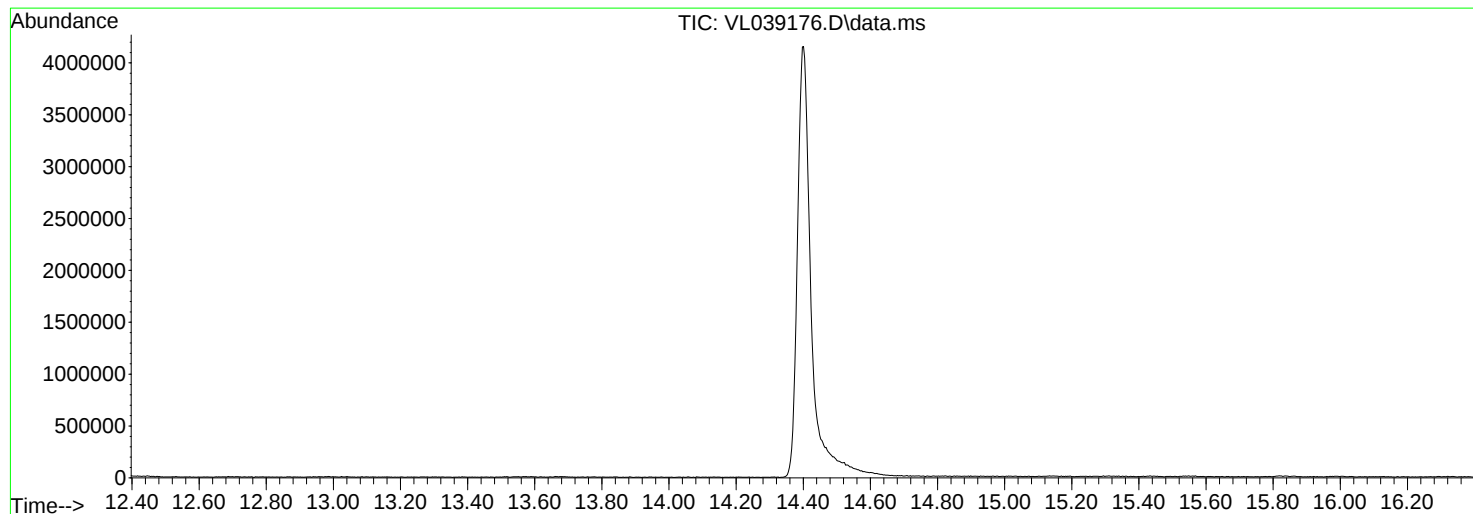

AutoFind: Scans 3610, 3611, 3612; Background Corrected with Scan 3579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.5	194325	PASS
75	95	30	66	51.5	465557	PASS
95	95	100	100	100.0	903381	PASS
96	95	5	9	6.4	57685	PASS
173	174	0.00	2	1.0	5947	PASS
174	95	50	120	64.2	579755	PASS
175	174	4	9	7.7	44739	PASS
176	174	93	101	95.3	552405	PASS
177	176	5	9	6.4	35125	PASS

Average of 14.394 to 14.401 min.: VL039176.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	210	47.00	6391	56.00	12665	66.00	61
36.05	8369	47.20	3168	57.05	26960	67.05	272
37.05	45995	47.90	3015	58.05	1319	68.05	9975
38.05	41936	48.10	1532	59.10	270	69.05	10198
39.05	17416	49.05	39296	60.05	7586	70.05	7422
40.00	1043	50.10	194325	61.05	37787	71.00	127
41.10	76	51.05	59805	62.10	41973	71.25	297
43.10	377	52.10	3070	63.05	32928	72.05	4248
44.05	5575	52.90	158	64.00	3300	73.05	39635
45.05	9140	53.90	142	64.80	255	74.10	151445
46.05	597	55.05	2122	65.25	245	75.10	465557

Average of 14.394 to 14.401 min.: VL039176.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	41451	85.70	202	97.10	2100	111.70	253
76.90	1191	86.05	619	102.80	410	111.95	474
77.05	3557	87.00	27608	104.05	3286	112.90	439
77.80	1034	88.00	27144	104.80	379	114.20	52
78.00	1458	90.90	821	104.95	1018	114.50	93
79.00	20446	91.05	1664	105.95	3508	114.95	1148
80.05	5747	92.05	24557	106.95	792	115.95	2916
80.95	20559	93.05	38925	108.00	80	116.95	5210
81.95	4686	94.10	108781	109.70	80	117.80	842
82.90	784	95.10	903381	110.00	135	118.00	2115
83.20	341	96.05	57685	110.85	875	119.00	3873

Average of 14.394 to 14.401 min.: VL039176.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.85	162	128.75	674	136.95	1884	144.60	271
120.90	131	129.00	925	138.60	241	144.90	357
122.10	85	129.90	3366	138.80	162	145.20	221
123.80	120	130.95	973	139.10	87	145.85	838
124.15	273	131.90	145	139.65	487	146.95	880
125.00	299	133.90	205	139.90	125	148.05	1812
125.75	349	134.20	69	141.00	7887	149.00	744
126.00	145	134.90	1197	142.15	1343	149.70	212
126.90	282	135.80	229	143.00	8492	150.10	875
127.80	1725	136.10	121	143.70	194	151.90	72
128.10	1384	136.50	222	144.05	311	152.05	343

Average of 14.394 to 14.401 min.: VL039176.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.90	432	166.35	191	171.40	263	214.90	54
153.85	529	166.90	217	172.05	1869	253.80	136
154.95	1663	167.55	359	173.05	5947		
155.60	58	167.90	88	174.00	579755		
156.10	253	168.35	368	175.00	44739		
156.90	722	168.85	243	176.00	552405		
157.10	358	169.30	704	177.05	35125		
158.90	899	169.80	246	177.90	421		
161.00	1000	170.20	284	178.20	844		
163.05	213	170.60	427	199.20	227		
165.45	212	170.80	446	204.20	52		