


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL061319\
Data File : VL033898.D
Acq On : 13 Jun 2019 12:59
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL060719AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
Last Update : Fri Jun 07 08:53:27 2019

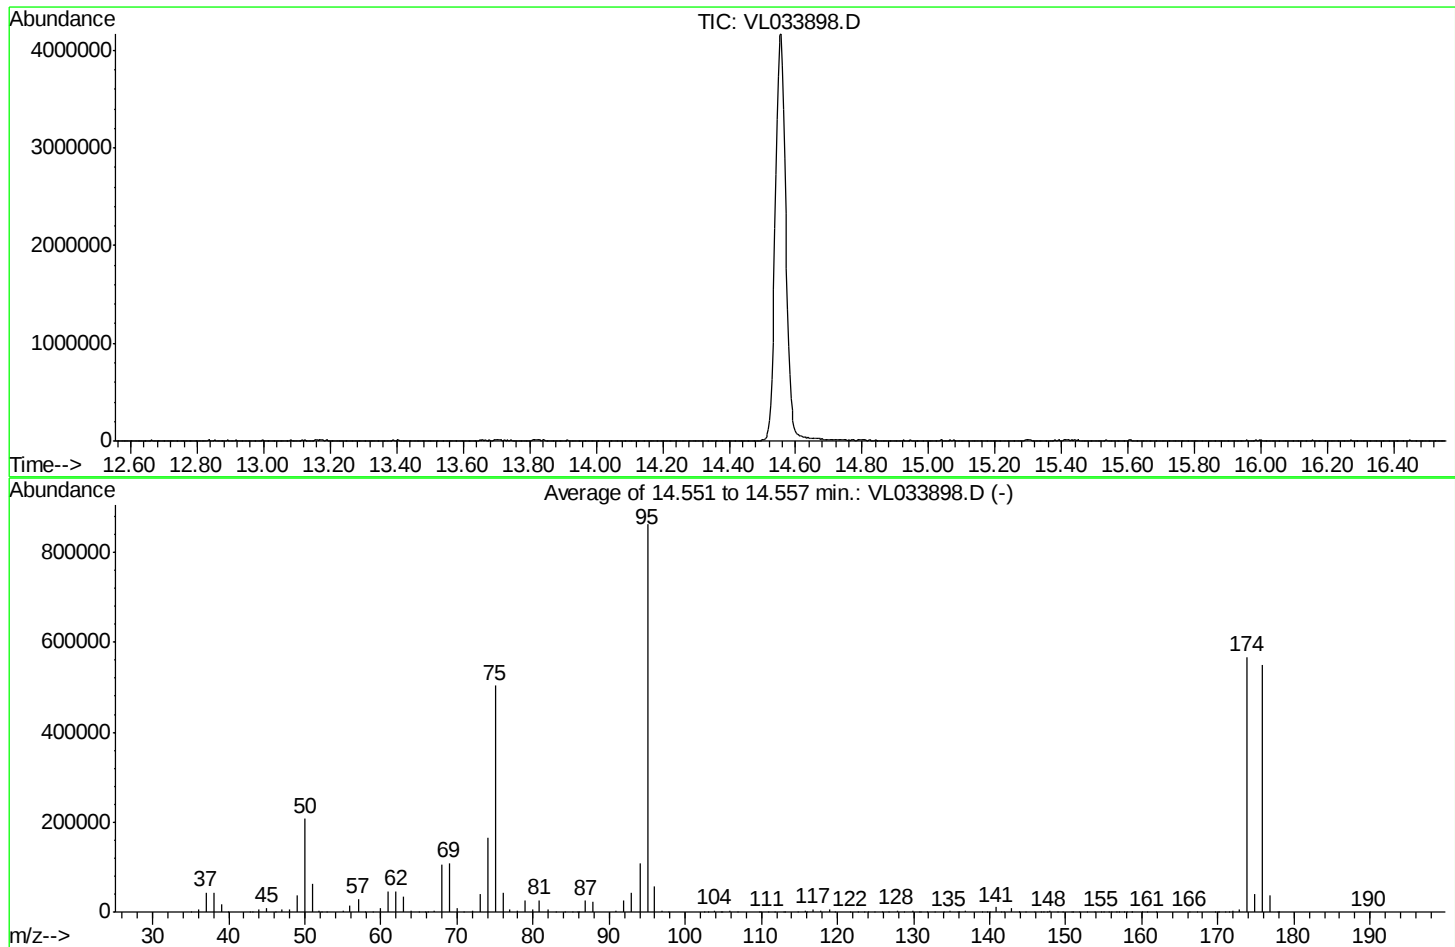

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	206869	PASS
75	95	30	66	58.3	502976	PASS
95	95	100	100	100.0	862506	PASS
96	95	5	9	6.7	57658	PASS
173	174	0.00	2	0.8	4506	PASS
174	95	50	120	65.7	566890	PASS
175	174	4	9	7.2	40664	PASS
176	174	93	101	96.9	549546	PASS
177	176	5	9	6.9	38152	PASS