

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061522\
 Data File : VL039300.D
 Acq On : 15 Jun 2022 17:04
 Operator : SY/AP
 Sample : VL0615ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0615ABL01

Quant Time: Jun 16 04:35:51 2022
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 QLast Update : Wed Jun 01 01:22:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.658	49	1269258	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.166	114	3669816	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.073	117	3193930	10.000	ppbv	-0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.400	95	2466065	9.339	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	93.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061522\
Data File : VL039300.D
Acq On : 15 Jun 2022 17:04
Operator : SY/AP
Sample : VL0615ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0615ABL01

Quant Time: Jun 16 04:35:51 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
QLast Update : Wed Jun 01 01:22:18 2022
Response via : Initial Calibration




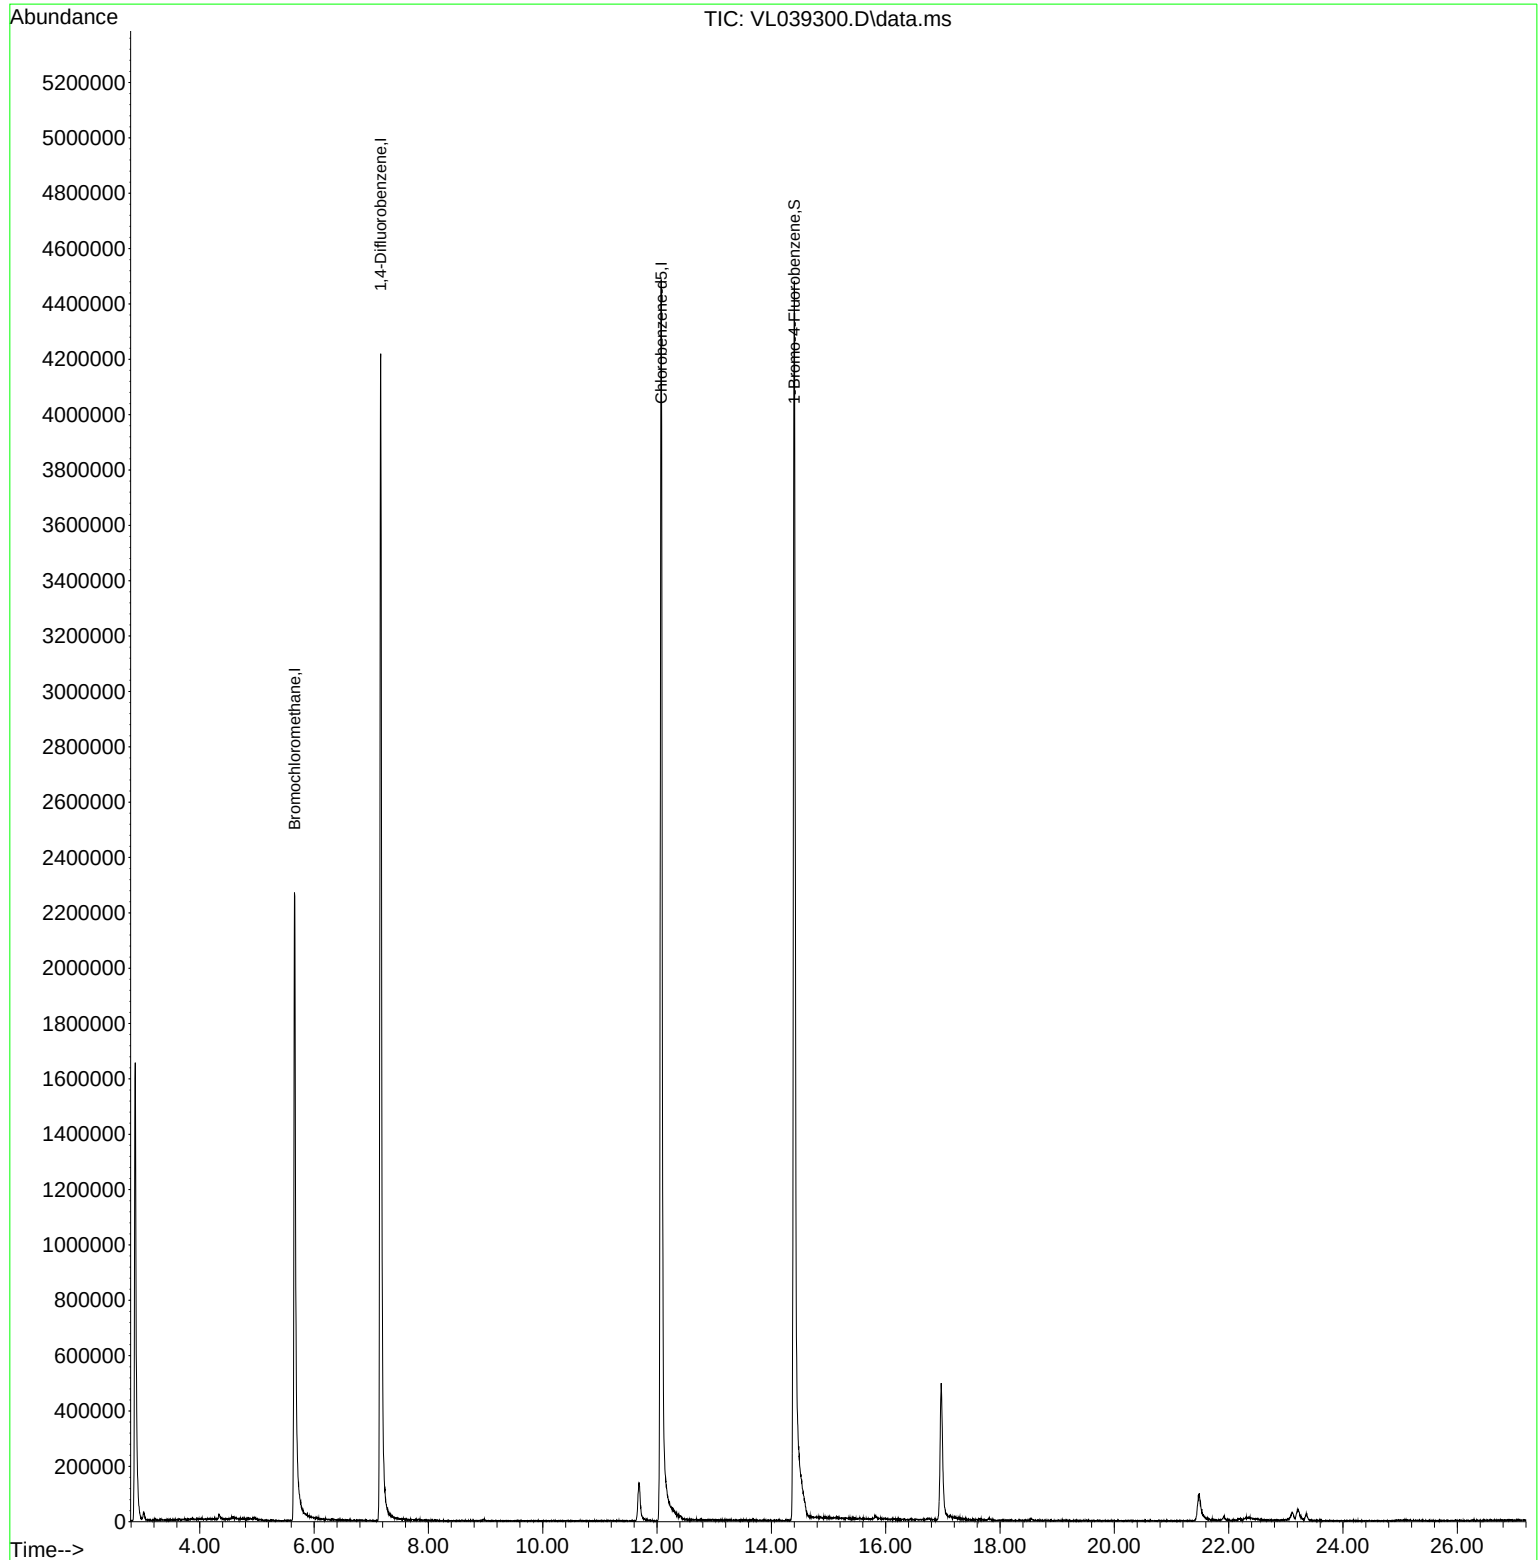


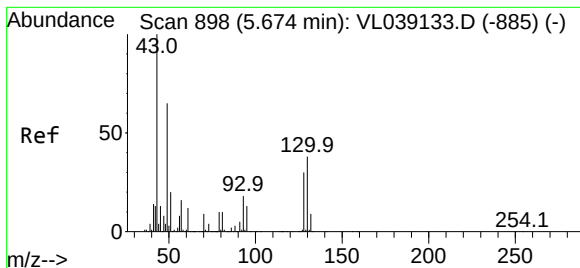

#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.658 min Scan# 893
 Delta R.T. -0.016 min
 Lab File: VL039300.D
 Acq: 15 Jun 2022 17:04




Instrument :
 MSVOA_L
 ClientSampleId :
 VL0615ABL01


Tgt Ion: 49 Resp: 1269258
 Ion Ratio Lower Upper
 49 100
 128 54.7 24.7 74.1
 130 71.8 31.4 94.0

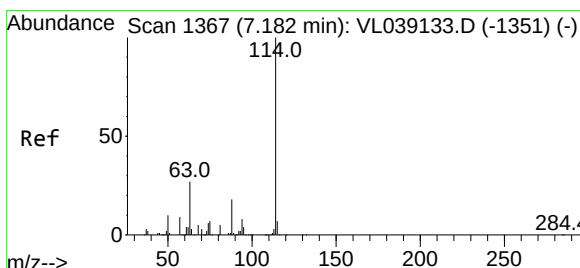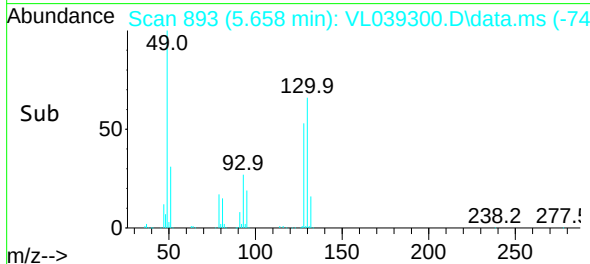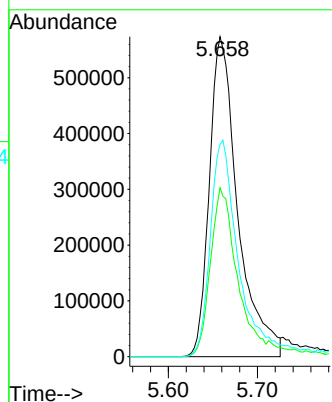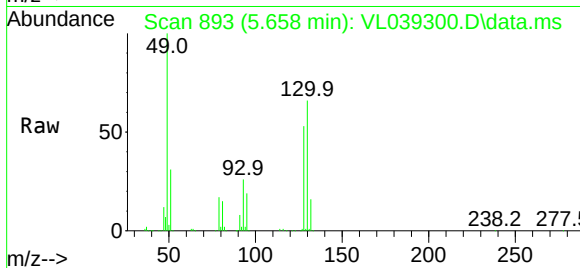

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.166 min Scan# 1362
 Delta R.T. -0.016 min
 Lab File: VL039300.D
 Acq: 15 Jun 2022 17:04

Tgt Ion: 114 Resp: 3669816
 Ion Ratio Lower Upper
 114 100
 63 24.9 21.7 32.5
 88 18.1 14.8 22.2


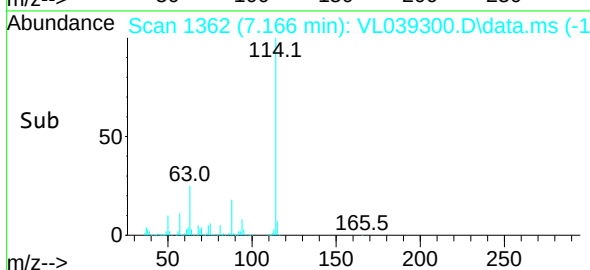
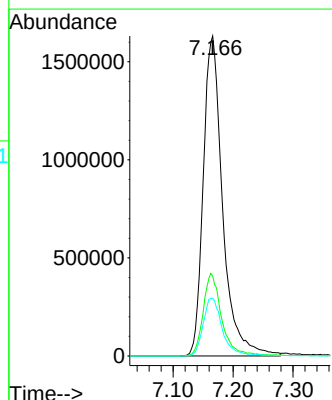
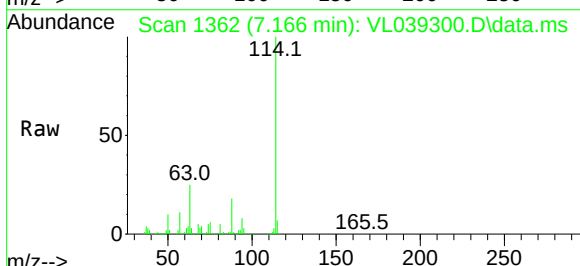


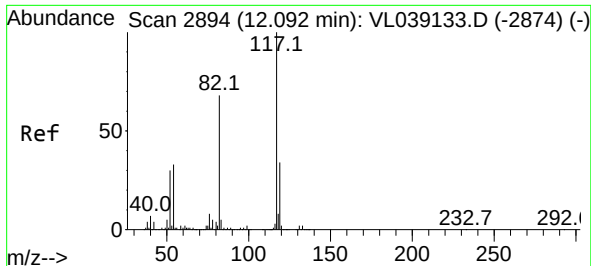

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.073 min Scan# 2888
Delta R.T. -0.019 min
Lab File: VL039300.D
Acq: 15 Jun 2022 17:04

Instrument :
MSVOA_L
ClientSampleId :
VL0615ABL01

Tgt Ion: 117 Resp: 3193930
Ion Ratio Lower Upper
117 100
82 65.6 55.1 82.7
119 33.6 24.7 37.1

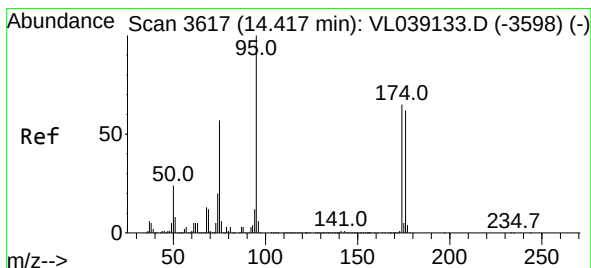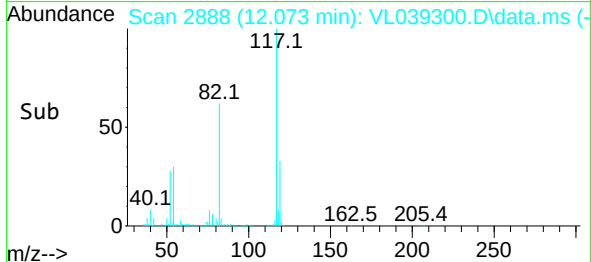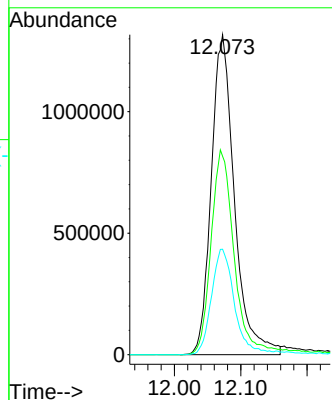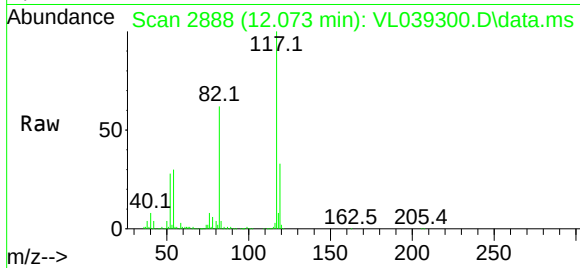

#68
1-Bromo-4-Fluorobenzene
Concen: 9.339 ppbv
RT: 14.400 min Scan# 3612
Delta R.T. -0.016 min
Lab File: VL039300.D
Acq: 15 Jun 2022 17:04

Tgt Ion: 95 Resp: 2466065
Ion Ratio Lower Upper
95 100
174 71.4 53.8 80.8
175 5.0 4.1 6.1

