

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061522\
 Data File : VL039302.D
 Acq On : 15 Jun 2022 19:14
 Operator : SY/AP
 Sample : N3326-03
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022
 Supervised By :Mahesh Dadoda 06/17/2022

Quant Time: Jun 16 04:36:46 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 0

QLast Update : Wed Jun 01 01:22:18 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.655	49	1176631	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.163	114	3281690	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.069	117	2971429	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.397	95	2335637	9.508	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.100%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	3.041	85	50068	0.242	ppbv	93
3) Chlorodifluoromethane	2.983	51	61428	0.410	ppbv #	90
4) Chloromethane	3.137	50	44719	0.582	ppbv	95
9) Propene	3.018	41	243947m	3.737	ppbv	
10) Heptane	8.108	43	89472	0.588	ppbv	96
11) Trichlorofluoromethane	3.944	101	42340	0.226	ppbv	92
13) Ethanol	3.591	45	520849	146.302	ppbv #	100
15) Acetone	3.835	43	3558870	29.036	ppbv	91
17) tert-Butyl alcohol	4.288	59	69158m	0.727	ppbv	
19) Isopropyl Alcohol	3.951	45	1221061	21.241	ppbv #	97
20) Methylene Chloride	4.337	84	248804	4.817	ppbv	92
26) Hexane	5.677	57	407578	3.357	ppbv #	39
28) Methyl tert-Butyl Ether	5.021	73	27522m	0.205	ppbv	
30) Cyclohexane	7.118	84	46157m	0.453	ppbv	
34) 2-Butanone	5.237	43	146402	0.821	ppbv	95
35) Carbon Tetrachloride	7.005	117	13297m	0.056	ppbv	
36) Benzene	6.877	78	135675	0.509	ppbv	96
37) 1,2-Dichloroethane	6.295	62	33043	0.188	ppbv #	94
44) 2,2,4-Trimethylpentane	7.854	57	1386892	2.976	ppbv	96
52) Tetrachloroethene	11.220	164	3505m	0.034	ppbv	
53) Toluene	9.790	91	925922	3.018	ppbv	99
58) Ethyl Benzene	12.693	91	226806	0.554	ppbv	97
59) m/p-Xylene	12.950	91	706651m	1.961	ppbv	
60) o-Xylene	13.674	91	271117	0.800	ppbv	99
61) Styrene	13.507	104	113835m	0.628	ppbv	
65) tert-Butylbenzene	16.751	119	51848m	0.113	ppbv	
72) 4-Ethyltoluene	15.825	105	135793m	0.342	ppbv	
73) 1,3,5-Trimethylbenzene	15.979	105	110062	0.307	ppbv	96
74) 1,2,4-Trimethylbenzene	16.741	105	403020m	1.009	ppbv	
79) Naphthalene	22.175	128	40969m	0.133	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061522\
Data File : VL039302.D
Acq On : 15 Jun 2022 19:14
Operator : SY/AP
Sample : N3326-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
IA1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022


Quant Time: Jun 16 04:36:46 2022


Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun

QLast Update : Wed Jun 01 01:22:18 2022


Response via : Initial Calibration

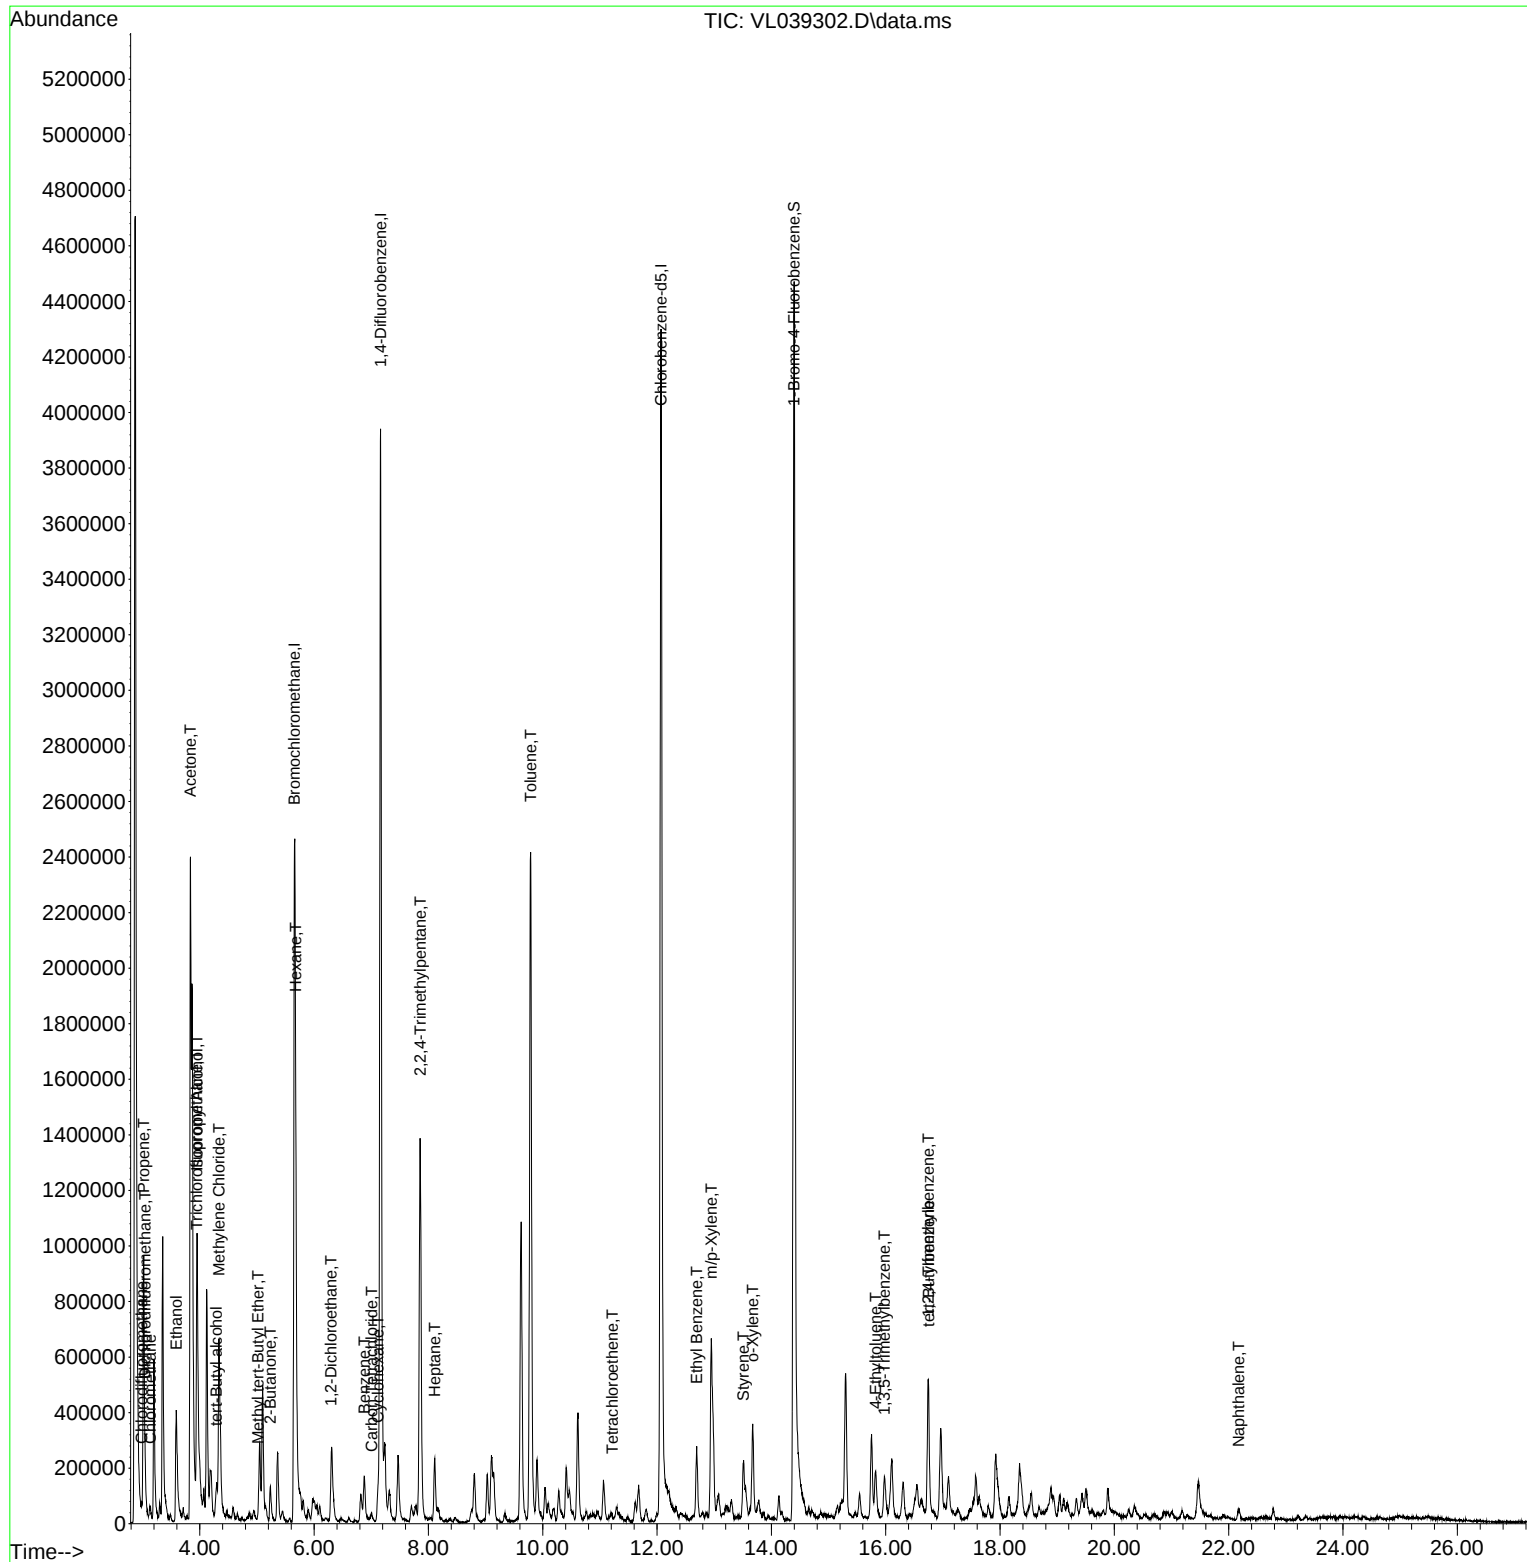



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.655 min Scan# 89
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion: 49 Resp: 117663
Ion Ratio Lower Upper
49 100
128 52.8 24.7 74.1
130 68.2 31.4 94.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

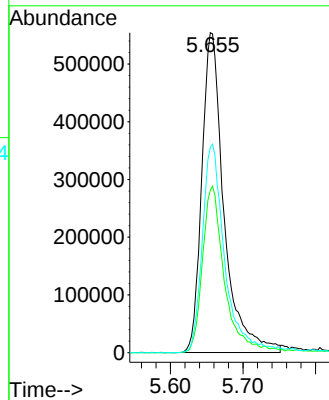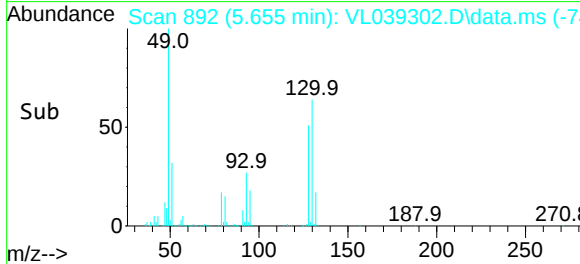


#2
Dichlorodifluoromethane
Concen: 0.242 ppbv
RT: 3.041 min Scan# 79
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14

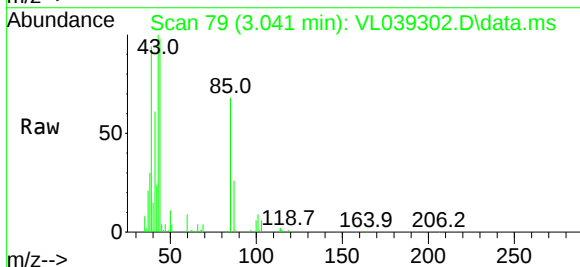


Tgt Ion: 85 Resp: 50068
Ion Ratio Lower Upper
85 100
87 37.4 26.9 40.3

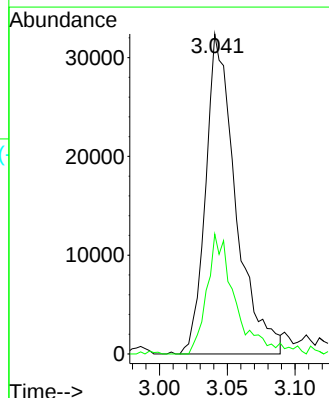



#3
Chlorodifluoromethane
Concen: 0.410 ppbv
RT: 2.983 min Scan# 61
Delta R.T. -0.016 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion: 51 Resp: 61428
Ion Ratio Lower Upper
51 100
67 15.8 16.2 24.4

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022




#4
Chloromethane
Concen: 0.582 ppbv
RT: 3.137 min Scan# 109
Delta R.T. -0.013 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14

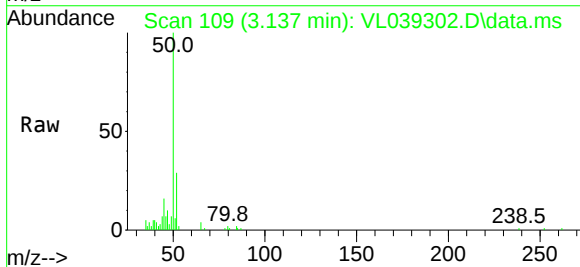


Tgt Ion: 50 Resp: 44719
Ion Ratio Lower Upper
50 100
52 29.4 25.9 38.9

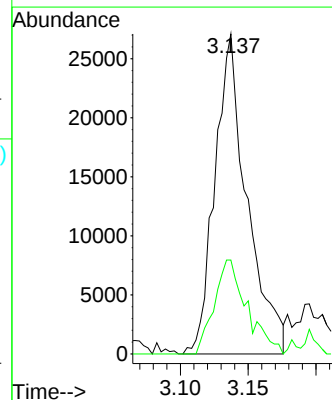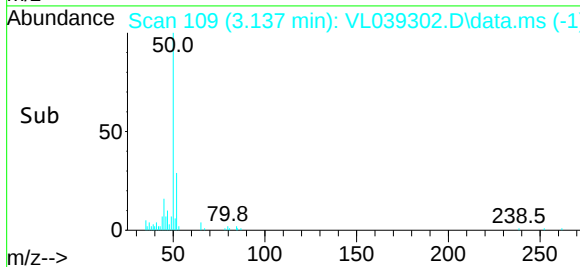



#9
 Propene
 Concen: 3.737 ppbv m
 RT: 3.018 min Scan# 70
 Delta R.T. -0.000 min
 Lab File: VL039302.D
 Acq: 15 Jun 2022 19:14




Instrument :
 MSVOA_L
 ClientSampleId :
 IA1



Tgt Ion: 41 Resp: 24394
 Ion Ratio Lower Upper
 41 100
 42 54.5 55.4 83.2




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
 Supervised By :Mahesh Dadoda 06/17/2022



#10
 Heptane
 Concen: 0.588 ppbv
 RT: 8.108 min Scan# 1655
 Delta R.T. -0.019 min
 Lab File: VL039302.D
 Acq: 15 Jun 2022 19:14


Tgt Ion: 43 Resp: 89472
 Ion Ratio Lower Upper
 43 100
 57 54.9 41.4 62.2





#11
Trichlorofluoromethane
Concen: 0.226 ppbv
RT: 3.944 min Scan# 30
Delta R.T. -0.016 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion:101 Resp: 42340
Ion Ratio Lower Upper
101 100
103 58.3 51.7 77.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

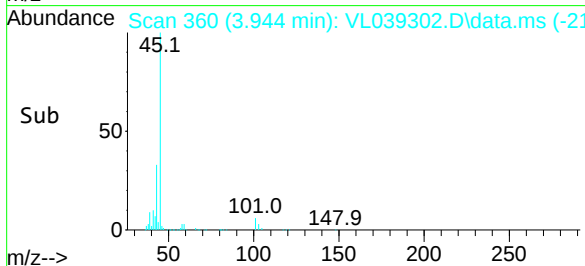

#13
Ethanol
Concen: 146.302 ppbv
RT: 3.591 min Scan# 250
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14


Tgt Ion: 45 Resp: 520849
Ion Ratio Lower Upper
45 100
46 38.9 0.0 0.0#

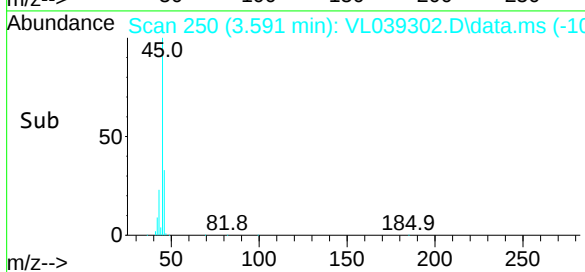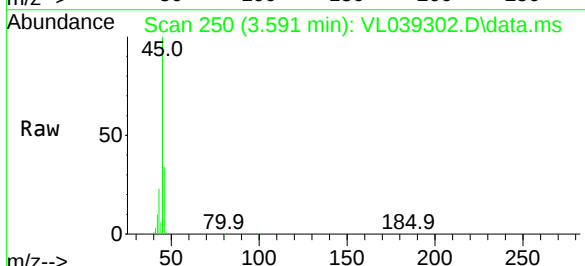



#15
Acetone
Concen: 29.036 ppbv
RT: 3.835 min Scan# 31
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 43 Resp: 3558870
Ion Ratio Lower Upper
43 100
58 23.5 22.5 33.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022



#17
tert-Butyl alcohol
Concen: 0.727 ppbv m
RT: 4.288 min Scan# 467
Delta R.T. -0.000 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14


Tgt Ion: 59 Resp: 69158
Ion Ratio Lower Upper
59 100
57 0.0 9.1 13.7#





#19
Isopropyl Alcohol
Concen: 21.241 ppbv
RT: 3.951 min Scan# 30
Delta R.T. -0.013 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion: 45 Resp: 122106
Ion Ratio Lower Upper
45 100
58 3.5 1.8 2.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

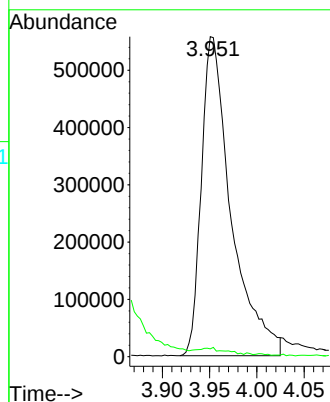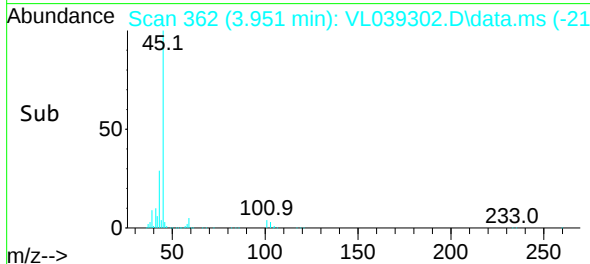


#20
Methylene Chloride
Concen: 4.817 ppbv
RT: 4.337 min Scan# 482
Delta R.T. -0.016 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14

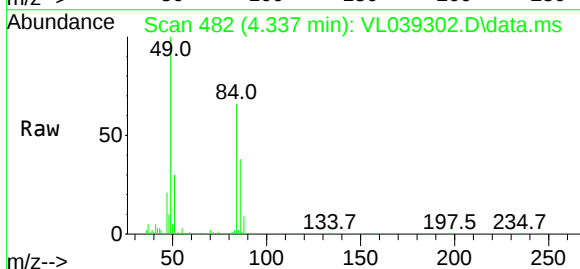


Tgt Ion: 84 Resp: 248804
Ion Ratio Lower Upper
84 100
49 151.0 111.1 166.7
51 44.0 35.3 52.9
86 57.4 51.9 77.9

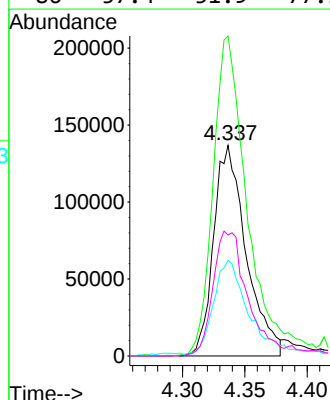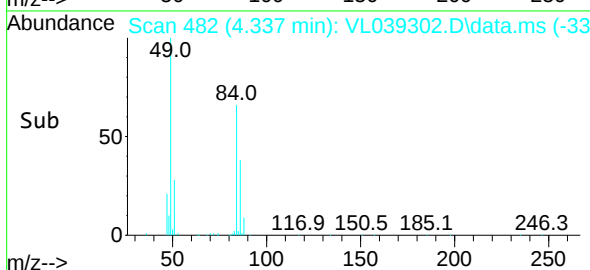



#26
Hexane
Concen: 3.357 ppbv
RT: 5.677 min Scan# 899
Delta R.T. -0.016 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 57 Resp: 407578
Ion Ratio Lower Upper
57 100
41 101.1 72.4 108.6
43 77.8 187.0 280.6
56 55.6 41.8 62.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

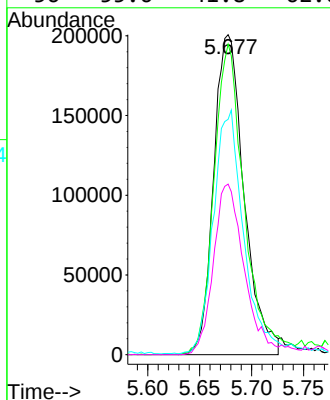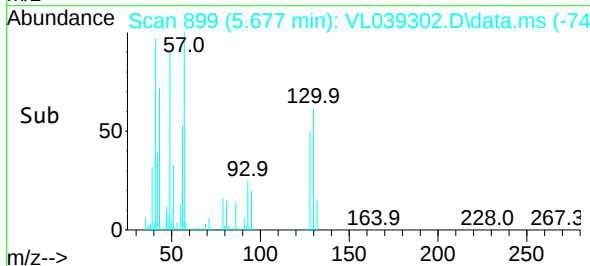

#28
Methyl tert-Butyl Ether
Concen: 0.205 ppbv m
RT: 5.021 min Scan# 695
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14


Tgt Ion: 73 Resp: 27522
Ion Ratio Lower Upper
73 100
57 29.6 18.6 27.8#

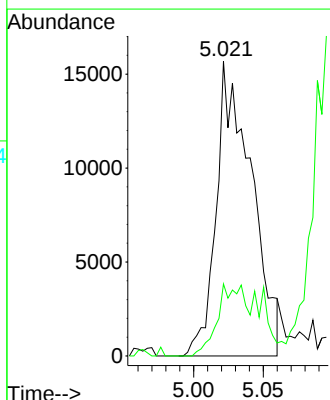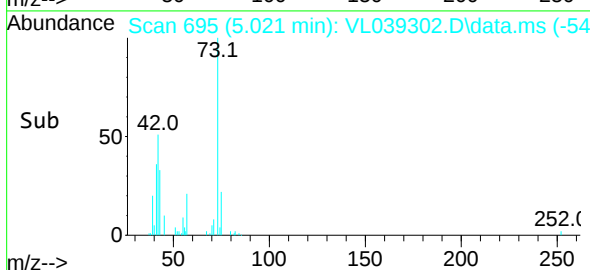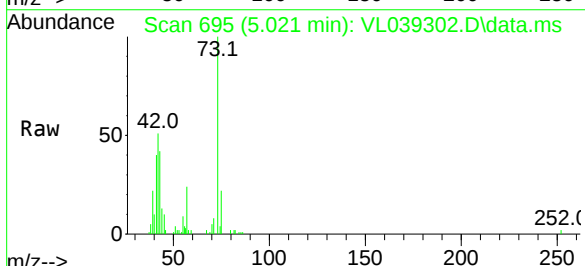



#30
Cyclohexane
Concen: 0.453 ppbv m
RT: 7.118 min Scan# 1347
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion: 84 Resp: 4615
Ion Ratio Lower Upper
84 100
56 99.4 110.6 165.8
41 89.0 68.9 103.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

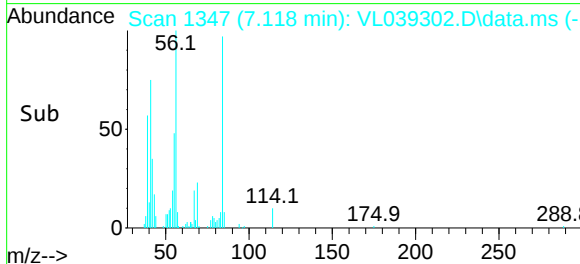


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.163 min Scan# 1361
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Tgt Ion:114 Resp: 3281690
Ion Ratio Lower Upper
114 100
63 25.3 21.7 32.5
88 18.2 14.8 22.2

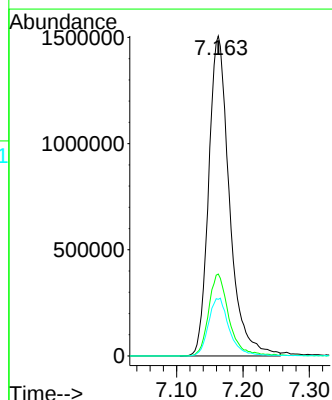



#34
2-Butanone
Concen: 0.821 ppbv
RT: 5.237 min Scan# 766
Delta R.T. -0.013 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 43 Resp: 14640
Ion Ratio Lower Upper
43 100
72 25.1 18.2 27.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

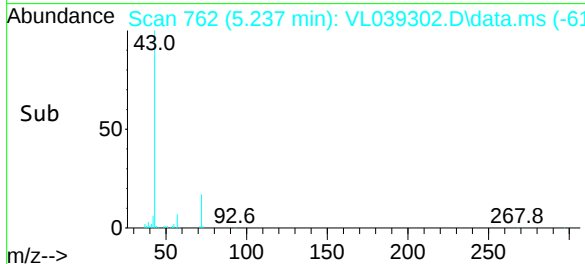

#35
Carbon Tetrachloride
Concen: 0.056 ppbv m
RT: 7.005 min Scan# 1312
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14

Tgt Ion:117 Resp: 13297
Ion Ratio Lower Upper
117 100
119 73.9 78.6 118.0#
121 19.0 25.4 38.0#

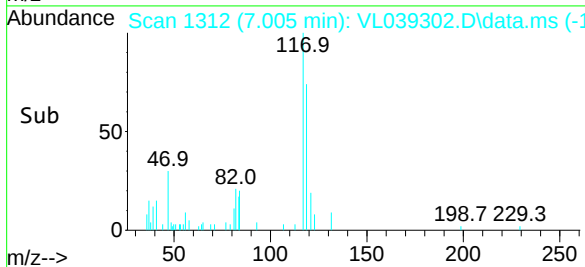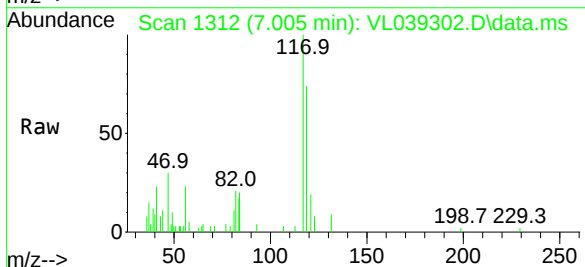



#36

Benzene

Concen: 0.509 ppbv

RT: 6.877 min Scan# 1091

Delta R.T. -0.023 min

Lab File: VL039302.D


Acq: 15 Jun 2022 19:14

Instrument :

MSVOA_L

ClientSampleId :

IA1



Tgt Ion: 78 Resp: 135679

Ion Ratio Lower Upper

78 100

77 20.0 18.6 27.8




50 19.6 15.8 23.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022

Supervised By :Mahesh Dadoda 06/17/2022

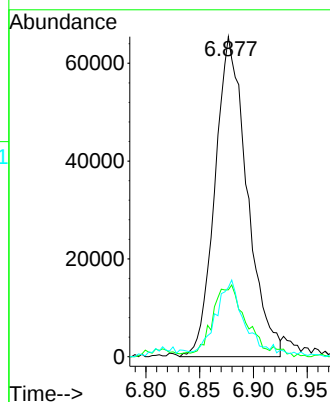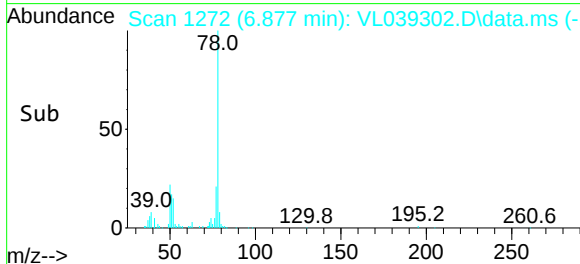

#37

1,2-Dichloroethane

Concen: 0.188 ppbv

RT: 6.295 min Scan# 1091

Delta R.T. -0.019 min

Lab File: VL039302.D




Acq: 15 Jun 2022 19:14


Tgt Ion: 62 Resp: 33043

Ion Ratio Lower Upper

62 100

98 7.4 4.3 6.5#

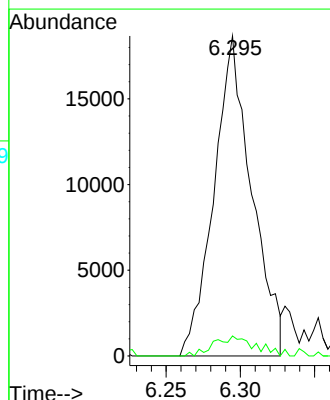



#44

2,2,4-Trimethylpentane

Concen: 2.976 ppbv

RT: 7.854 min Scan# 1

Delta R.T. -0.023 min

Lab File: VL039302.D

Acq: 15 Jun 2022 19:14

Instrument :

MSVOA_L

ClientSampleId :

IA1

Tgt Ion: 57 Resp: 138689

Ion Ratio Lower Upper

57 100

41 35.3 26.2 39.4





56 32.5 24.7 37.1

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022

Supervised By :Mahesh Dadoda 06/17/2022

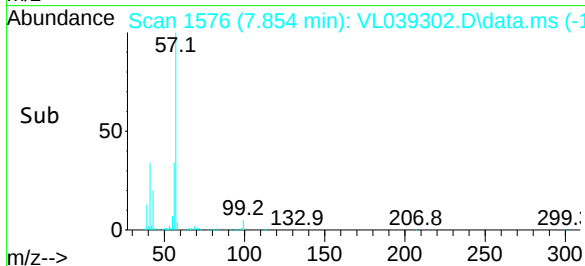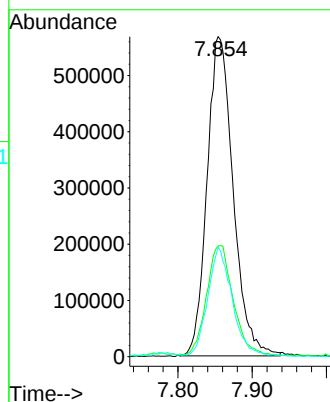

#52

Tetrachloroethene

Concen: 0.034 ppbv m

RT: 11.220 min Scan# 2623

Delta R.T. -0.010 min

Lab File: VL039302.D

Acq: 15 Jun 2022 19:14

Tgt Ion:164 Resp: 3505




Ion Ratio Lower Upper


164 100

166 82.5 96.3 144.5#

129 66.1 82.5 123.7#


131 46.0 82.1 123.1#

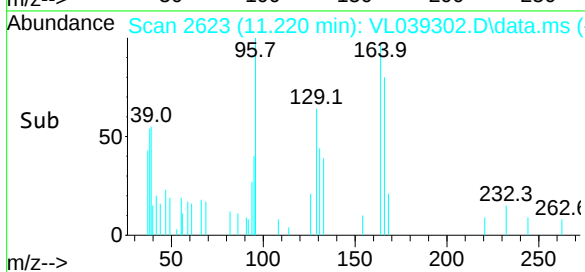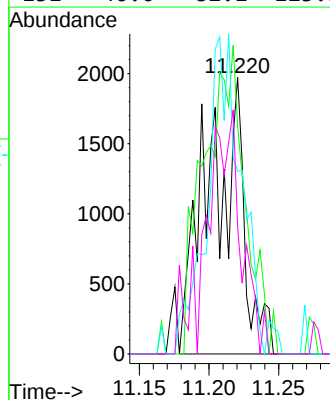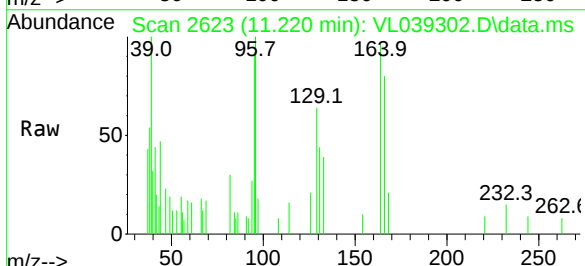

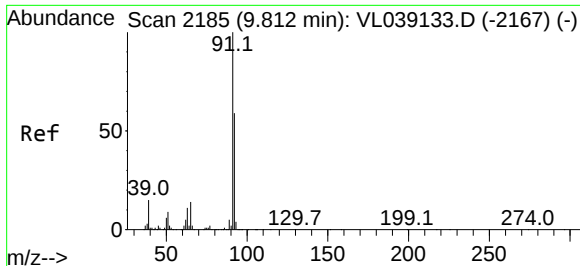

#53
Toluene
Concen: 3.018 ppbv
RT: 9.790 min Scan# 2185
Delta R.T. -0.023 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1




Tgt Ion: 91 Resp: 92592
Ion Ratio Lower Upper
91 100
92 60.6 48.1 72.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

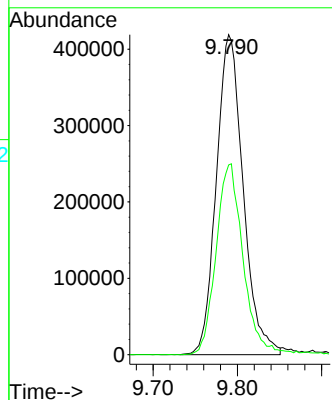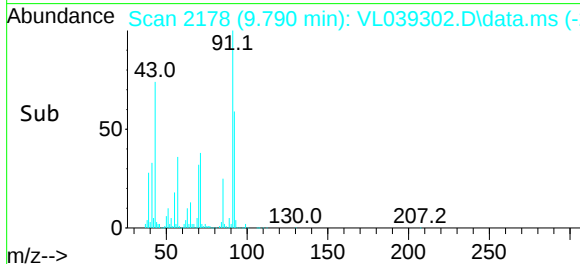


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.069 min Scan# 2887
Delta R.T. -0.023 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14

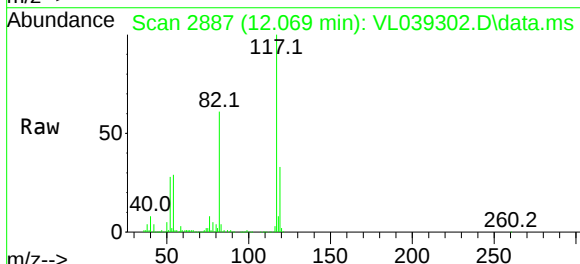


Tgt Ion:117 Resp: 2971429
Ion Ratio Lower Upper
117 100
82 66.8 55.1 82.7
119 34.1 24.7 37.1

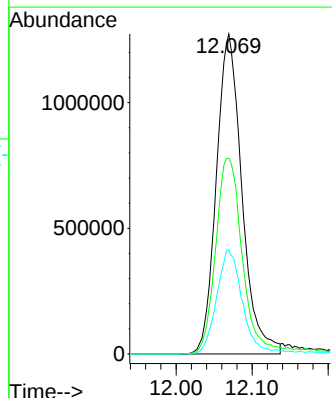

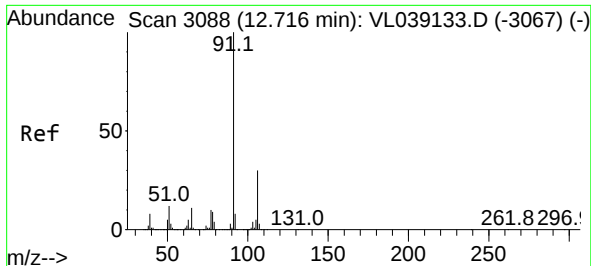

#58
Ethyl Benzene
Concen: 0.554 ppbv
RT: 12.693 min Scan# 3088
Delta R.T. -0.023 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 91 Resp: 226800
Ion Ratio Lower Upper
91 100
106 28.9 24.2 36.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

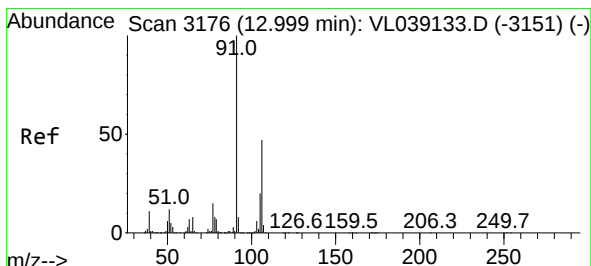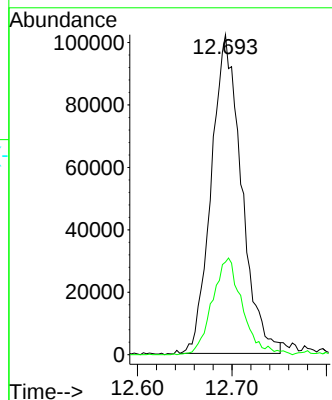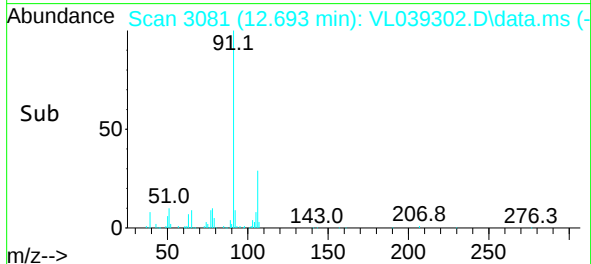

#59
m/p-Xylene
Concen: 1.961 ppbv m
RT: 12.950 min Scan# 3161
Delta R.T. -0.048 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14

Tgt Ion: 91 Resp: 706651
Ion Ratio Lower Upper
91 100
106 0.0 34.3 51.5#

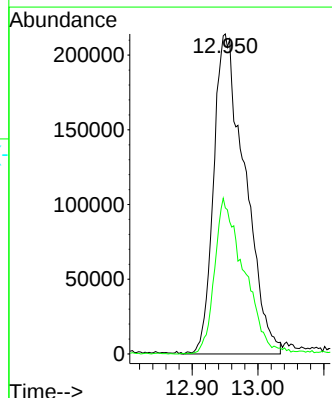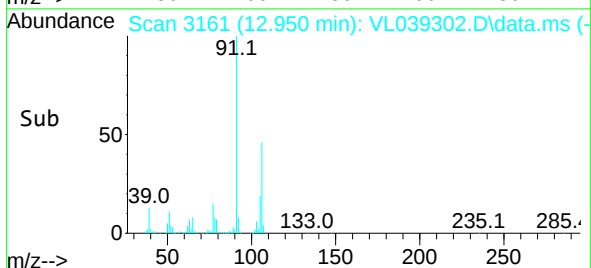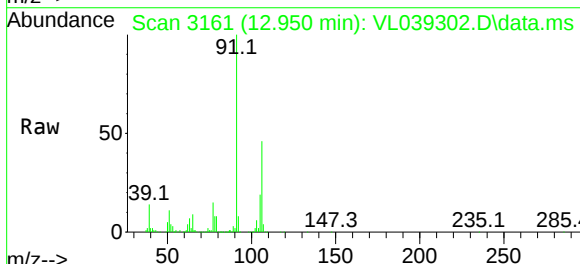

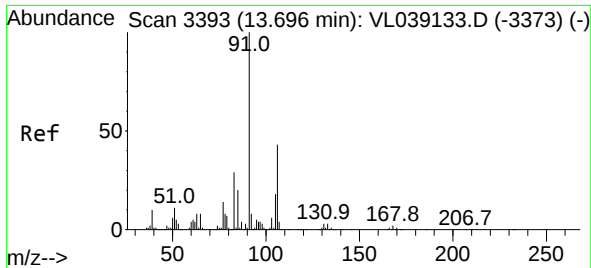





#60
o-Xylene
Concen: 0.800 ppbv
RT: 13.674 min Scan# 311
Delta R.T. -0.023 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion: 91 Resp: 27111
Ion Ratio Lower Upper
91 100
106 44.0 22.3 66.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

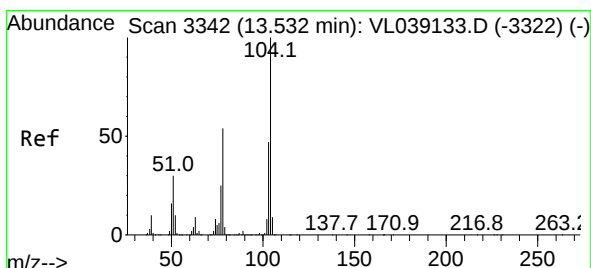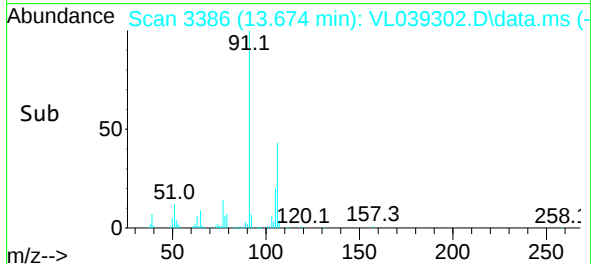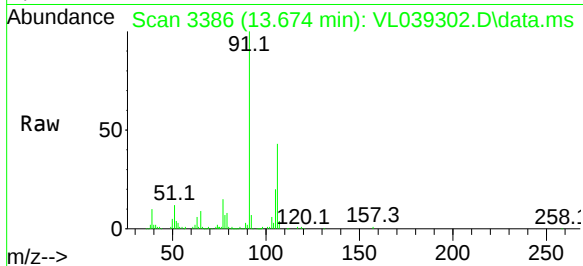

#61
Styrene
Concen: 0.628 ppbv m
RT: 13.507 min Scan# 3334
Delta R.T. -0.026 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14


Tgt Ion:104 Resp: 113835
Ion Ratio Lower Upper
104 100
78 53.5 45.7 68.5
103 52.7 39.6 59.4

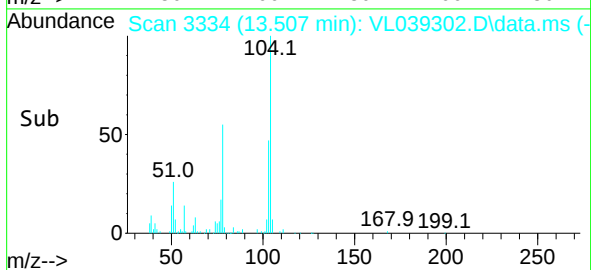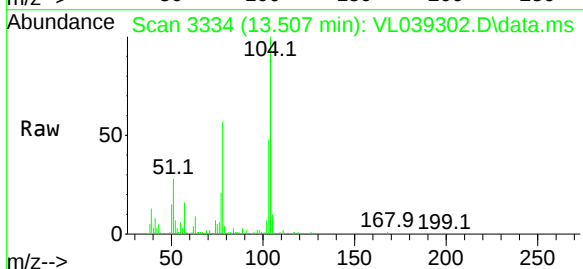

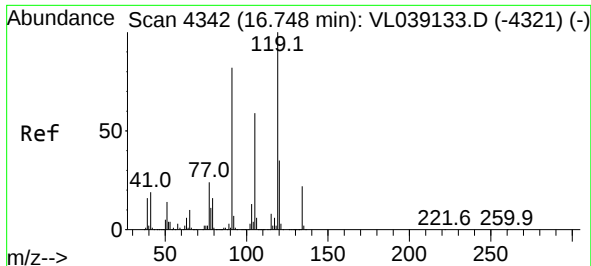

#65
tert-Butylbenzene
Concen: 0.113 ppbv m
RT: 16.751 min Scan# 4342
Delta R.T. 0.003 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14




Instrument :
MSVOA_L
ClientSampleId :
IA1

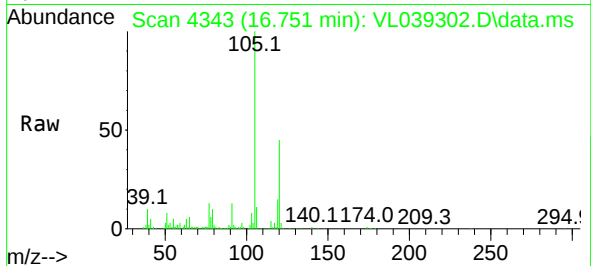


Tgt Ion: 119 Resp: 5184
Ion Ratio Lower Upper
119 100
91 99.8 67.1 100.7
134 0.5 15.8 23.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

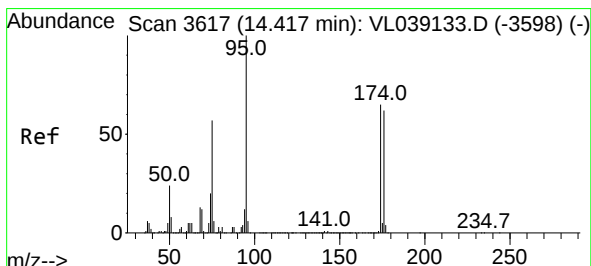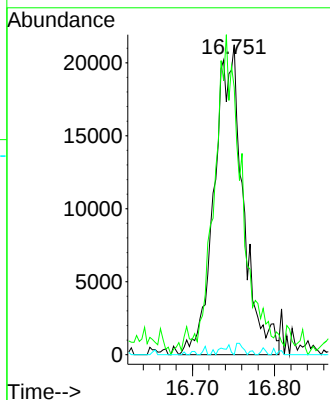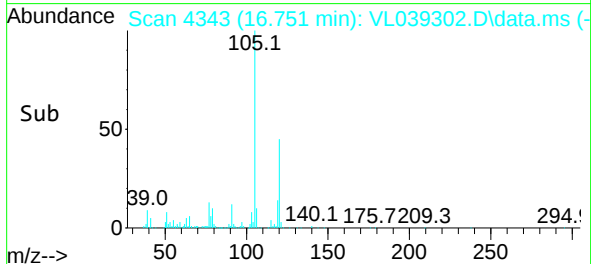


#68
1-Bromo-4-Fluorobenzene
Concen: 9.508 ppbv
RT: 14.397 min Scan# 3611
Delta R.T. -0.019 min
Lab File: VL039302.D
Acq: 15 Jun 2022 19:14

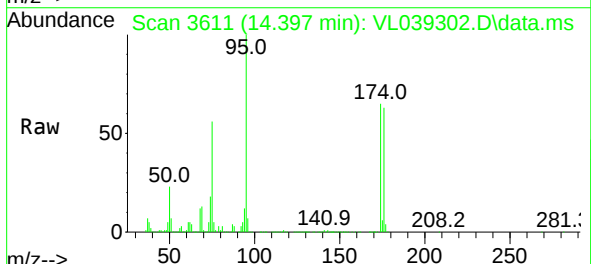

Tgt Ion: 95 Resp: 2335637
Ion Ratio Lower Upper
95 100
174 71.8 53.8 80.8
175 5.5 4.1 6.1

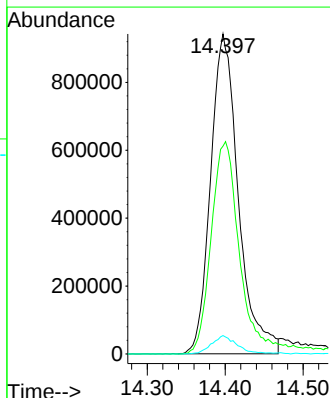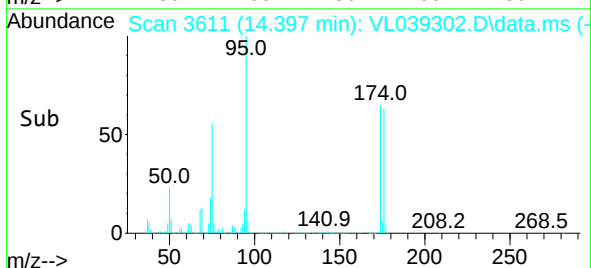

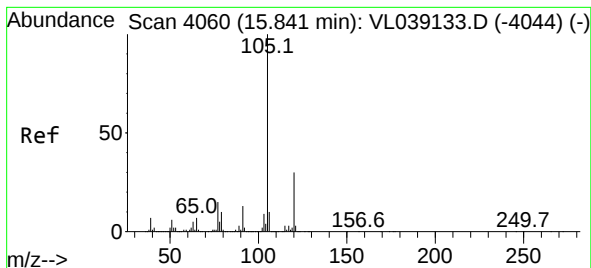

#72

4-Ethyltoluene

Concen: 0.342 ppbv

RT: 15.825 min Scan# 4060

Delta R.T. -0.016 min

Lab File: VL039302.D

Acq: 15 Jun 2022 19:14

Instrument :

MSVOA_L

ClientSampleId :

IA1





Tgt Ion:105	Resp: 13579
Ion Ratio	Lower Upper
105 100	
120 0.0	23.9 35.9
91 0.0	10.6 16.0
77 0.0	11.7 17.5

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022

Supervised By :Mahesh Dadoda 06/17/2022

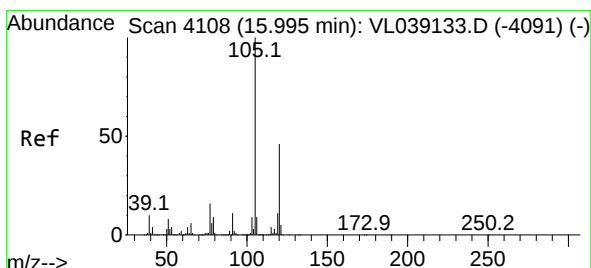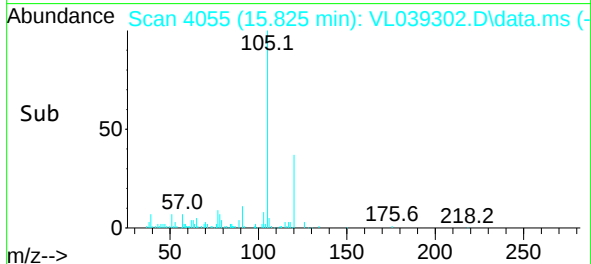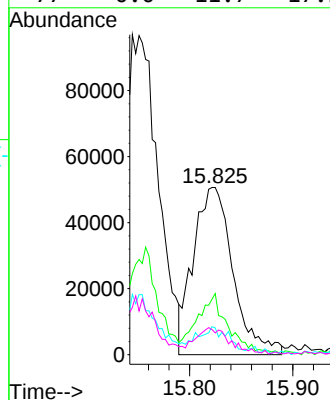

#73

1,3,5-Trimethylbenzene

Concen: 0.307 ppbv




RT: 15.979 min Scan# 4103


Delta R.T. -0.016 min

Lab File: VL039302.D

Acq: 15 Jun 2022 19:14

Tgt Ion:105	Resp: 110062
Ion Ratio	Lower Upper
105 100	
120 43.4	36.7 55.1

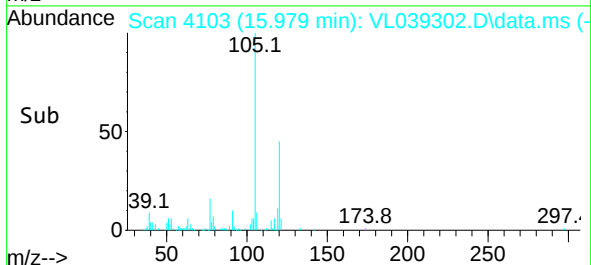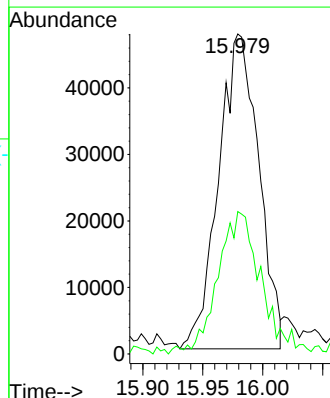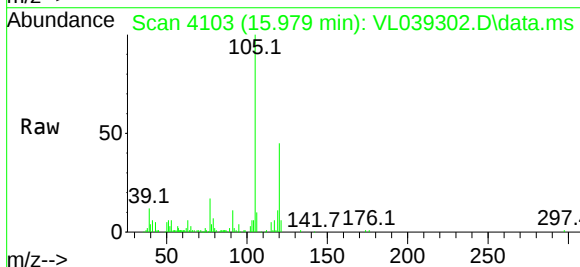

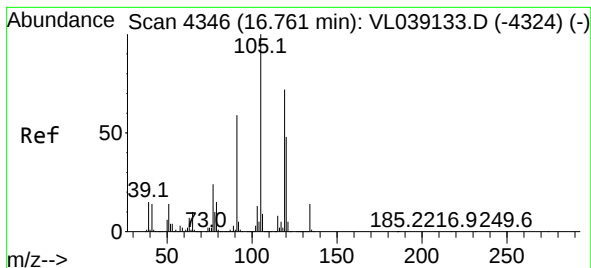

#74

1,2,4-Trimethylbenzene

Concen: 1.009 ppbv m

RT: 16.741 min Scan# 4346

Delta R.T. -0.019 min

Lab File: VL039302.D

Acq: 15 Jun 2022 19:14

Instrument :

MSVOA_L

ClientSampleId :

IA1





Tgt Ion:105 Resp: 403020

Ion	Ratio	Lower	Upper
105	100		
120	43.4	38.1	57.1
91	13.7	47.4	71.0
77	14.7	19.5	29.3

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/17/2022

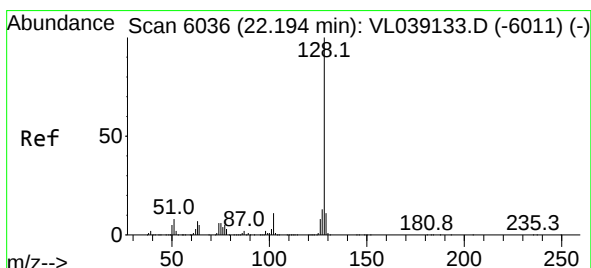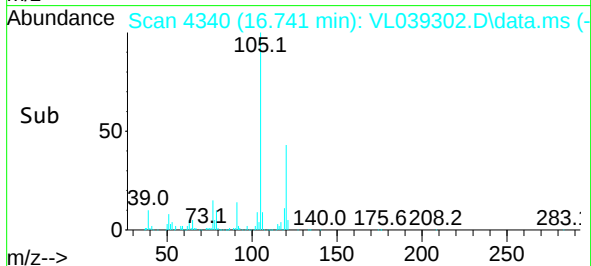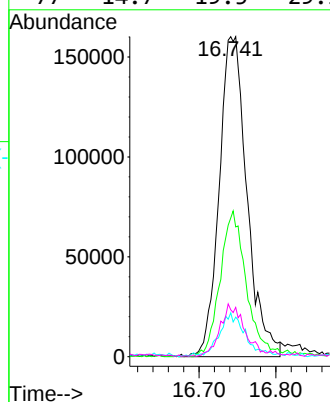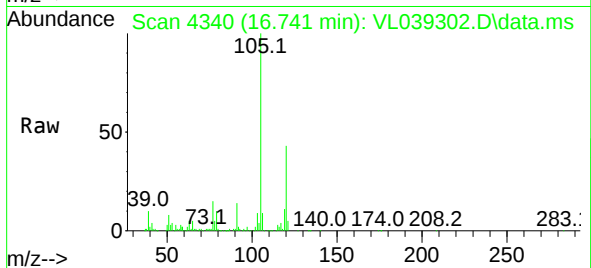

#79

Naphthalene

Concen: 0.133 ppbv m

RT: 22.175 min Scan# 6030

Delta R.T. -0.019 min

Lab File: VL039302.D

Acq: 15 Jun 2022 19:14

Tgt Ion:128 Resp: 40969

Ion	Ratio	Lower	Upper
128	100		
127	13.7	10.4	15.6
129	11.1	9.0	13.6

