


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061522\
 Data File : VL039298.D
 Acq On : 15 Jun 2022 15:34
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

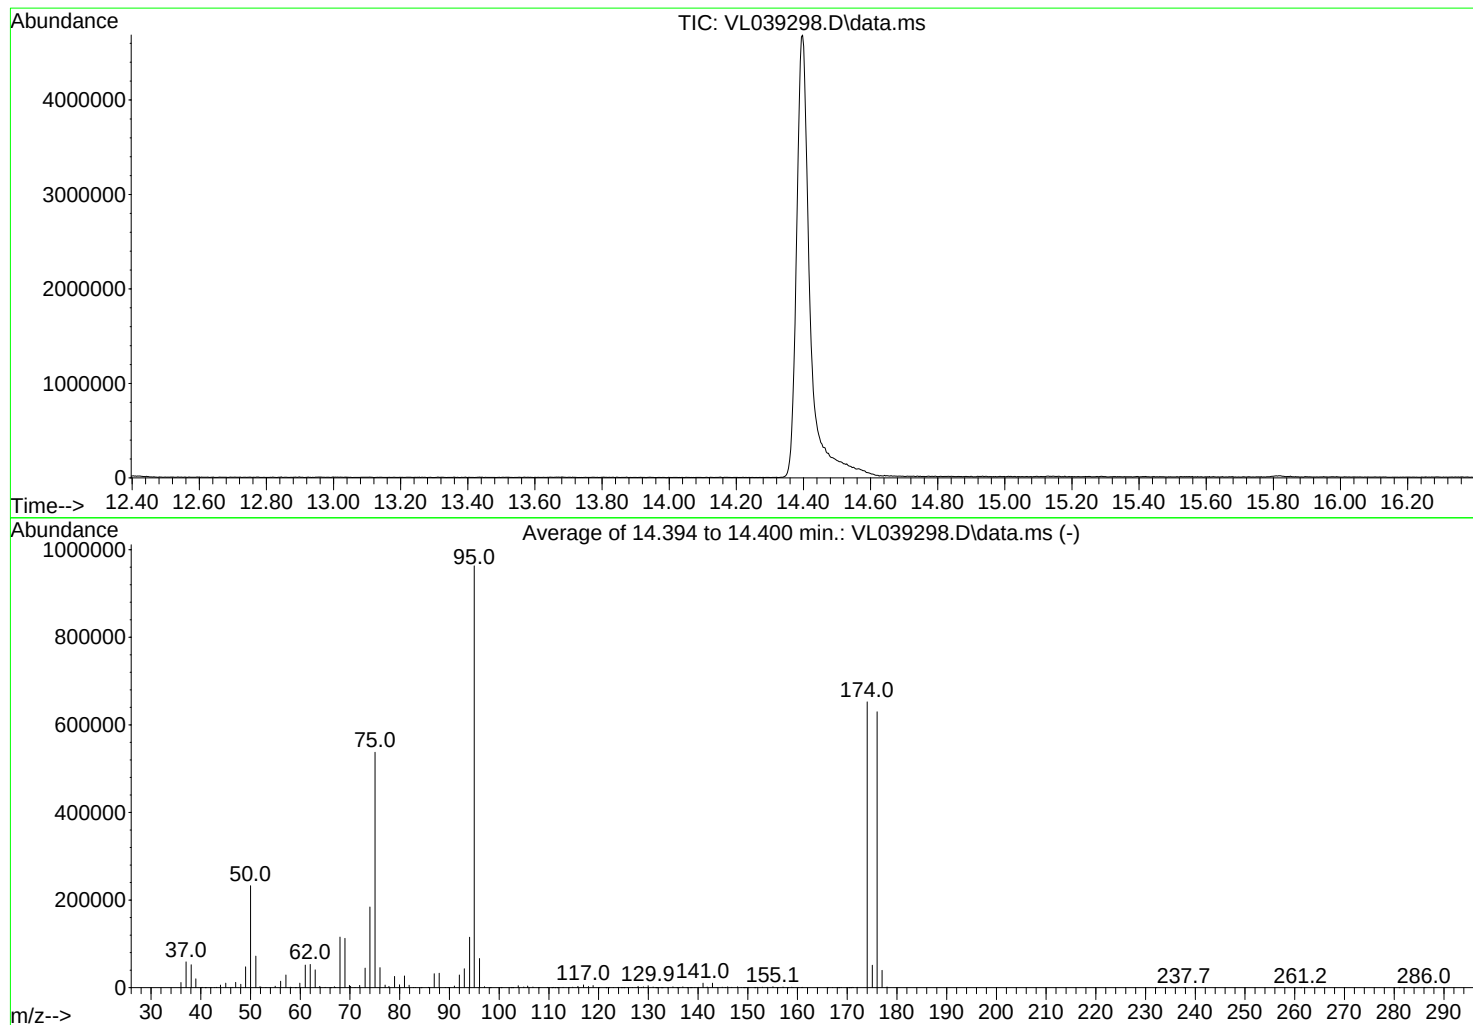

AutoFind: Scans 3610, 3611, 3612; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	232832	PASS
75	95	30	66	55.8	537387	PASS
95	95	100	100	100.0	963051	PASS
96	95	5	9	6.9	66685	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.8	652651	PASS
175	174	4	9	7.9	51264	PASS
176	174	93	101	96.5	629717	PASS
177	176	5	9	6.3	39627	PASS

Average of 14.394 to 14.400 min.: VL039298.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	11556	45.00	10427	53.95	233	63.90	249
37.05	58963	46.05	704	54.95	3276	64.10	94
38.05	52176	46.30	649	56.05	14747	65.00	89
39.00	20133	47.00	12057	57.10	28965	66.10	18
39.90	176	48.05	7823	58.00	962	66.85	2246
40.25	779	49.00	47493	58.20	294	67.10	541
40.90	55	50.00	232832	59.00	81	68.00	115616
41.90	108	51.05	71861	59.90	10131	69.00	112613
42.80	305	51.90	2345	61.00	51683	69.90	5228
43.15	689	52.10	998	62.00	53112	70.10	3125
43.95	5964	53.10	255	63.00	40744	71.00	436

Average of 14.394 to 14.400 min.: VL039298.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
71.95	5151	82.75	527	93.00	43037	104.95	1372
73.05	44512	83.10	510	94.05	115264	105.75	3753
74.00	184043	84.30	60	95.00	963051	106.80	1357
75.05	537387	85.80	602	96.05	66685	107.90	86
76.05	45579	86.00	420	97.05	2263	109.80	887
77.05	5732	86.95	31899	98.20	145	110.60	87
77.85	2885	87.95	33013	100.40	55	110.90	658
78.95	25771	89.15	241	102.40	140	111.20	177
79.95	6690	89.75	319	102.70	156	111.70	103
80.95	26688	91.00	3513	102.95	480	112.00	410
81.90	5507	92.00	28928	103.85	4241	112.85	830

Average of 14.394 to 14.400 min.: VL039298.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
113.90	133	124.60	102	131.80	154	139.35	341
114.80	1000	124.90	244	132.60	99	140.05	627
115.85	2835	125.10	100	132.80	51	141.00	10422
116.95	6342	125.85	337	133.85	206	141.85	1377
117.95	2749	126.80	441	134.95	1760	142.90	10395
118.90	4757	127.95	3034	135.80	164	143.85	570
120.00	141	128.60	362	136.20	338	144.85	982
121.50	81	129.00	1695	136.95	1863	145.50	375
122.00	61	129.95	4336	137.80	82	145.95	1705
122.95	266	130.95	1390	138.50	135	146.80	866
123.90	653	131.50	75	138.80	366	147.95	1872

Average of 14.394 to 14.400 min.: VL039298.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.70	512	156.05	258	168.30	82	177.00	39627
149.10	232	157.10	1522	168.80	472	178.00	1489
149.30	105	158.00	198	169.95	442	232.00	63
149.70	326	158.85	1009	170.35	6	237.70	64
150.05	595	159.10	403	170.70	58	261.20	76
151.40	86	160.25	361	171.00	692	281.00	134
151.90	592	160.80	319	171.20	292	286.00	176
152.95	1018	161.05	832	172.00	696		
153.90	733	166.00	56	174.00	652651		
155.05	2283	167.05	255	175.05	51264		
155.90	58	168.05	230	176.00	629717		