


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL061621\
 Data File : VL037163.D
 Acq On : 16 Jun 2021 8:31
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL061621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jun 16 14:06:32 2021
 Last Update : Wed Jun 16 14:06:32 2021

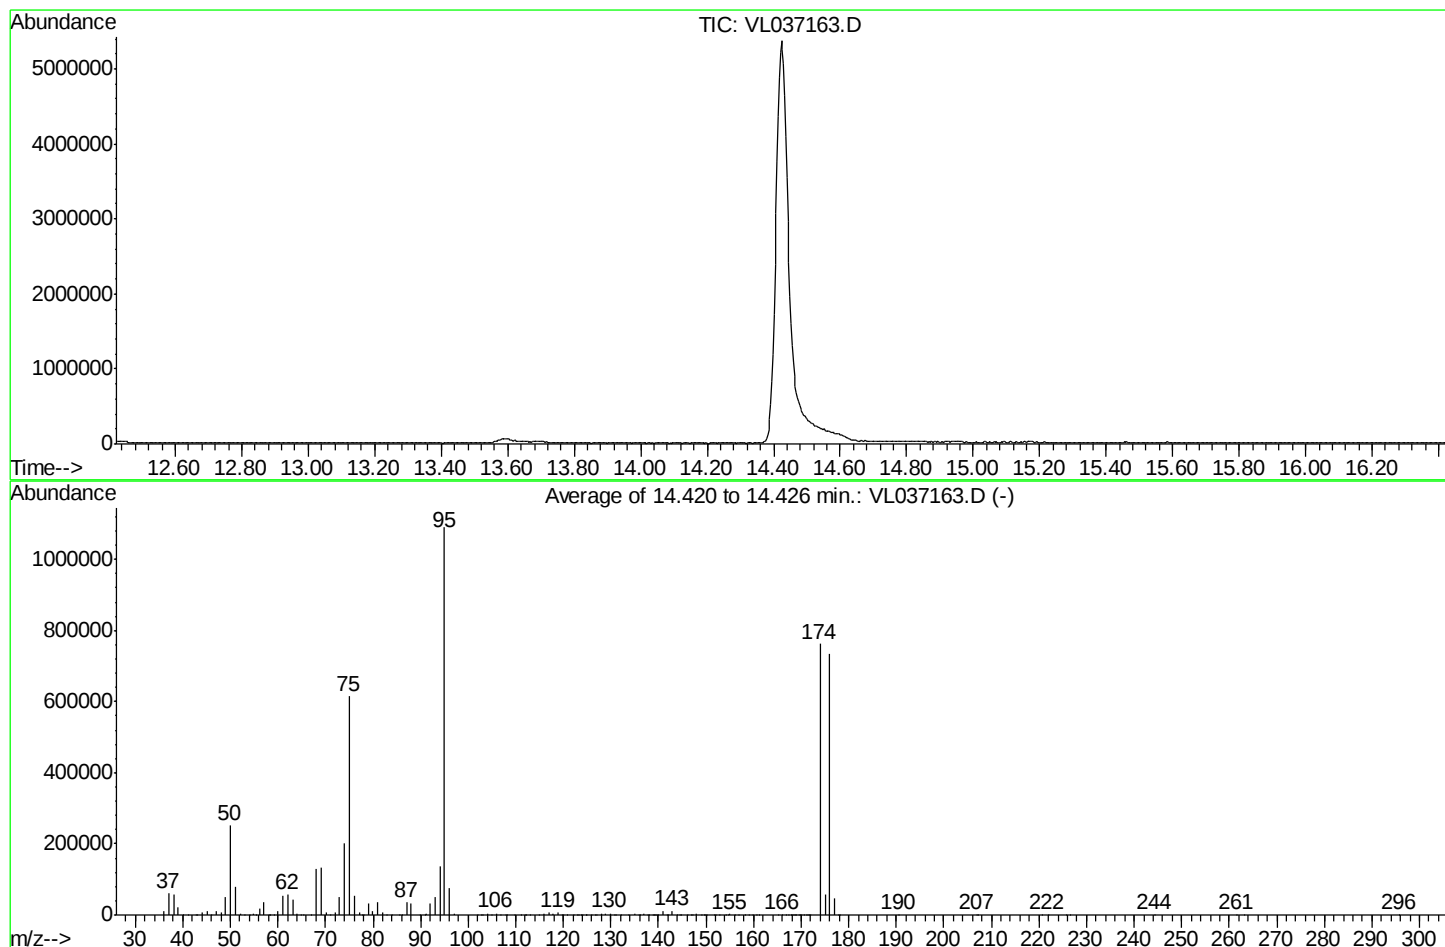

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	251136	PASS
75	95	30	66	56.5	615509	PASS
95	95	100	100	100.0	1090218	PASS
96	95	5	9	6.9	75541	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.9	762197	PASS
175	174	4	9	7.8	59152	PASS
176	174	93	101	96.6	735978	PASS
177	176	5	9	6.6	48594	PASS