
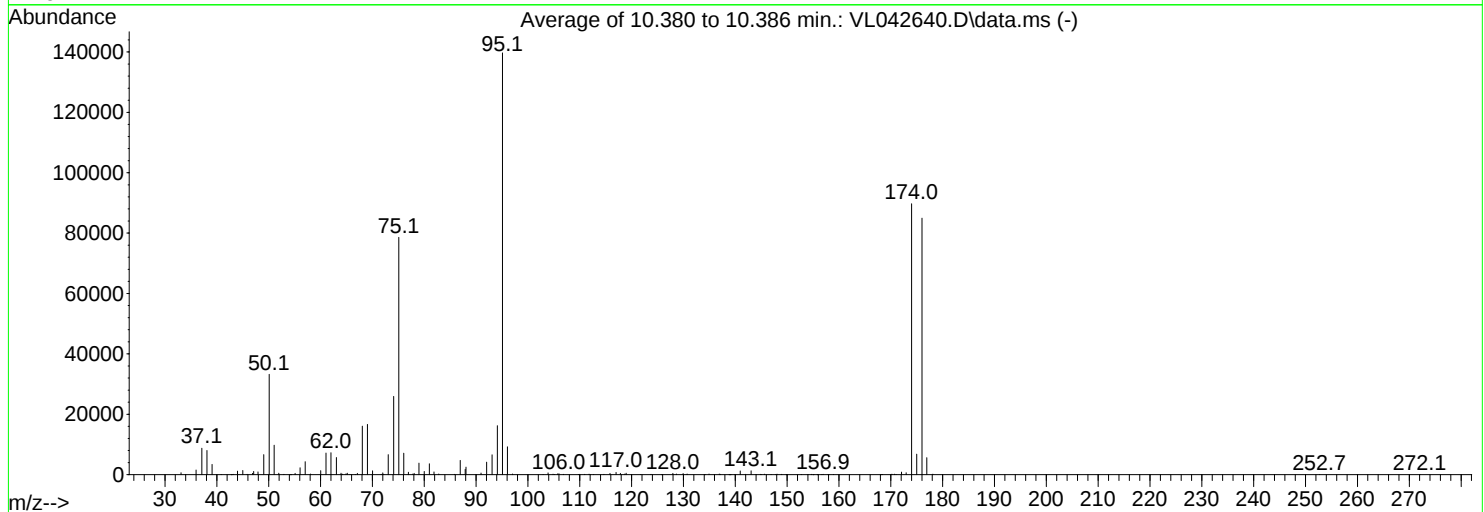


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061725\
Data File : VL042640.D
Acq On : 17 Jun 2025 08:40
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052925AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 30 02:01:56 2025

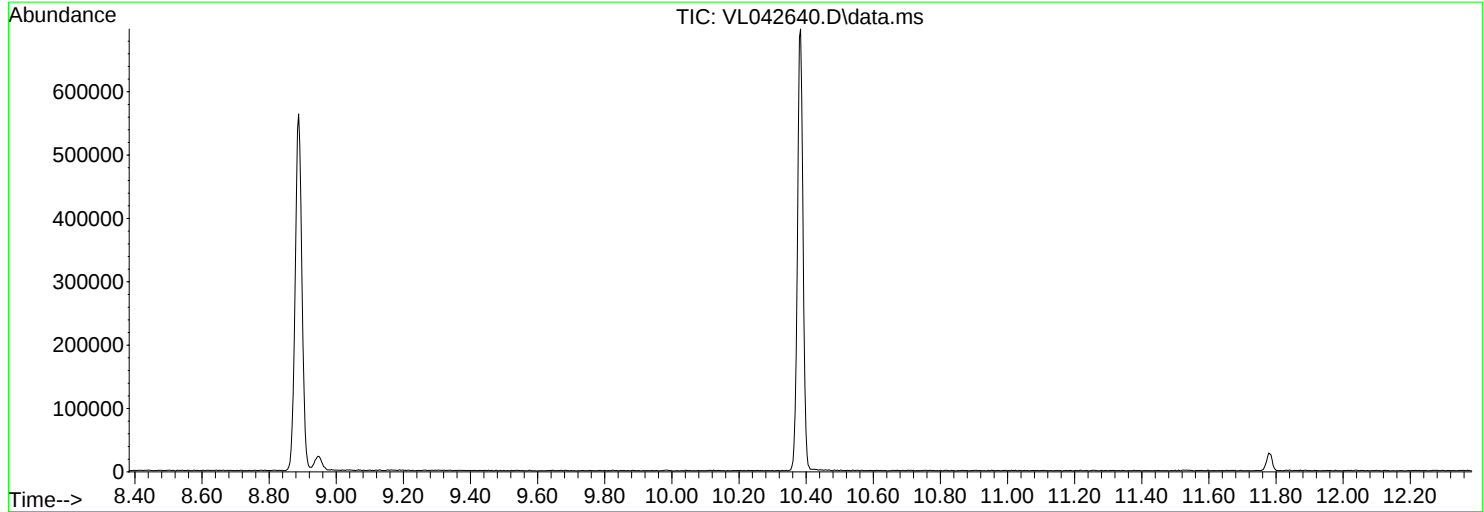

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	33224	PASS
75	95	30	66	56.2	78568	PASS
95	95	100	100	100.0	139704	PASS
96	95	5	9	6.6	9242	PASS
173	174	0.00	2	0.7	650	PASS
174	95	50	120	64.2	89696	PASS
175	174	4	9	7.6	6796	PASS
176	174	93	101	94.7	84944	PASS
177	176	5	9	6.6	5645	PASS

Average of 10.380 to 10.386 min.: VL042640.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	671	45.85	110	56.05	2304	65.70	41
34.00	46	46.90	445	57.05	4280	66.70	8
36.00	1515	47.10	1090	58.10	204	67.10	41
37.10	8753	47.95	899	60.05	1346	68.05	1608
38.10	8013	49.05	6600	61.05	7170	69.05	16670
39.10	3381	50.10	33224	62.00	7277	70.05	1258
40.85	67	51.05	9753	63.05	5651	71.70	109
42.80	24	51.95	470	63.95	505	72.00	607
43.15	99	52.95	101	64.20	144	72.20	89
44.00	1149	54.20	28	64.90	282	73.05	6652
45.00	1382	55.10	451	65.15	496	74.10	25933

Average of 10.380 to 10.386 min.: VL042640.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	78568	86.95	4709	102.95	58	112.00	41
76.05	7114	87.90	1733	103.90	577	112.70	44
76.95	820	88.05	2517	104.85	186	114.65	101
77.80	208	90.00	76	105.10	49	115.85	433
78.05	439	90.95	546	105.75	268	117.00	769
79.00	3798	92.05	4117	106.00	315	117.85	433
80.00	1080	93.10	6582	106.85	110	118.70	195
81.00	3585	94.10	16236	109.80	49	118.95	484
81.90	913	95.10	139704	110.00	98	121.75	66
82.80	212	96.05	9242	110.95	124	123.75	104
85.85	109	97.05	237	111.80	141	125.80	21

Average of 10.380 to 10.386 min.: VL042640.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.95	421	139.95	85	148.95	106	158.95	62
128.65	192	140.95	1245	149.80	18	168.00	26
129.95	387	141.95	133	150.00	86	168.40	72
130.70	229	143.05	1266	152.75	84	170.00	32
134.00	22	144.00	37	154.00	42	170.20	170
134.95	225	144.85	112	154.70	106	170.70	137
135.95	62	145.10	60	155.00	26	171.00	60
136.90	227	145.60	155	155.80	18	172.05	878
137.10	94	146.90	68	156.70	48	172.95	650
138.80	21	147.80	83	156.95	115	174.00	89696
139.00	21	148.05	148	157.90	23	175.00	6796

Average of 10.380 to 10.386 min.: VL042640.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	84944						
176.95	5645						
178.10	154						
244.00	33						
252.70	42						
272.05	40						