

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
 Data File : VL040501.D
 Acq On : 23 Jun 2023 10:13
 Operator : SY/MD
 Sample : 03397-04 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV-4DL

Quant Time: Jun 26 02:15:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Jun 06 06:22:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	5.185	49	1079178	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.645	114	2775408	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.458	117	2474865	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.767	95	2037323	9.974	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.700%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.722	85	24518	0.104	ppbv #	83
3) Chlorodifluoromethane	2.668	51	9927	0.056	ppbv	95
9) Propene	2.700	41	25870	0.475	ppbv	86
10) Heptane	7.571	43	106791	0.866	ppbv	99
11) Trichlorofluoromethane	3.555	101	188459	0.985	ppbv	98
13) Ethanol	3.237	45	206482	18.293	ppbv	99
15) Acetone	3.465	43	1014048	7.790	ppbv	97
16) 1,3-Butadiene	2.964	39	19932	0.315	ppbv #	25
19) Isopropyl Alcohol	3.578	45	8580	0.137	ppbv #	1
20) Methylene Chloride	3.931	84	70682	1.272	ppbv	95
21) Allyl Chloride	3.951	41	22102	0.301	ppbv #	54
23) Vinyl Acetate	4.600	43	31456	0.247	ppbv #	1
25) Ethyl Acetate	5.205	43	121641	0.516	ppbv #	78
26) Hexane	5.205	57	177154	1.586	ppbv #	43
27) Carbon Disulfide	4.118	76	76620	0.549	ppbv #	91
30) Cyclohexane	6.590	84	27912	0.310	ppbv #	90
34) 2-Butanone	4.787	43	70244	0.525	ppbv	92
36) Benzene	6.359	78	170788	0.774	ppbv	95
39) 1,2-Dichloropropane	6.645	63	679480	7.984	ppbv #	22
44) 2,2,4-Trimethylpentane	7.320	57	168020	0.466	ppbv #	80
51) 2-Hexanone	9.549	43	4378	0.035	ppbv #	31
52) Tetrachloroethene	10.610	164	60709	0.876	ppbv	91
53) Toluene	9.211	91	1432891	6.162	ppbv	99
58) Ethyl Benzene	12.082	91	656262	2.189	ppbv	95
59) m/p-Xylene	12.336	91	2197149	7.973	ppbv	95
60) o-Xylene	13.053	91	813861	3.114	ppbv	99
64) n-propylbenzene	14.899	120	10141	0.103	ppbv #	1
65) tert-Butylbenzene	16.098	119	69567	0.209	ppbv #	56
66) Benzyl Chloride	16.207	91	974	0.038	ppbv #	71
71) 2-Chlorotoluene	14.908	91	170034	0.589	ppbv #	45
72) 4-Ethyltoluene	15.185	105	215335	0.731	ppbv	98
73) 1,3,5-Trimethylbenzene	15.339	105	63066	0.242	ppbv	88
74) 1,2,4-Trimethylbenzene	16.101	105	680145	2.222	ppbv #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040501.D
Acq On : 23 Jun 2023 10:13
Operator : SY/MD
Sample : 03397-04 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-4DL

Quant Time: Jun 26 02:15:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Jun 06 06:22:12 2023
Response via : Initial Calibration




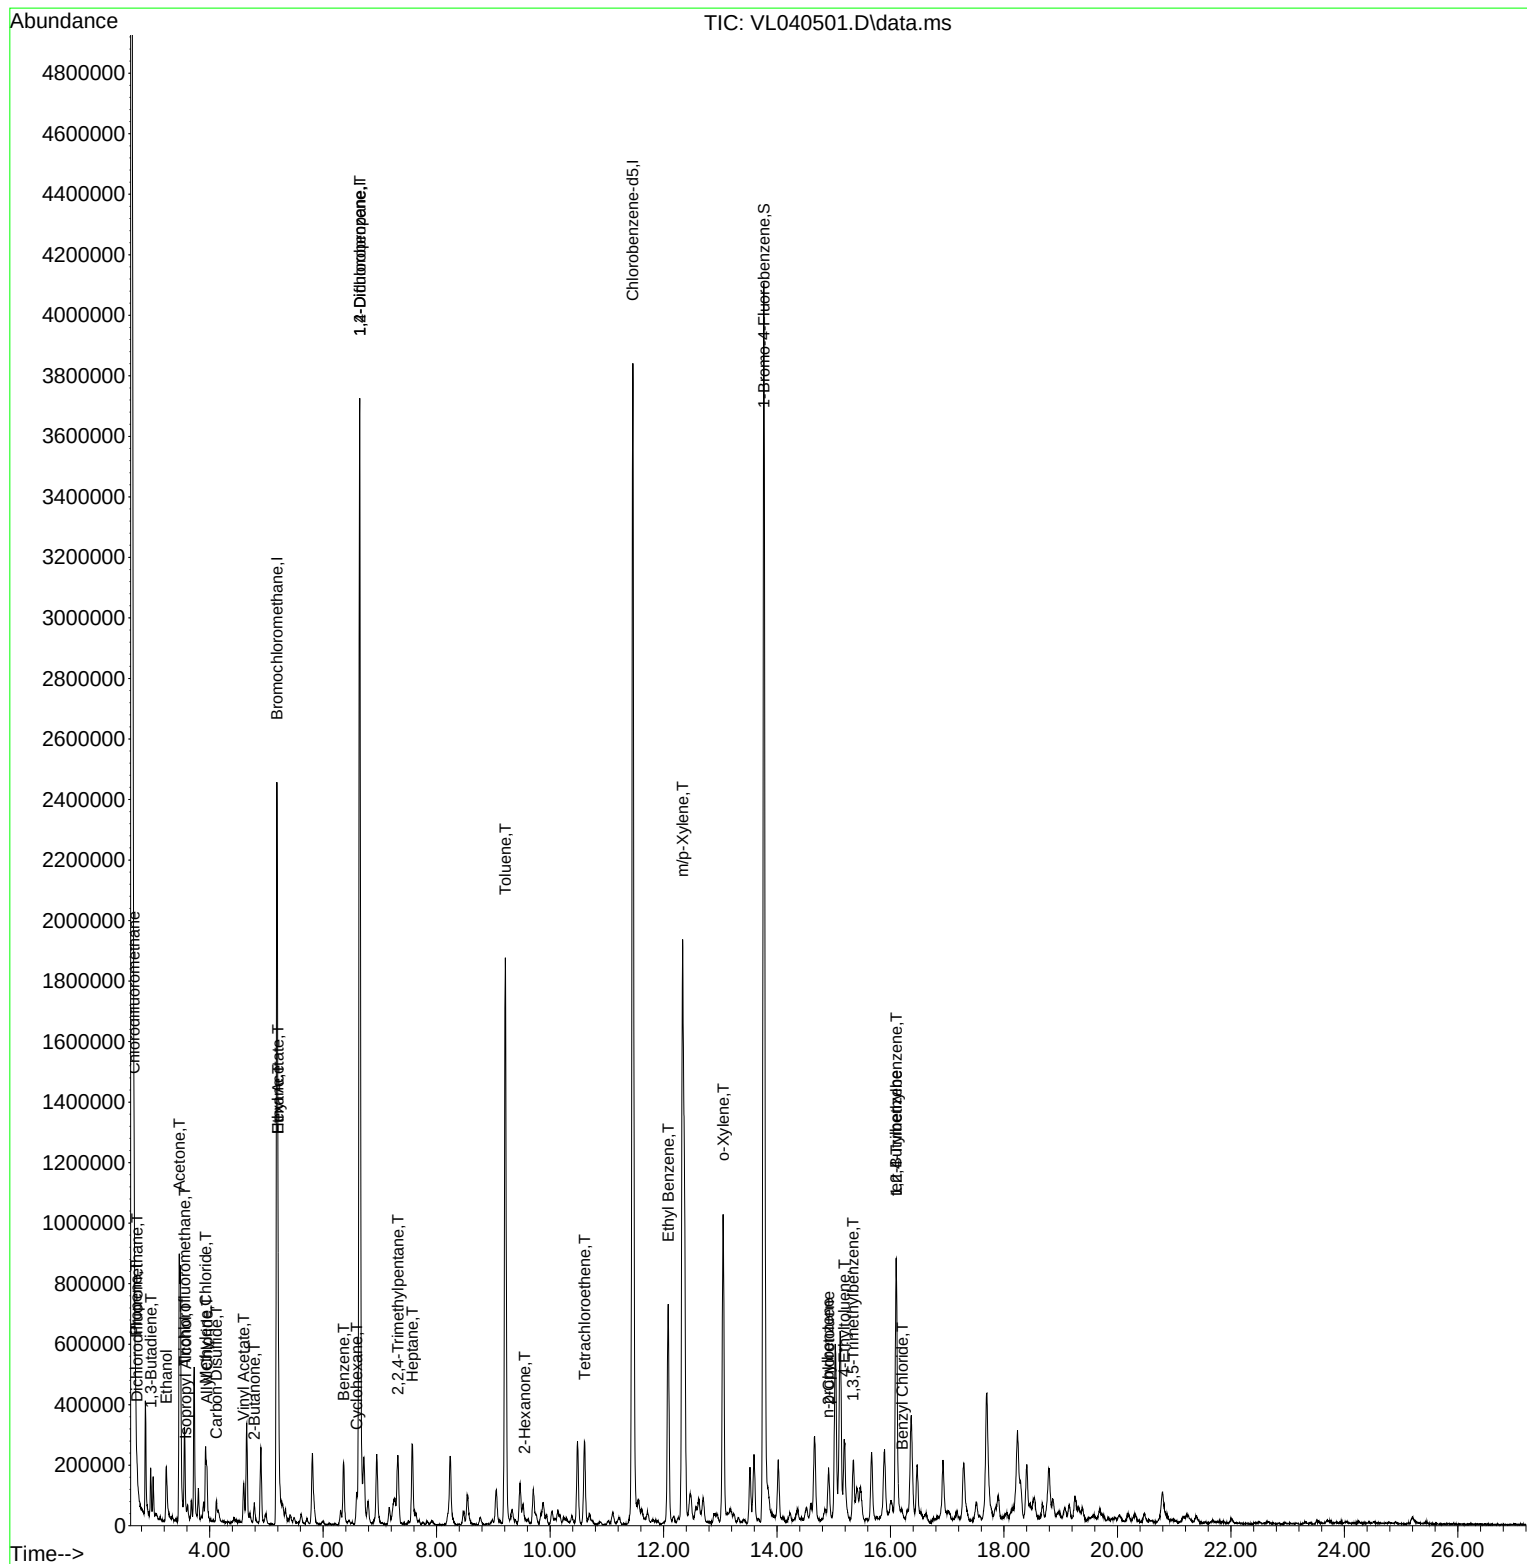




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.185 min Scan# 80
Delta R.T. -0.004 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 49 Resp: 1079178
Ion Ratio Lower Upper
49 100
128 48.7 24.7 74.1
130 62.8 31.4 94.2

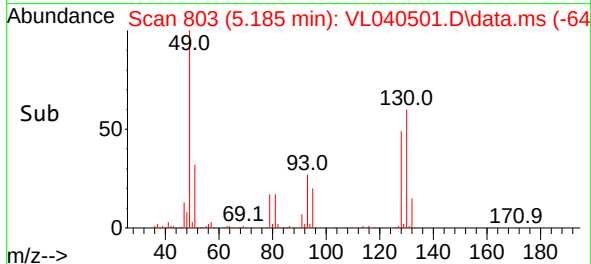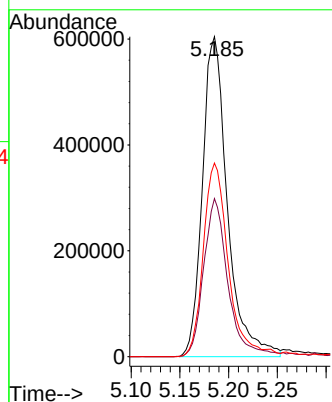

#2
Dichlorodifluoromethane
Concen: 0.104 ppbv
RT: 2.722 min Scan# 37
Delta R.T. 0.006 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 85 Resp: 24518
Ion Ratio Lower Upper
85 100
87 23.8 26.6 39.8


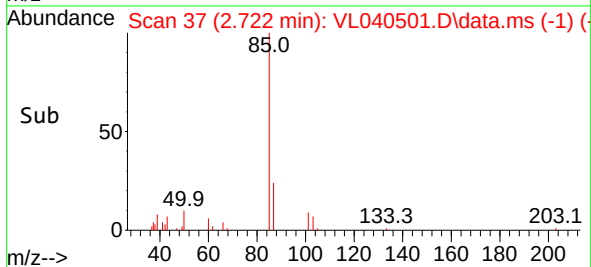
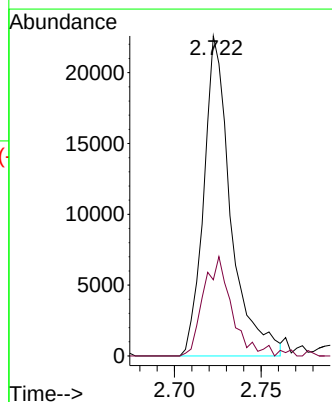
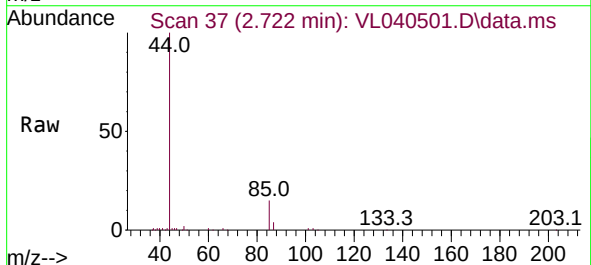


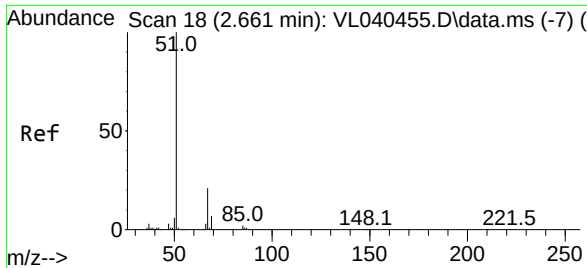

#3
Chlorodifluoromethane
Concen: 0.056 ppbv
RT: 2.668 min Scan# 20
Delta R.T. 0.006 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 51 Resp: 9927
Ion Ratio Lower Upper
51 100
67 18.1 16.3 24.5

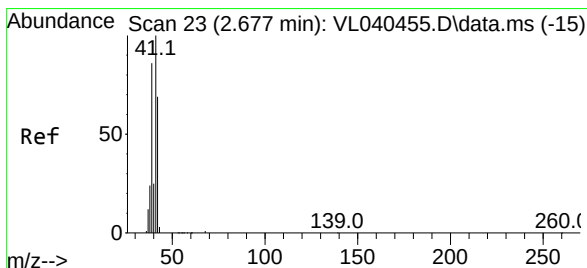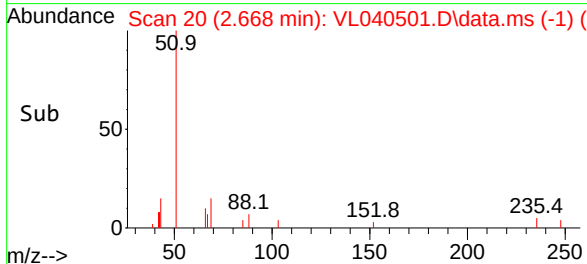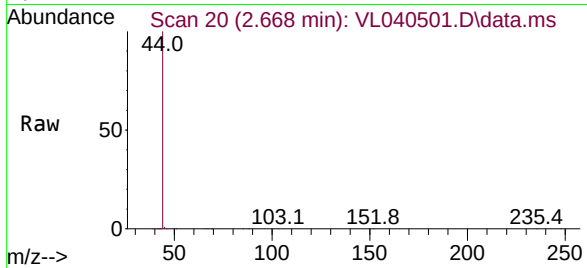

#9
Propene
Concen: 0.475 ppbv
RT: 2.700 min Scan# 30
Delta R.T. 0.022 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 41 Resp: 25870
Ion Ratio Lower Upper
41 100
42 59.1 56.2 84.2


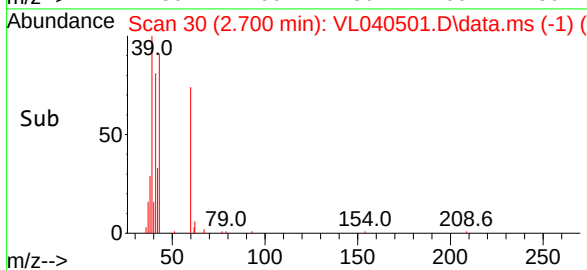

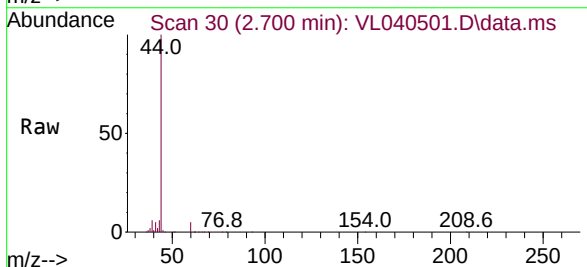




#10
Heptane
Concen: 0.866 ppbv
RT: 7.571 min Scan# 11
Delta R.T. -0.013 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 43 Resp: 106791
Ion Ratio Lower Upper
43 100
57 53.6 42.5 63.7

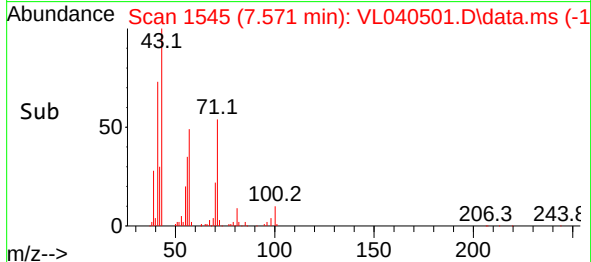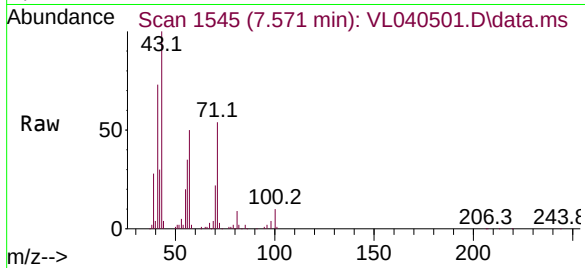

#11
Trichlorofluoromethane
Concen: 0.985 ppbv
RT: 3.555 min Scan# 296
Delta R.T. 0.003 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion:101 Resp: 188459
Ion Ratio Lower Upper
101 100
103 66.3 51.7 77.5


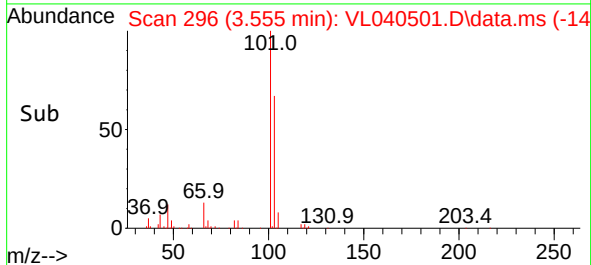

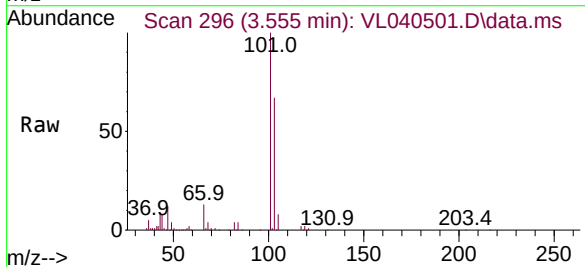




#13
 Ethanol
 Concen: 18.293 ppbv
 RT: 3.237 min Scan# 194
 Delta R.T. 0.010 min
 Lab File: VL040501.D
 Acq: 23 Jun 2023 10:13




Instrument :
 MSVOA_L
 ClientSampleId :
 SV-4DL


Tgt Ion: 45 Resp: 206482
 Ion Ratio Lower Upper
 45 100
 46 37.0 14.5 58.1

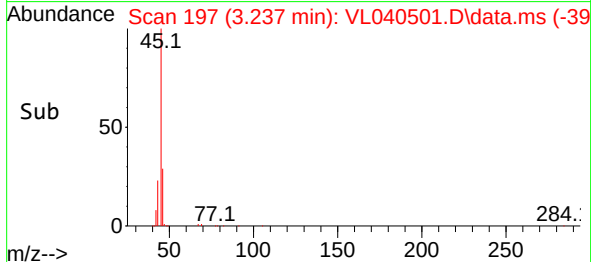

#15
 Acetone
 Concen: 7.790 ppbv
 RT: 3.465 min Scan# 268
 Delta R.T. 0.010 min
 Lab File: VL040501.D
 Acq: 23 Jun 2023 10:13

Tgt Ion: 43 Resp: 1014048
 Ion Ratio Lower Upper
 43 100
 58 25.4 21.6 32.4


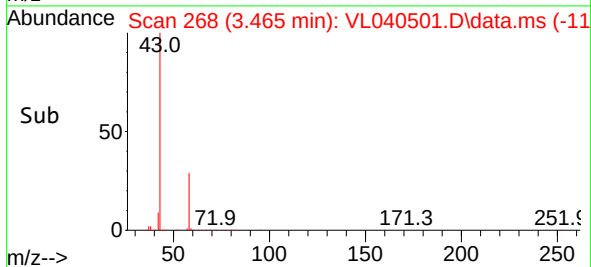

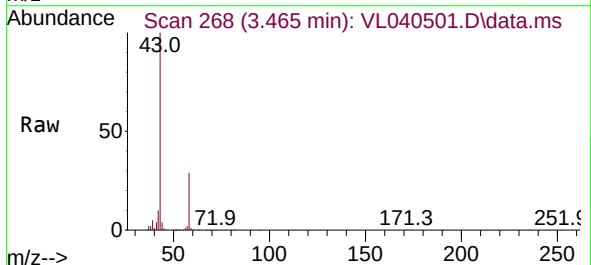




#16
1,3-Butadiene
Concen: 0.315 ppbv
RT: 2.964 min Scan# 114
Delta R.T. -0.006 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 39 Resp: 19932
Ion Ratio Lower Upper
39 100
54 15.5 66.9 100.3#

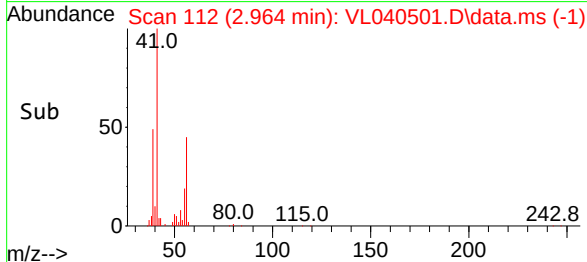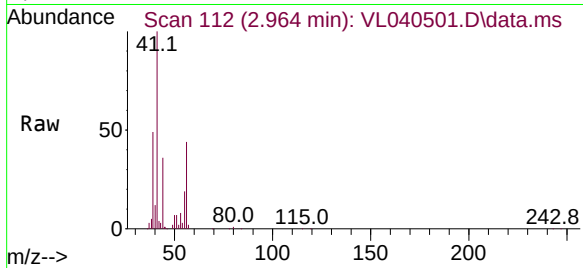

#19
Isopropyl Alcohol
Concen: 0.137 ppbv
RT: 3.578 min Scan# 303
Delta R.T. 0.016 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 45 Resp: 8580
Ion Ratio Lower Upper
45 100
58 3002.9 2.6 4.0#

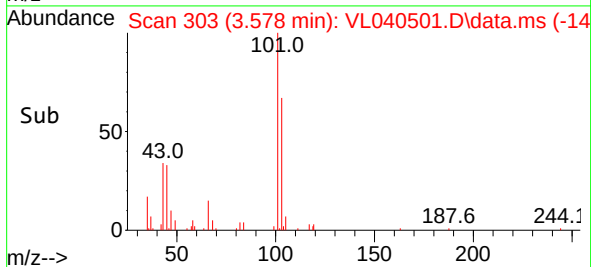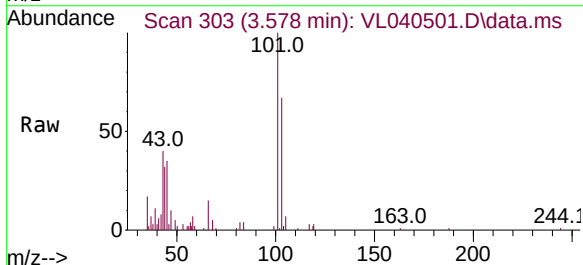







#20
Methylene Chloride
Concen: 1.272 ppbv
RT: 3.931 min Scan# 411
Delta R.T. 0.006 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Instrument :
MSVOA_L
ClientSampleId :
SV-4DL

Tgt Ion: 84 Resp: 70682




Ion	Ratio	Lower	Upper
84	100		
49	161.1	126.2	189.2
51	43.9	38.7	58.1
86	69.7	50.6	75.8

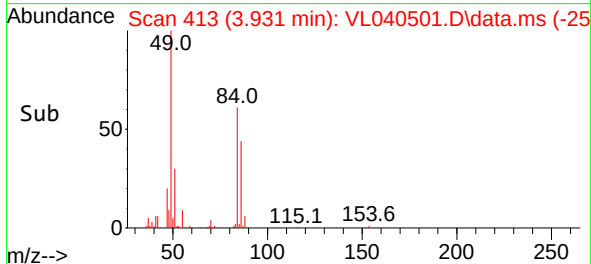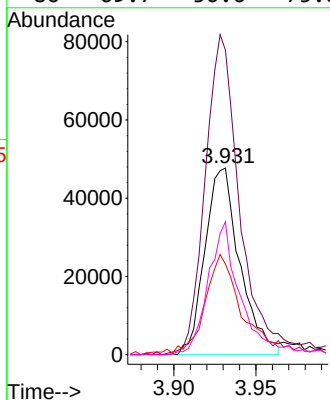


#21
Allyl Chloride
Concen: 0.301 ppbv
RT: 3.951 min Scan# 419
Delta R.T. -0.039 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 41 Resp: 22102

Ion	Ratio	Lower	Upper
41	100		
76	0.0	26.1	39.1#
39	115.7	63.9	95.9#


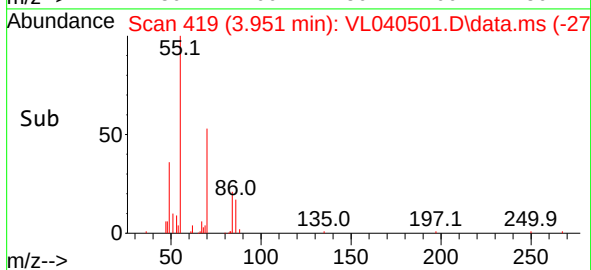
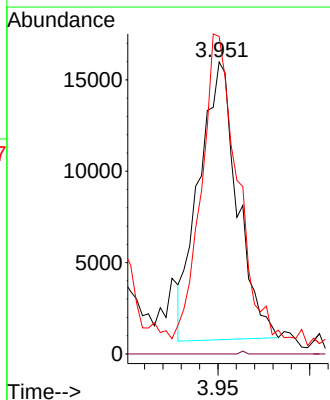
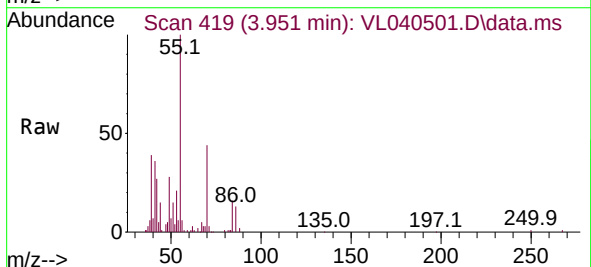




#23
 Vinyl Acetate
 Concen: 0.247 ppbv
 RT: 4.600 min Scan# 61
 Delta R.T. -0.019 min
 Lab File: VL040501.D
 Acq: 23 Jun 2023 10:13




Instrument :
 MSVOA_L
 ClientSampleId :
 SV-4DL


Tgt Ion: 43	Resp: 31456
Ion Ratio	Lower Upper
43 100	
86 2.7	5.8 8.6#
42 104.6	7.4 11.2#
44 0.9	5.3 7.9#

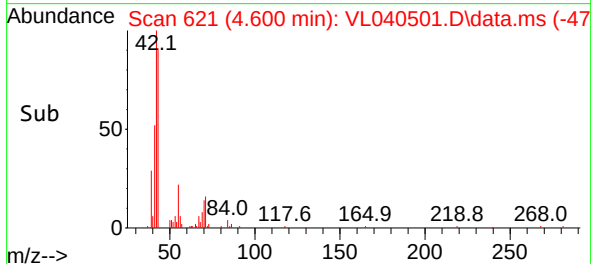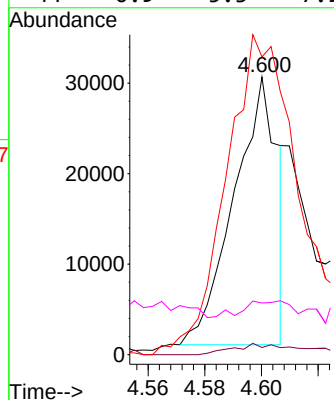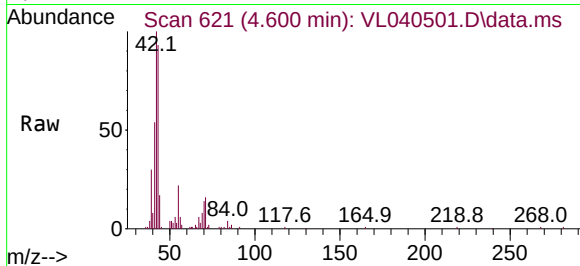

#25
 Ethyl Acetate
 Concen: 0.516 ppbv
 RT: 5.205 min Scan# 809
 Delta R.T. 0.003 min
 Lab File: VL040501.D
 Acq: 23 Jun 2023 10:13

Tgt	Ion: 43	Resp:	121641
Ion	Ratio	Lower	Upper
43	100		
45	1.3	8.0	12.0#
61	0.5	8.1	12.1#
70	2.5	5.8	8.6#

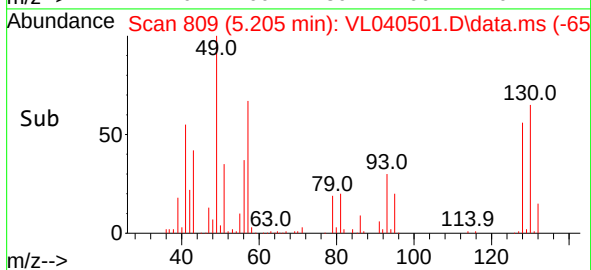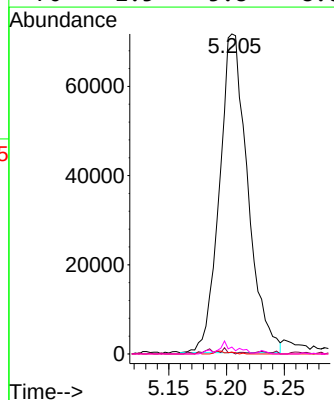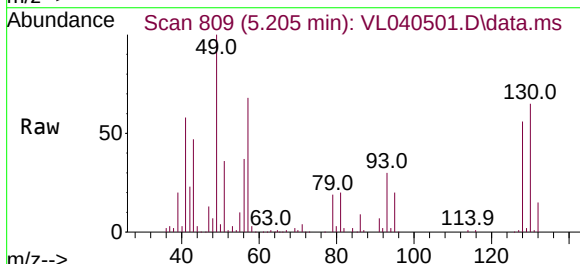







#26
Hexane
Concen: 1.586 ppbv
RT: 5.205 min Scan# 810
Delta R.T. -0.003 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Instrument :
MSVOA_L
ClientSampleId :
SV-4DL

Tgt Ion: 57 Resp: 177154




Ion	Ratio	Lower	Upper
57	100		
41	95.9	73.0	109.6
43	73.7	177.5	266.3#
56	57.2	43.6	65.4

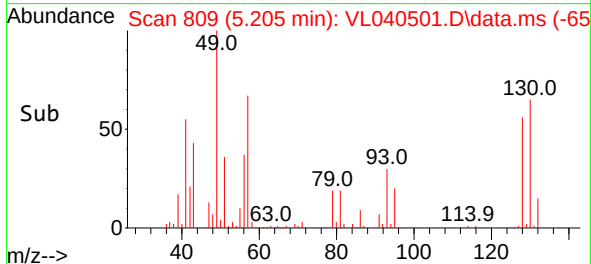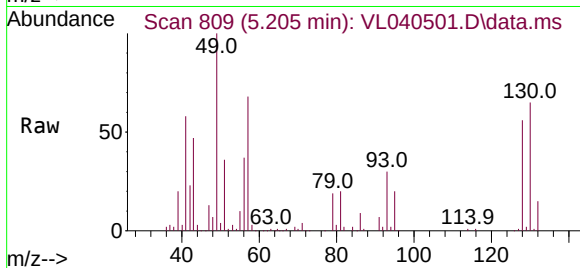


#27
Carbon Disulfide
Concen: 0.549 ppbv
RT: 4.118 min Scan# 471
Delta R.T. 0.003 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 76 Resp: 76620

Ion	Ratio	Lower	Upper
76	100		
44	23.7	14.6	22.0#
78	10.8	7.6	11.4


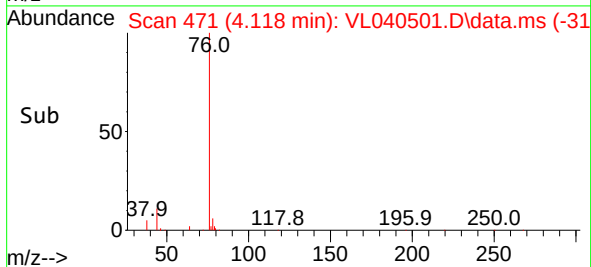

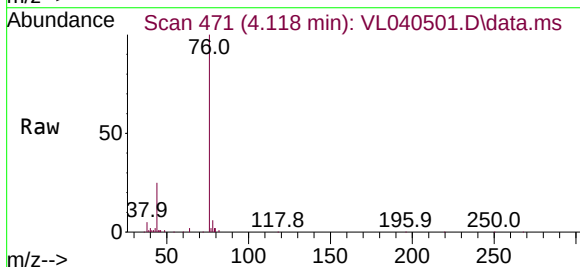




#30
Cyclohexane
Concen: 0.310 ppbv
RT: 6.590 min Scan# 11
Delta R.T. -0.010 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 84 Resp: 27912
Ion Ratio Lower Upper
84 100
56 135.2 106.0 159.0
41 102.7 66.8 100.2#

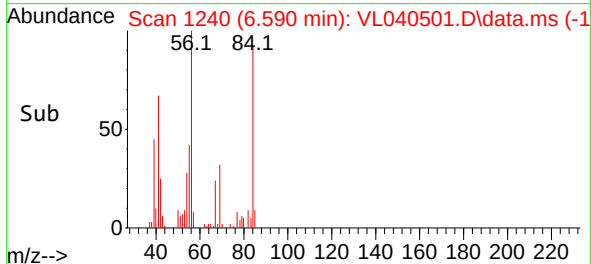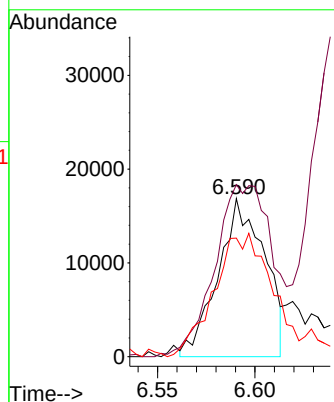

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.645 min Scan# 1257
Delta R.T. -0.010 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 114 Resp: 2775408
Ion Ratio Lower Upper
114 100
63 25.0 21.0 31.6
88 17.9 14.5 21.7


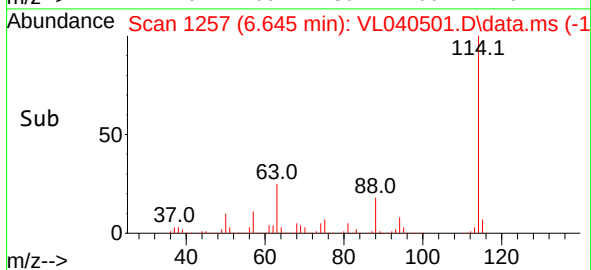
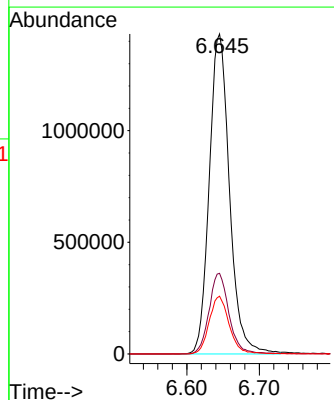
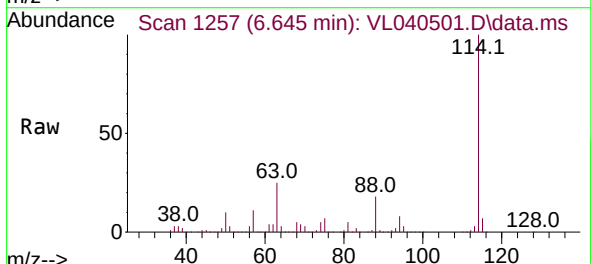




#34
2-Butanone
Concen: 0.525 ppbv
RT: 4.787 min Scan# 61
Delta R.T. 0.006 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_1
ClientSampleId :
SV-4DL


Tgt Ion: 43 Resp: 70244
Ion Ratio Lower Upper
43 100
72 26.4 18.1 27.1

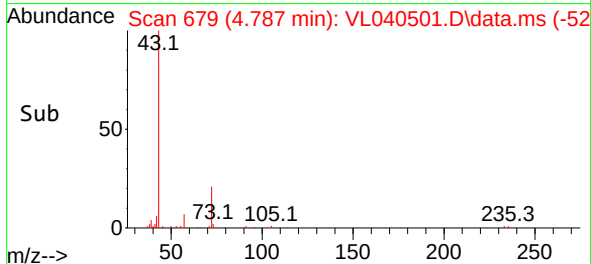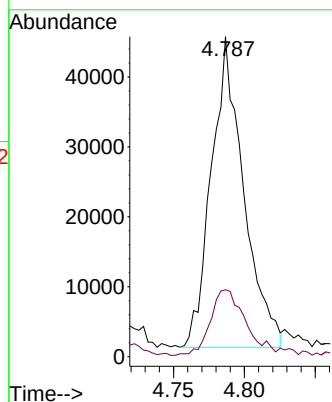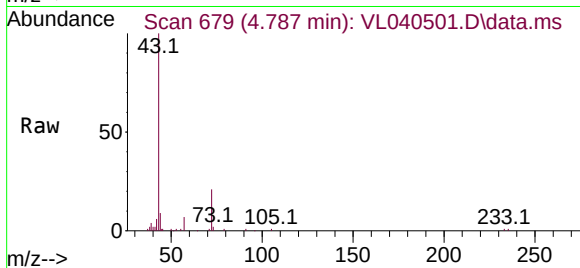

#36
Benzene
Concen: 0.774 ppbv
RT: 6.359 min Scan# 1168
Delta R.T. -0.013 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 78 Resp: 170788
Ion Ratio Lower Upper
78 100
77 20.2 18.5 27.7
50 18.4 16.1 24.1

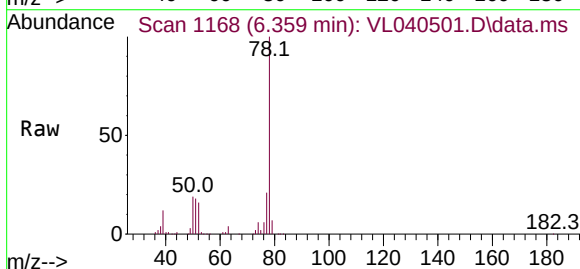

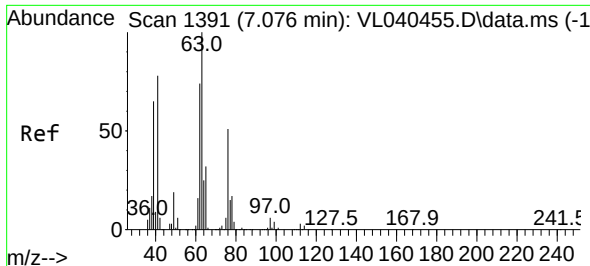

#39

1,2-Dichloropropane

Concen: 7.984 ppbv

RT: 6.645 min Scan# 11

Delta R.T. -0.431 min

Lab File: VL040501.D

Acq: 23 Jun 2023 10:13

Instrument :

MSVOA_L

ClientSampleId :

SV-4DL





Tgt Ion: 63 Resp: 679480

Ion Ratio Lower Upper

63 100

41 0.0 62.2 93.2#

62 17.4 59.0 88.4#

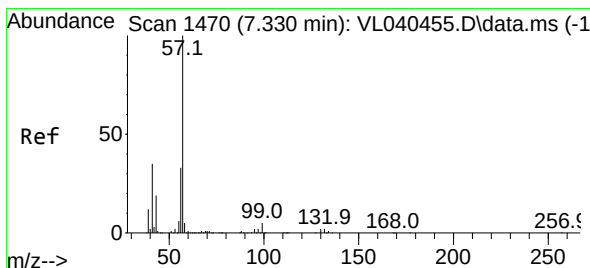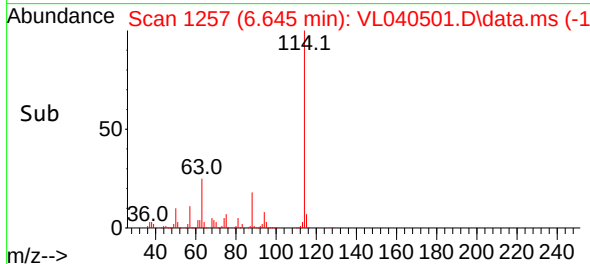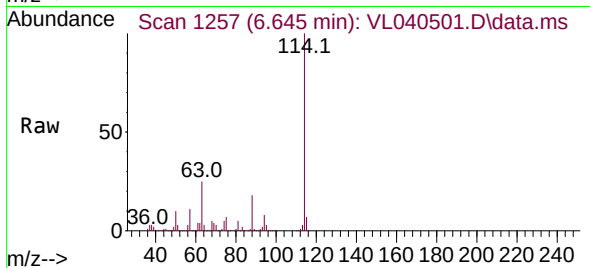

#44

2,2,4-Trimethylpentane

Concen: 0.466 ppbv

RT: 7.320 min Scan# 1467

Delta R.T. -0.010 min

Lab File: VL040501.D

Acq: 23 Jun 2023 10:13




Tgt Ion: 57 Resp: 168020


Ion Ratio Lower Upper

57 100

41 44.6 27.8 41.8#

56 45.0 25.3 37.9#


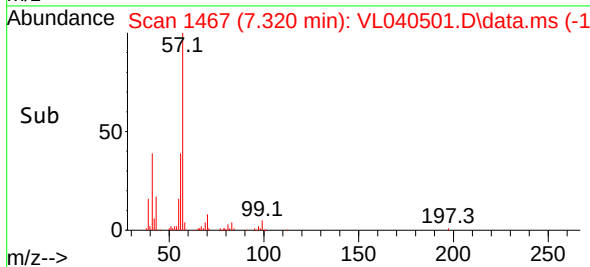

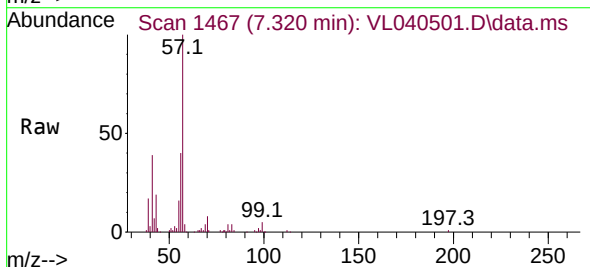




#51
2-Hexanone
Concen: 0.035 ppbv
RT: 9.549 min Scan# 2162
Delta R.T. -0.006 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 43 Resp: 4378
Ion Ratio Lower Upper
43 100
58 0.0 37.1 55.7#
98 0.0 0.5 0.7#

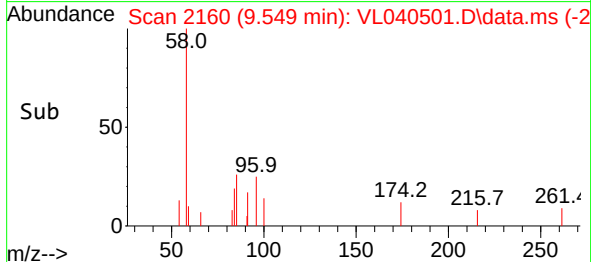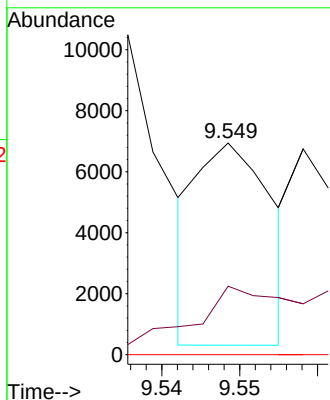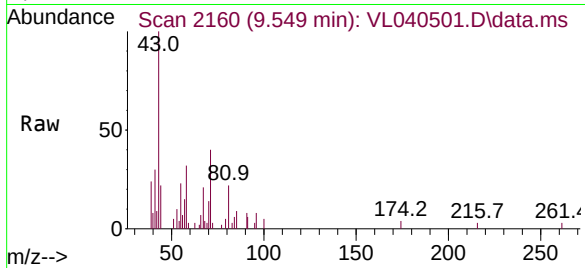

#52
Tetrachloroethene
Concen: 0.876 ppbv
RT: 10.610 min Scan# 2490
Delta R.T. -0.016 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 164 Resp: 60709
Ion Ratio Lower Upper
164 100
166 122.2 102.7 154.1
129 116.0 84.6 126.8
131 94.4 85.1 127.7


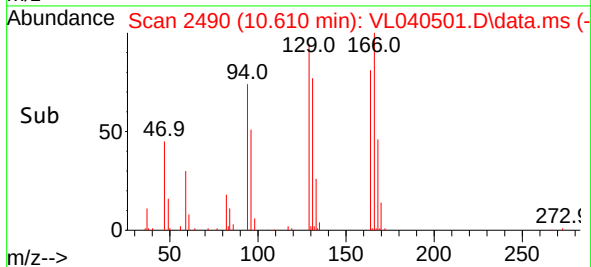
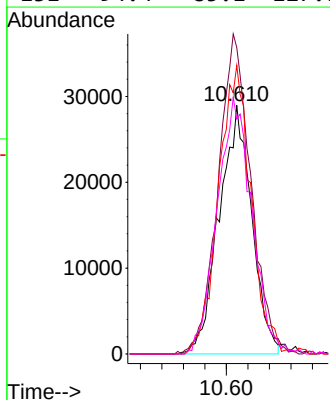
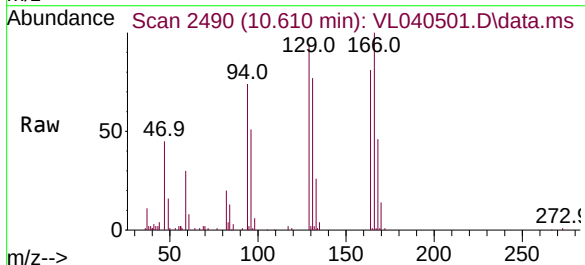




#53
Toluene
Concen: 6.162 ppbv
RT: 9.211 min Scan# 2060
Delta R.T. -0.016 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 91 Resp: 1432891
Ion Ratio Lower Upper
91 100
92 61.0 49.1 73.7

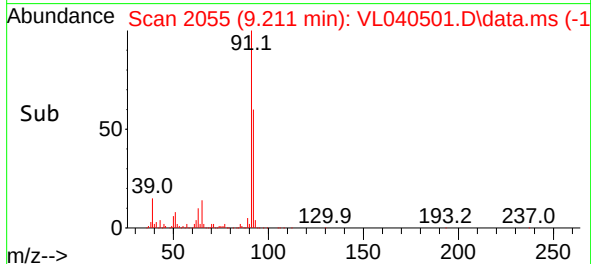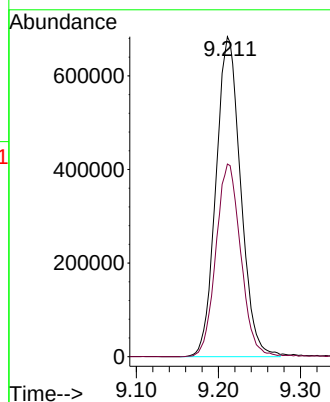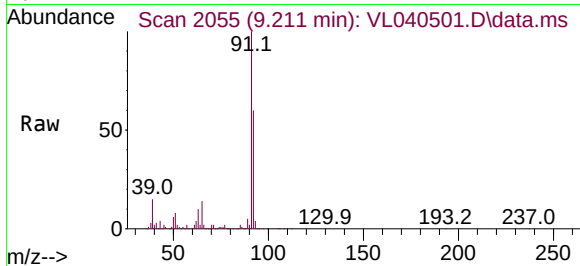

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.458 min Scan# 2754
Delta R.T. -0.019 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 117 Resp: 2474865
Ion Ratio Lower Upper
117 100
82 65.9 53.0 79.4
119 33.3 24.4 36.6


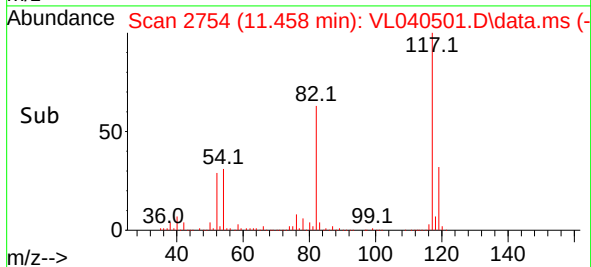
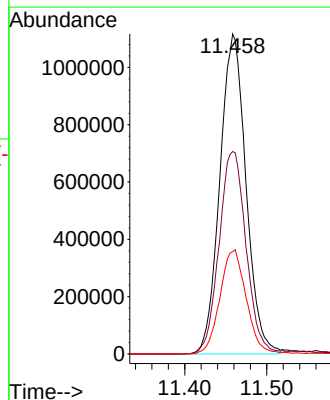
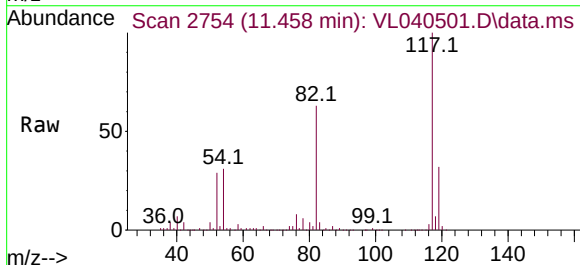




#58
Ethyl Benzene
Concen: 2.189 ppbv
RT: 12.082 min Scan# 2954
Delta R.T. -0.019 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 91 Resp: 656262
Ion Ratio Lower Upper
91 100
106 32.5 23.7 35.5

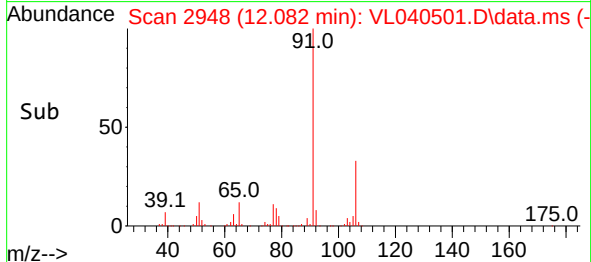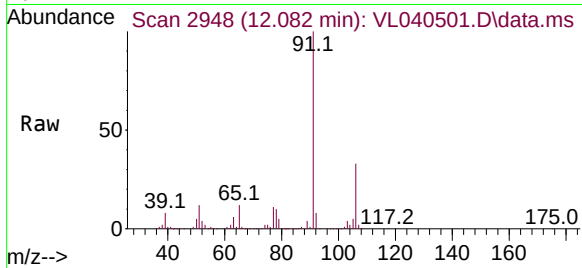

#59
m/p-Xylene
Concen: 7.973 ppbv
RT: 12.336 min Scan# 3027
Delta R.T. -0.045 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 91 Resp: 2197149
Ion Ratio Lower Upper
91 100
106 46.7 34.6 52.0


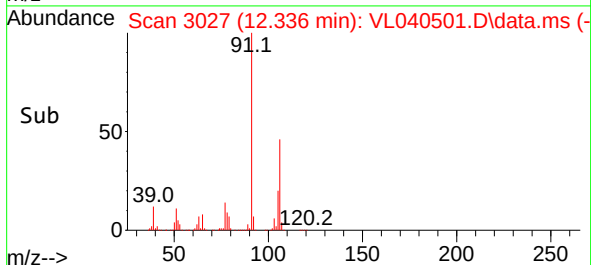
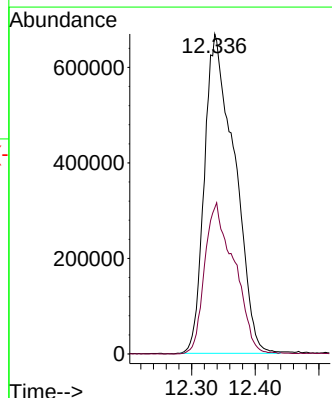
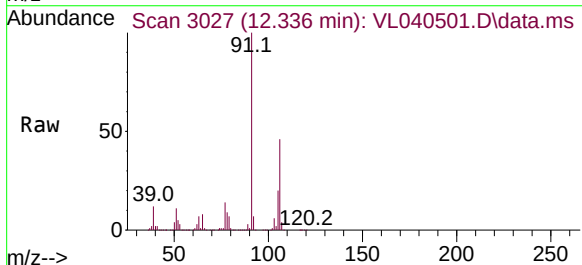


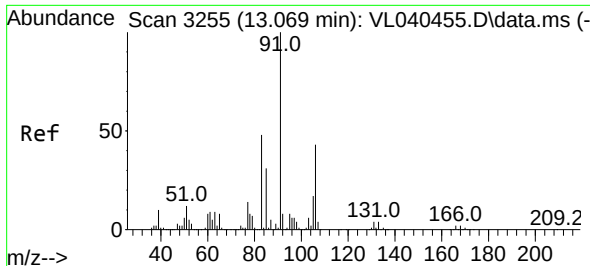

#60
o-Xylene
Concen: 3.114 ppbv
RT: 13.053 min Scan# 31
Delta R.T. -0.016 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 91 Resp: 813861
Ion Ratio Lower Upper
91 100
106 43.7 22.1 66.1

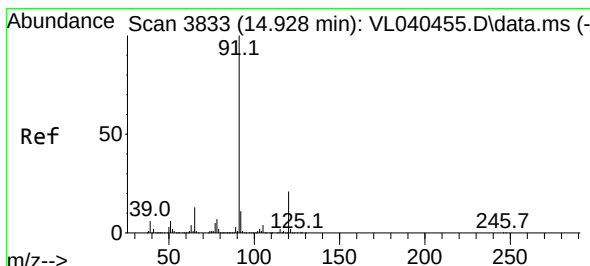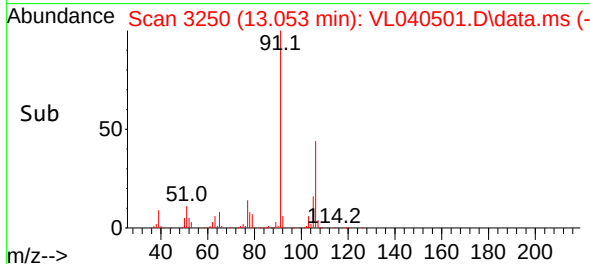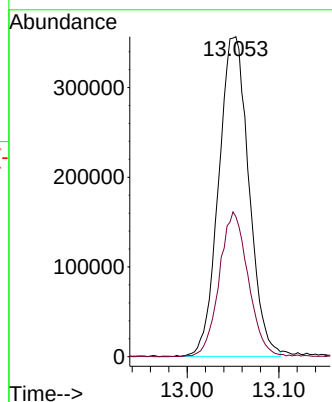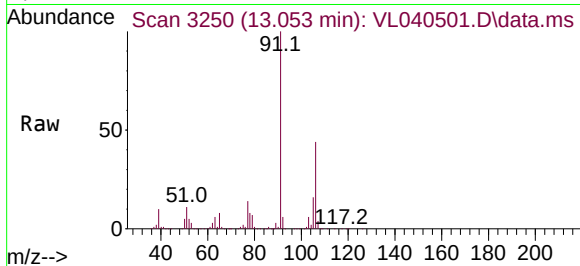

#64
n-propylbenzene
Concen: 0.103 ppbv
RT: 14.899 min Scan# 3824
Delta R.T. -0.029 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 120 Resp: 10141
Ion Ratio Lower Upper
120 100
91 0.0 388.5 582.7#


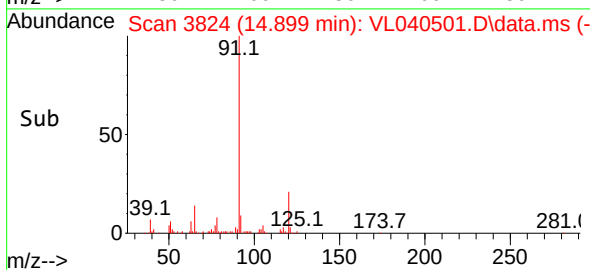
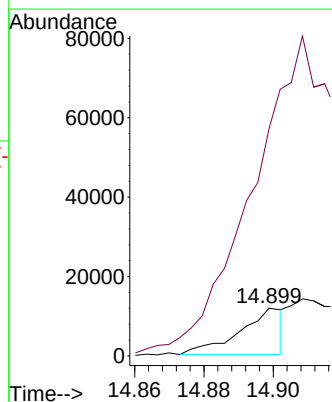
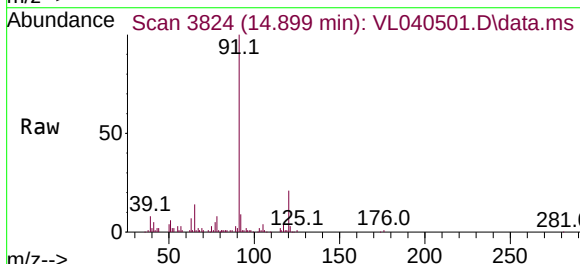




#65
tert-Butylbenzene
Concen: 0.209 ppbv
RT: 16.098 min Scan# 4199
Delta R.T. -0.006 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion:119 Resp: 69567
Ion Ratio Lower Upper
119 100
91 129.6 70.5 105.7#
134 1.4 15.6 23.4#

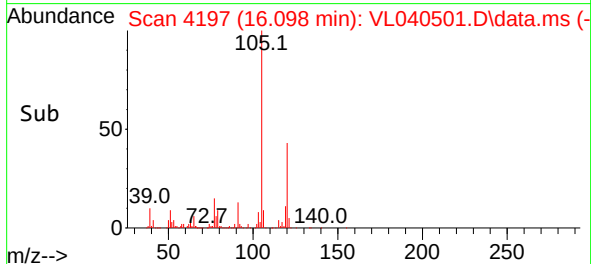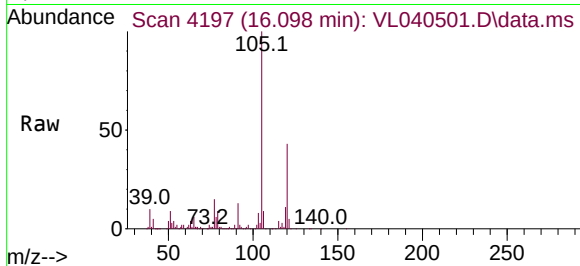

#66
Benzyl Chloride
Concen: 0.038 ppbv
RT: 16.207 min Scan# 4231
Delta R.T. -0.132 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 91 Resp: 974
Ion Ratio Lower Upper
91 100
126 0.0 13.2 19.8#
128 6.5 4.6 6.8


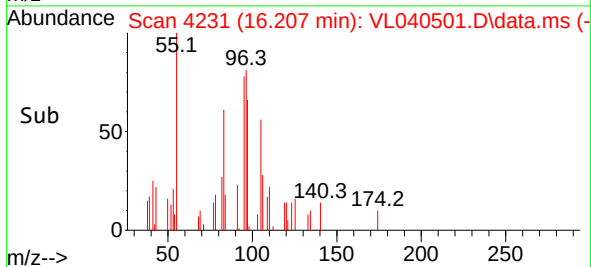

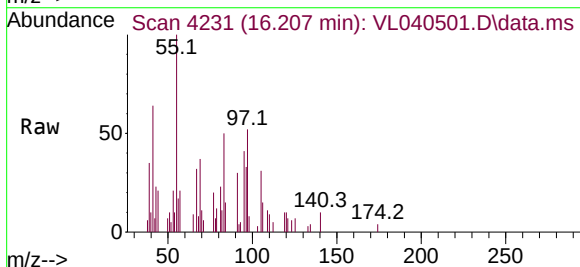




#68
1-Bromo-4-Fluorobenzene
Concen: 9.974 ppbv
RT: 13.767 min Scan# 3478
Delta R.T. -0.019 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_L
ClientSampleId :
SV-4DL


Tgt Ion: 95 Resp: 2037323
Ion Ratio Lower Upper
95 100
174 61.6 47.7 71.5
175 4.3 3.5 5.3

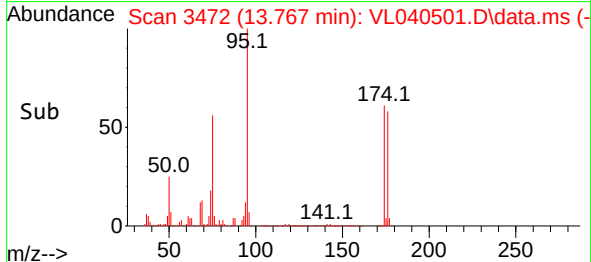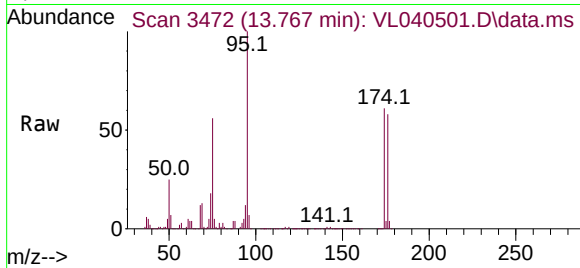

#71
2-Chlorotoluene
Concen: 0.589 ppbv
RT: 14.908 min Scan# 3827
Delta R.T. 0.096 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13

Tgt Ion: 91 Resp: 170034
Ion Ratio Lower Upper
91 100
126 0.0 12.0 48.2#


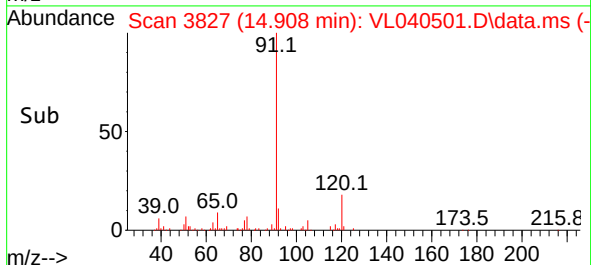
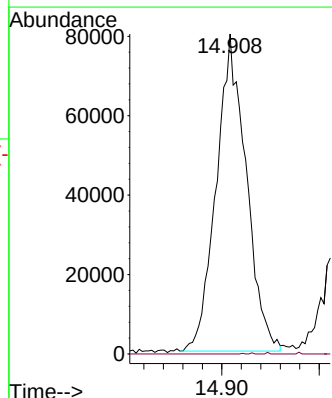
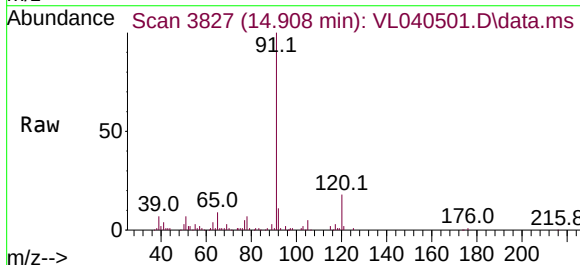


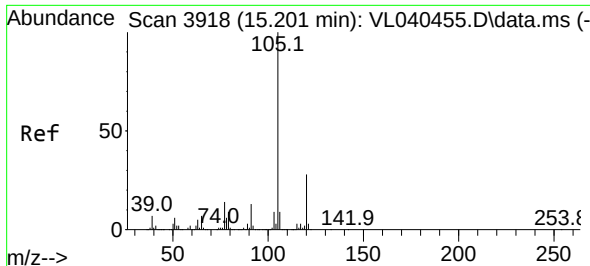

#72
4-Ethyltoluene
Concen: 0.731 ppbv
RT: 15.185 min Scan# 3913
Delta R.T. -0.016 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13




Instrument :
MSVOA_1
ClientSampleId :
SV-4DL


Tgt Ion:105 Resp: 215335
Ion Ratio Lower Upper
105 100
120 30.7 23.4 35.0
91 14.7 11.1 16.7
77 15.3 12.1 18.1

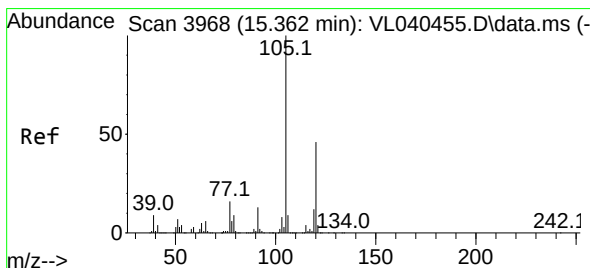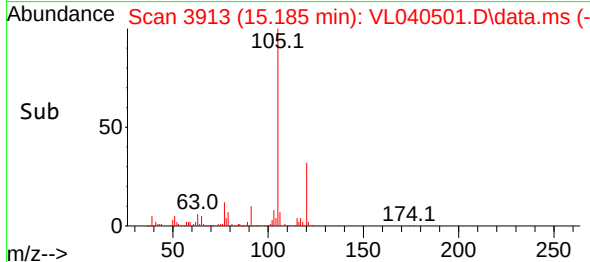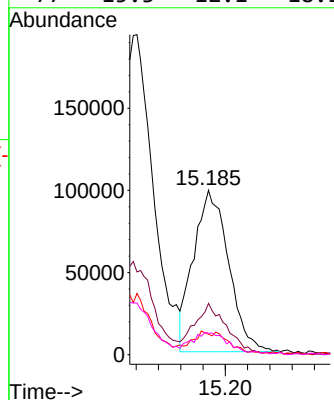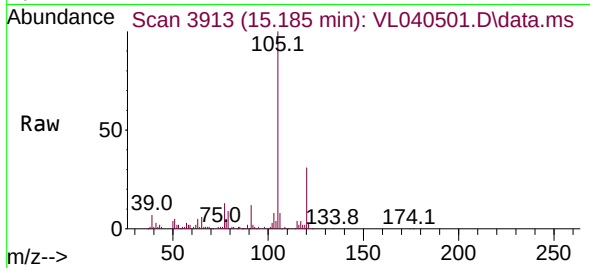

#73
1,3,5-Trimethylbenzene
Concen: 0.242 ppbv
RT: 15.339 min Scan# 3961
Delta R.T. -0.023 min
Lab File: VL040501.D
Acq: 23 Jun 2023 10:13


Tgt Ion:105 Resp: 63066
Ion Ratio Lower Upper
105 100
120 37.4 36.4 54.6

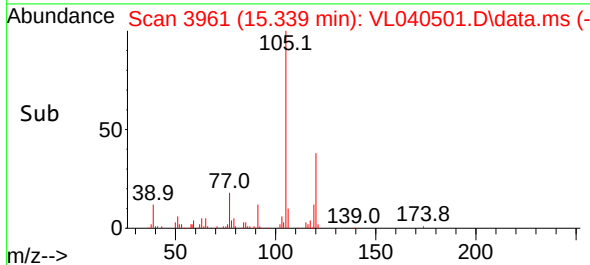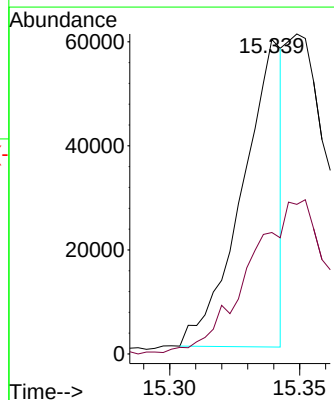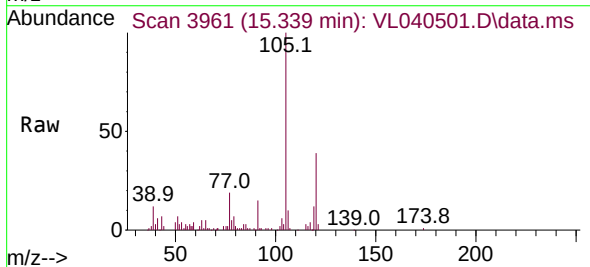

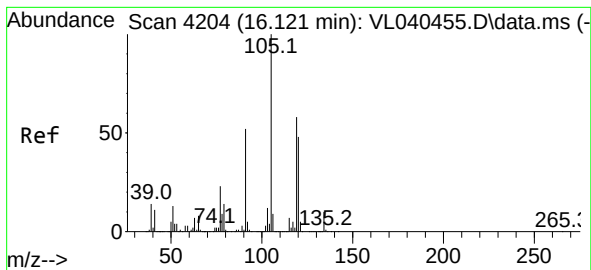

#74
 1,2,4-Trimethylbenzene
 Concen: 2.222 ppbv
 RT: 16.101 min Scan# 4198
 Delta R.T. -0.019 min
 Lab File: VL040501.D
 Acq: 23 Jun 2023 10:13

Instrument :
 MSVOA_L
 ClientSampleId :
 SV-4DL

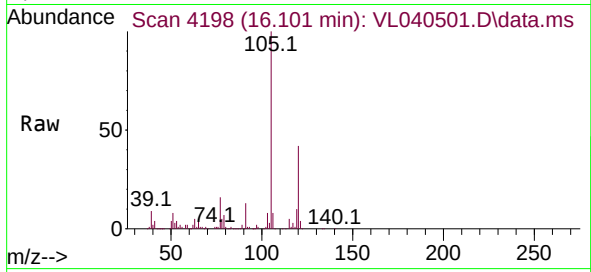

Tgt Ion:	105	Resp:	680145
Ion	Ratio	Lower	Upper
105	100		
120	42.2	38.4	57.6
91	12.7	41.3	61.9#
77	15.2	18.6	28.0#

