

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
 Data File : VL040487.D
 Acq On : 22 Jun 2023 16:03
 Operator : SY/MD
 Sample : 03300-03
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 AI-1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/26/2023
 Supervised By :Mahesh Dadoda 06/27/2023

Quant Time: Jun 23 01:31:05 2023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jun 06 06:22:12 2023

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.179	49	1001060	10.000	ppbv	-0.01
33) 1,4-Difluorobenzene	6.639	114	2507924	10.000	ppbv	-0.02
55) Chlorobenzene-d5	11.452	117	2169064	10.000	ppbv	-0.03

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 13.760 95 1687756 9.428 ppbv -0.03
 Spiked Amount 10.000 Range 65 - 135 Recovery = 94.300%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	2.729	85	90855m	0.417	ppbv	
3) Chlorodifluoromethane	2.668	51	59297m	0.362	ppbv	
4) Chloromethane	2.809	50	36158	0.570	ppbv #	85
9) Propene	2.693	41	586671	11.603	ppbv	87
10) Heptane	7.565	43	74104m	0.648	ppbv	
11) Trichlorofluoromethane	3.555	101	42726	0.241	ppbv	100
12) 1,1,2-Trichlorotrifluo...	4.057	101	8300	0.067	ppbv	91
13) Ethanol	3.227	45	891717	85.167	ppbv	99
15) Acetone	3.462	43	517808	4.289	ppbv #	85
19) Isopropyl Alcohol	3.568	45	206662	3.551	ppbv #	97
20) Methylene Chloride	3.925	84	130147	2.526	ppbv	98
26) Hexane	5.205	57	157829	1.523	ppbv #	54
29) Chloroform	5.266	83	12440	0.070	ppbv	87
30) Cyclohexane	6.590	84	32755m	0.392	ppbv	
34) 2-Butanone	4.780	43	68586	0.567	ppbv	96
35) Carbon Tetrachloride	6.475	117	10984m	0.064	ppbv	
36) Benzene	6.356	78	718573	3.602	ppbv	95
44) 2,2,4-Trimethylpentane	7.311	57	889064	2.727	ppbv	96
52) Tetrachloroethene	10.600	164	4859m	0.078	ppbv	
53) Toluene	9.204	91	1428836	6.800	ppbv	100
58) Ethyl Benzene	12.076	91	395499	1.505	ppbv	94
59) m/p-Xylene	12.326	91	1141687	4.727	ppbv	97
60) o-Xylene	13.040	91	410884	1.794	ppbv	99
61) Styrene	12.886	104	32609	0.331	ppbv	92
62) Isopropylbenzene	14.018	105	54212	0.159	ppbv	99
72) 4-Ethyltoluene	15.178	105	75530	0.293	ppbv #	94
73) 1,3,5-Trimethylbenzene	15.339	105	59993m	0.263	ppbv	
74) 1,2,4-Trimethylbenzene	16.095	105	248781	0.927	ppbv #	72
76) 1,4-Dichlorobenzene	16.458	146	20926m	0.143	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040487.D
Acq On : 22 Jun 2023 16:03
Operator : SY/MD
Sample : 03300-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
AI-1

Quant Time: Jun 23 01:31:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jun 06 06:22:12 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 06/26/2023
Supervised By : Mahesh Dadoda 06/27/2023

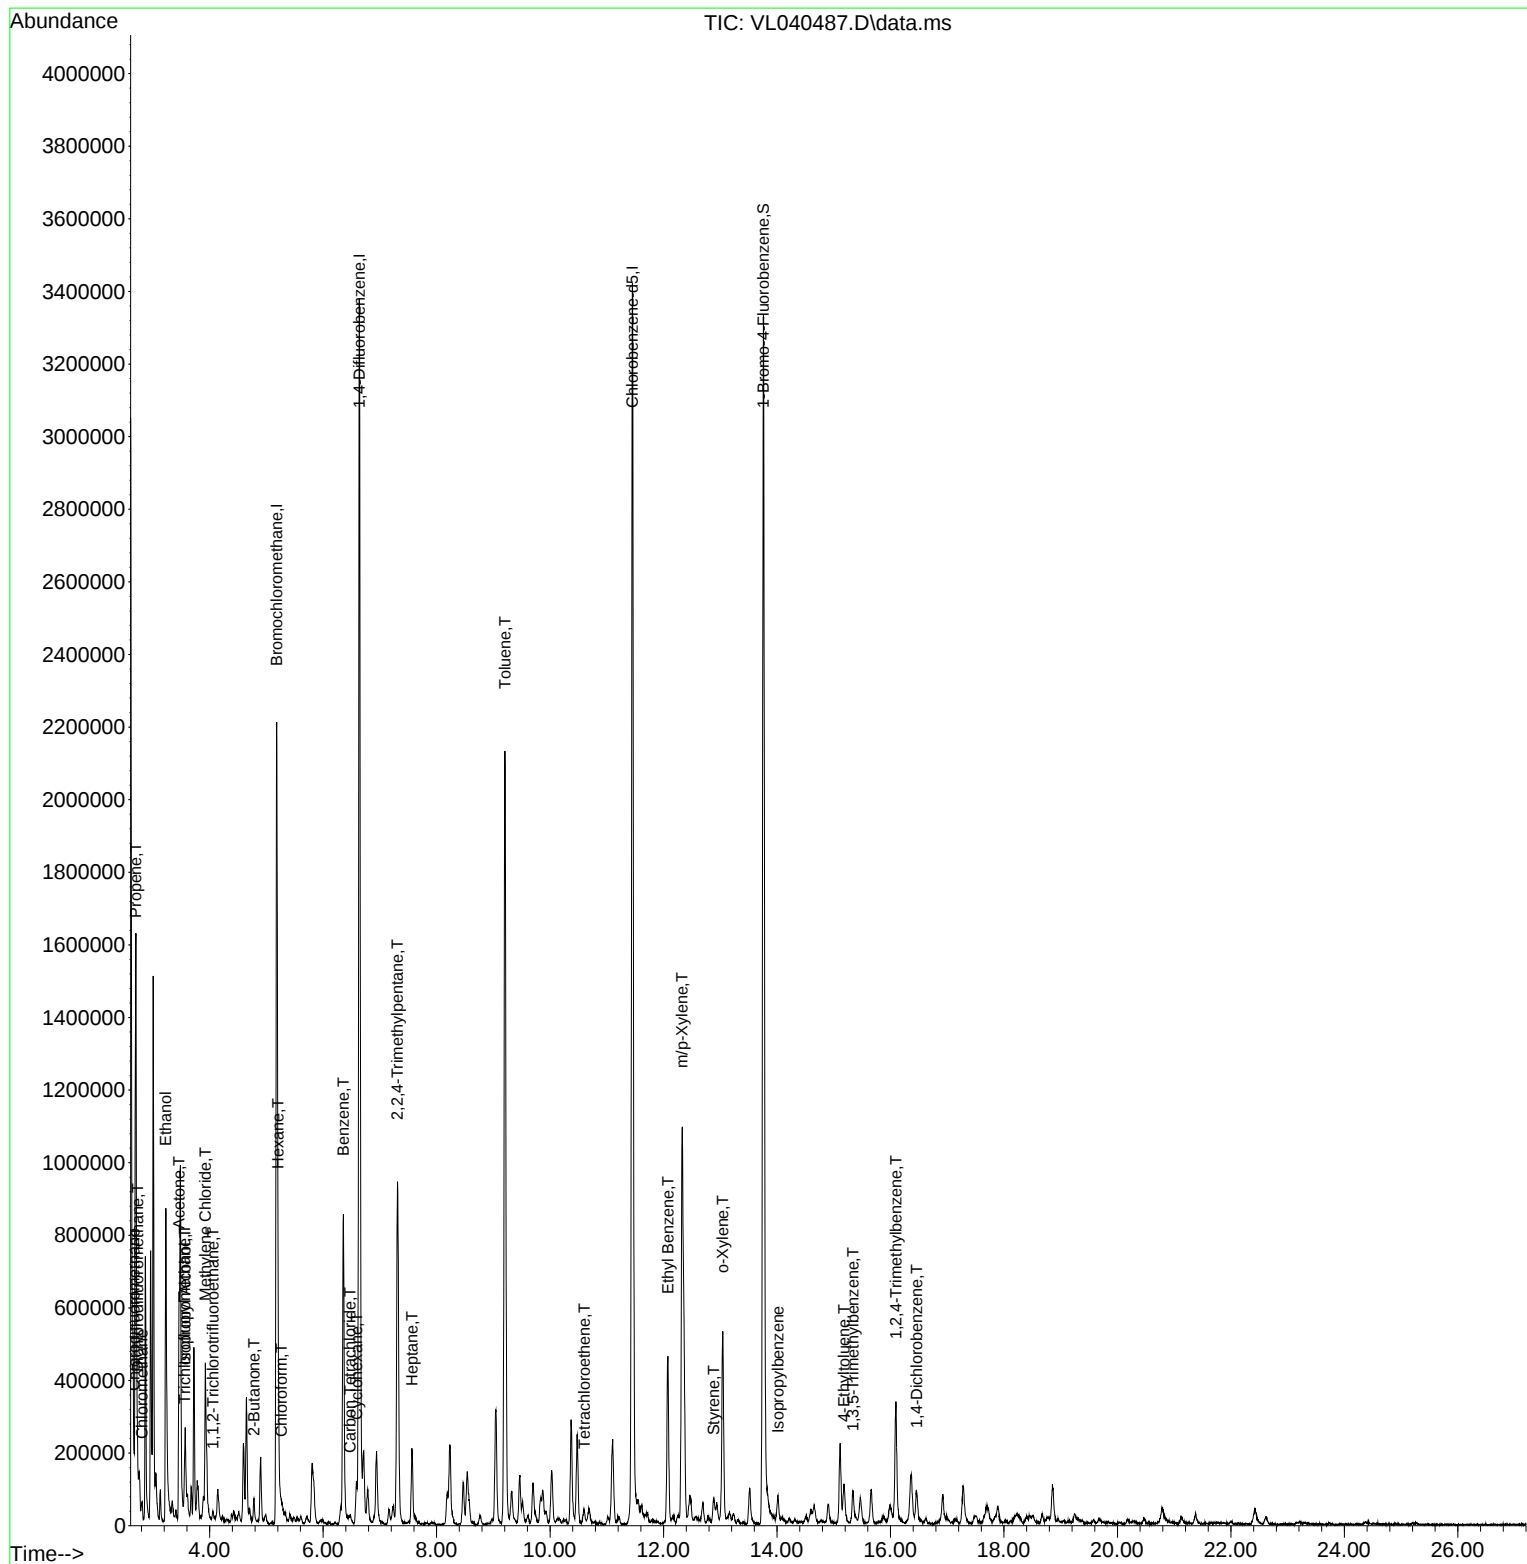



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.179 min Scan# 80
Delta R.T. -0.010 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument :
MSVOA_L
ClientSampleId :
AI-1

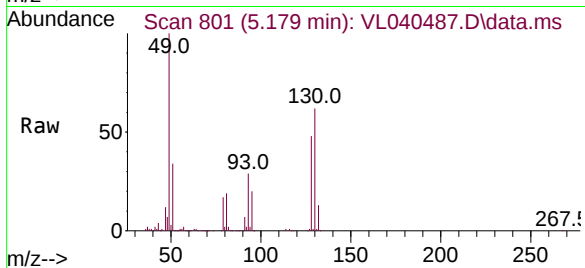

Tgt Ion: 49 Resp: 1001060
Ion Ratio Lower Upper
49 100
128 47.7 24.7 74.1
130 61.4 31.4 94.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023



#2
Dichlorodifluoromethane
Concen: 0.417 ppbv m
RT: 2.729 min Scan# 39
Delta R.T. 0.013 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

Tgt Ion: 85 Resp: 90855
Ion Ratio Lower Upper
85 100
87 24.9 26.6 39.8#

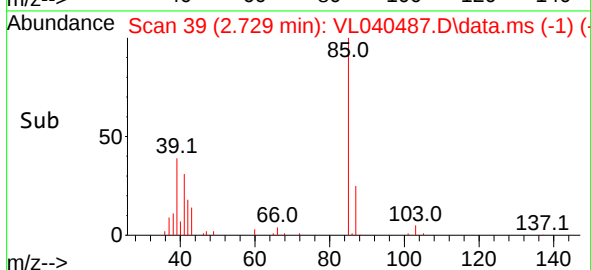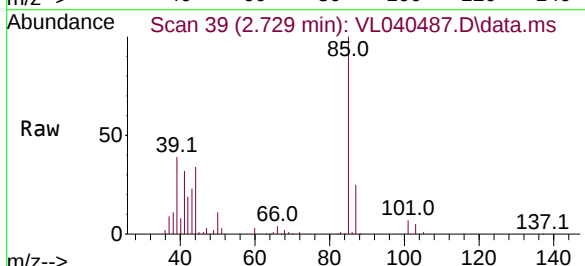

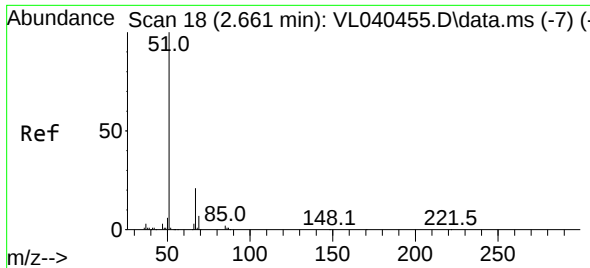





#3
Chlorodifluoromethane
Concen: 0.362 ppbv m
RT: 2.668 min Scan# 20
Delta R.T. 0.006 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

Instrument :
MSVOA_L
ClientSampleId :
AI-1

Tgt Ion: 51 Resp: 5929
Ion Ratio Lower Upper
51 100
67 15.1 16.3 24.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

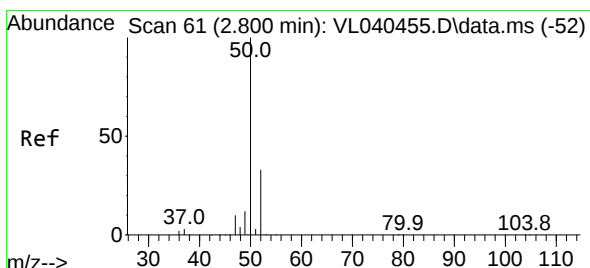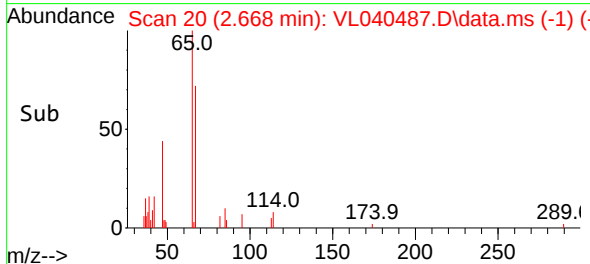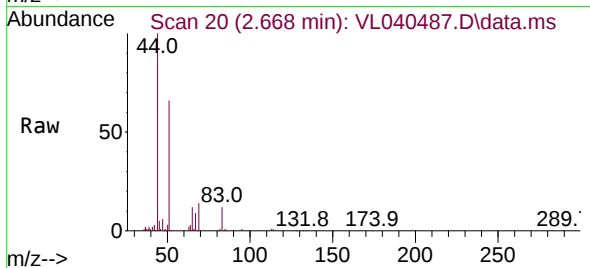

#4
Chloromethane
Concen: 0.570 ppbv
RT: 2.809 min Scan# 64
Delta R.T. 0.010 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03


Tgt Ion: 50 Resp: 36158
Ion Ratio Lower Upper
50 100
52 41.2 26.3 39.5

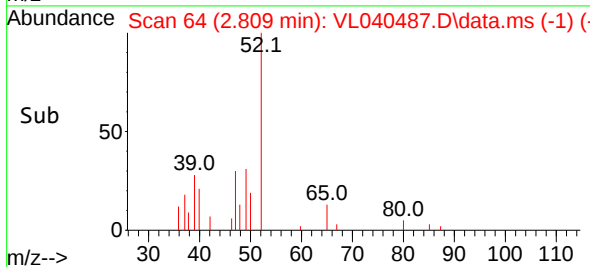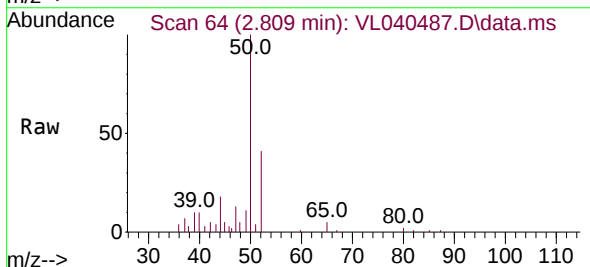

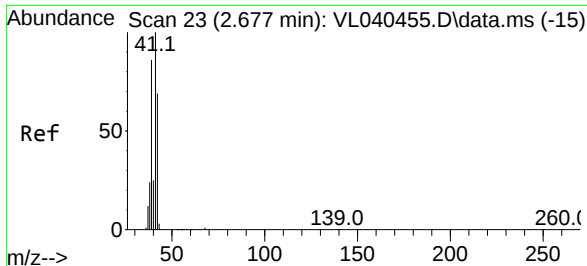

#9
 Propene
 Concen: 11.603 ppbv
 RT: 2.693 min Scan# 21
 Delta R.T. 0.016 min
 Lab File: VL040487.D
 Acq: 22 Jun 2023 16:03




Instrument :
 MSVOA_L
 ClientSampleId :
 AI-1

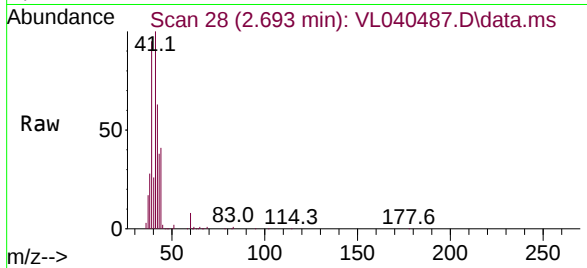

Tgt Ion: 41 Resp: 58667
 Ion Ratio Lower Upper
 41 100
 42 59.3 56.2 84.2




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
 Supervised By :Mahesh Dadoda 06/27/2023

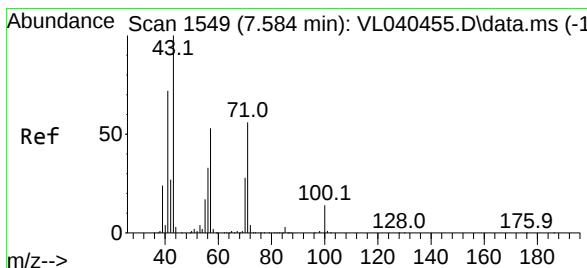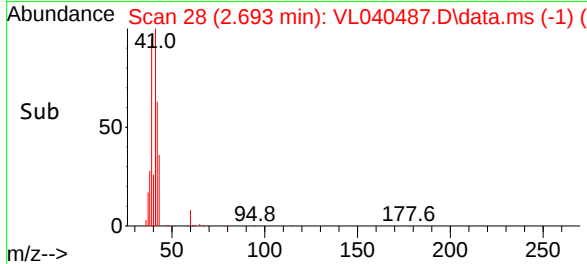

#10
 Heptane
 Concen: 0.648 ppbv m
 RT: 7.565 min Scan# 1543
 Delta R.T. -0.019 min
 Lab File: VL040487.D
 Acq: 22 Jun 2023 16:03


Tgt Ion: 43 Resp: 74104
 Ion Ratio Lower Upper
 43 100
 57 56.4 42.5 63.7

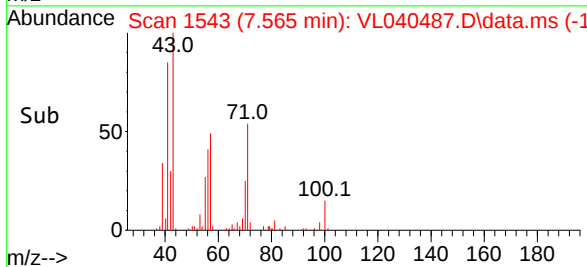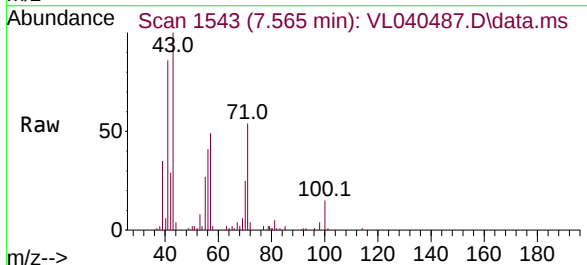



#11
 Trichlorofluoromethane
 Concen: 0.241 ppbv
 RT: 3.555 min Scan# 295
 Delta R.T. 0.003 min
 Lab File: VL040487.D
 Acq: 22 Jun 2023 16:03




Instrument :
 MSVOA_L
 ClientSampleId :
 AI-1

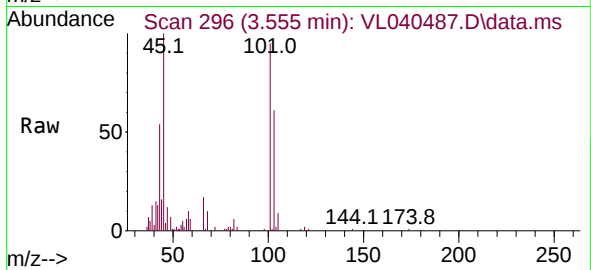


Tgt Ion:101 Resp: 42720
 Ion Ratio Lower Upper
 101 100
 103 64.8 51.7 77.5

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 06/26/2023
 Supervised By :Mahesh Dadoda 06/27/2023

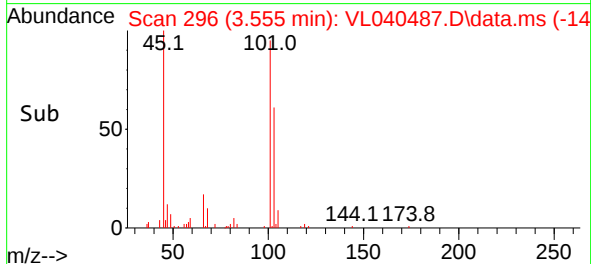


#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.067 ppbv
 RT: 4.057 min Scan# 452
 Delta R.T. -0.000 min
 Lab File: VL040487.D
 Acq: 22 Jun 2023 16:03

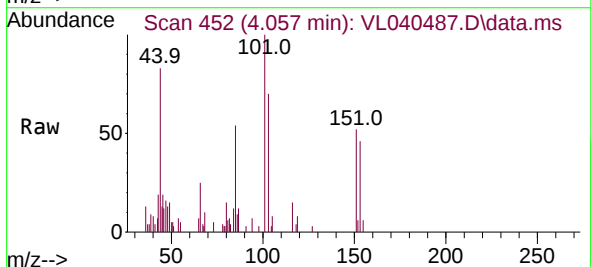


Tgt Ion:101 Resp: 8300
 Ion Ratio Lower Upper
 101 100
 151 75.2 54.3 81.5





#13
Ethanol
Concen: 85.167 ppbv
RT: 3.227 min Scan# 194
Delta R.T. -0.000 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument : MSVOA_L
Client Sample Id : AI-1




Tgt Ion: 45 Resp: 89171
Ion Ratio Lower Upper
45 100
46 35.5 14.5 58.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

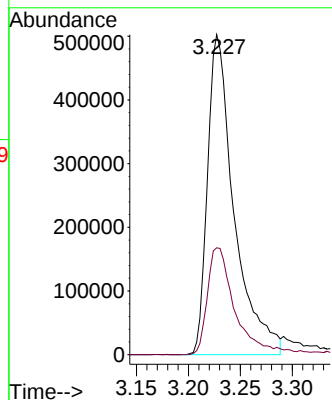


#15
Acetone
Concen: 4.289 ppbv
RT: 3.462 min Scan# 267
Delta R.T. 0.006 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

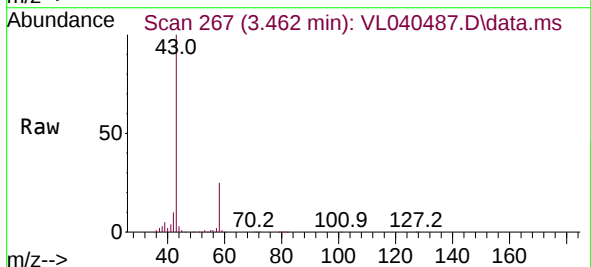

Tgt Ion: 43 Resp: 517808
Ion Ratio Lower Upper
43 100
58 34.8 21.6 32.4#

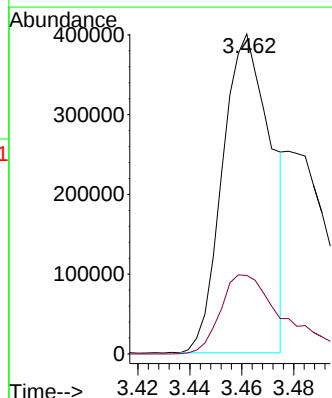







#19
Isopropyl Alcohol
Concen: 3.551 ppbv
RT: 3.568 min Scan# 300
Delta R.T. 0.006 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

Instrument :
MSVOA_L
ClientSampleId :
AI-1

Tgt Ion: 45 Resp: 206662
Ion Ratio Lower Upper
45 100
58 4.3 2.6 4.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

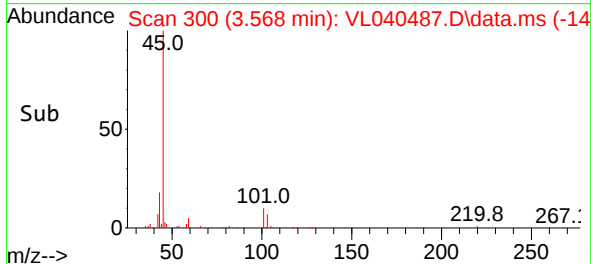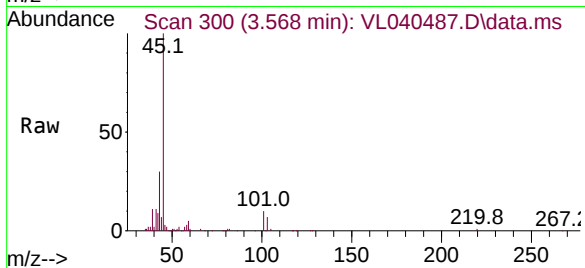

#20
Methylene Chloride
Concen: 2.526 ppbv
RT: 3.925 min Scan# 411
Delta R.T. -0.000 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03


Tgt Ion: 84 Resp: 130147
Ion Ratio Lower Upper
84 100
49 154.4 126.2 189.2
51 47.9 38.7 58.1
86 65.1 50.6 75.8

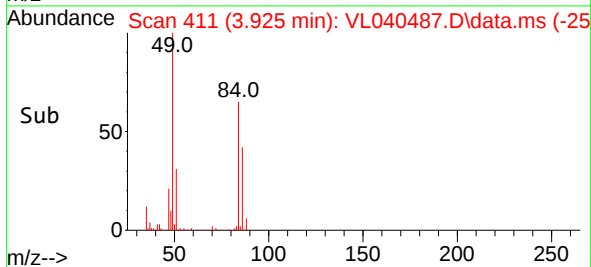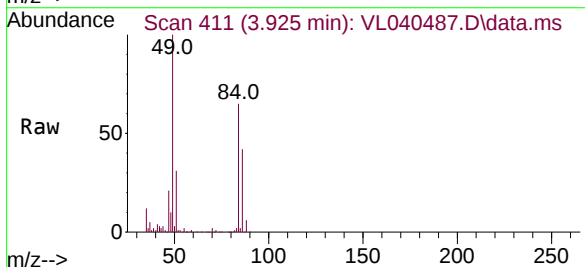



#26
Hexane
Concen: 1.523 ppbv
RT: 5.205 min Scan# 809
Delta R.T. -0.003 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument :
MSVOA_L
ClientSampleId :
AI-1

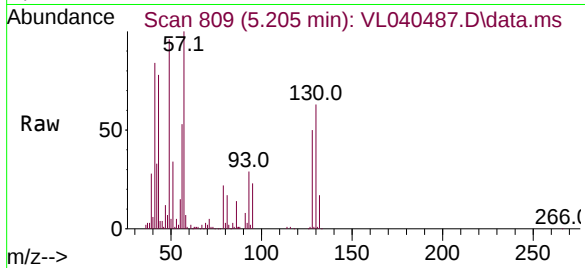

Tgt Ion: 57 Resp: 157829
Ion Ratio Lower Upper
57 100
41 97.2 73.0 109.6
43 104.2 177.5 266.3
56 57.9 43.6 65.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

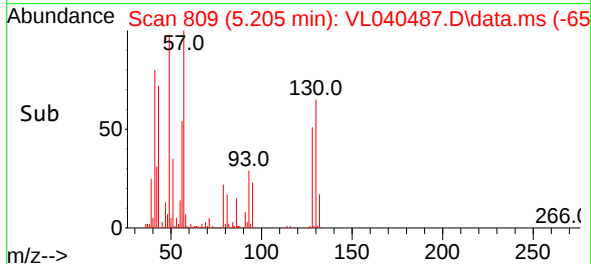

#29
Chloroform
Concen: 0.070 ppbv
RT: 5.266 min Scan# 828
Delta R.T. -0.007 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03


Tgt Ion: 83 Resp: 12440
Ion Ratio Lower Upper
83 100
85 54.1 51.1 76.7

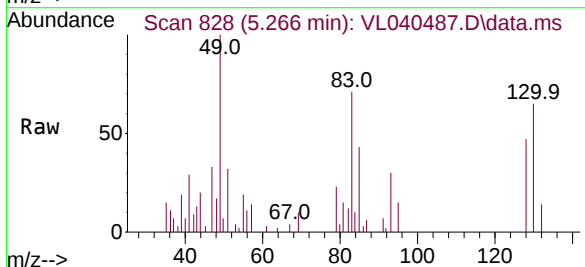



#30
Cyclohexane
Concen: 0.392 ppbv m
RT: 6.590 min Scan# 1243
Delta R.T. -0.010 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument :
MSVOA_L
ClientSampleId :
AI-1



Tgt Ion: 84 Resp: 3275
Ion Ratio Lower Upper
84 100
56 123.7 106.0 159.0
41 99.2 66.8 100.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

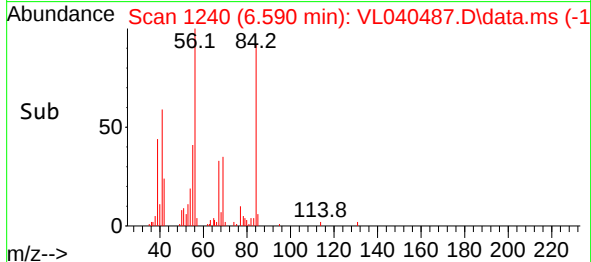

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.639 min Scan# 1255
Delta R.T. -0.016 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03


Tgt Ion:114 Resp: 2507924
Ion Ratio Lower Upper
114 100
63 25.4 21.0 31.6
88 17.8 14.5 21.7

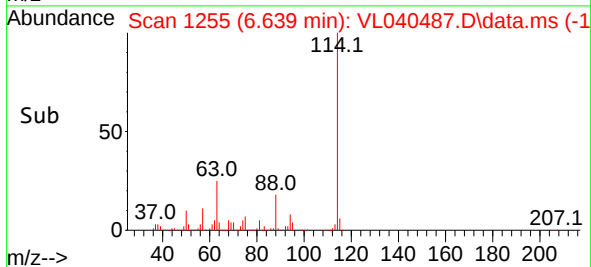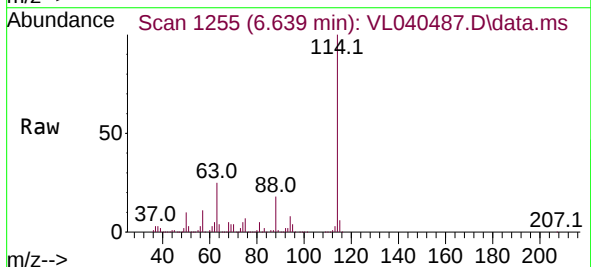



#34
2-Butanone
Concen: 0.567 ppbv
RT: 4.780 min Scan# 61
Delta R.T. -0.000 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument :
MSVOA_L
ClientSampleId :
AI-1

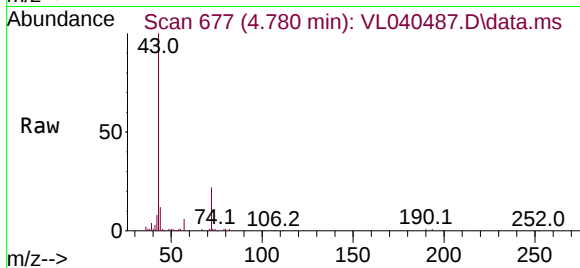


Tgt Ion: 43 Resp: 6858
Ion Ratio Lower Upper
43 100
72 24.4 18.1 27.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

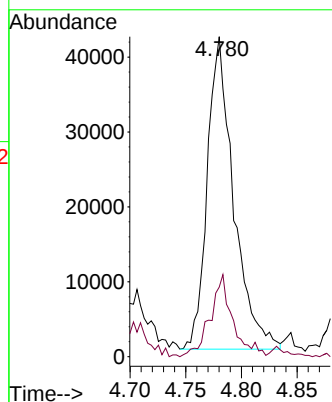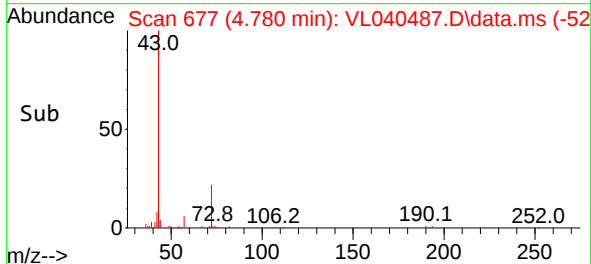


#35
Carbon Tetrachloride
Concen: 0.064 ppbv m
RT: 6.475 min Scan# 1204
Delta R.T. -0.019 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

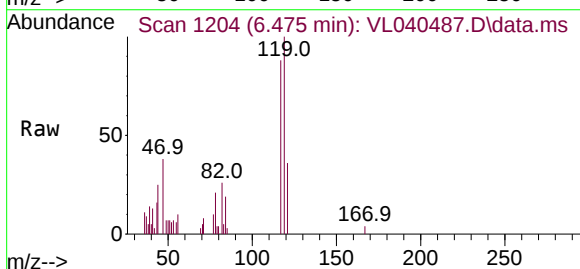


Tgt Ion:117 Resp: 10984
Ion Ratio Lower Upper
117 100
119 113.2 79.1 118.7
121 40.2 26.0 39.0#

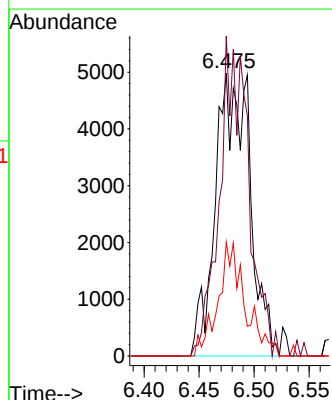



#36
Benzene
Concen: 3.602 ppbv
RT: 6.356 min Scan# 1172
Delta R.T. -0.016 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument :
MSVOA_L
ClientSampleId :
AI-1



Tgt Ion: 78 Resp: 71857
Ion Ratio Lower Upper
78 100
77 20.4 18.5 27.7
50 17.6 16.1 24.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

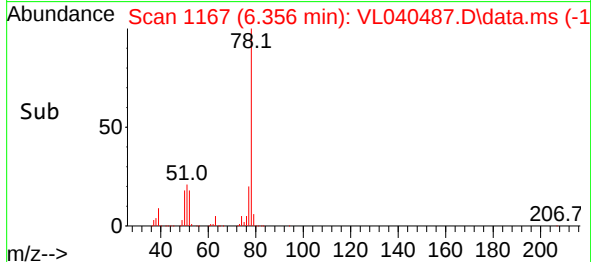

#44
2,2,4-Trimethylpentane
Concen: 2.727 ppbv
RT: 7.311 min Scan# 1464
Delta R.T. -0.019 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03


Tgt Ion: 57 Resp: 889064
Ion Ratio Lower Upper
57 100
41 35.9 27.8 41.8
56 34.6 25.3 37.9

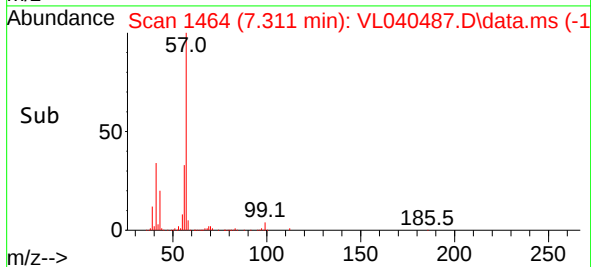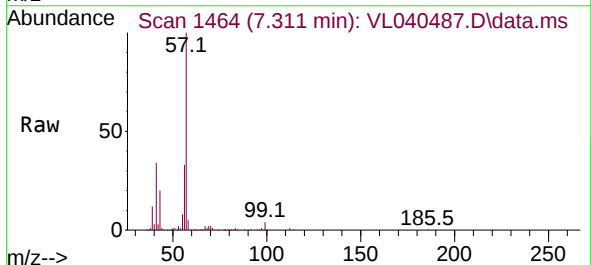



#52
Tetrachloroethene
Concen: 0.078 ppbv m
RT: 10.600 min Scan# 2495
Delta R.T. -0.026 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument :
MSVOA_L
ClientSampleId :
AI-1



Tgt Ion:164 Resp: 4859
Ion Ratio Lower Upper
164 100
166 106.5 102.7 154.1
129 124.1 84.6 126.8
131 134.6 85.1 127.7#




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

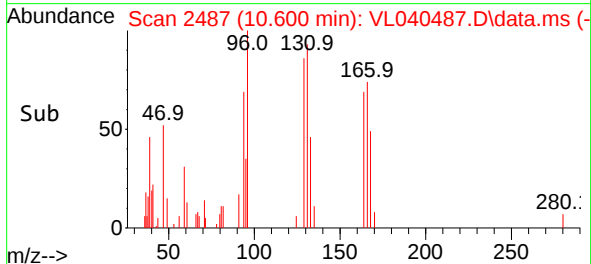

#53
Toluene
Concen: 6.800 ppbv
RT: 9.204 min Scan# 2053
Delta R.T. -0.023 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03


Tgt Ion: 91 Resp: 1428836
Ion Ratio Lower Upper
91 100
92 61.2 49.1 73.7

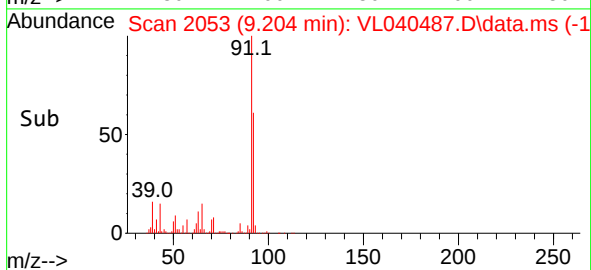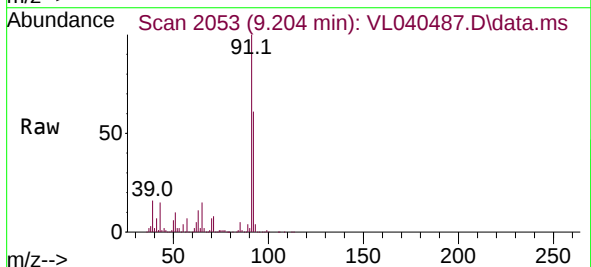

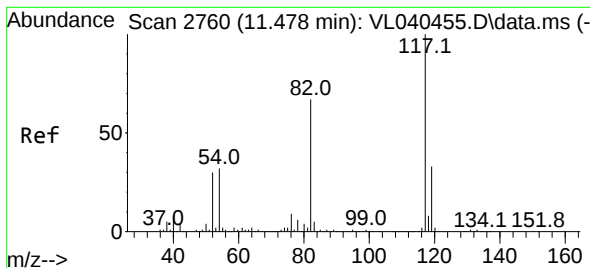

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.452 min Scan# 21
Delta R.T. -0.026 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument :
MSVOA_L
ClientSampleId :
AI-1

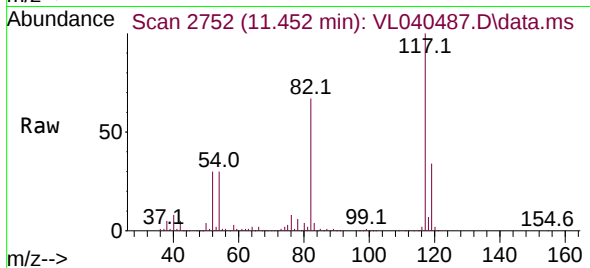

Tgt Ion: 117 Resp: 216906
Ion Ratio Lower Upper
117 100
82 66.7 53.0 79.4
119 33.1 24.4 36.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

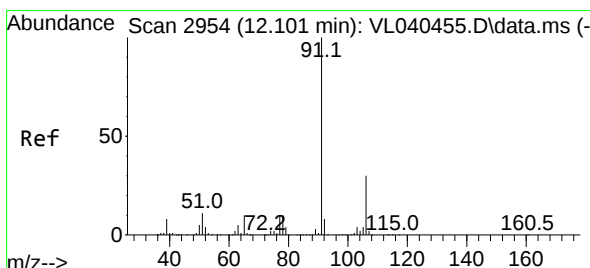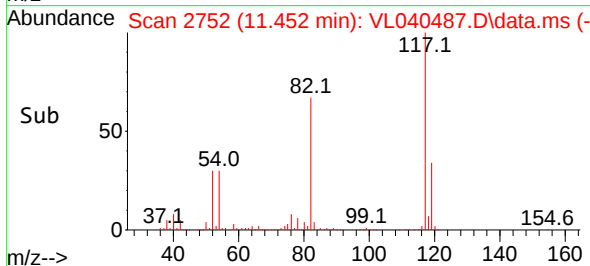

#58
Ethyl Benzene
Concen: 1.505 ppbv
RT: 12.076 min Scan# 2946
Delta R.T. -0.026 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

Tgt Ion: 91 Resp: 395499
Ion Ratio Lower Upper
91 100
106 26.6 23.7 35.5

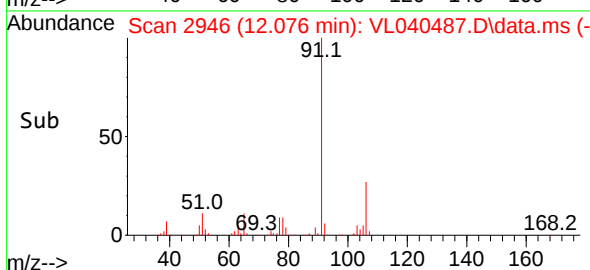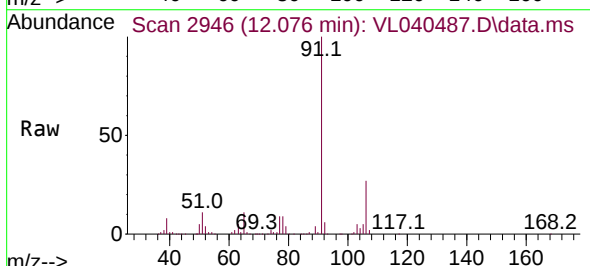







#59
m/p-Xylene
Concen: 4.727 ppbv
RT: 12.326 min Scan# 3041
Delta R.T. -0.055 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

Instrument :
MSVOA_L
ClientSampleId :
AI-1

Tgt Ion: 91 Resp: 114168
Ion Ratio Lower Upper
91 100
106 45.5 34.6 52.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

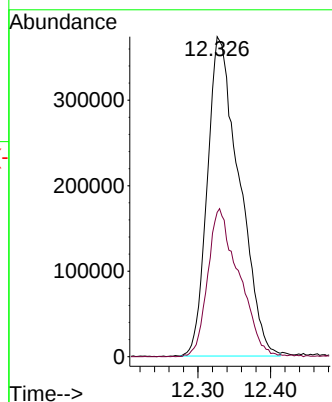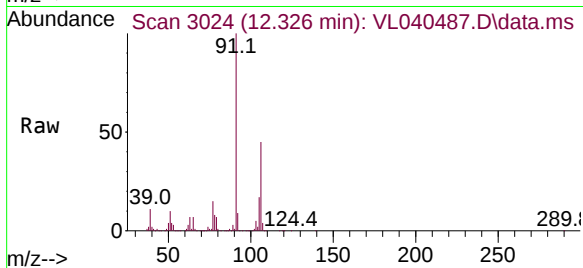

#60
o-Xylene
Concen: 1.794 ppbv
RT: 13.040 min Scan# 3246
Delta R.T. -0.029 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

Tgt Ion: 91 Resp: 410884
Ion Ratio Lower Upper
91 100
106 43.4 22.1 66.1

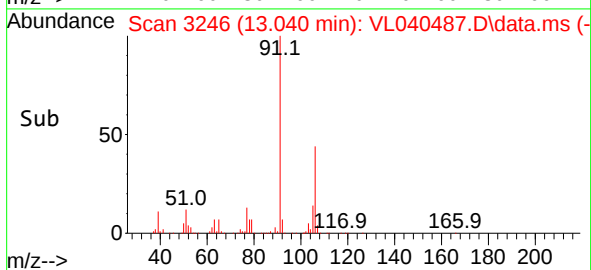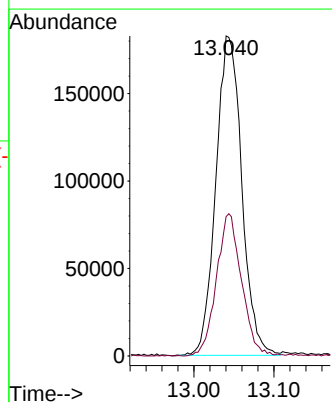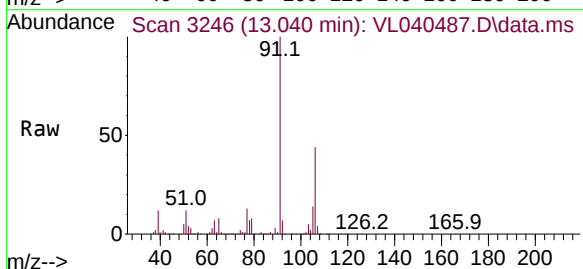



#61

Styrene

Concen: 0.331 ppbv

RT: 12.886 min Scan# 3198

Delta R.T. -0.023 min

Lab File: VL040487.D

Acq: 22 Jun 2023 16:03

Instrument :

MSVOA_L

ClientSampleId :





AI-1

Tgt Ion:104 Resp: 32609
 Ion Ratio Lower Upper
 104 100
 78 61.5 43.1 64.7
 103 49.3 37.1 55.7

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/26/2023
 Supervised By :Mahesh Dadoda 06/27/2023



#62

Isopropylbenzene

Concen: 0.159 ppbv




RT: 14.018 min Scan# 3550


Delta R.T. -0.023 min

Lab File: VL040487.D

Acq: 22 Jun 2023 16:03


Tgt Ion:105 Resp: 54212
 Ion Ratio Lower Upper
 105 100
 120 25.6 20.2 30.4

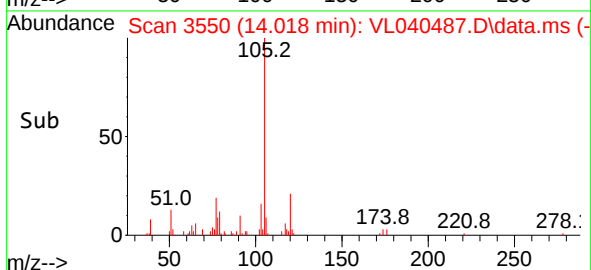



#68
1-Bromo-4-Fluorobenzene
Concen: 9.428 ppbv
RT: 13.760 min Scan# 3478
Delta R.T. -0.026 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03




Instrument :
MSVOA_L
ClientSampleId :
AI-1

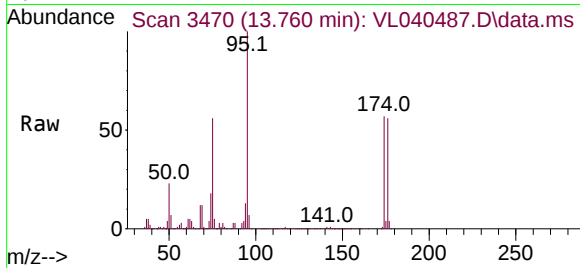


Tgt Ion: 95 Resp: 1687750
Ion Ratio Lower Upper
95 100
174 60.4 47.7 71.5
175 4.2 3.5 5.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

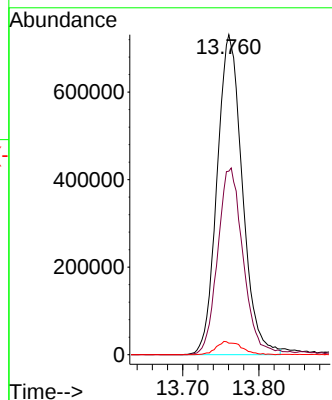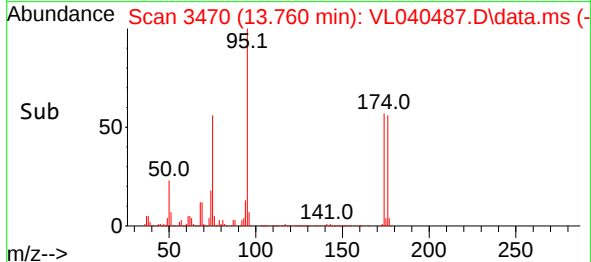


#72
4-Ethyltoluene
Concen: 0.293 ppbv
RT: 15.178 min Scan# 3911
Delta R.T. -0.023 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

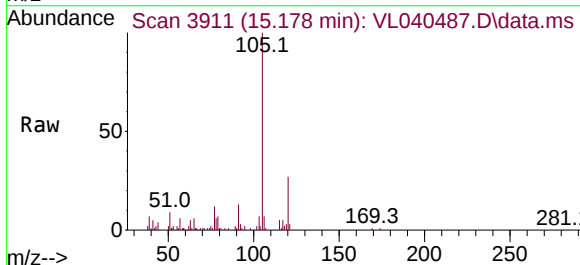

Tgt Ion:105 Resp: 75530
Ion Ratio Lower Upper
105 100
120 31.4 23.4 35.0
91 17.4 11.1 16.7#
77 18.6 12.1 18.1#

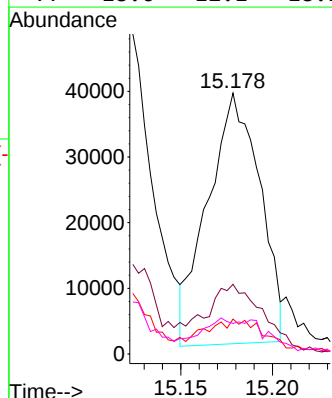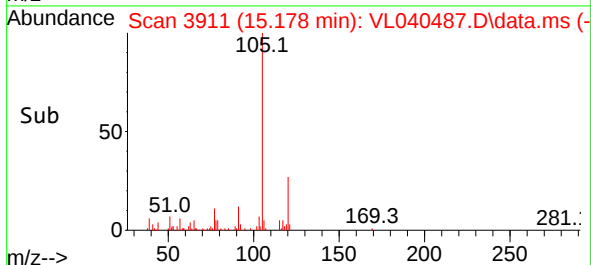







#73
1,3,5-Trimethylbenzene
Concen: 0.263 ppbv m
RT: 15.339 min Scan# 3968
Delta R.T. -0.023 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

Instrument :
MSVOA_L
ClientSampleId :
AI-1

Tgt Ion:105 Resp: 5999
Ion Ratio Lower Upper
105 100
120 34.2 36.4 54.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

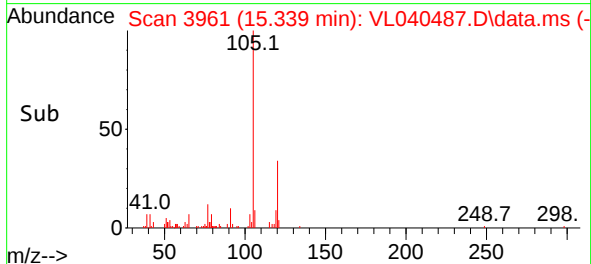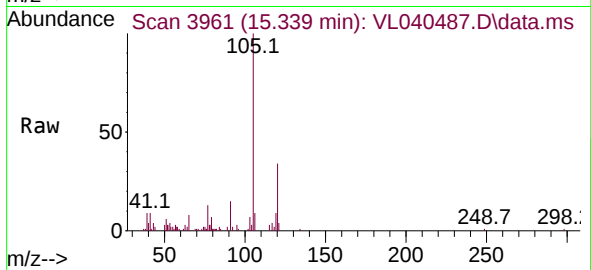

#74
1,2,4-Trimethylbenzene
Concen: 0.927 ppbv
RT: 16.095 min Scan# 4196
Delta R.T. -0.026 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03


Tgt Ion:105 Resp: 248781
Ion Ratio Lower Upper
105 100
120 42.4 38.4 57.6
91 15.0 41.3 61.9#
77 15.3 18.6 28.0#

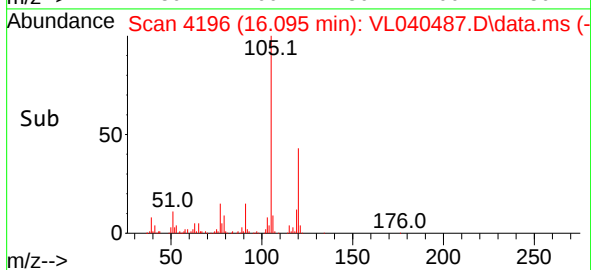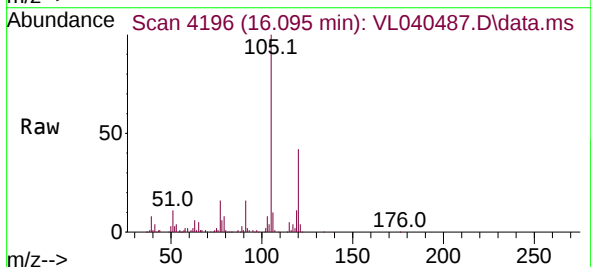



#76
1,4-Dichlorobenzene
Concen: 0.143 ppbv m
RT: 16.458 min Scan# 41
Delta R.T. -0.029 min
Lab File: VL040487.D
Acq: 22 Jun 2023 16:03

Instrument :
MSVOA_L
ClientSampleId :
AI-1



Tgt Ion	Ratio	Lower	Upper
146	100		
111	0.0	23.8	71.5
148	0.0	32.9	98.6

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/26/2023
Supervised By :Mahesh Dadoda 06/27/2023

