

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
 Data File : VL040487.D
 Acq On : 22 Jun 2023 16:03
 Operator : SY/MD
 Sample : 03300-03
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 AI-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 3

Min Area: 3 % of largest Peak

Start Thrs: 0.001

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 0

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

Signal : TIC: VL040487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.700	21	30	44	rVB5	1503846	2470083	31.19%	3.662%
2	2.761	48	49	56	rVB3	105869	83261	1.05%	0.123%
3	2.809	56	64	72	rVB2	49848	86111	1.09%	0.128%
4	2.867	72	82	99	rBV	724519	929623	11.74%	1.378%
5	2.960	103	111	119	rBV	734413	1034237	13.06%	1.533%
6	3.005	119	125	135	rVV	1466973	1794050	22.65%	2.660%
7	3.050	135	139	153	rVB5	122576	209267	2.64%	0.310%
8	3.131	157	164	174	rVB	84647	110486	1.40%	0.164%
9	3.227	184	194	214	rBV	862888	1572229	19.85%	2.331%
10	3.462	259	267	268	rBV	625393	566628	7.15%	0.840%
11	3.484	268	274	289	rVV3	972428	1588927	20.06%	2.356%
12	3.568	289	300	310	rVV2	249903	503201	6.35%	0.746%
13	3.607	310	312	325	rVV9	66349	92945	1.17%	0.138%
14	3.674	325	333	340	rVV3	86352	121846	1.54%	0.181%
15	3.722	340	348	357	rVV	469463	656386	8.29%	0.973%
16	3.780	357	366	368	rVV3	102583	130116	1.64%	0.193%
17	3.796	368	371	380	rVB3	87176	105239	1.33%	0.156%
18	3.890	389	400	404	rBV6	59587	97925	1.24%	0.145%
19	3.925	404	411	425	rVB2	397341	700278	8.84%	1.038%
20	4.144	466	479	494	rVB10	82858	178219	2.25%	0.264%
21	4.597	608	620	628	rBV2	214896	404088	5.10%	0.599%
22	4.648	628	636	648	rVV	342544	607502	7.67%	0.901%
23	4.780	667	677	695	rVB2	64538	109399	1.38%	0.162%
24	4.899	703	714	727	rBV2	177043	313492	3.96%	0.465%
25	5.182	789	802	824	rBV6	2208770	4715727	59.54%	6.991%
26	5.809	983	997	1021	rVB6	163375	538746	6.80%	0.799%
27	6.359	1155	1168	1187	rVB2	840743	1650416	20.84%	2.447%
28	6.587	1225	1239	1243	rBV5	118468	208143	2.63%	0.309%
29	6.639	1243	1255	1271	rVV	3368326	6554559	82.76%	9.717%
30	6.716	1271	1279	1291	rVV3	192149	435817	5.50%	0.646%
31	6.780	1291	1299	1300	rVV3	85859	90228	1.14%	0.134%
32	6.787	1300	1301	1313	rVB4	85136	97877	1.24%	0.145%
33	6.941	1335	1349	1368	rVB5	192598	441594	5.58%	0.655%
34	7.311	1448	1464	1489	rVB	936003	2213796	27.95%	3.282%
35	7.565	1530	1543	1555	rBV3	205745	413219	5.22%	0.613%
36	8.192	1723	1738	1741	rBV7	83569	165398	2.09%	0.245%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
 Data File : VL040487.D
 Acq On : 22 Jun 2023 16:03
 Operator : SY/MD
 Sample : 03300-03
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 AI-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 3

Min Area: 3 % of largest Peak

Start Thrs: 0.001

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 0

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

37	8.233	1741	1751	1764	rVB6	197766	464552	5.87%	0.689%
38	8.468	1809	1824	1836	rBV3	114453	270974	3.42%	0.402%
39	8.539	1836	1846	1870	rVB6	140178	429858	5.43%	0.637%
40	9.040	1987	2002	2020	rBV3	306997	733360	9.26%	1.087%
41	9.204	2033	2053	2076	rBV3	2128166	4794645	60.54%	7.108%
42	9.317	2078	2088	2089	rVV5	73897	84966	1.07%	0.126%
43	9.327	2089	2091	2103	rVB4	75773	89446	1.13%	0.133%
44	9.468	2119	2135	2143	rBV3	130766	292904	3.70%	0.434%
45	9.516	2143	2150	2165	rVB9	56112	117903	1.49%	0.175%
46	9.700	2191	2207	2217	rBV6	111817	265517	3.35%	0.394%
47	9.835	2236	2249	2253	rVV5	68178	140033	1.77%	0.208%
48	9.873	2253	2261	2271	rVV9	87307	217331	2.74%	0.322%
49	10.028	2293	2309	2327	rBV3	146075	367161	4.64%	0.544%
50	10.372	2402	2416	2436	rBV2	282998	636999	8.04%	0.944%
51	10.478	2436	2449	2463	rVB2	240723	536544	6.77%	0.795%
52	11.105	2626	2644	2660	rVB3	229045	594346	7.50%	0.881%
53	11.452	2725	2752	2777	rBV	3414980	7866901	99.33%	11.662%
54	12.076	2931	2946	2962	rBV2	454810	997945	12.60%	1.479%
55	12.330	3008	3025	3050	rBV2	1077789	3289433	41.53%	4.876%
56	12.465	3050	3067	3068	rVV5	68334	111612	1.41%	0.165%
57	12.471	3068	3069	3084	rVB4	64147	88162	1.11%	0.131%
58	12.886	3184	3198	3206	rBV8	68039	163836	2.07%	0.243%
59	13.043	3229	3247	3265	rBV2	518263	1172661	14.81%	1.738%
60	13.519	3379	3395	3418	rBV5	99147	267232	3.37%	0.396%
61	13.760	3449	3470	3492	rBV3	3332199	7920062	100.00%	11.741%
62	14.018	3540	3550	3561	rVB4	65807	131208	1.66%	0.195%
63	14.654	3740	3748	3762	rVB4	44038	102684	1.30%	0.152%
64	15.111	3871	3890	3902	rBV2	220799	524699	6.62%	0.778%
65	15.178	3902	3911	3929	rVB2	103336	263796	3.33%	0.391%
66	15.333	3947	3959	3960	rBV	82737	95320	1.20%	0.141%
67	15.468	3987	4001	4019	rVB5	68281	189779	2.40%	0.281%
68	15.664	4041	4062	4075	rBV4	93966	238287	3.01%	0.353%
69	16.095	4179	4196	4216	rVB	322584	769871	9.72%	1.141%
70	16.365	4262	4280	4297	rBV5	125819	388082	4.90%	0.575%
71	16.458	4297	4309	4321	rVB5	79280	182755	2.31%	0.271%
72	16.918	4439	4452	4454	rBV2	69913	97983	1.24%	0.145%
73	17.281	4546	4565	4583	rBV2	104687	326635	4.12%	0.484%
74	18.854	5040	5054	5057	rBV5	96142	152536	1.93%	0.226%
75	18.866	5057	5058	5070	rVB7	85516	85846	1.08%	0.127%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040487.D
Acq On : 22 Jun 2023 16:03
Operator : SY/MD
Sample : 03300-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
AI-1

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 3 Min Area: 3 % of largest Peak
Start Thrs: 0.001 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 0

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022




Sum of corrected areas: 67454922

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040487.D
Acq On : 22 Jun 2023 16:03
Operator : SY/MD
Sample : 03300-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
AI-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

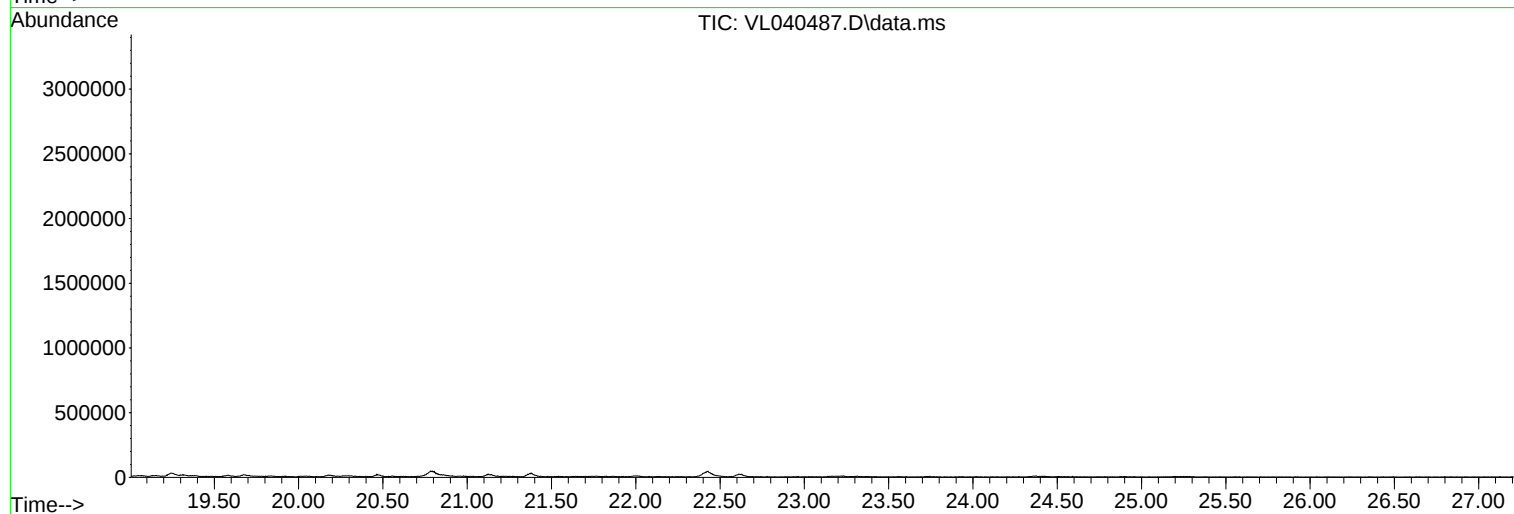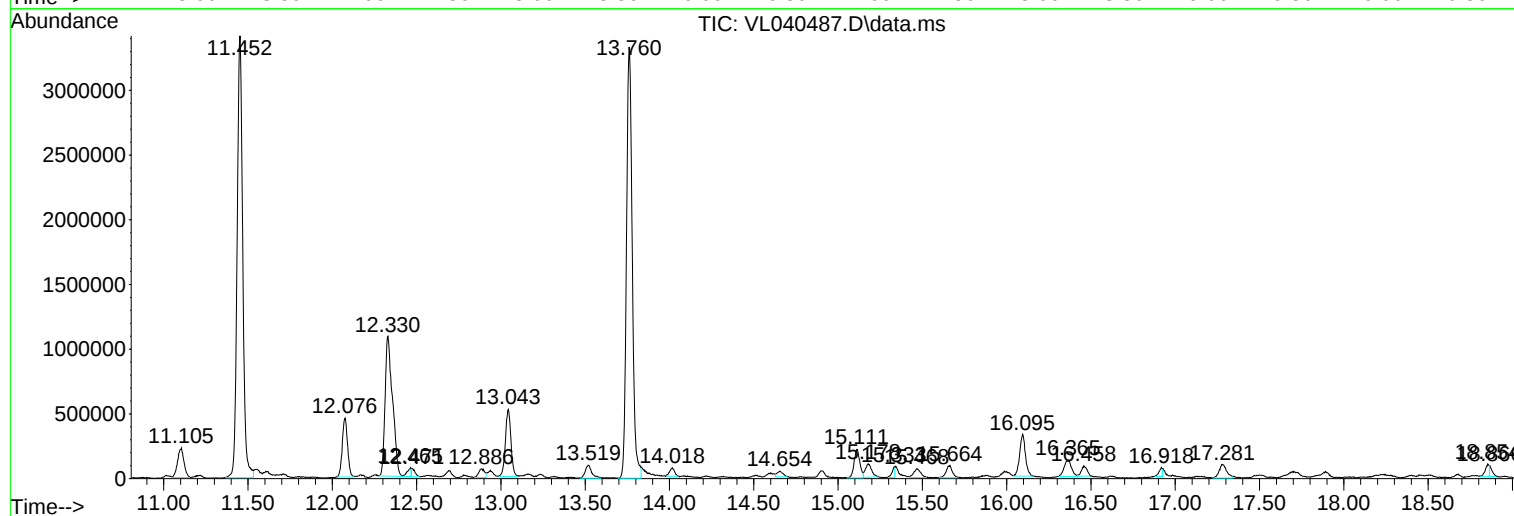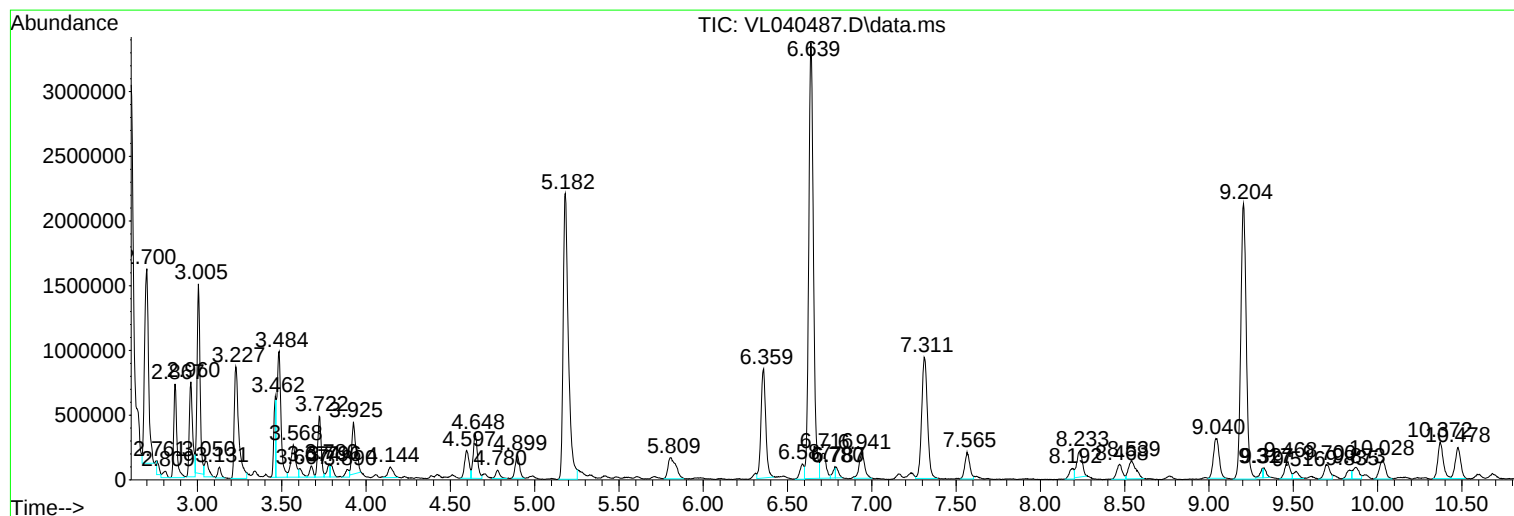

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040487.D
Acq On : 22 Jun 2023 16:03
Operator : SY/MD
Sample : 03300-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
AI-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040487.D
Acq On : 22 Jun 2023 16:03
Operator : SY/MD
Sample : 03300-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
AI-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------