

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
 Data File : VL040492.D
 Acq On : 22 Jun 2023 19:25
 Operator : SY/MD
 Sample : 03300-01 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 3

Min Area: 3 % of largest Peak

Start Thrs: 0.001

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 0

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

Signal : TIC: VL040492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.649	10	14	21	rVB2	459075	489026	5.86%	1.207%
2	2.700	21	30	42	rVV5	824342	1265407	15.16%	3.122%
3	2.752	42	46	56	rVB2	71803	96395	1.16%	0.238%
4	2.867	74	82	94	rBV	426103	529208	6.34%	1.306%
5	2.961	103	111	118	rBV2	142353	186914	2.24%	0.461%
6	3.006	118	125	135	rVV	381858	481112	5.76%	1.187%
7	3.076	138	147	158	rVV	572737	790694	9.47%	1.951%
8	3.227	186	194	213	rBV	1109607	1950202	23.37%	4.812%
9	3.459	255	266	290	rBV	1020794	1813754	21.73%	4.475%
10	3.568	290	300	328	rVV	1484924	2633694	31.56%	6.498%
11	3.723	339	348	357	rVB4	104503	147870	1.77%	0.365%
12	3.925	402	411	435	rVB2	1092210	1716742	20.57%	4.236%
13	4.157	474	483	501	rVB2	303741	540451	6.48%	1.334%
14	4.780	667	677	688	rBV	70583	117578	1.41%	0.290%
15	5.182	789	802	830	rBV	2316068	4696153	56.27%	11.587%
16	5.555	909	918	929	rBV5	55010	100838	1.21%	0.249%
17	6.594	1226	1241	1243	rBV6	63407	107755	1.29%	0.266%
18	6.642	1243	1256	1285	rVB	3459728	6697139	80.25%	16.524%
19	11.455	2734	2753	2781	rBV2	3497168	7822231	93.73%	19.301%
20	13.764	3450	3471	3496	rBV3	3550583	8345462	100.00%	20.592%




Sum of corrected areas: 40528625

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040492.D
Acq On : 22 Jun 2023 19:25
Operator : SY/MD
Sample : 03300-01 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

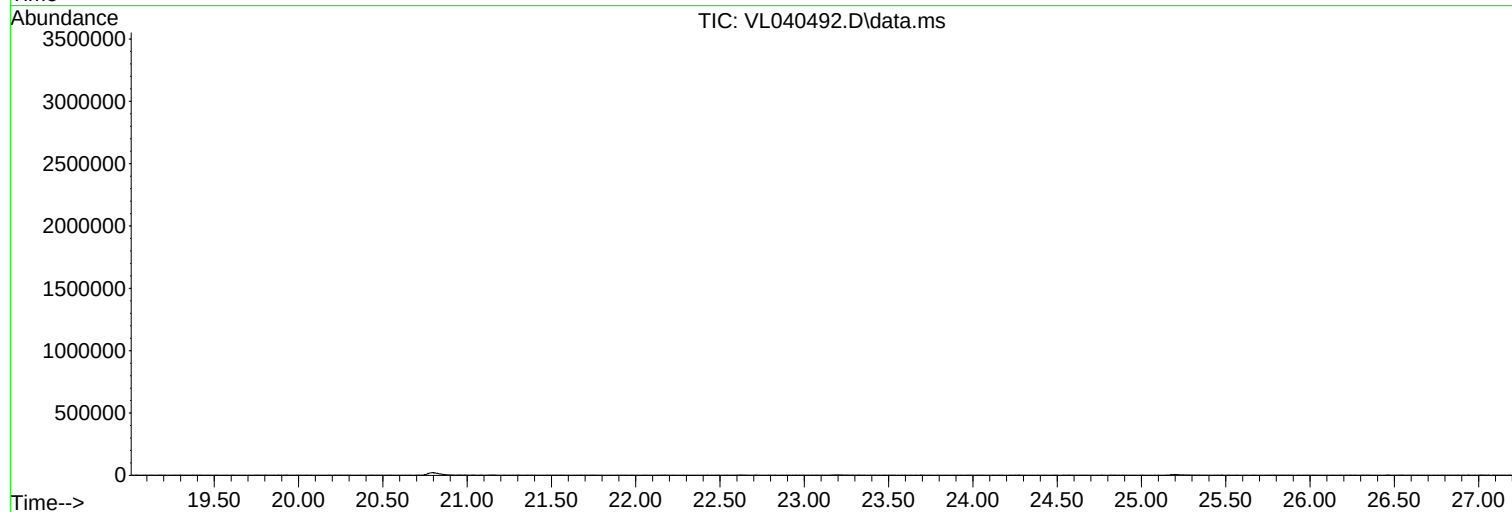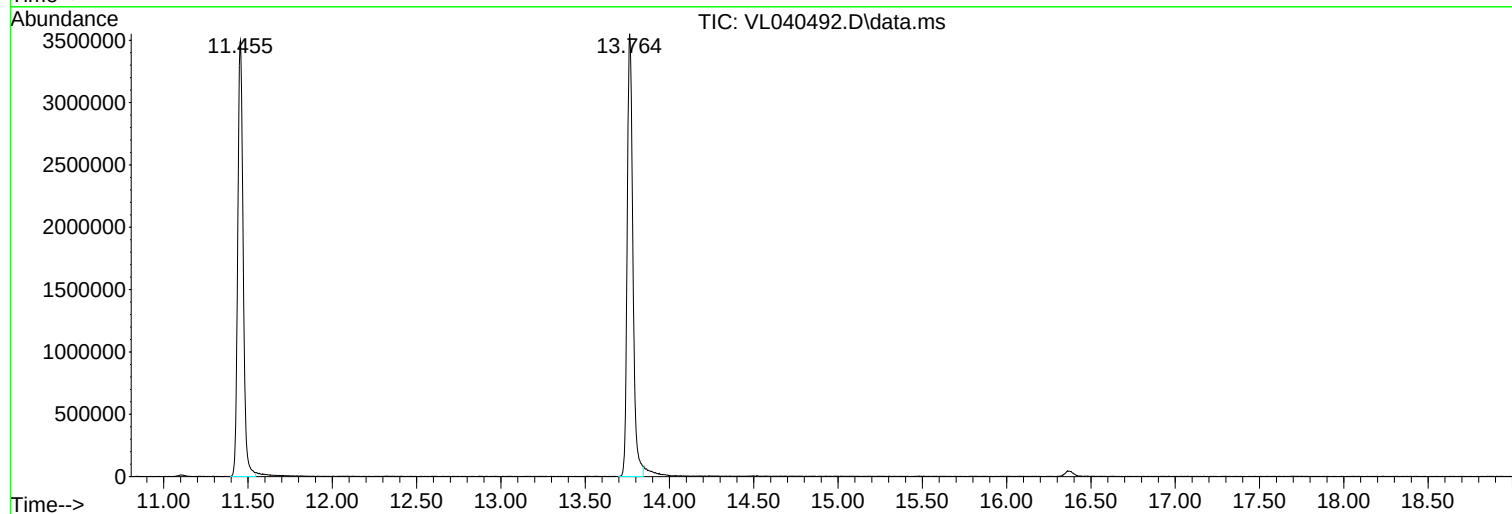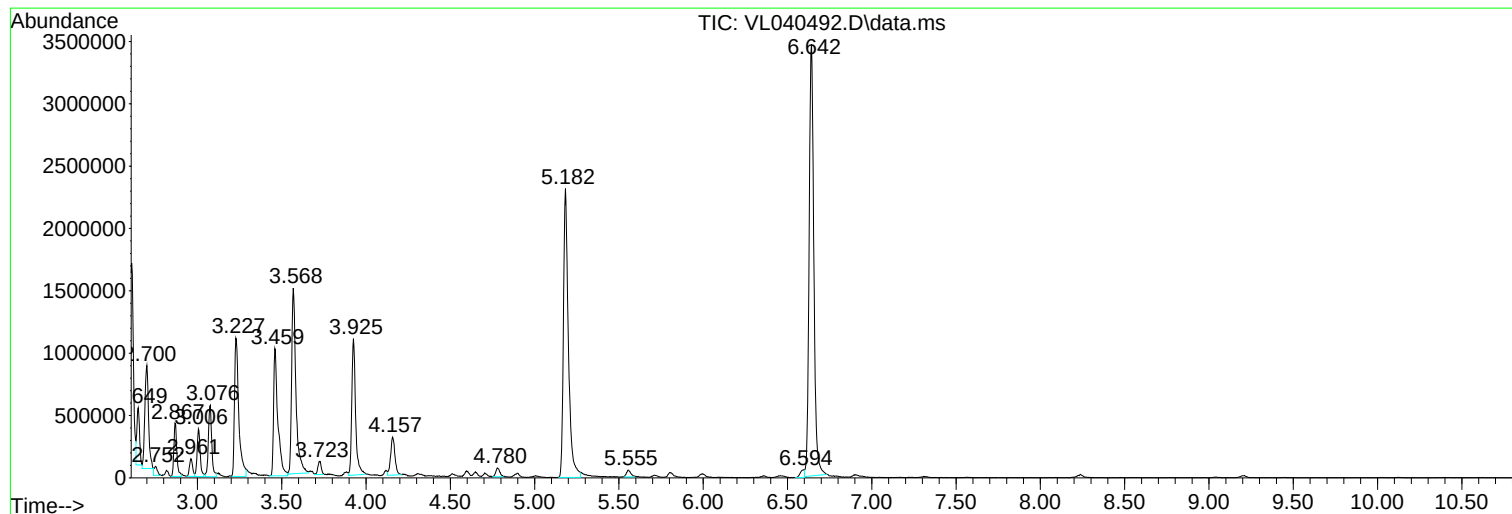

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040492.D
Acq On : 22 Jun 2023 19:25
Operator : SY/MD
Sample : 03300-01 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040492.D
Acq On : 22 Jun 2023 19:25
Operator : SY/MD
Sample : 03300-01 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc