

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
 Data File : VL040496.D
 Acq On : 22 Jun 2023 22:07
 Operator : SY/MD
 Sample : 03300-04 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 3

Min Area: 3 % of largest Peak

Start Thrs: 0.001

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 0

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

Signal : TIC: VL040496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.230	186	195	227	rBV	1230602	2232848	3.94%	1.943%
2	3.459	257	266	288	rBV	1632881	2549391	4.50%	2.219%
3	3.568	291	300	324	rVV	1457509	2487537	4.39%	2.165%
4	4.777	665	676	691	rBV	441499	743173	1.31%	0.647%
5	5.182	789	802	824	rBV	2301742	4525695	7.98%	3.939%
6	6.642	1242	1256	1274	rBV	3484515	6574955	11.60%	5.723%
7	9.204	2034	2053	2072	rBV4	843900	1997044	3.52%	1.738%
8	9.825	2231	2246	2255	rBV3	449341	1000267	1.76%	0.871%
9	10.484	2434	2451	2471	rVB5	287231	668394	1.18%	0.582%
10	11.101	2627	2643	2662	rVV3	420008	1092554	1.93%	0.951%
11	11.214	2662	2678	2696	rVB3	510577	1222332	2.16%	1.064%
12	11.455	2723	2753	2769	rBV	3797801	8938701	15.77%	7.780%
13	12.336	3014	3027	3050	rVB2	416400	1301733	2.30%	1.133%
14	13.764	3449	3471	3494	rBV	4078087	9405265	16.59%	8.186%
15	16.362	4247	4279	4303	rBV	18724243	56689922	100.00%	49.343%
16	16.465	4303	4311	4328	rVB3	247421	602189	1.06%	0.524%
17	17.278	4545	4564	4584	rBV6	536360	1344377	2.37%	1.170%
18	18.214	4837	4855	4876	rBV9	164533	661464	1.17%	0.576%
19	20.773	5623	5651	5698	rBV2	3161541	10851813	19.14%	9.445%




Sum of corrected areas: 114889654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040496.D
Acq On : 22 Jun 2023 22:07
Operator : SY/MD
Sample : 03300-04 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

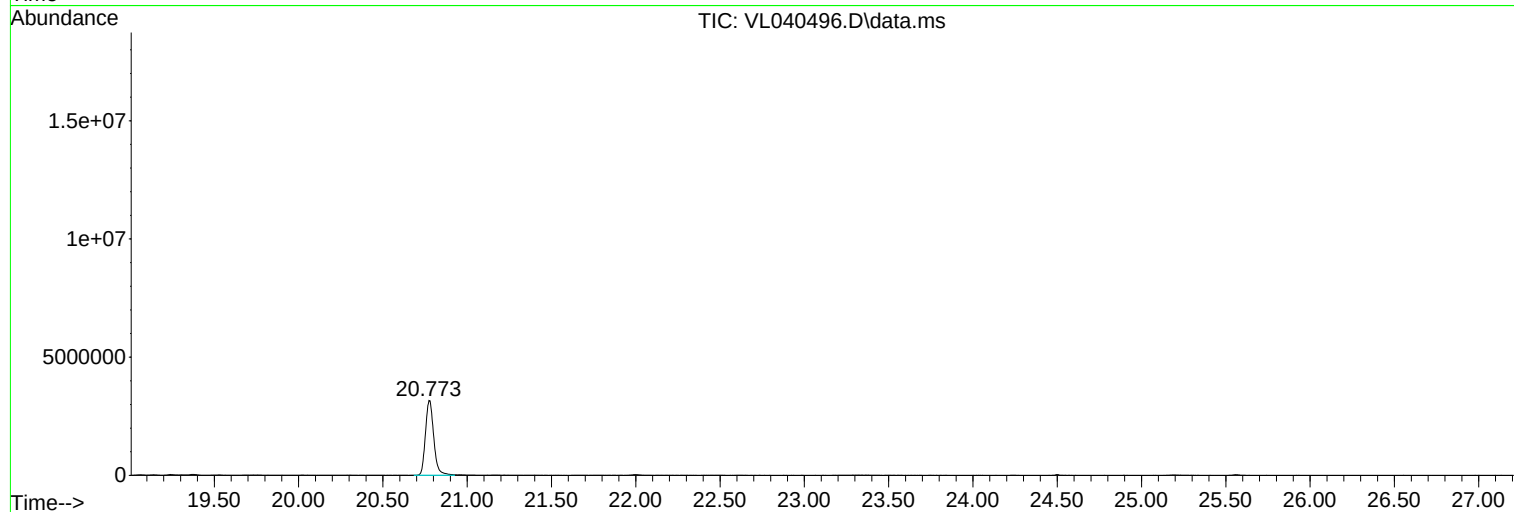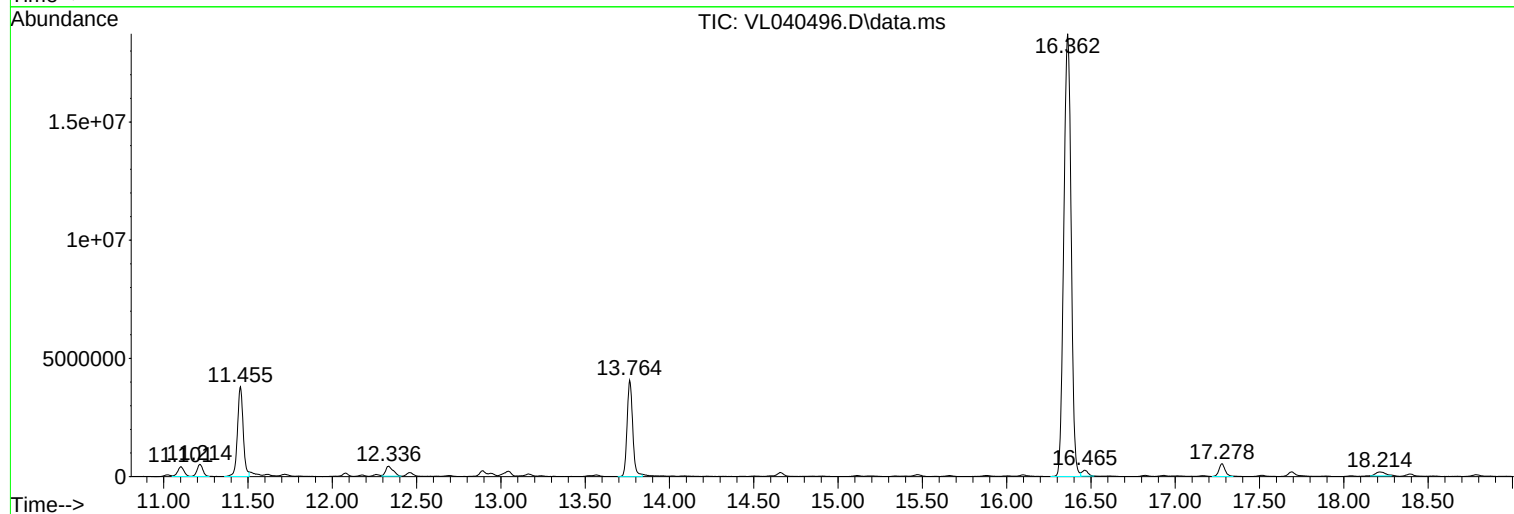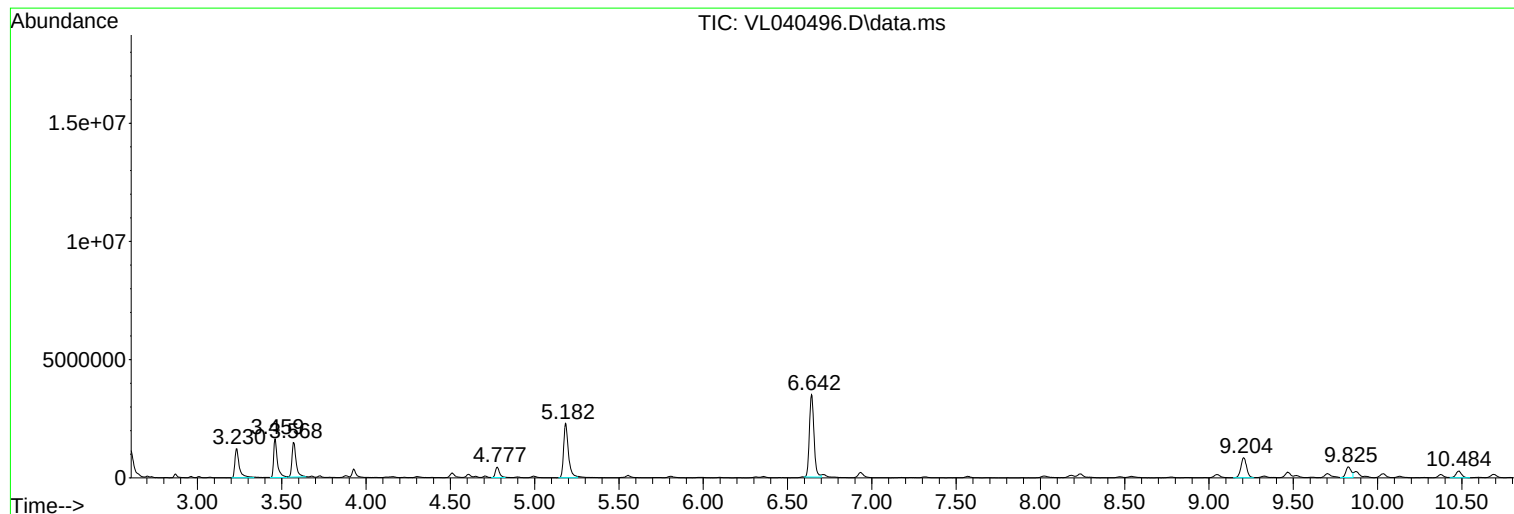

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040496.D
Acq On : 22 Jun 2023 22:07
Operator : SY/MD
Sample : 03300-04 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040496.D
Acq On : 22 Jun 2023 22:07
Operator : SY/MD
Sample : 03300-04 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc