
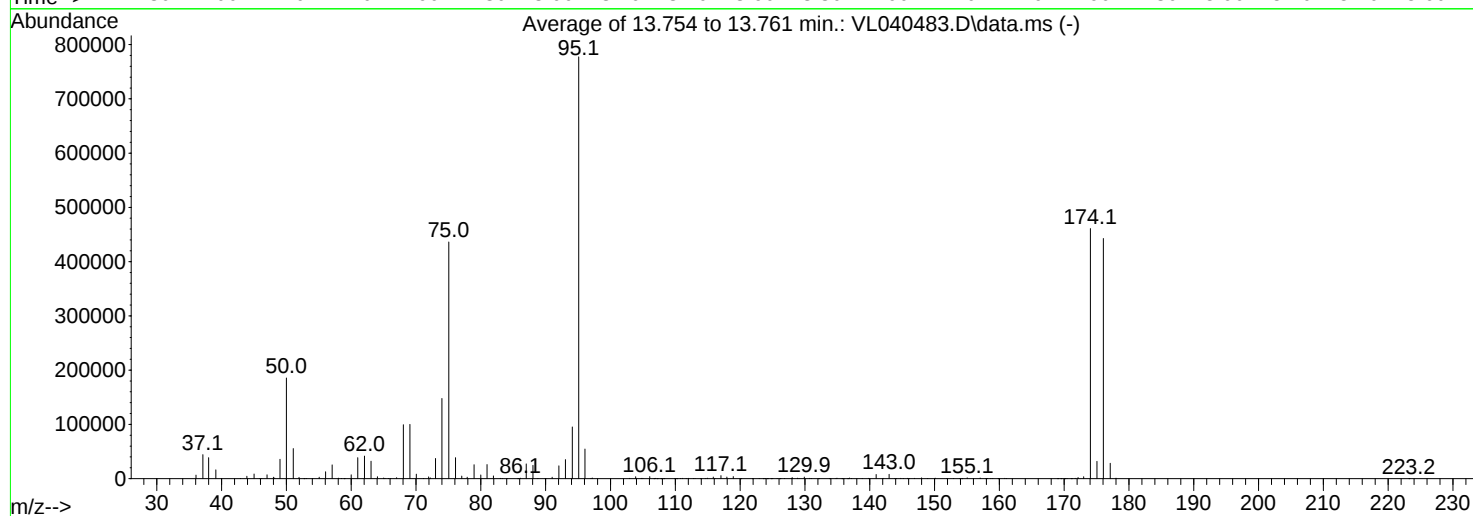


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062223\
Data File : VL040483.D
Acq On : 22 Jun 2023 12:42
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jun 06 06:22:12 2023

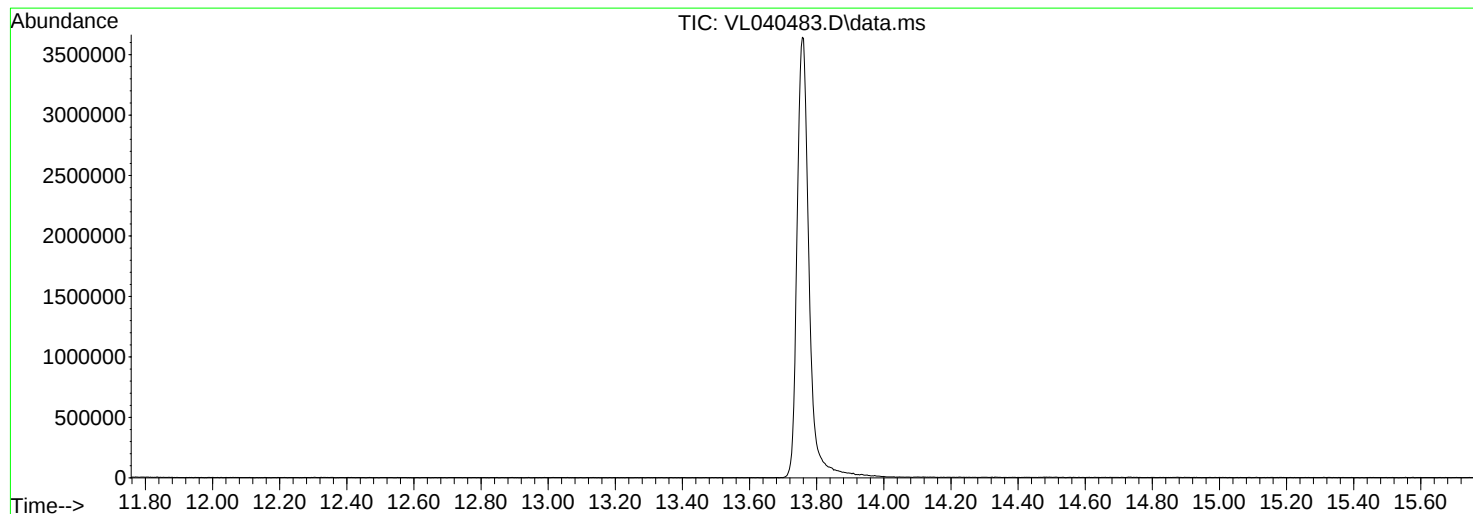

AutoFind: Scans 3468, 3469, 3470; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	185493	PASS
75	95	30	66	56.1	436245	PASS
95	95	100	100	100.0	777451	PASS
96	95	5	9	7.0	54525	PASS
173	174	0.00	2	0.8	3578	PASS
174	95	50	120	59.3	460885	PASS
175	174	4	9	6.9	31856	PASS
176	174	93	101	96.1	442752	PASS
177	176	5	9	6.4	28429	PASS

Average of 13.754 to 13.761 min.: VL040483.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6487	48.00	2548	57.05	25429	65.75	271
37.10	44344	48.20	1223	58.05	908	66.10	281
38.00	38688	49.00	35669	58.50	190	67.00	191
39.10	16160	50.00	185493	58.90	142	68.05	9945
40.00	388	51.05	55493	60.00	6955	69.05	99984
42.90	299	51.95	2371	61.00	38811	70.05	8271
43.90	4376	52.70	53	62.05	41491	71.15	475
45.00	8706	53.10	196	63.05	32240	71.95	3144
45.90	419	54.05	198	64.05	3473	72.20	1409
46.20	321	55.05	2547	65.00	1258	73.00	37208
47.00	7034	56.05	12706	65.20	623	74.00	147648

Average of 13.754 to 13.761 min.: VL040483.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.05	436245	85.70	143	96.05	54525	107.80	151
76.10	38659	86.10	1019	97.00	535	108.20	80
77.05	4673	87.00	27088	97.20	1283	109.90	384
77.90	2548	88.05	24627	102.95	513	110.20	159
78.95	25776	88.80	268	103.90	3492	110.80	265
80.00	6887	89.90	61	104.75	631	111.10	598
80.95	25824	91.00	2569	105.00	503	111.70	173
81.95	4899	92.05	23635	106.05	3864	112.05	552
83.00	508	93.05	35157	106.70	71	112.80	373
83.30	205	94.10	95323	106.95	543	113.05	256
84.05	353	95.10	777451	107.20	127	113.90	79

Average of 13.754 to 13.761 min.: VL040483.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.70	255	123.90	286	129.90	3024	137.20	278
114.95	790	124.20	149	130.75	644	138.85	196
115.85	3052	124.80	75	131.00	260	139.85	605
116.10	598	125.05	184	132.10	78	141.00	7813
117.05	5599	125.70	196	133.80	55	142.05	648
117.95	2995	126.15	124	134.80	299	143.00	8074
118.95	3858	126.85	164	134.95	879	143.85	215
120.10	157	127.90	1055	135.70	116	144.10	223
121.90	136	128.05	1908	136.00	262	144.80	498
122.95	325	128.85	1036	136.60	146	145.20	280
123.60	92	129.10	402	136.90	1136	145.85	571

Average of 13.754 to 13.761 min.: VL040483.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
146.10	354	157.05	1292	170.45	179		
146.90	697	157.90	141	171.10	148		
148.00	1533	158.15	394	171.70	559		
148.95	438	158.70	435	172.15	2227		
150.10	901	159.00	280	173.00	3578		
151.90	287	159.80	57	174.05	460885		
152.95	291	160.85	531	175.05	31856		
153.90	389	161.10	410	176.05	442752		
154.20	127	169.00	104	177.10	28429		
155.05	1550	169.50	56	178.00	776		
156.00	301	170.10	105	223.20	119		