

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062722\
 Data File : VL039388.D
 Acq On : 28 Jun 2022 11:11
 Operator : SY/AP
 Sample : N3453-01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-1

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 06/29/2022
 Supervised By : Mahesh Dadoda 06/30/2022

Quant Time: Jun 29 06:05:36 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jun 01 01:22:18 2022

QLast Update : Wed Jun 01 01:22:18 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.655	49	1049977	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.160	114	2926712	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.066	117	2644575	10.000	ppbv	-0.03
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.394	95	2043568	9.347	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	93.500%
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	3.044	85	44158m	0.239	ppbv	
3) Chlorodifluoromethane	2.986	51	31184m	0.233	ppbv	
4) Chloromethane	3.131	50	15148	0.221	ppbv	92
9) Propene	3.012	41	222532m	3.820	ppbv	
10) Heptane	8.105	43	49933	0.367	ppbv	98
11) Trichlorofluoromethane	3.941	101	37743	0.226	ppbv	91
13) Ethanol	3.591	45	483855	152.305	ppbv #	100
15) Acetone	3.838	43	1103904	10.093	ppbv	100
17) tert-Butyl alcohol	4.288	59	20870m	0.246	ppbv	
19) Isopropyl Alcohol	3.957	45	43658m	0.851	ppbv	
20) Methylene Chloride	4.337	84	1802486	39.106	ppbv	95
26) Hexane	5.674	57	2739789	25.291	ppbv #	39
27) Carbon Disulfide	4.539	76	70391m	0.627	ppbv	
30) Cyclohexane	7.124	84	44070m	0.484	ppbv	
34) 2-Butanone	5.234	43	121873	0.766	ppbv	96
36) Benzene	6.877	78	176245m	0.742	ppbv	
52) Tetrachloroethene	11.198	164	5172m	0.056	ppbv	
53) Toluene	9.790	91	752795	2.751	ppbv	99
58) Ethyl Benzene	12.684	91	174436m	0.479	ppbv	
59) m/p-Xylene	12.941	91	567403	1.769	ppbv	96
60) o-Xylene	13.668	91	213956m	0.710	ppbv	
62) Isopropylbenzene	14.639	105	65410m	0.146	ppbv	
64) n-propylbenzene	15.542	120	17425	0.158	ppbv	86
69) p-Isopropyltoluene	17.626	119	55056m	0.117	ppbv	
70) n-Butylbenzene	18.523	91	71817m	0.148	ppbv	
72) 4-Ethyltoluene	15.815	105	126379m	0.358	ppbv	
73) 1,3,5-Trimethylbenzene	15.976	105	219956	0.690	ppbv	95
74) 1,2,4-Trimethylbenzene	16.735	105	974363	2.740	ppbv #	62
79) Naphthalene	22.169	128	54606m	0.199	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062722\
Data File : VL039388.D
Acq On : 28 Jun 2022 11:11
Operator : SY/AP
Sample : N3453-01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SG-1

Quant Time: Jun 29 06:05:36 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun
QLast Update : Wed Jun 01 01:22:18 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

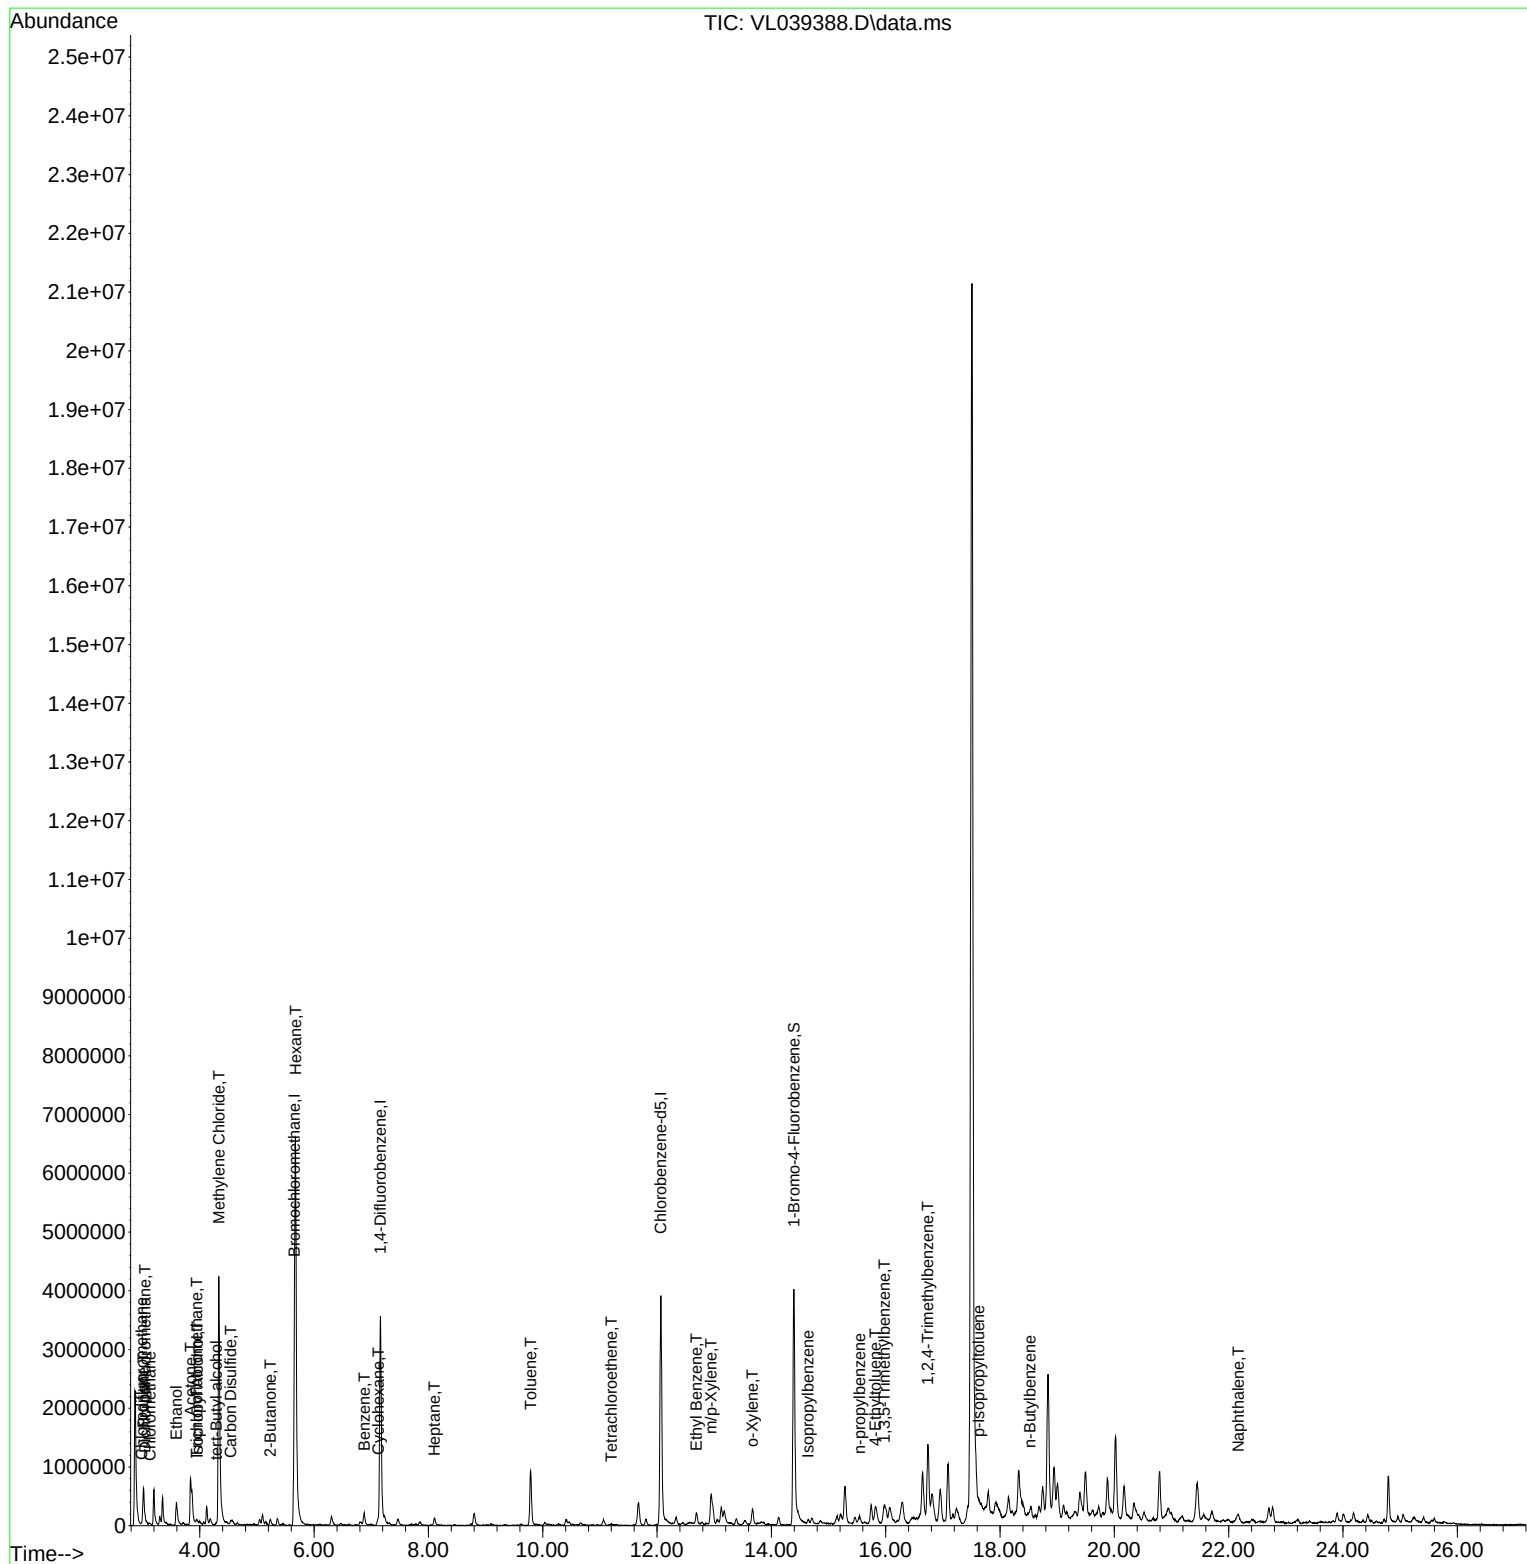

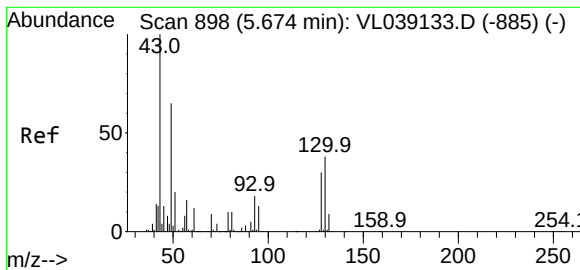

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.655 min Scan# 80
Delta R.T. -0.019 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1

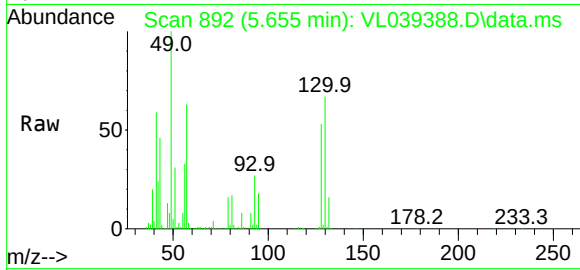

Tgt Ion: 49 Resp: 104997
Ion Ratio Lower Upper
49 100
128 53.7 24.7 74.1
130 68.6 31.4 94.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

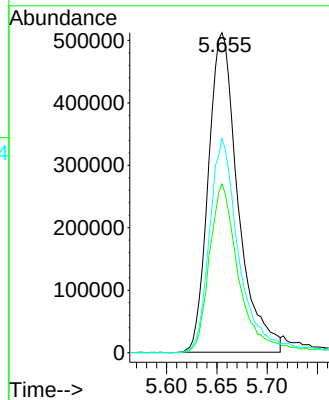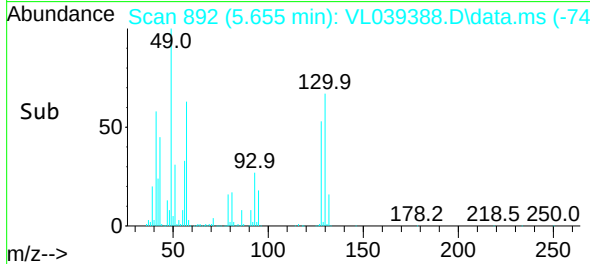

#2
Dichlorodifluoromethane
Concen: 0.239 ppbv m
RT: 3.044 min Scan# 80
Delta R.T. -0.016 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

Tgt Ion: 85 Resp: 44158
Ion Ratio Lower Upper
85 100
87 23.7 26.9 40.3

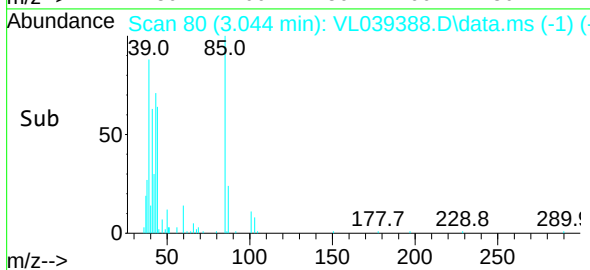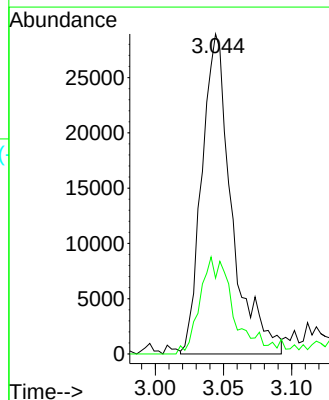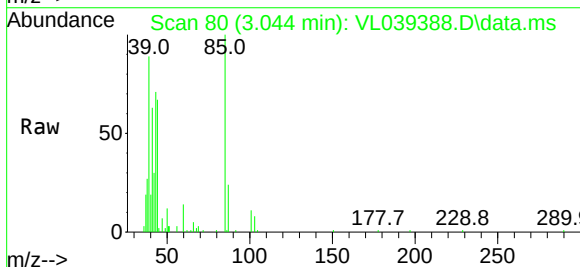

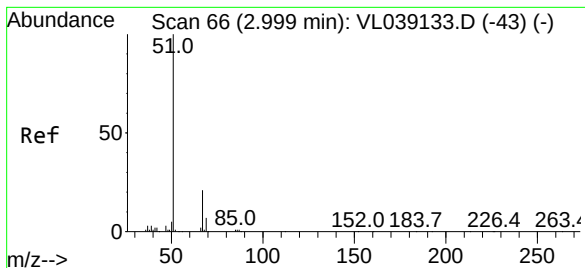





#3
Chlorodifluoromethane
Concen: 0.233 ppbv m
RT: 2.986 min Scan# 61
Delta R.T. -0.013 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tgt Ion: 51 Resp: 31184
Ion Ratio Lower Upper
51 100
67 21.6 16.2 24.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

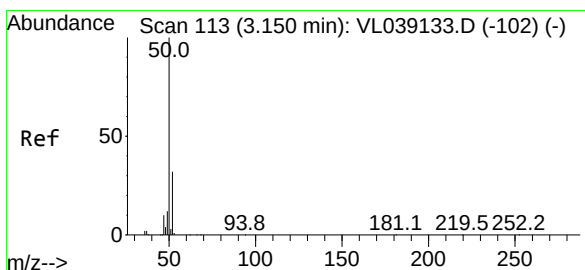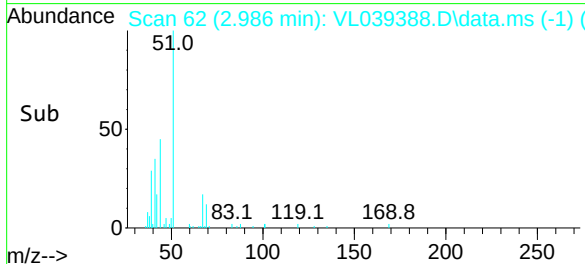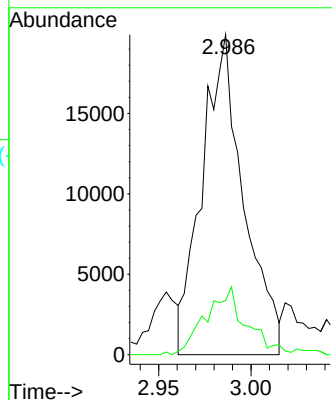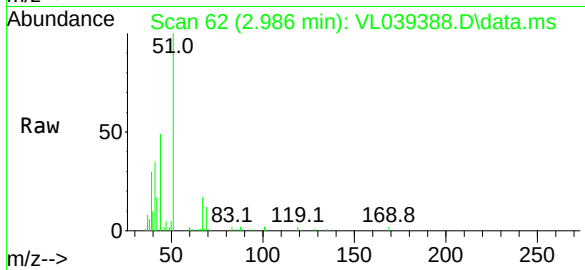

#4
Chloromethane
Concen: 0.221 ppbv
RT: 3.131 min Scan# 107
Delta R.T. -0.019 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11


Tgt Ion: 50 Resp: 15148
Ion Ratio Lower Upper
50 100
52 27.8 25.9 38.9

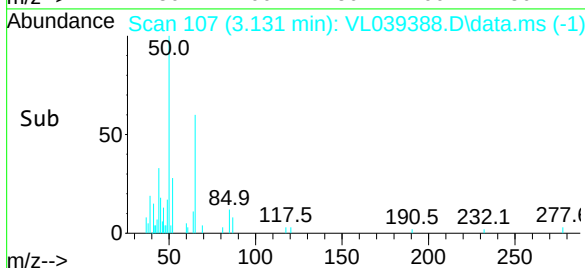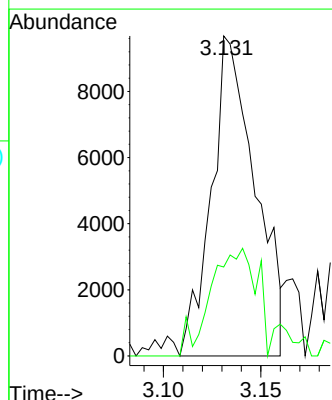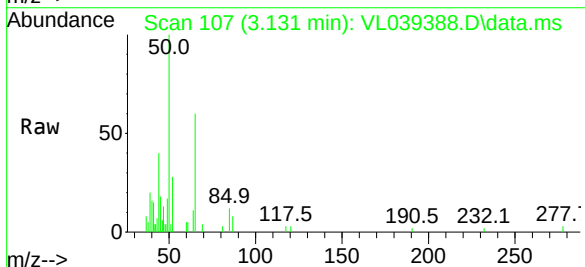



#9
 Propene
 Concen: 3.820 ppbv m
 RT: 3.012 min Scan# 70
 Delta R.T. -0.006 min
 Lab File: VL039388.D
 Acq: 28 Jun 2022 11:11




Instrument :
 MSVOA_L
 ClientSampleId :
 SG-1



Tgt Ion: 41 Resp: 22253
 Ion Ratio Lower Upper
 41 100
 42 50.7 55.4 83.2




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
 Supervised By :Mahesh Dadoda 06/30/2022

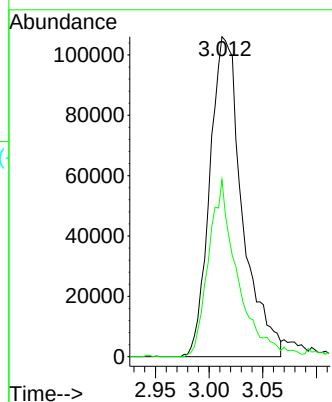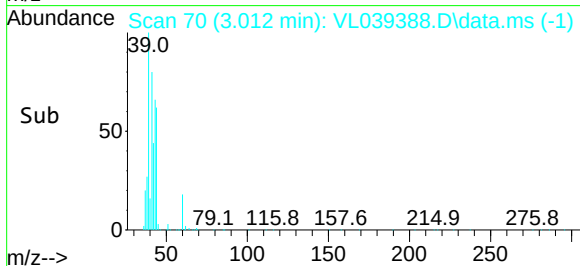

#10
 Heptane
 Concen: 0.367 ppbv
 RT: 8.105 min Scan# 1654
 Delta R.T. -0.022 min
 Lab File: VL039388.D
 Acq: 28 Jun 2022 11:11


Tgt Ion: 43 Resp: 49933
 Ion Ratio Lower Upper
 43 100
 57 50.6 41.4 62.2

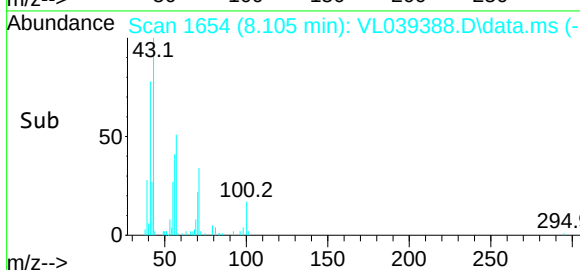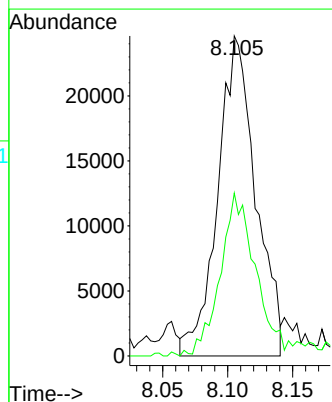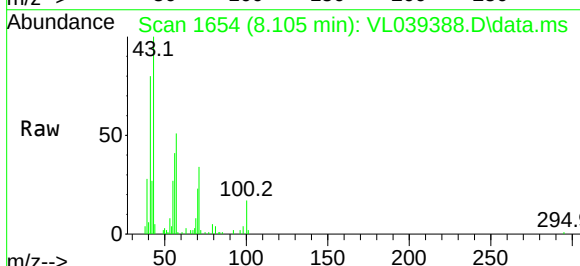

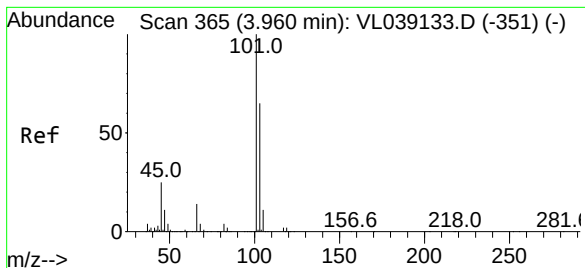

#11
Trichlorofluoromethane
Concen: 0.226 ppbv
RT: 3.941 min Scan# 30
Delta R.T. -0.019 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1

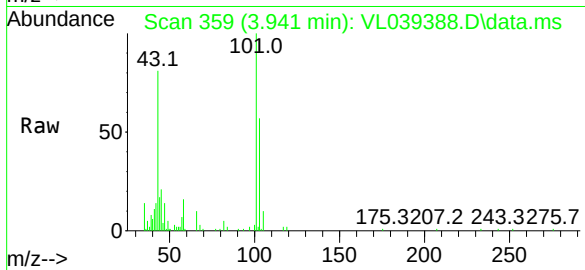

Tgt Ion:101 Resp: 3774
Ion Ratio Lower Upper
101 100
103 57.3 51.7 77.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

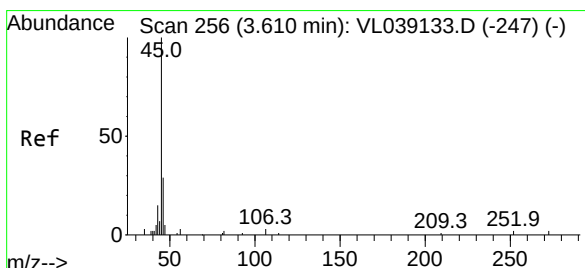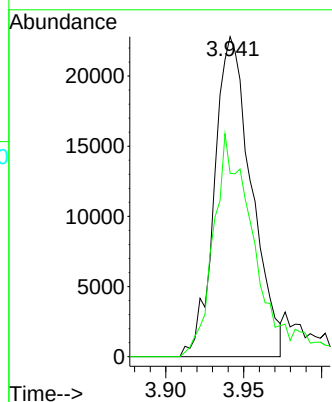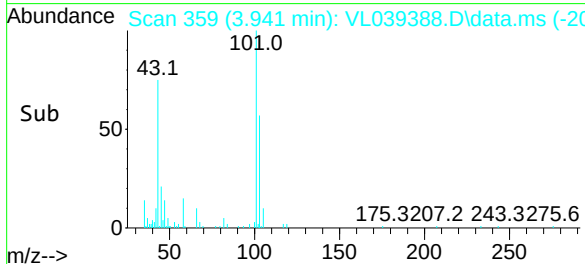

#13
Ethanol
Concen: 152.305 ppbv
RT: 3.591 min Scan# 250
Delta R.T. -0.019 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

Tgt Ion: 45 Resp: 483855
Ion Ratio Lower Upper
45 100
46 38.0 0.0 0.0#

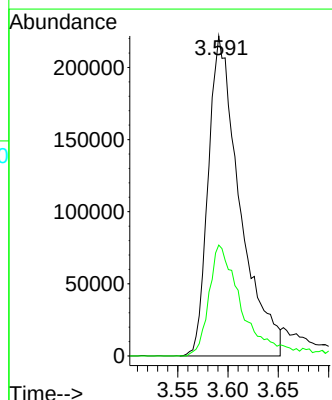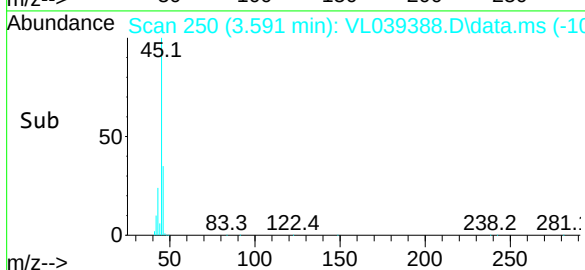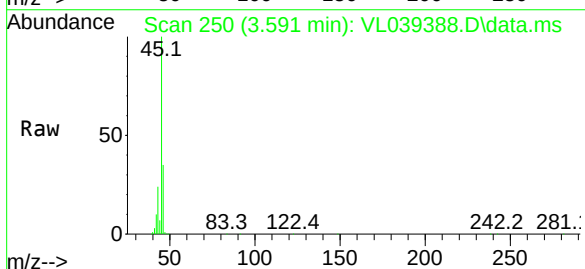

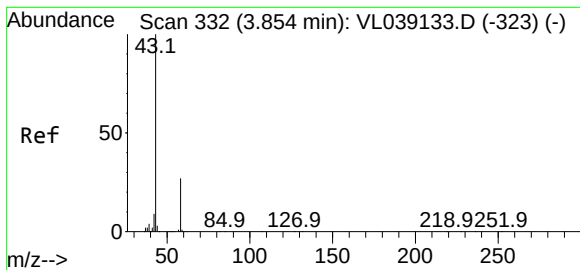





#15
Acetone
Concen: 10.093 ppbv
RT: 3.838 min Scan# 311
Delta R.T. -0.016 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

Instrument : MSVOA_L
ClientSampleId : SG-1

Tgt Ion: 43 Resp: 1103904
Ion Ratio Lower Upper
43 100
58 28.3 22.5 33.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

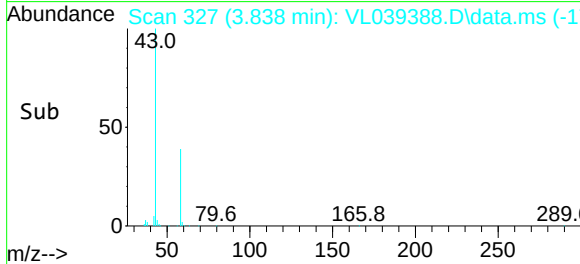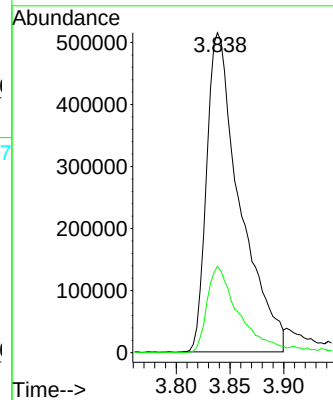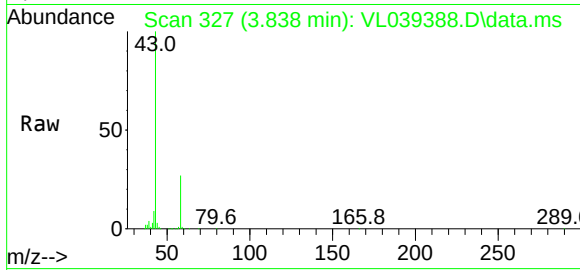

#17
tert-Butyl alcohol
Concen: 0.246 ppbv m
RT: 4.288 min Scan# 467
Delta R.T. 0.000 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

Tgt Ion: 59 Resp: 20870
Ion Ratio Lower Upper
59 100
57 0.0 9.1 13.7#

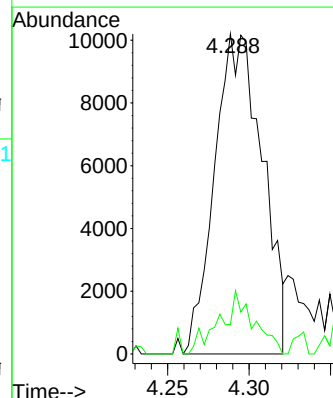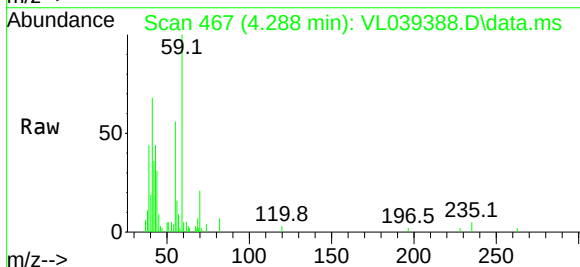







#19
Isopropyl Alcohol
Concen: 0.851 ppbv m
RT: 3.957 min Scan# 30
Delta R.T. -0.006 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tgt Ion: 45 Resp: 43658
Ion Ratio Lower Upper
45 100
58 696.2 1.8 2.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

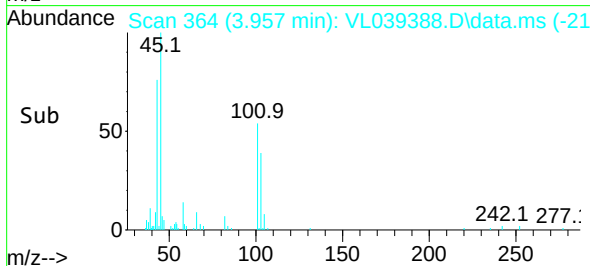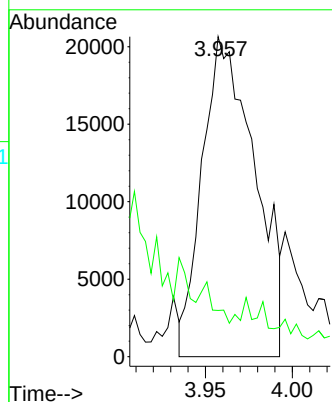

#20
Methylene Chloride
Concen: 39.106 ppbv
RT: 4.337 min Scan# 482
Delta R.T. -0.016 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11


Tgt Ion: 84 Resp: 1802486
Ion Ratio Lower Upper
84 100
49 147.4 111.1 166.7
51 45.1 35.3 52.9
86 62.4 51.9 77.9

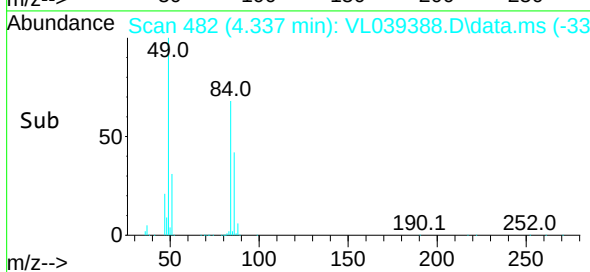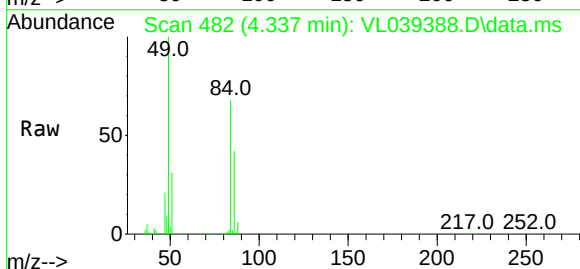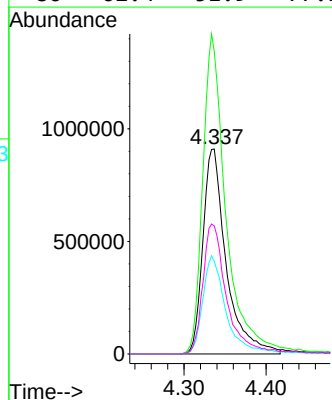



#26
Hexane
Concen: 25.291 ppbv
RT: 5.674 min Scan# 898
Delta R.T. -0.019 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1



Tgt Ion: 57 Resp: 2739789
Ion Ratio Lower Upper
57 100
41 91.2 72.4 108.6
43 70.0 187.0 280.6
56 53.3 41.8 62.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

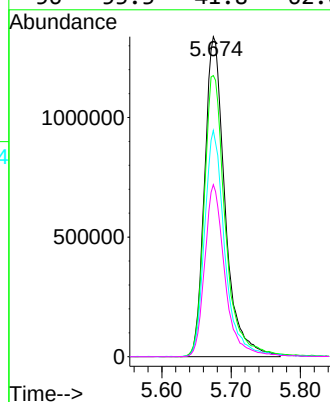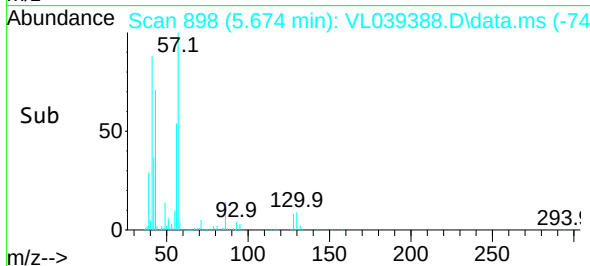

#27
Carbon Disulfide
Concen: 0.627 ppbv m
RT: 4.539 min Scan# 545
Delta R.T. -0.019 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11


Tgt Ion: 76 Resp: 70391
Ion Ratio Lower Upper
76 100
44 32.9 14.4 21.6
78 11.4 7.7 11.5

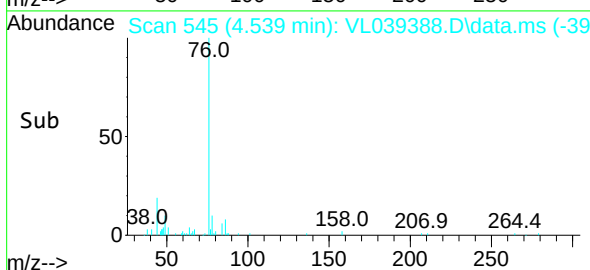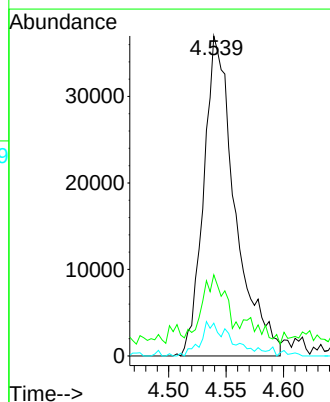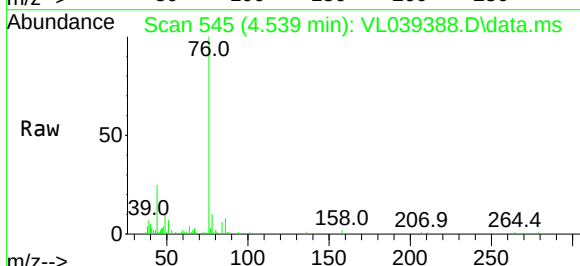

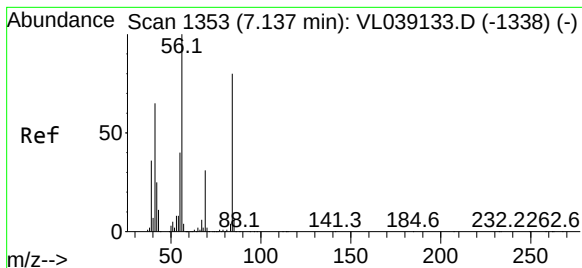

#30
Cyclohexane
Concen: 0.484 ppbv m
RT: 7.124 min Scan# 1349
Delta R.T. -0.013 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1

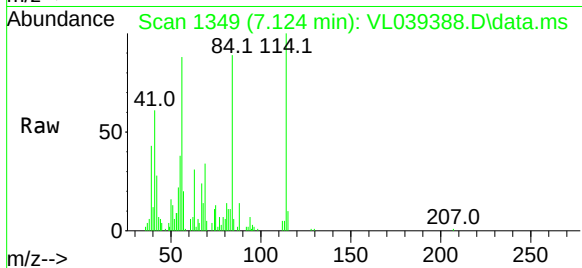


Tgt Ion: 84 Resp: 44070
Ion Ratio Lower Upper
84 100
56 0.0 110.6 165.8
41 78.6 68.9 103.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

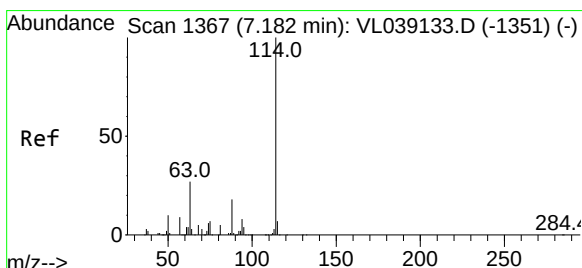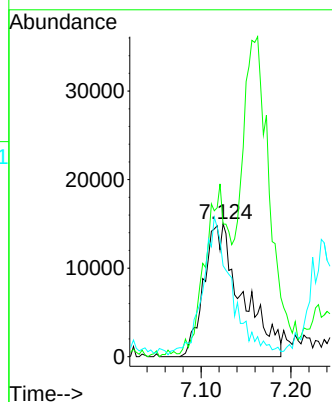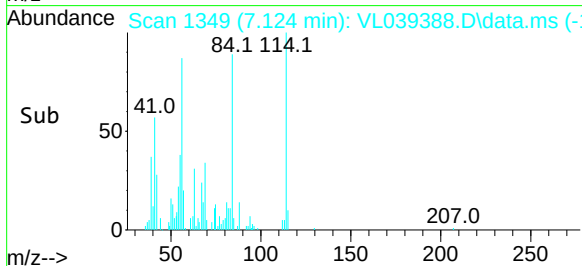


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.160 min Scan# 1360
Delta R.T. -0.022 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

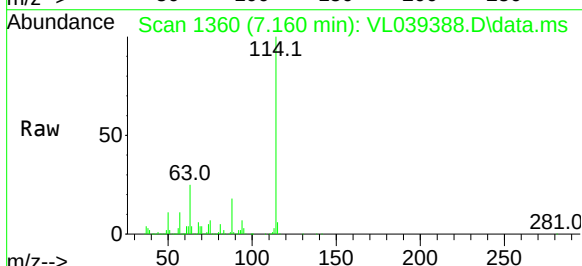


Tgt Ion:114 Resp: 2926712
Ion Ratio Lower Upper
114 100
63 25.3 21.7 32.5
88 18.2 14.8 22.2

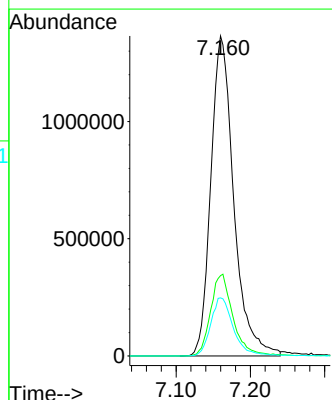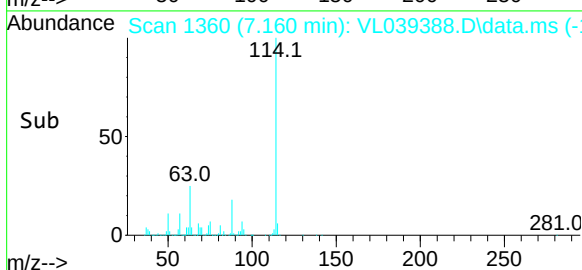

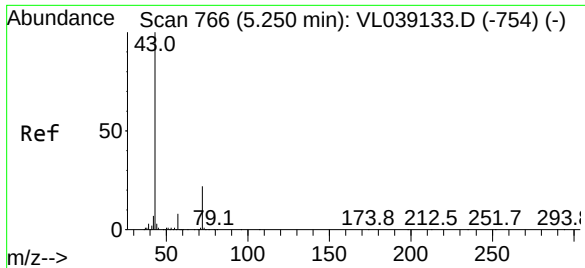

#34
2-Butanone
Concen: 0.766 ppbv
RT: 5.234 min Scan# 761
Delta R.T. -0.016 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1

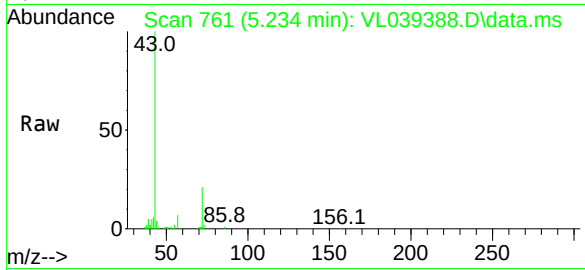

Tgt Ion: 43 Resp: 12187
Ion Ratio Lower Upper
43 100
72 24.7 18.2 27.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

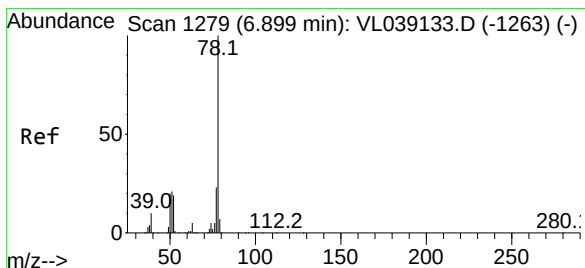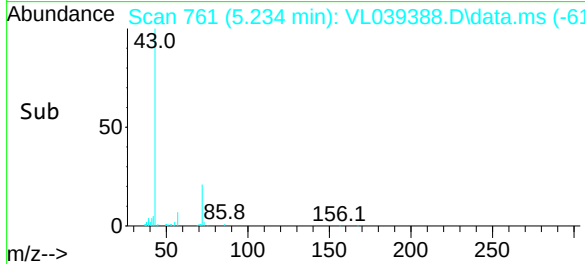

#36
Benzene
Concen: 0.742 ppbv m
RT: 6.877 min Scan# 1272
Delta R.T. -0.022 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11


Tgt Ion: 78 Resp: 176245
Ion Ratio Lower Upper
78 100
77 23.5 18.6 27.8
50 17.2 15.8 23.8

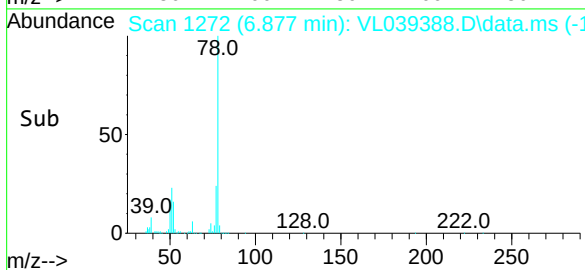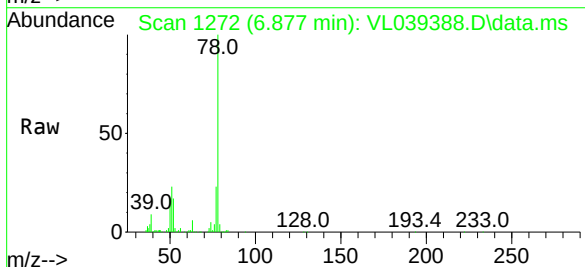



#52
Tetrachloroethene
Concen: 0.056 ppbv m
RT: 11.198 min Scan# 2616
Delta R.T. -0.032 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1




Tgt Ion:164 Resp: 5172
Ion Ratio Lower Upper
164 100
166 227.0 96.3 144.5
129 154.3 82.5 123.7
131 96.0 82.1 123.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

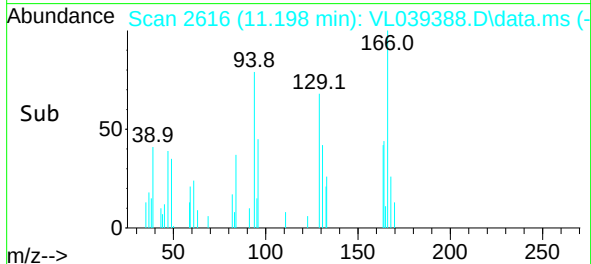


#53
Toluene
Concen: 2.751 ppbv
RT: 9.790 min Scan# 2178
Delta R.T. -0.022 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

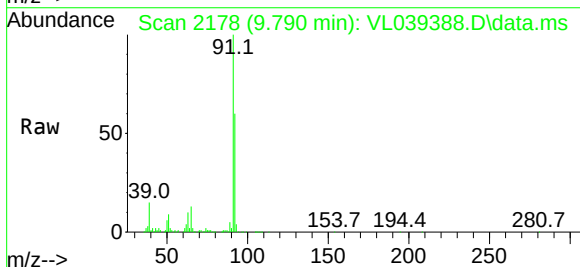


Tgt Ion: 91 Resp: 752795
Ion Ratio Lower Upper
91 100
92 59.2 48.1 72.1

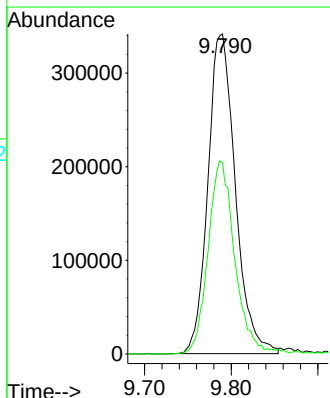

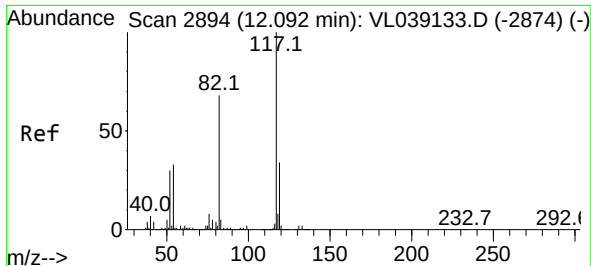

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.066 min Scan# 2886
Delta R.T. -0.026 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument : MSVOA_L
ClientSampleId : SG-1




Tgt Ion: 117 Resp: 264457
Ion Ratio Lower Upper
117 100
82 65.3 55.1 82.7
119 33.3 24.7 37.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

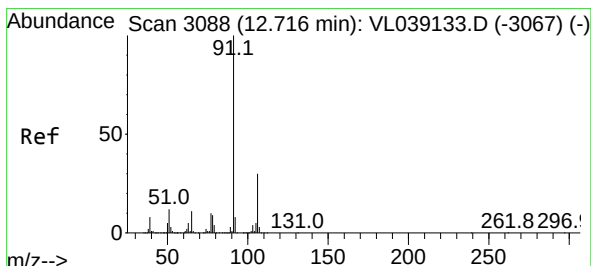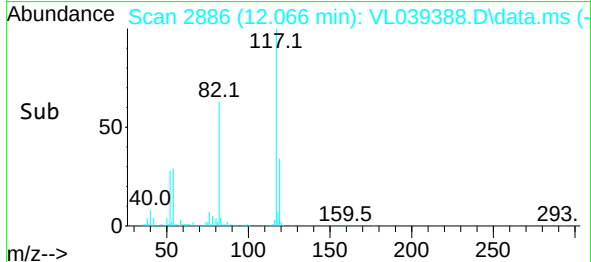


#58
Ethyl Benzene
Concen: 0.479 ppbv m
RT: 12.684 min Scan# 3078
Delta R.T. -0.032 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

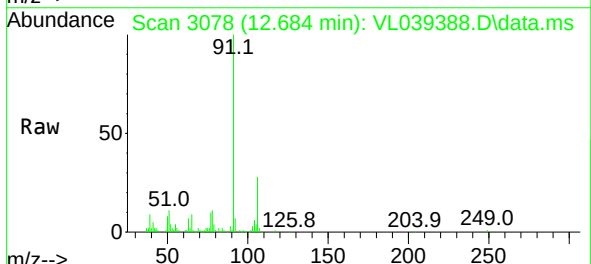


Tgt Ion: 91 Resp: 174436
Ion Ratio Lower Upper
91 100
106 27.8 24.2 36.4

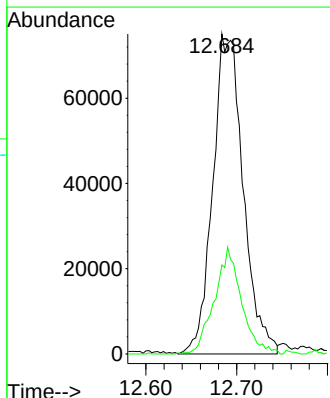



#59
m/p-Xylene
Concen: 1.769 ppbv
RT: 12.941 min Scan# 3176
Delta R.T. -0.058 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1



Tgt Ion: 91 Resp: 56740
Ion Ratio Lower Upper
91 100
106 45.2 34.3 51.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

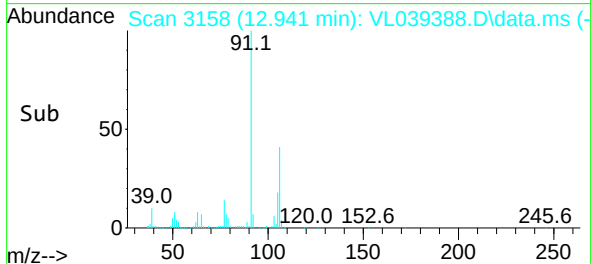

#60
o-Xylene
Concen: 0.710 ppbv m
RT: 13.668 min Scan# 3384
Delta R.T. -0.029 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11


Tgt Ion: 91 Resp: 213956
Ion Ratio Lower Upper
91 100
106 0.0 22.3 66.9#

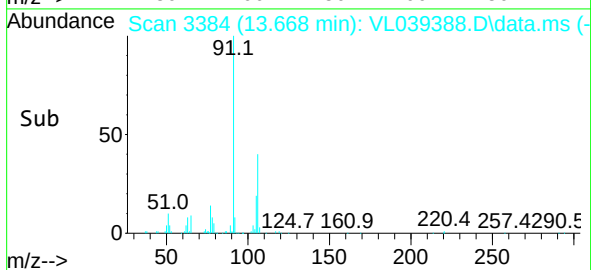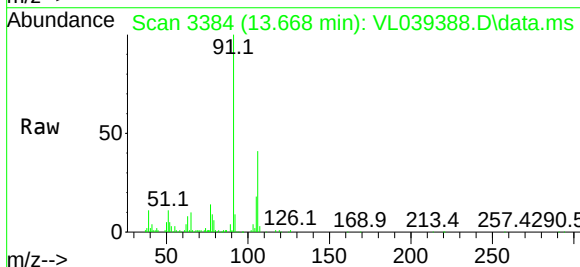



#62
Isopropylbenzene
Concen: 0.146 ppbv m
RT: 14.639 min Scan# 3686
Delta R.T. -0.032 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1




Tgt Ion:105 Resp: 65410
Ion Ratio Lower Upper
105 100
120 0.0 20.3 30.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

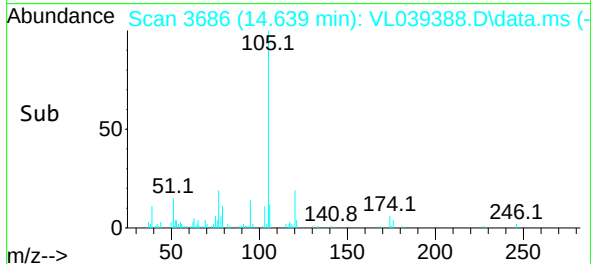


#64
n-propylbenzene
Concen: 0.158 ppbv
RT: 15.542 min Scan# 3967
Delta R.T. -0.019 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

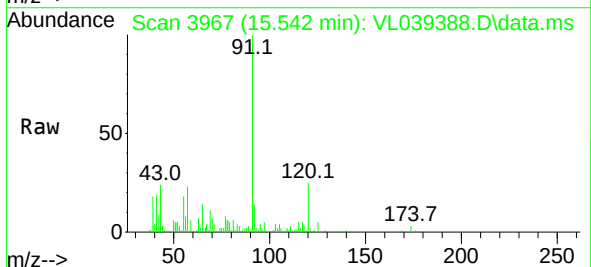


Tgt Ion:120 Resp: 17425
Ion Ratio Lower Upper
120 100
91 522.3 388.4 582.6

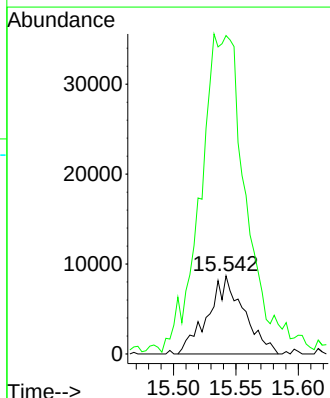

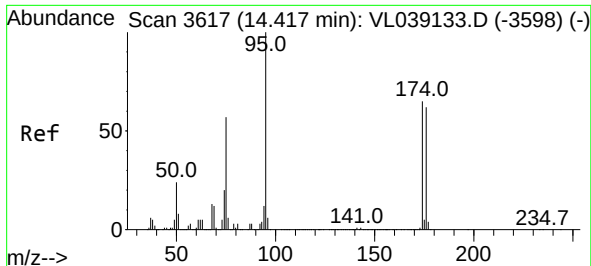

#68
1-Bromo-4-Fluorobenzene
Concen: 9.347 ppbv
RT: 14.394 min Scan# 3610
Delta R.T. -0.022 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1




Tgt Ion: 95 Resp: 204356
Ion Ratio Lower Upper
95 100
174 69.6 53.8 80.8
175 5.3 4.1 6.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

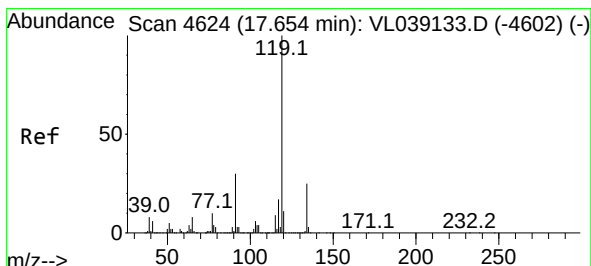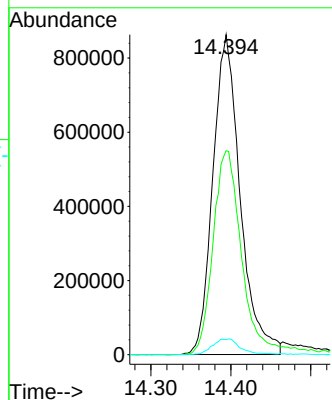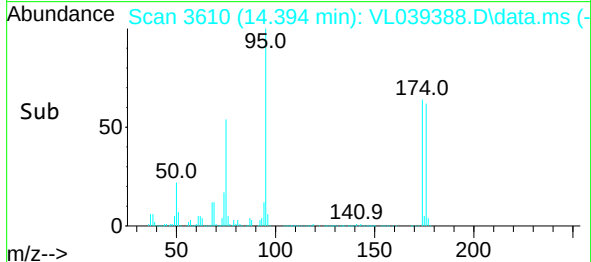


#69
p-Isopropyltoluene
Concen: 0.117 ppbv m
RT: 17.626 min Scan# 4615
Delta R.T. -0.029 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

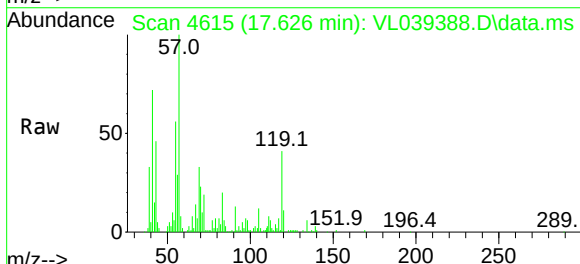


Tgt Ion:119 Resp: 55056
Ion Ratio Lower Upper
119 100
134 0.0 20.4 30.6#
91 0.0 24.2 36.4#

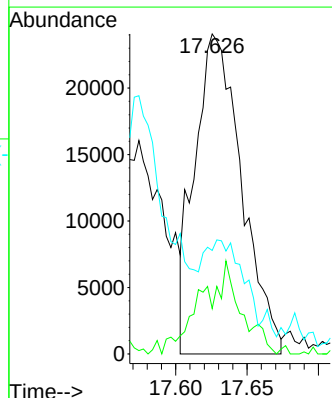

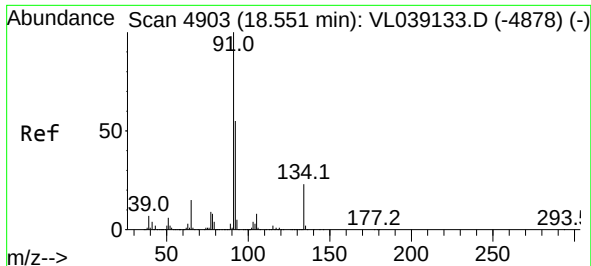

#70
n-Butylbenzene
Concen: 0.148 ppbv m
RT: 18.523 min Scan# 41
Delta R.T. -0.029 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11




Instrument :
MSVOA_L
ClientSampleId :
SG-1




Tgt Ion: 91 Resp: 7181
Ion Ratio Lower Upper
91 100
92 38.9 43.6 65.4
134 0.0 17.7 26.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

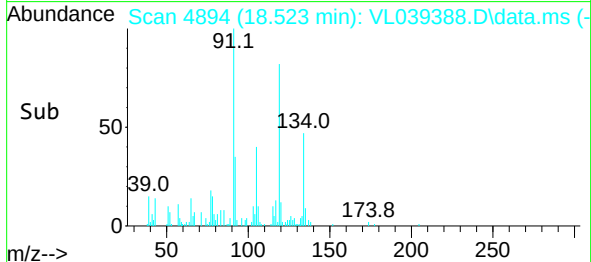


#72
4-Ethyltoluene
Concen: 0.358 ppbv m
RT: 15.815 min Scan# 4052
Delta R.T. -0.026 min
Lab File: VL039388.D
Acq: 28 Jun 2022 11:11

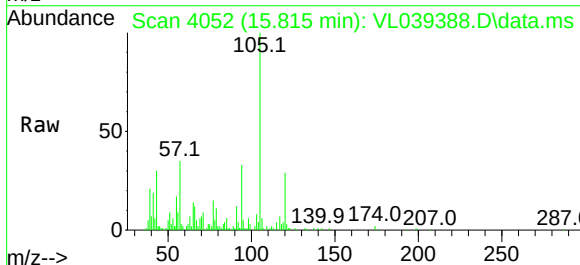

Tgt Ion:105 Resp: 126379
Ion Ratio Lower Upper
105 100
120 28.6 23.9 35.9
91 0.0 10.6 16.0
77 14.3 11.7 17.5

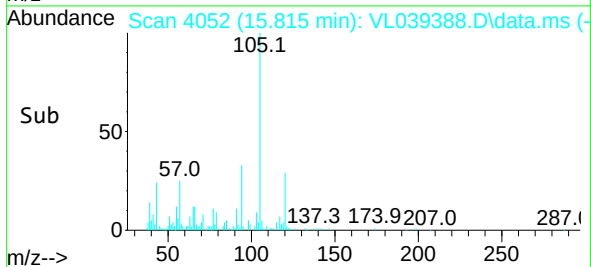



#73

1,3,5-Trimethylbenzene

Concen: 0.690 ppbv

RT: 15.976 min Scan# 4108

Delta R.T. -0.019 min

Lab File: VL039388.D

Acq: 28 Jun 2022 11:11

Instrument :

MSVOA_L

ClientSampleId :

SG-1

Tgt Ion:105 Resp: 219950

Ion Ratio Lower Upper

105 100





120 42.9 36.7 55.1

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022

Supervised By :Mahesh Dadoda 06/30/2022

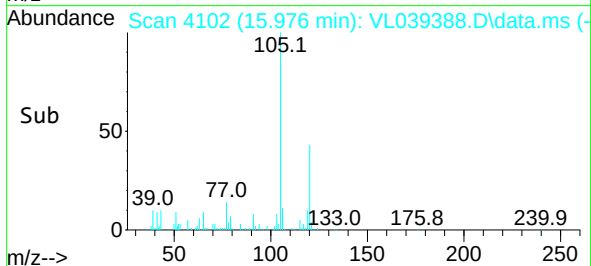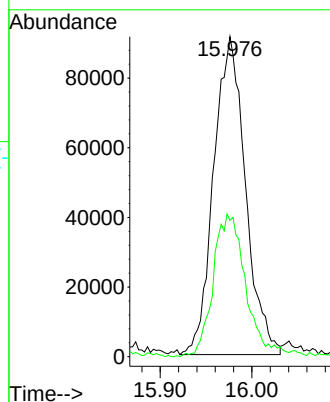

#74

1,2,4-Trimethylbenzene

Concen: 2.740 ppbv

RT: 16.735 min Scan# 4338

Delta R.T. -0.026 min

Lab File: VL039388.D

Acq: 28 Jun 2022 11:11

Tgt Ion:105 Resp: 974363




Ion Ratio Lower Upper


105 100

120 39.5 38.1 57.1

91 10.6 47.4 71.0#

77 12.4 19.5 29.3#

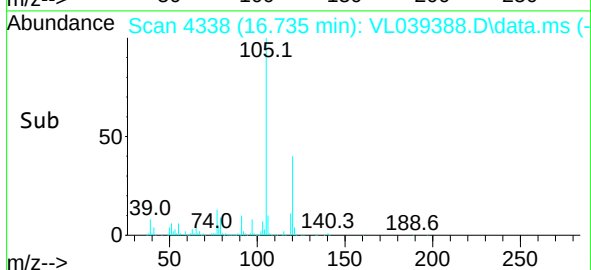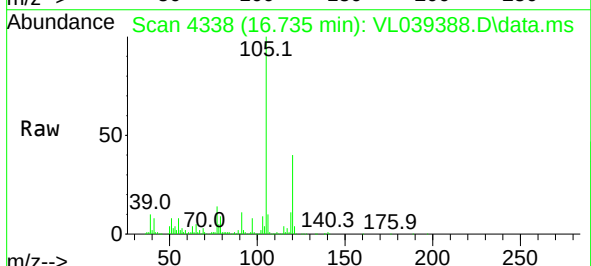

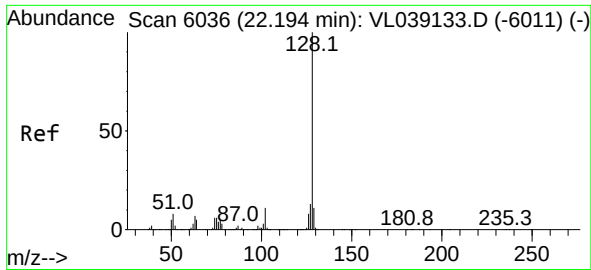

#79

Naphthalene

Concen: 0.199 ppbv m

RT: 22.169 min Scan# 60

Delta R.T. -0.026 min

Lab File: VL039388.D


Acq: 28 Jun 2022 11:11

Instrument :

MSVOA_L

ClientSampleId :

SG-1

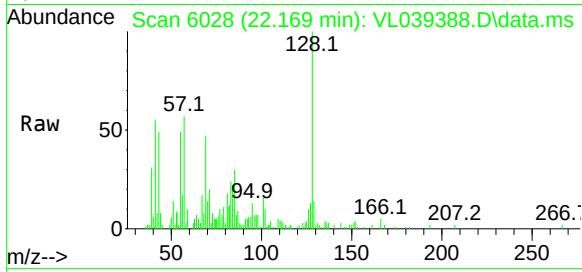

Tgt Ion:128 Resp: 54600

Ion Ratio Lower Upper

128 100

127 12.8 10.4 15.6

129 14.3 9.0 13.6

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022

Supervised By :Mahesh Dadoda 06/30/2022

