

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062722\
 Data File : VL039389.D
 Acq On : 28 Jun 2022 11:52
 Operator : SY/AP
 Sample : N3453-02
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022
 Supervised By :Mahesh Dadoda 06/30/2022

Quant Time: Jun 29 06:05:52 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022

QLast Update : Wed Jun 01 01:22:18 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.652	49	1142333	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.160	114	3158061	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.066	117	2708000	10.000	ppbv	-0.03
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.394	95	2131503	9.521	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.200%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	3.041	85	34352	0.171	ppbv	97
3) Chlorodifluoromethane	2.983	51	31244m	0.215	ppbv	
4) Chloromethane	3.140	50	10263m	0.137	ppbv	
9) Propene	3.018	41	212674m	3.356	ppbv	
10) Heptane	8.105	43	86981m	0.588	ppbv	
11) Trichlorofluoromethane	3.941	101	40519m	0.223	ppbv	
13) Ethanol	3.591	45	419550	121.386	ppbv #	100
15) Acetone	3.835	43	2068840	17.386	ppbv	96
17) tert-Butyl alcohol	4.285	59	21615m	0.234	ppbv	
19) Isopropyl Alcohol	3.960	45	40068m	0.718	ppbv	
20) Methylene Chloride	4.333	84	260229	5.189	ppbv	94
26) Hexane	5.674	57	3083503	26.162	ppbv #	39
27) Carbon Disulfide	4.542	76	72313m	0.592	ppbv	
30) Cyclohexane	7.111	84	48638m	0.491	ppbv	
34) 2-Butanone	5.230	43	122358	0.713	ppbv	93
36) Benzene	6.870	78	280445m	1.094	ppbv	
52) Tetrachloroethene	11.208	164	14324m	0.143	ppbv	
53) Toluene	9.783	91	988490	3.348	ppbv	99
58) Ethyl Benzene	12.690	91	213193	0.572	ppbv #	87
59) m/p-Xylene	12.947	91	694191	2.113	ppbv	94
60) o-Xylene	13.671	91	274858	0.890	ppbv	98
62) Isopropylbenzene	14.645	105	77257m	0.168	ppbv	
64) n-propylbenzene	15.532	120	22078m	0.196	ppbv	
67) sec-Butylbenzene	17.272	105	63328m	0.111	ppbv	
69) p-Isopropyltoluene	17.629	119	67643m	0.140	ppbv	
70) n-Butylbenzene	18.535	91	91244m	0.184	ppbv	
72) 4-Ethyltoluene	15.815	105	144360	0.399	ppbv #	96
73) 1,3,5-Trimethylbenzene	15.976	105	264653	0.811	ppbv	99
74) 1,2,4-Trimethylbenzene	16.741	105	1081333	2.970	ppbv #	63
79) Naphthalene	22.175	128	69709m	0.249	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062722\
Data File : VL039389.D
Acq On : 28 Jun 2022 11:52
Operator : SY/AP
Sample : N3453-02
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SG-2

Quant Time: Jun 29 06:05:52 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun
QLast Update : Wed Jun 01 01:22:18 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

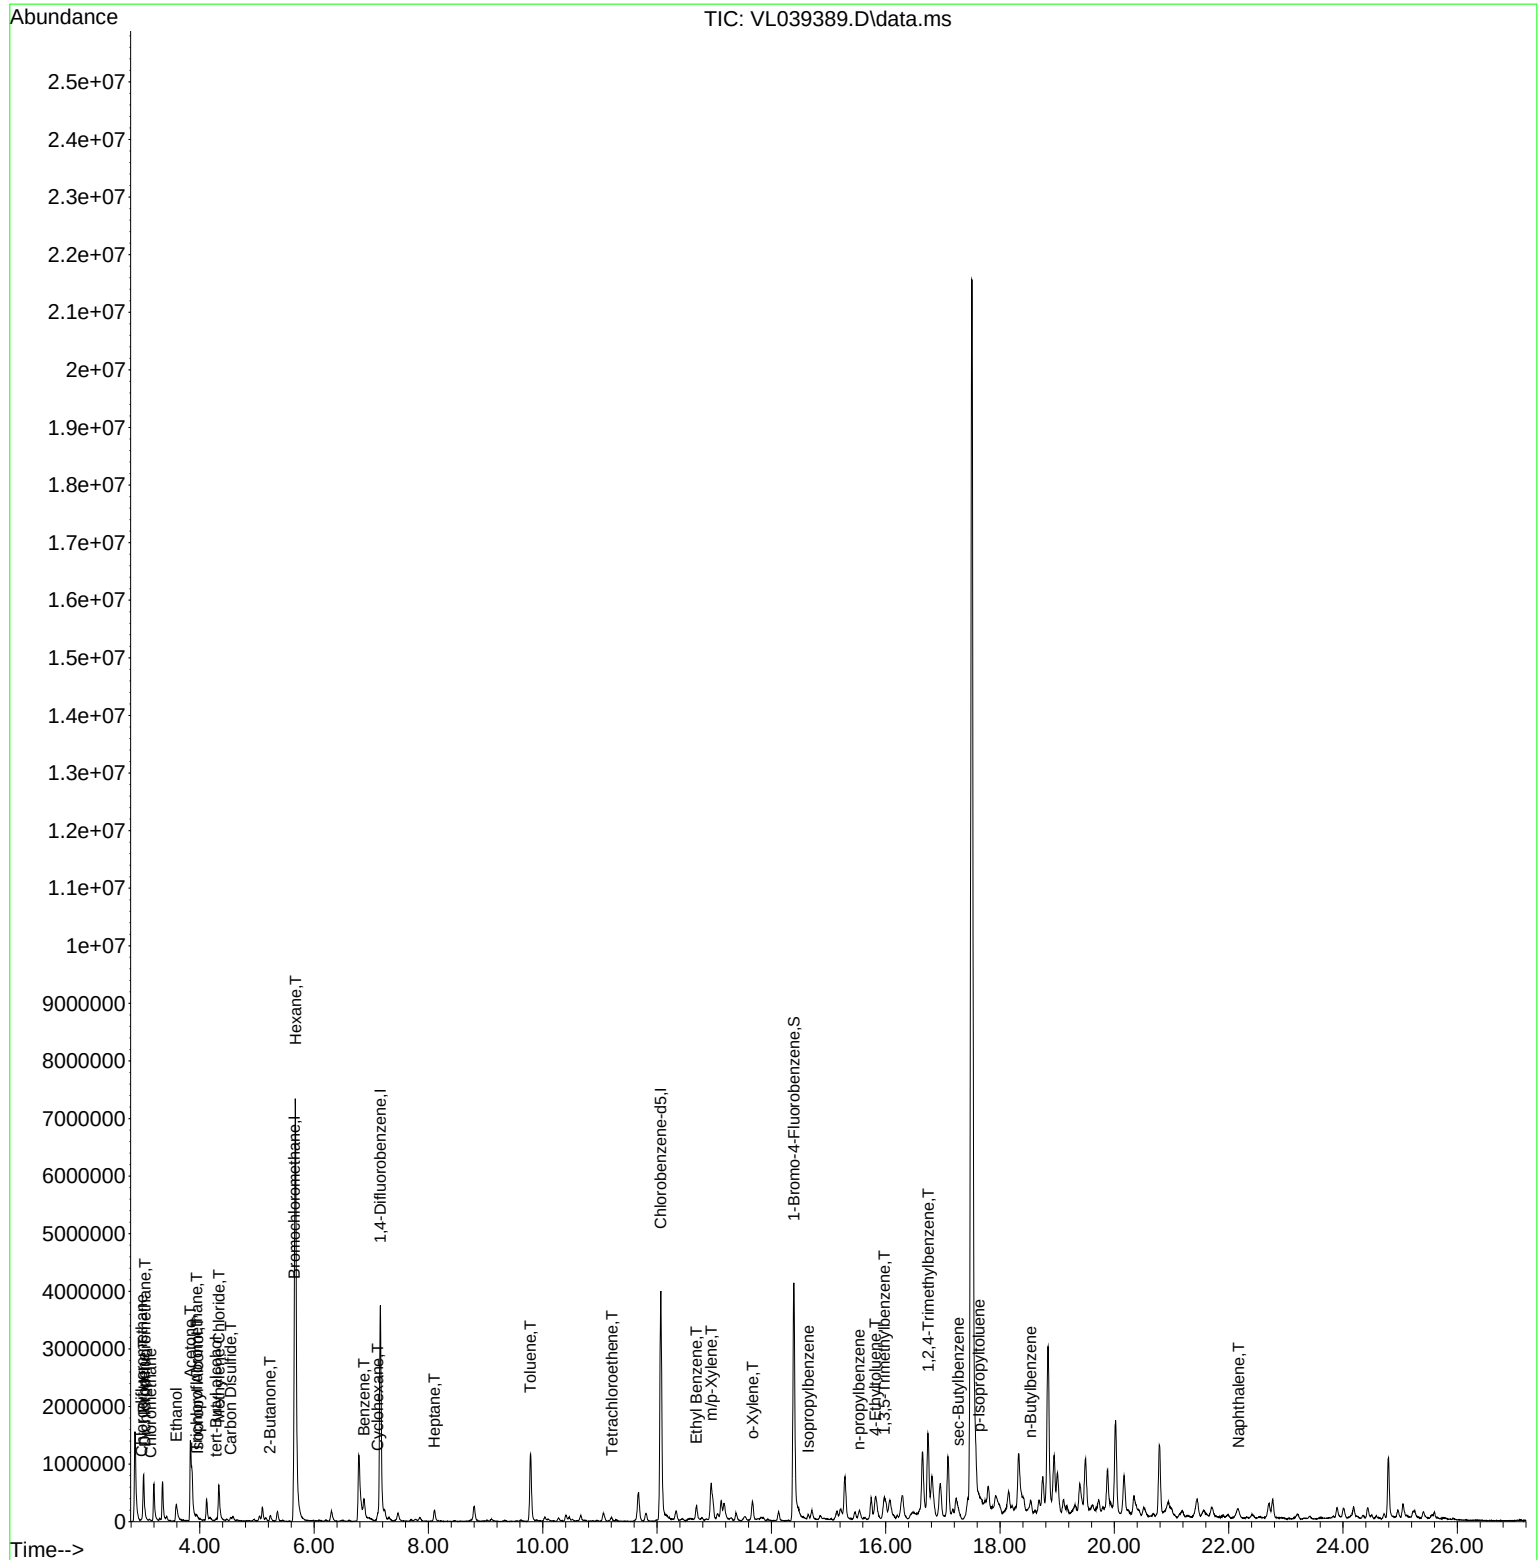



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.652 min Scan# 89
Delta R.T. -0.022 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2



Tgt Ion: 49 Resp: 114233
Ion Ratio Lower Upper
49 100
128 50.5 24.7 74.1
130 65.5 31.4 94.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

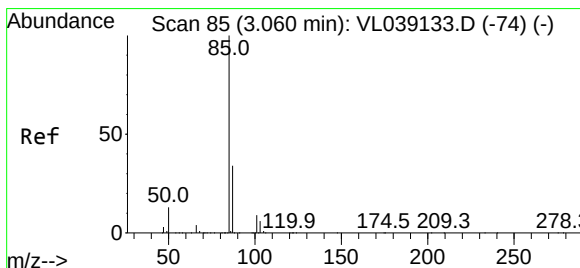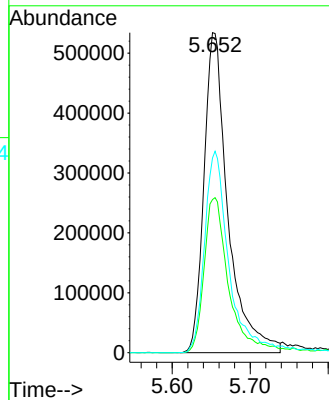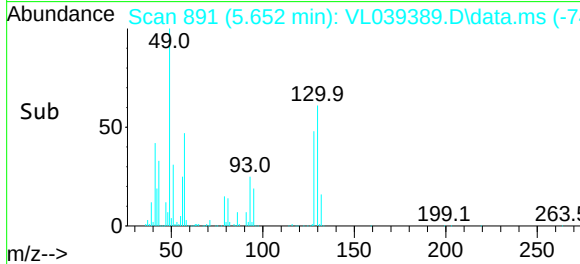

#2
Dichlorodifluoromethane
Concen: 0.171 ppbv
RT: 3.041 min Scan# 79
Delta R.T. -0.019 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52


Tgt Ion: 85 Resp: 34352
Ion Ratio Lower Upper
85 100
87 31.8 26.9 40.3

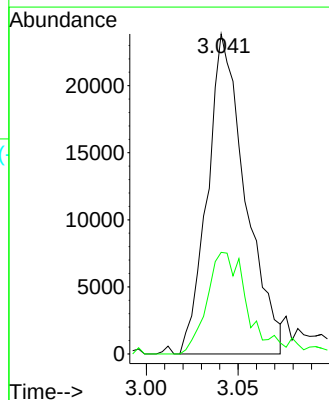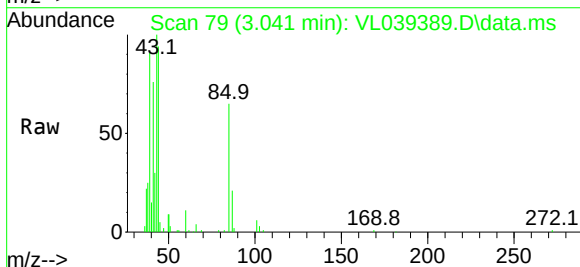



#3
Chlorodifluoromethane
Concen: 0.215 ppbv m
RT: 2.983 min Scan# 61
Delta R.T. -0.016 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2




Tgt Ion: 51 Resp: 31244
Ion Ratio Lower Upper
51 100
67 1.0 16.2 24.4

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

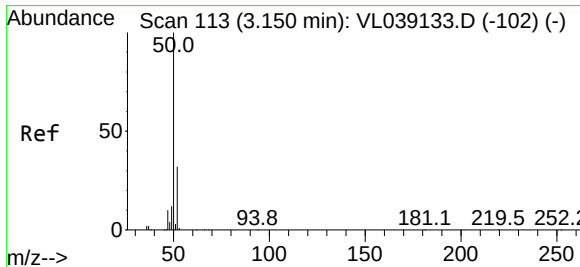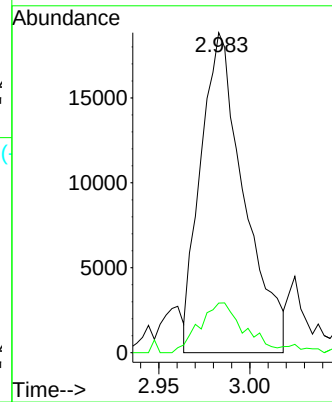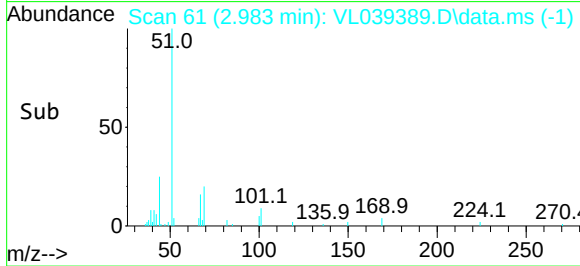


#4
Chloromethane
Concen: 0.137 ppbv m
RT: 3.140 min Scan# 110
Delta R.T. -0.010 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

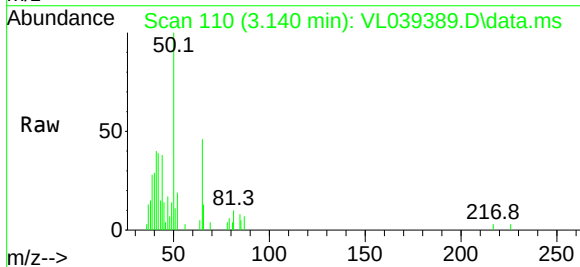


Tgt Ion: 50 Resp: 10263
Ion Ratio Lower Upper
50 100
52 19.4 25.9 38.9

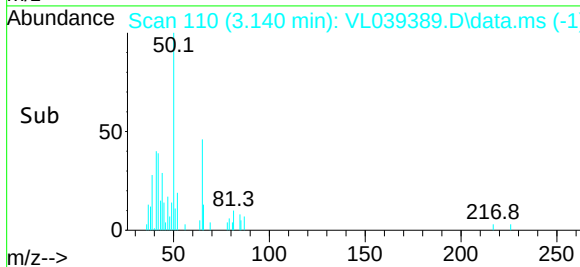



#9
 Propene
 Concen: 3.356 ppbv m
 RT: 3.018 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: VL039389.D
 Acq: 28 Jun 2022 11:52




Instrument :
 MSVOA_L
 ClientSampleId :
 SG-2



Tgt Ion: 41 Resp: 212674
 Ion Ratio Lower Upper
 41 100
 42 72.9 55.4 83.2




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
 Supervised By :Mahesh Dadoda 06/30/2022

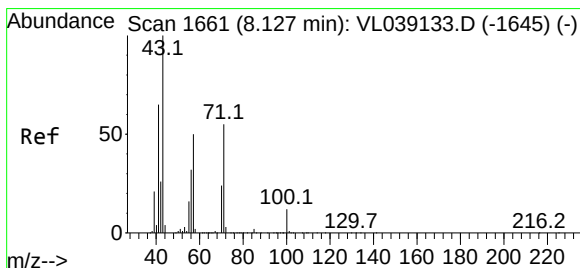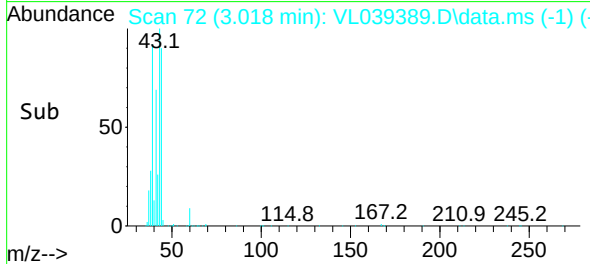

#10
 Heptane
 Concen: 0.588 ppbv m
 RT: 8.105 min Scan# 1654
 Delta R.T. -0.023 min
 Lab File: VL039389.D
 Acq: 28 Jun 2022 11:52


Tgt Ion: 43 Resp: 86981
 Ion Ratio Lower Upper
 43 100
 57 50.9 41.4 62.2

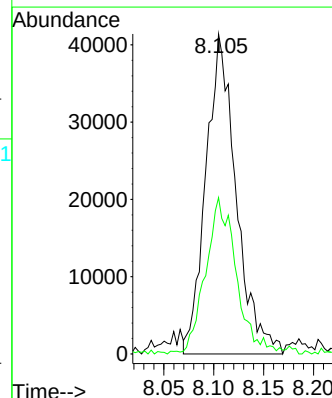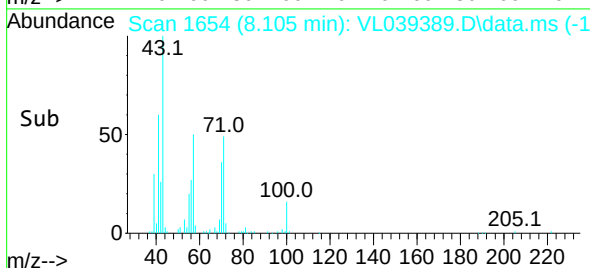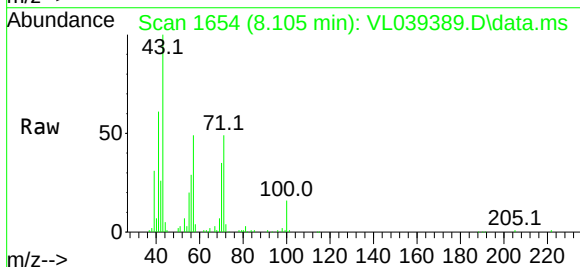

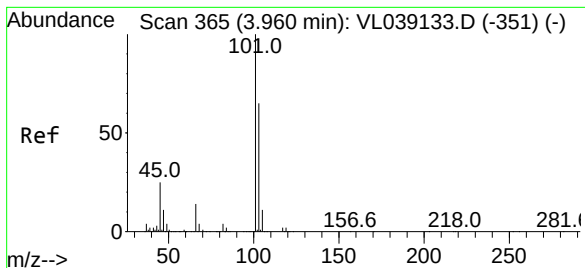

#11
 Trichlorofluoromethane
 Concen: 0.223 ppbv m
 RT: 3.941 min Scan# 3
 Delta R.T. -0.019 min
 Lab File: VL039389.D
 Acq: 28 Jun 2022 11:52




Instrument :
 MSVOA_L
 ClientSampleId :
 SG-2

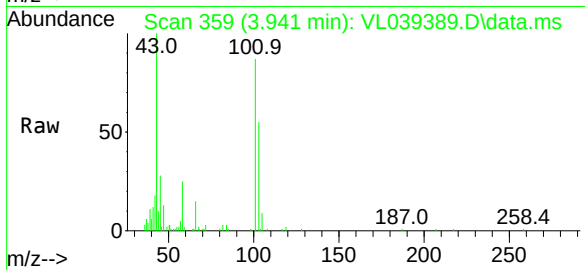

Tgt Ion:101 Resp: 40519
 Ion Ratio Lower Upper
 101 100
 103 62.9 51.7 77.5




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
 Supervised By :Mahesh Dadoda 06/30/2022

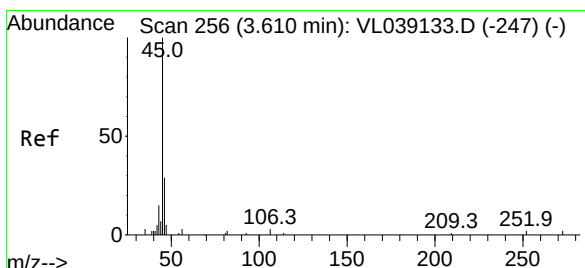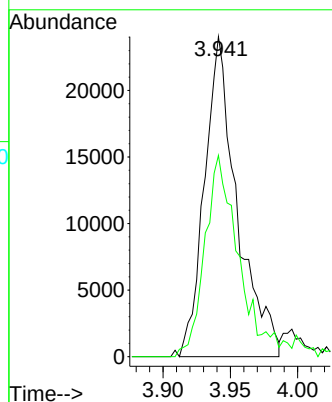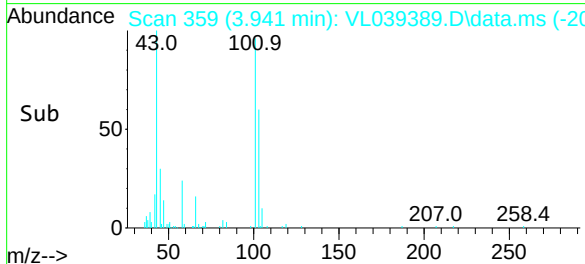

#13
 Ethanol
 Concen: 121.386 ppbv
 RT: 3.591 min Scan# 250
 Delta R.T. -0.019 min
 Lab File: VL039389.D
 Acq: 28 Jun 2022 11:52


Tgt Ion: 45 Resp: 419550
 Ion Ratio Lower Upper
 45 100
 46 40.8 0.0 0.0#

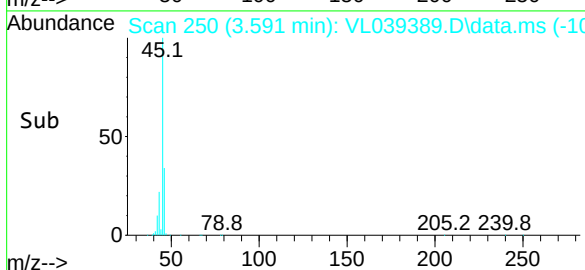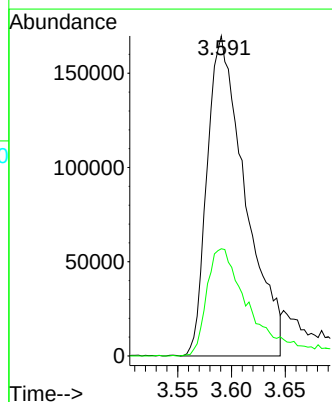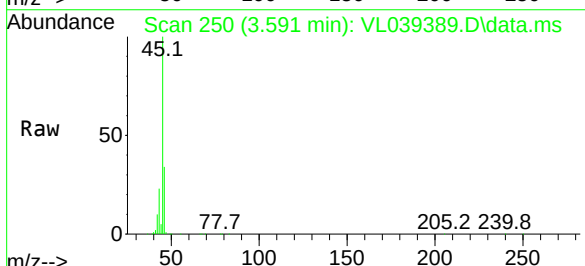

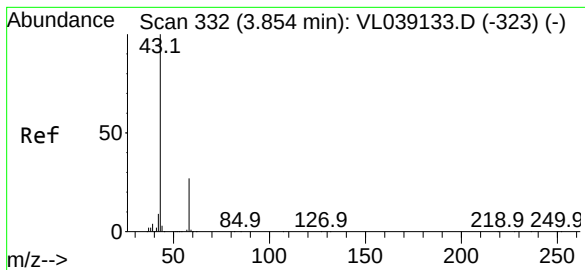

#15
Acetone
Concen: 17.386 ppbv
RT: 3.835 min Scan# 31
Delta R.T. -0.019 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2

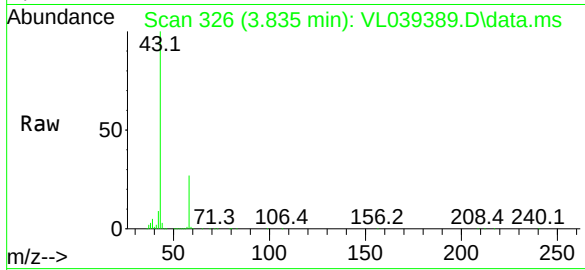

Tgt Ion: 43 Resp: 206884
Ion Ratio Lower Upper
43 100
58 26.0 22.5 33.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

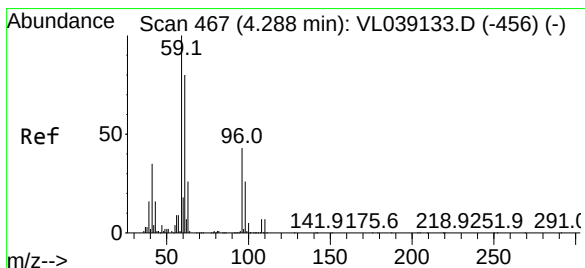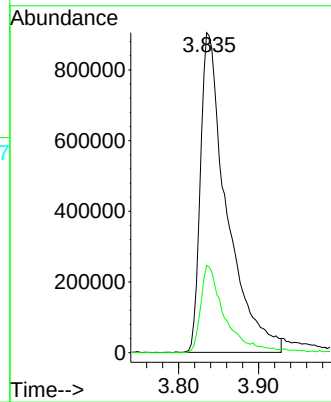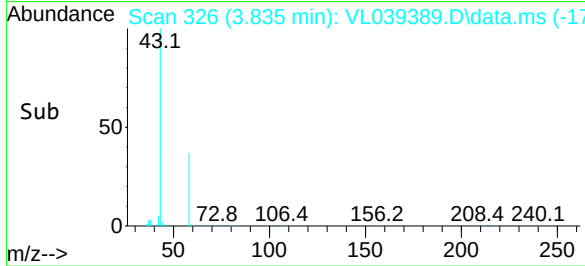

#17
tert-Butyl alcohol
Concen: 0.234 ppbv m
RT: 4.285 min Scan# 466
Delta R.T. -0.003 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52


Tgt Ion: 59 Resp: 21615
Ion Ratio Lower Upper
59 100
57 0.0 9.1 13.7#

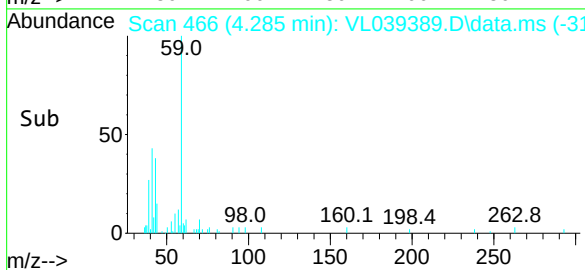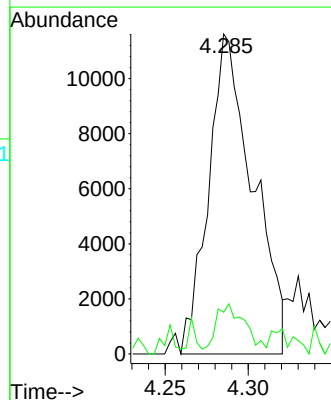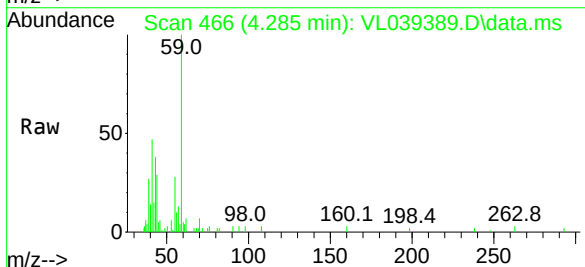



#19
Isopropyl Alcohol
Concen: 0.718 ppbv m
RT: 3.960 min Scan# 30
Delta R.T. -0.003 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2




Tgt Ion: 45 Resp: 4006
Ion Ratio Lower Upper
45 100
58 0.0 1.8 2.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

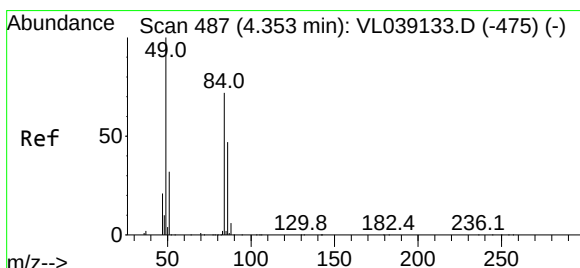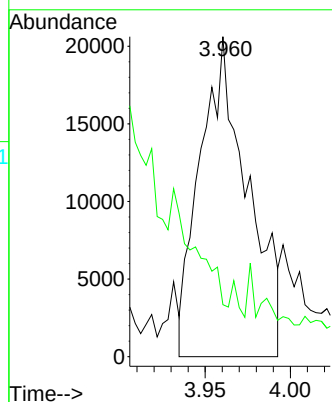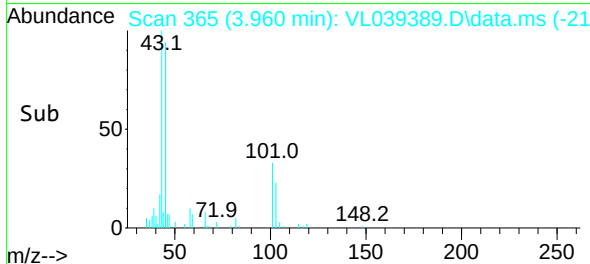


#20
Methylene Chloride
Concen: 5.189 ppbv
RT: 4.333 min Scan# 481
Delta R.T. -0.019 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

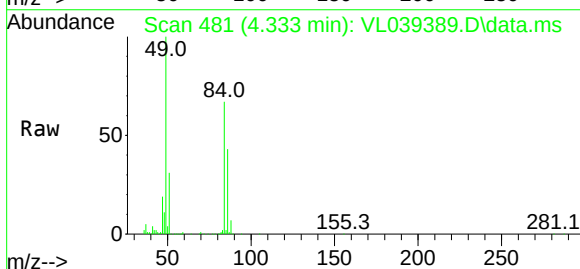


Tgt Ion: 84 Resp: 260229
Ion Ratio Lower Upper
84 100
49 149.5 111.1 166.7
51 45.9 35.3 52.9
86 63.9 51.9 77.9

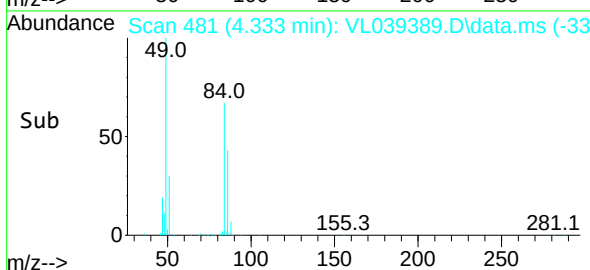



#26
Hexane
Concen: 26.162 ppbv
RT: 5.674 min Scan# 898
Delta R.T. -0.019 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2



Tgt Ion: 57 Resp: 308350
Ion Ratio Lower Upper
57 100
41 90.1 72.4 108.6
43 71.6 187.0 280.6
56 53.7 41.8 62.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

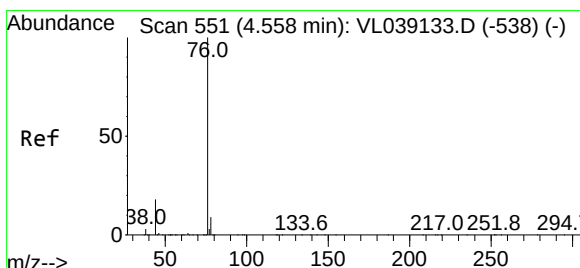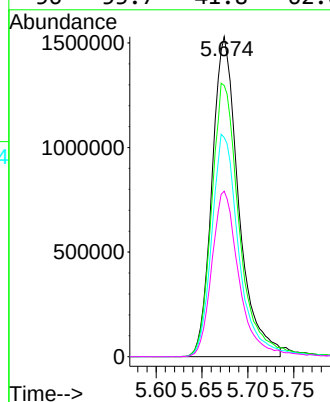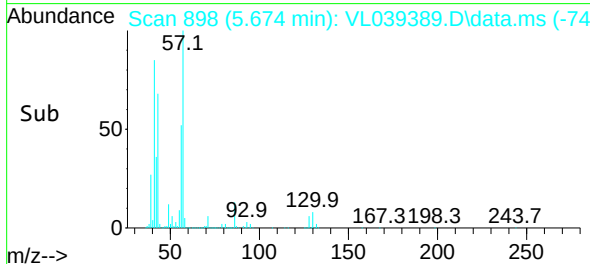

#27
Carbon Disulfide
Concen: 0.592 ppbv m
RT: 4.542 min Scan# 546
Delta R.T. -0.016 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52


Tgt Ion: 76 Resp: 72313
Ion Ratio Lower Upper
76 100
44 24.4 14.4 21.6
78 10.5 7.7 11.5

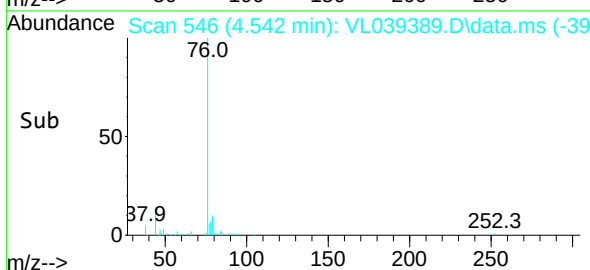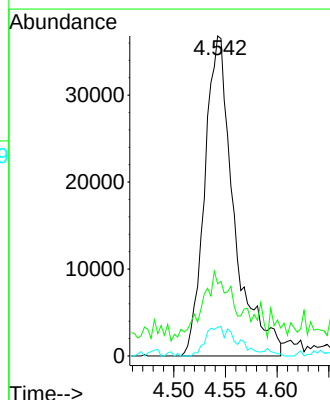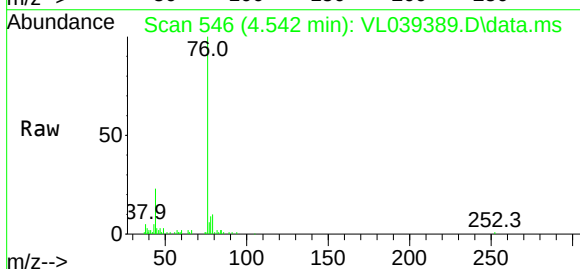

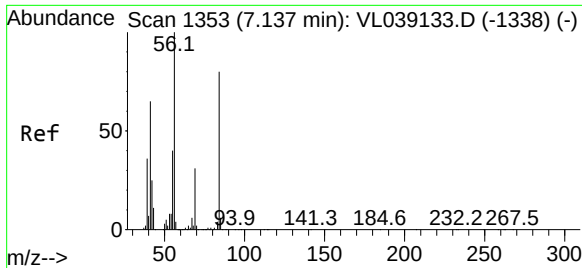

#30
Cyclohexane
Concen: 0.491 ppbv m
RT: 7.111 min Scan# 1345
Delta R.T. -0.026 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2

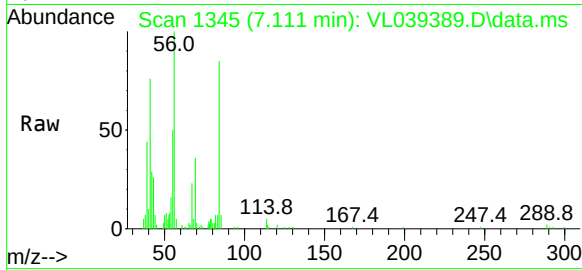


Tgt Ion: 84 Resp: 48638
Ion Ratio Lower Upper
84 100
56 0.0 110.6 165.8
41 86.6 68.9 103.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

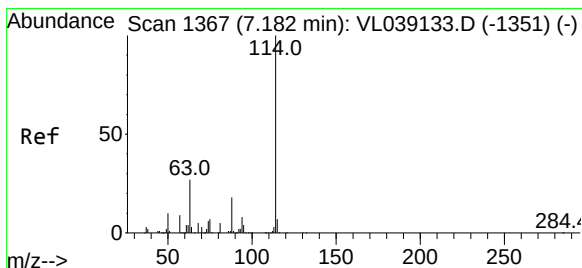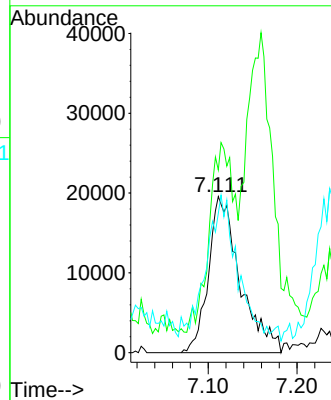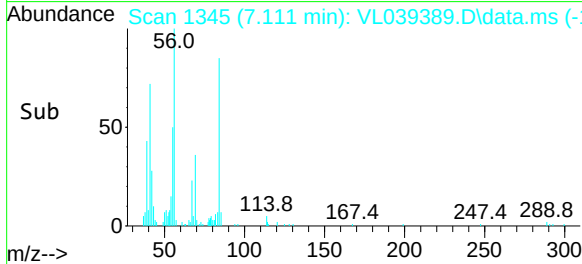


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.160 min Scan# 1360
Delta R.T. -0.023 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

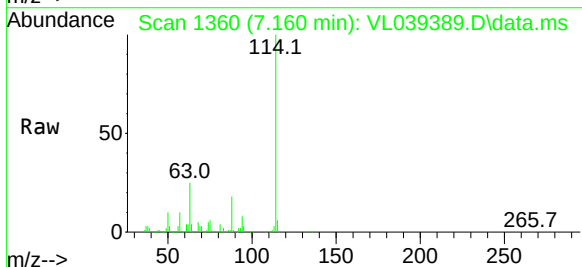


Tgt Ion:114 Resp: 3158061
Ion Ratio Lower Upper
114 100
63 24.7 21.7 32.5
88 18.4 14.8 22.2

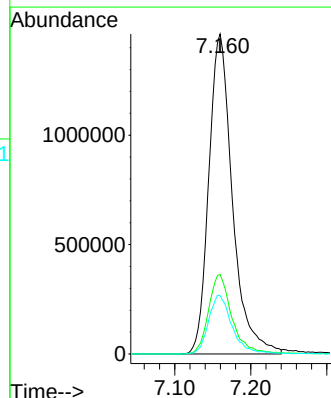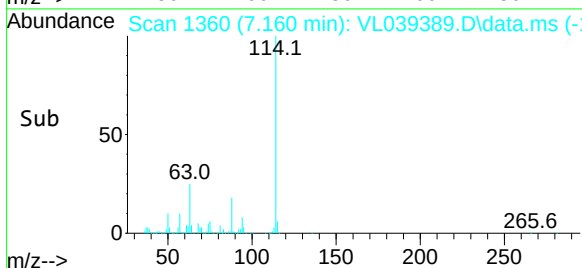

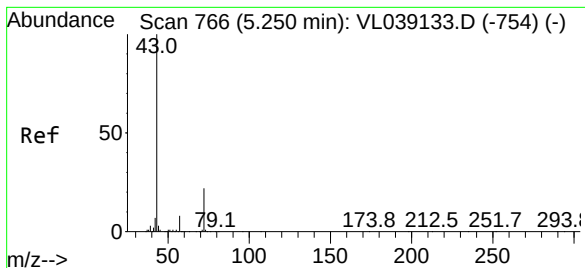

#34
2-Butanone
Concen: 0.713 ppbv
RT: 5.230 min Scan# 712
Delta R.T. -0.019 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2

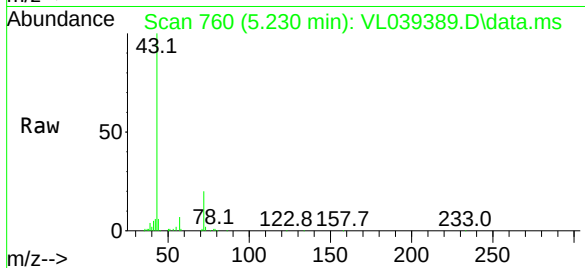

Tgt Ion: 43 Resp: 122358
Ion Ratio Lower Upper
43 100
72 25.9 18.2 27.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

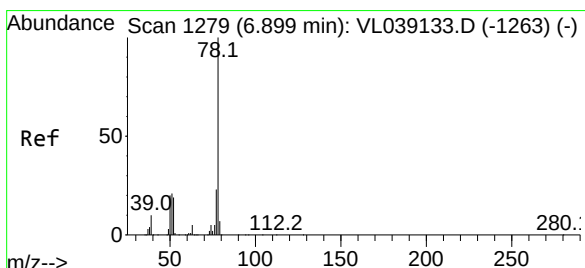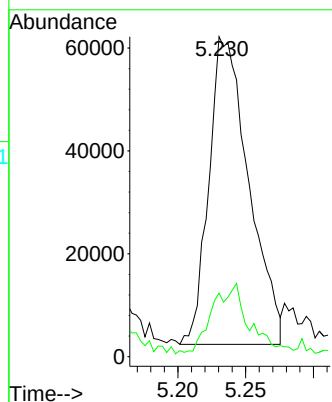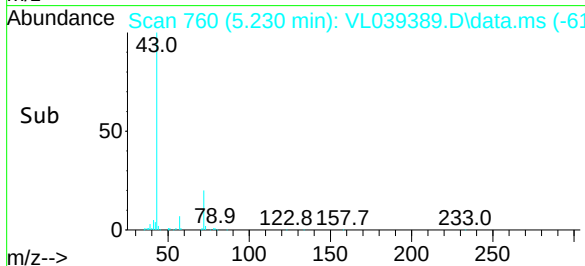

#36
Benzene
Concen: 1.094 ppbv m
RT: 6.870 min Scan# 1270
Delta R.T. -0.029 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52


Tgt Ion: 78 Resp: 280445
Ion Ratio Lower Upper
78 100
77 21.0 18.6 27.8
50 19.3 15.8 23.8

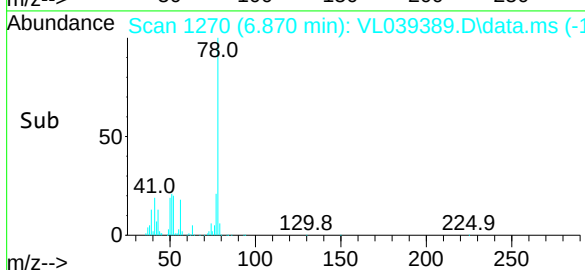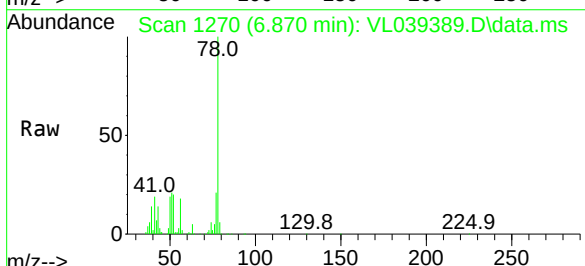

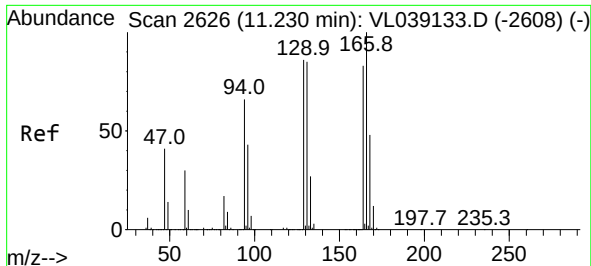

#52
Tetrachloroethene
Concen: 0.143 ppbv m
RT: 11.208 min Scan# 2169
Delta R.T. -0.023 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2

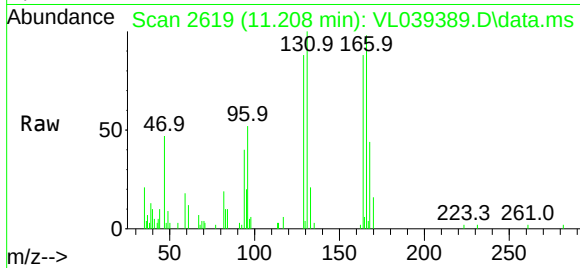


Tgt Ion:164 Resp: 14324
Ion Ratio Lower Upper
164 100
166 110.5 96.3 144.5
129 99.7 82.5 123.7
131 113.0 82.1 123.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

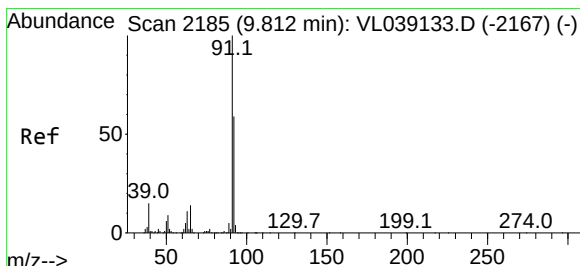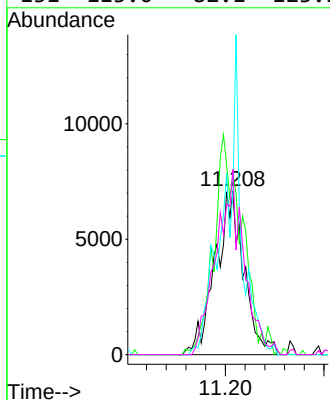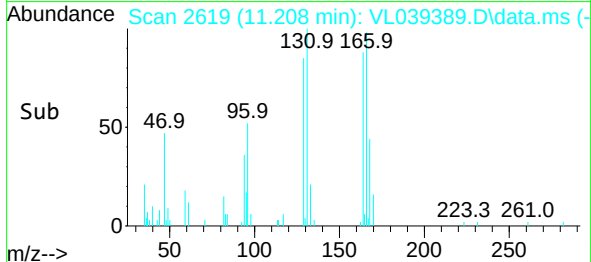


#53
Toluene
Concen: 3.348 ppbv
RT: 9.783 min Scan# 2176
Delta R.T. -0.029 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

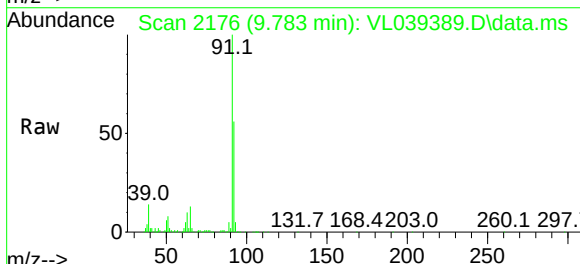


Tgt Ion: 91 Resp: 988490
Ion Ratio Lower Upper
91 100
92 59.7 48.1 72.1

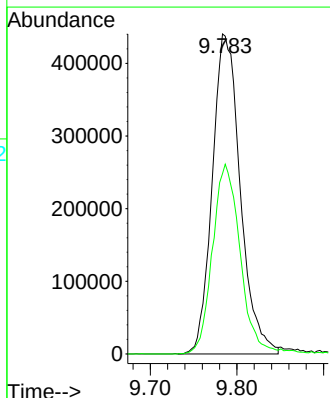

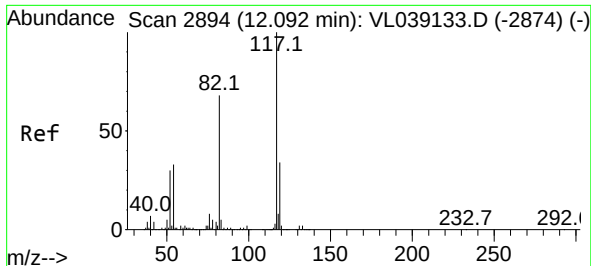

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.066 min Scan# 21
Delta R.T. -0.026 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2

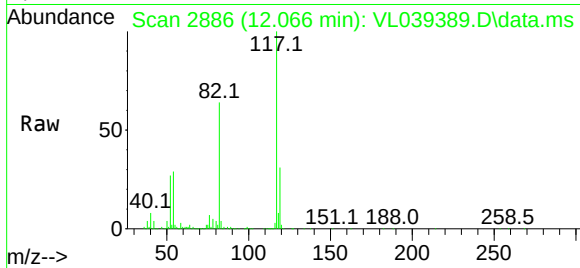


Tgt Ion: 117 Resp: 2708000
Ion Ratio Lower Upper
117 100
82 67.4 55.1 82.7
119 34.9 24.7 37.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

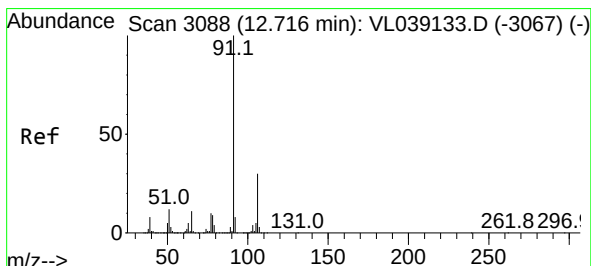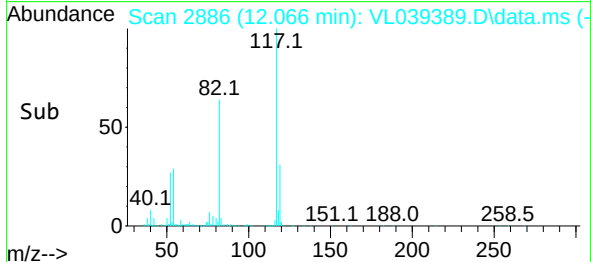


#58
Ethyl Benzene
Concen: 0.572 ppbv
RT: 12.690 min Scan# 3080
Delta R.T. -0.026 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

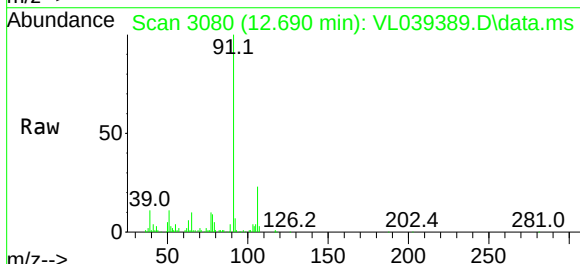

Tgt Ion: 91 Resp: 213193
Ion Ratio Lower Upper
91 100
106 23.1 24.2 36.4#

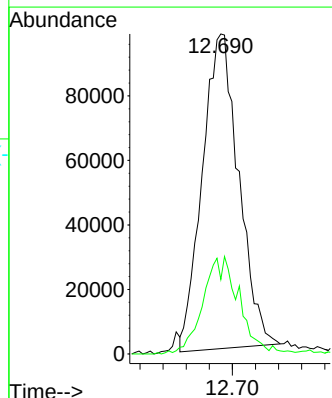







#59
m/p-Xylene
Concen: 2.113 ppbv
RT: 12.947 min Scan# 3176
Delta R.T. -0.051 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

Instrument :
MSVOA_L
ClientSampleId :
SG-2

Tgt Ion: 91 Resp: 69419
Ion Ratio Lower Upper
91 100
106 46.7 34.3 51.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

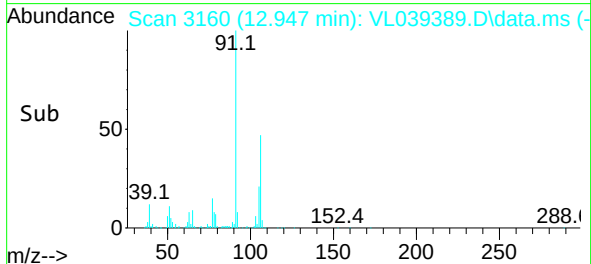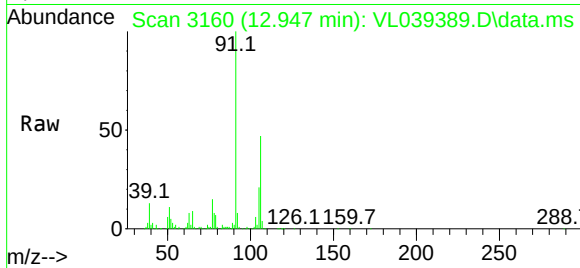

#60
o-Xylene
Concen: 0.890 ppbv
RT: 13.671 min Scan# 3385
Delta R.T. -0.026 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52


Tgt Ion: 91 Resp: 274858
Ion Ratio Lower Upper
91 100
106 43.3 22.3 66.9

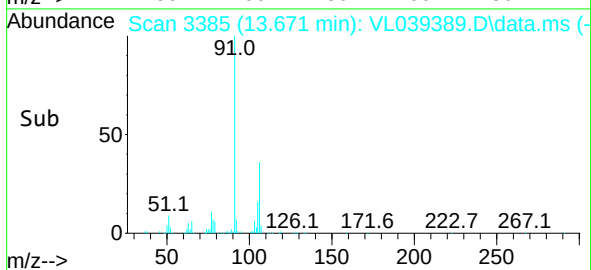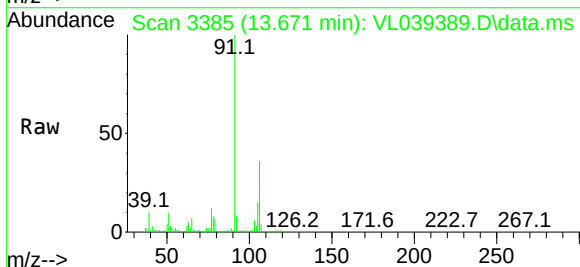



#62
Isopropylbenzene
Concen: 0.168 ppbv m
RT: 14.645 min Scan# 30
Delta R.T. -0.026 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52




Instrument :
MSVOA_L
ClientSampleId :
SG-2



Tgt Ion:105 Resp: 7725
Ion Ratio Lower Upper
105 100
120 27.0 20.3 30.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

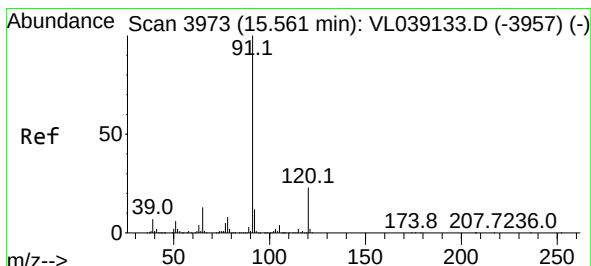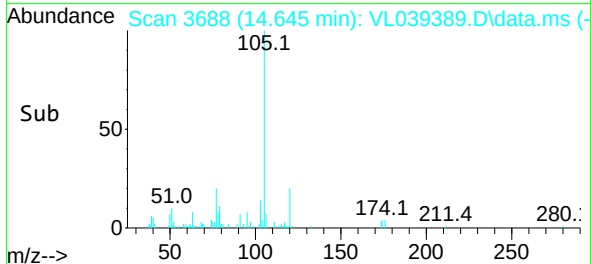

#64
n-propylbenzene
Concen: 0.196 ppbv m
RT: 15.532 min Scan# 3964
Delta R.T. -0.029 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

Tgt Ion:120 Resp: 22078
Ion Ratio Lower Upper
120 100
91 0.0 388.4 582.6#

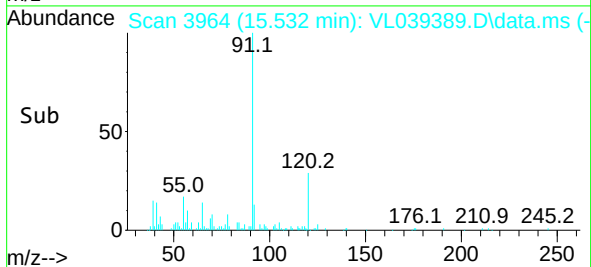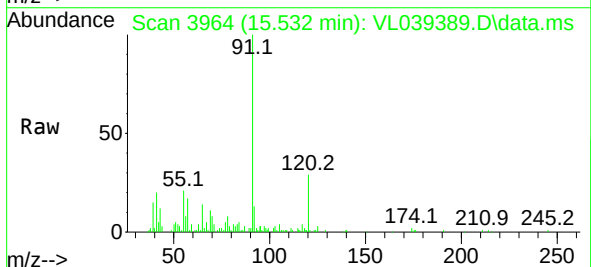

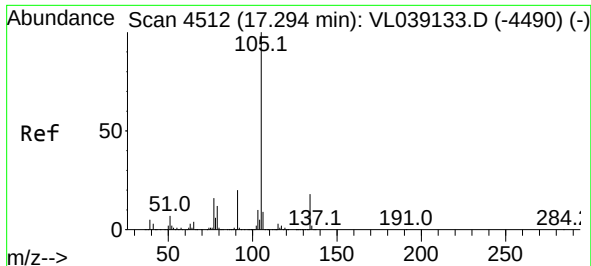

#67

sec-Butylbenzene

Concen: 0.111 ppbv m

RT: 17.272 min Scan# 4512

Delta R.T. -0.023 min

Lab File: VL039389.D


Acq: 28 Jun 2022 11:52

Instrument :

MSVOA_L

ClientSampleId :

SG-2

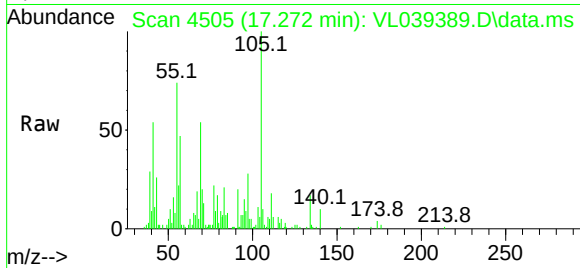

Tgt Ion: 105 Resp: 63328

Ion Ratio Lower Upper

105 100




134 18.6 14.4 21.6

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022

Supervised By :Mahesh Dadoda 06/30/2022

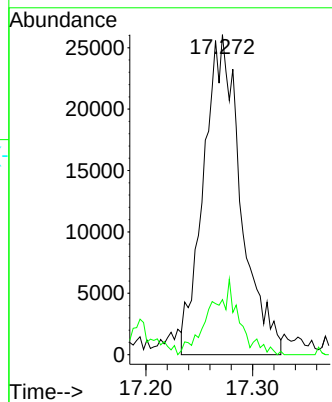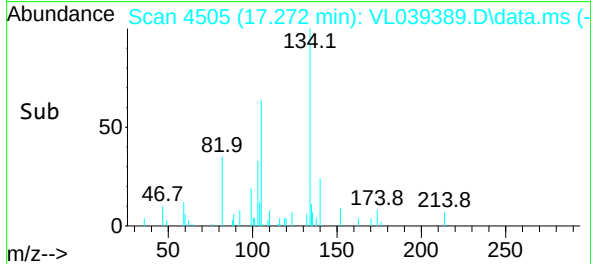

#68

1-Bromo-4-Fluorobenzene

Concen: 9.521 ppbv

RT: 14.394 min Scan# 3610

Delta R.T. -0.023 min

Lab File: VL039389.D

Acq: 28 Jun 2022 11:52




Tgt Ion: 95 Resp: 2131503


Ion Ratio Lower Upper

95 100

174 70.6 53.8 80.8

175 5.1 4.1 6.1

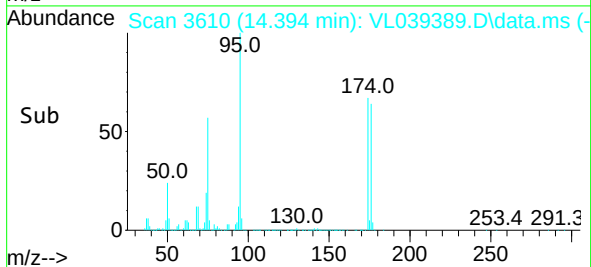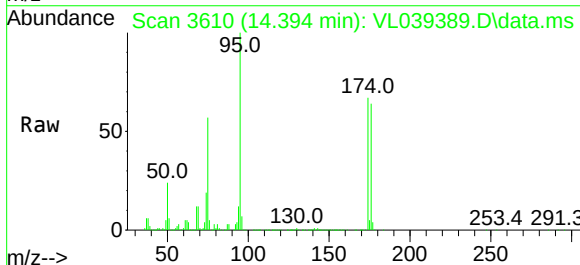

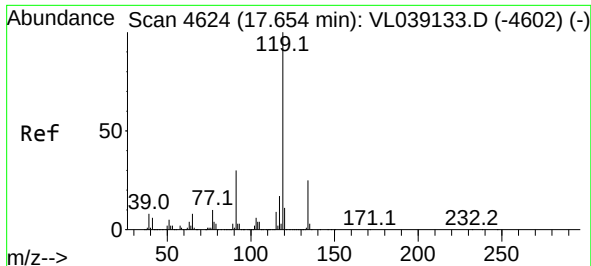





#69
p-Isopropyltoluene
Concen: 0.140 ppbv m
RT: 17.629 min Scan# 4616
Delta R.T. -0.026 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

Instrument :
MSVOA_L
ClientSampleId :
SG-2

Tgt Ion: 119 Resp: 6764
Ion Ratio Lower Upper
119 100
134 0.0 20.4 30.6
91 0.0 24.2 36.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/29/2022
Supervised By :Mahesh Dadoda 06/30/2022

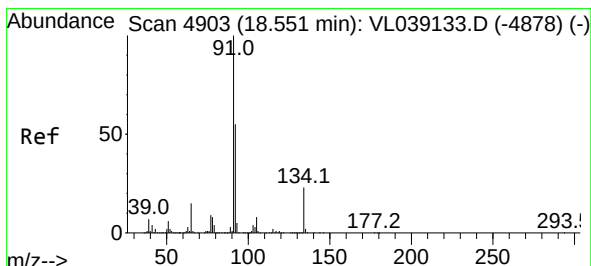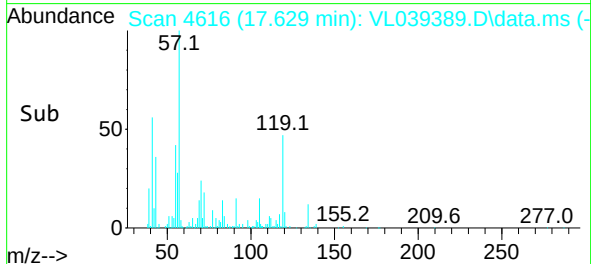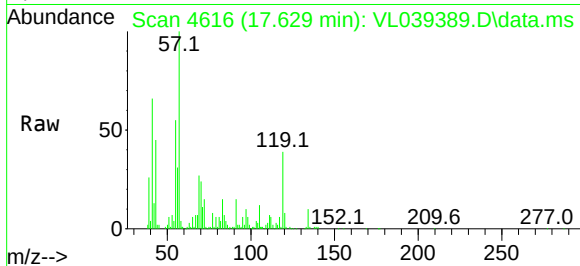

#70
n-Butylbenzene
Concen: 0.184 ppbv m
RT: 18.535 min Scan# 4898
Delta R.T. -0.016 min
Lab File: VL039389.D
Acq: 28 Jun 2022 11:52

Tgt Ion: 91 Resp: 91244
Ion Ratio Lower Upper
91 100
92 31.8 43.6 65.4#
134 77.4 17.7 26.5#

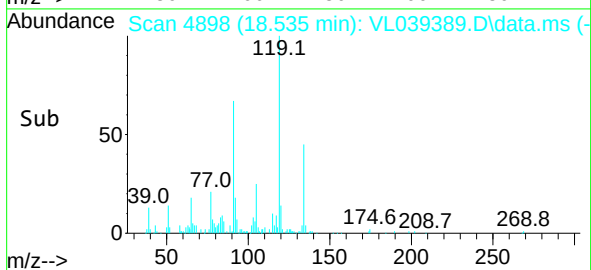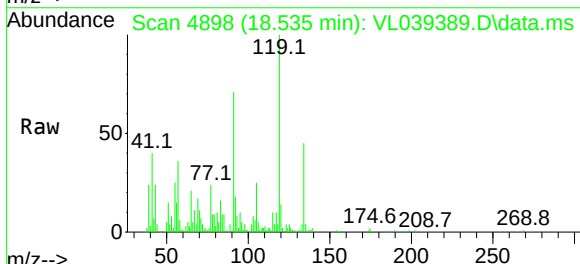



#72

4-Ethyltoluene

Concen: 0.399 ppbv

RT: 15.815 min Scan# 4060

Delta R.T. -0.026 min

Lab File: VL039389.D

Acq: 28 Jun 2022 11:52

Instrument :

MSVOA_L

ClientSampleId :

SG-2

Tgt Ion:105 Resp: 144360

Ion Ratio Lower Upper

105 100

120 31.6 23.9 35.9

91 13.4 10.6 16.0





77 17.7 11.7 17.5#

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022

Supervised By :Mahesh Dadoda 06/30/2022

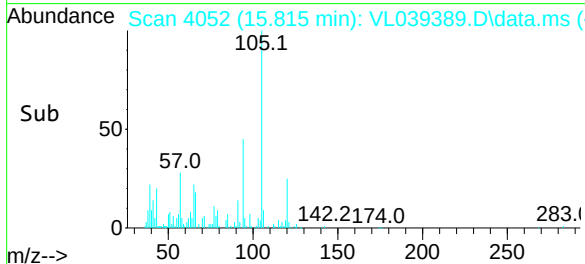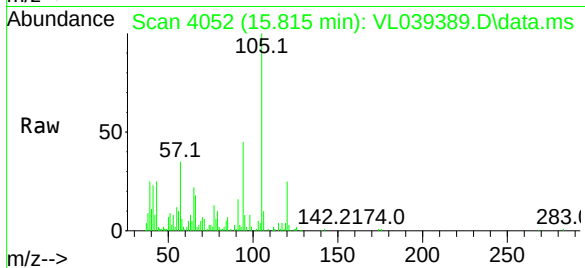

#73

1,3,5-Trimethylbenzene

Concen: 0.811 ppbv

RT: 15.976 min Scan# 4102

Delta R.T. -0.019 min

Lab File: VL039389.D




Acq: 28 Jun 2022 11:52


Tgt Ion:105 Resp: 264653

Ion Ratio Lower Upper

105 100

120 44.9 36.7 55.1

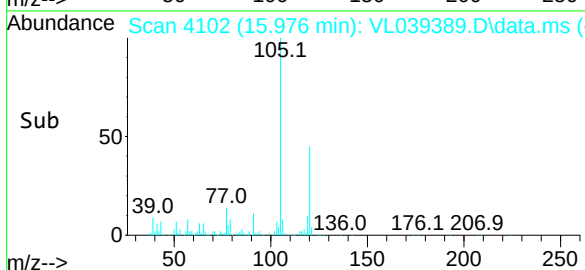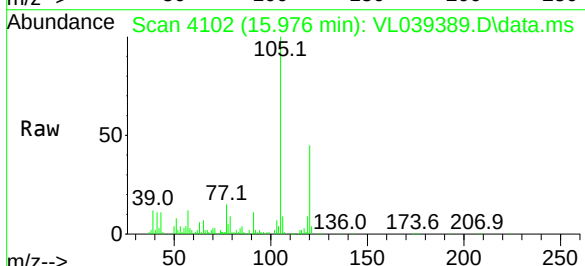



#74

1,2,4-Trimethylbenzene

Concen: 2.970 ppbv

RT: 16.741 min Scan# 41

Delta R.T. -0.019 min

Lab File: VL039389.D


Acq: 28 Jun 2022 11:52

Instrument :

MSVOA_L

ClientSampleId :

SG-2

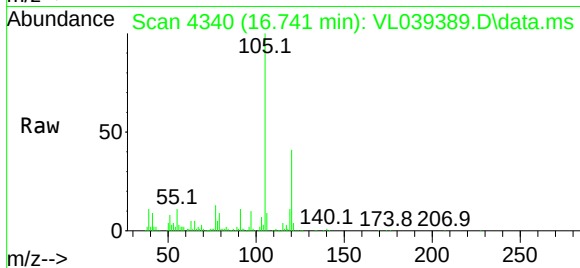

Tgt Ion:105 Resp: 108133

Ion Ratio Lower Upper

105 100

120 40.9 38.1 57.1

91 10.9 47.4 71.0




77 12.0 19.5 29.3

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2022

Supervised By :Mahesh Dadoda 06/30/2022

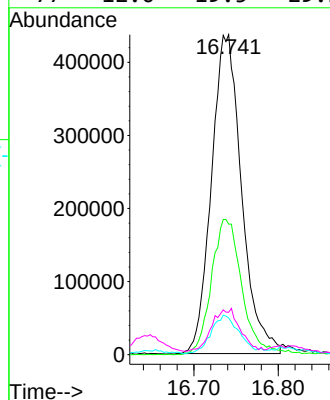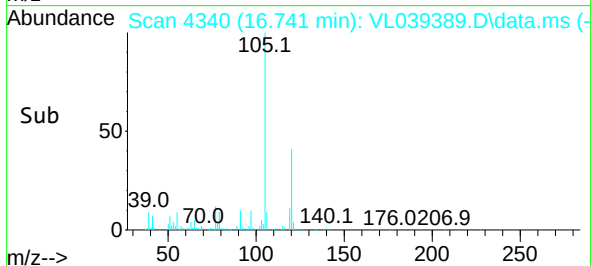

#79

Naphthalene

Concen: 0.249 ppbv m

RT: 22.175 min Scan# 6030

Delta R.T. -0.019 min

Lab File: VL039389.D

Acq: 28 Jun 2022 11:52

Tgt Ion:128 Resp: 69709

Ion Ratio Lower Upper

128 100

127 10.0 10.4 15.6

129 9.8 9.0 13.6

