
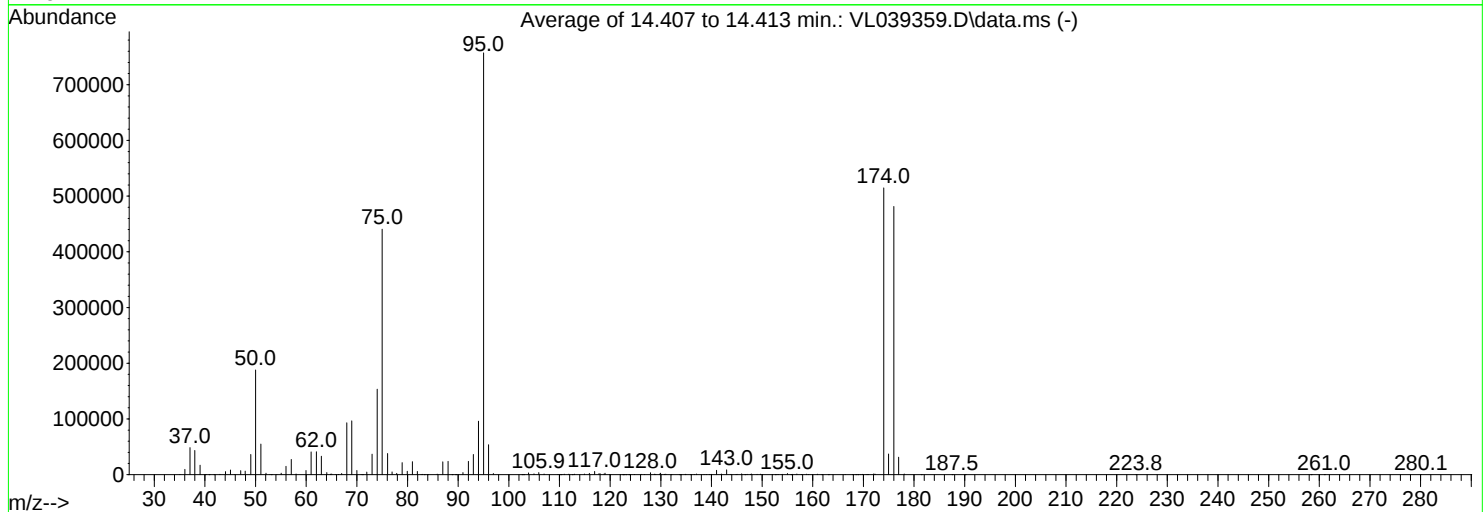


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062722\
 Data File : VL039359.D
 Acq On : 27 Jun 2022 13:05
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

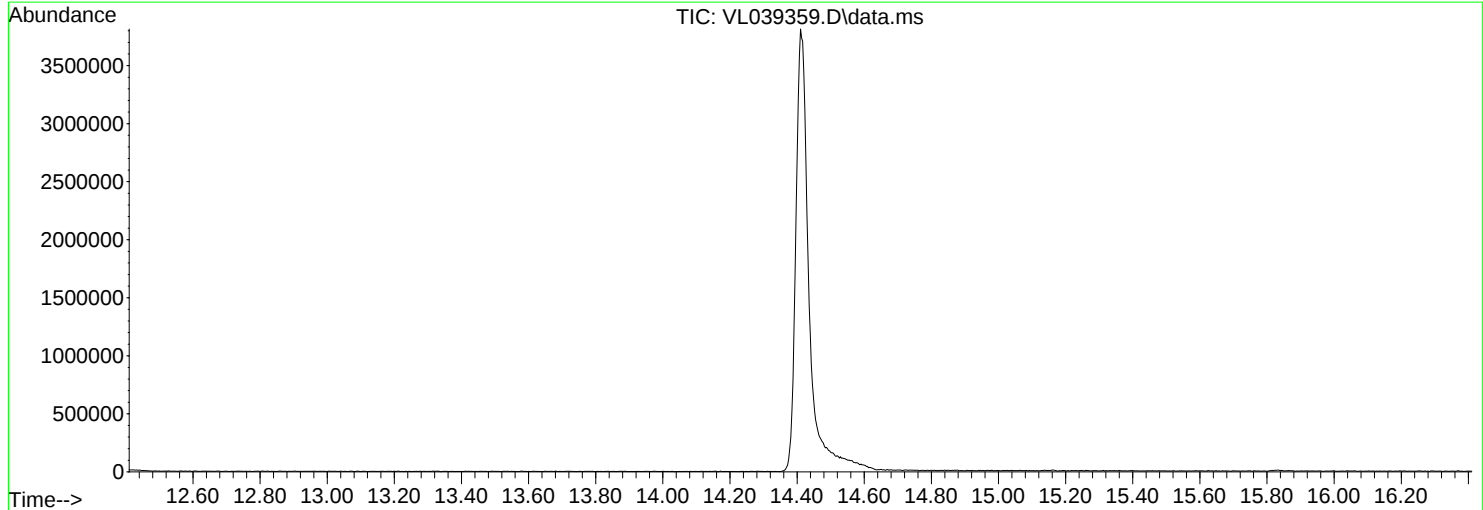

AutoFind: Scans 3614, 3615, 3616; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	187755	PASS
75	95	30	66	58.2	440576	PASS
95	95	100	100	100.0	757205	PASS
96	95	5	9	7.1	53621	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.0	514645	PASS
175	174	4	9	7.2	37183	PASS
176	174	93	101	93.5	481429	PASS
177	176	5	9	6.5	31227	PASS

Average of 14.407 to 14.413 min.: VL039359.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.05	192	45.05	8435	55.05	2510	65.85	241
36.05	9376	45.90	429	56.00	15030	66.35	400
37.05	48528	47.05	7325	57.05	27179	67.00	208
38.00	43357	47.95	6430	58.00	1135	68.00	9319
39.05	17054	49.05	36261	59.95	7528	69.00	96392
40.00	129	50.00	187755	60.95	40752	70.00	7482
40.20	326	51.05	54872	62.00	41200	70.85	160
40.80	99	52.05	2688	63.00	32952	71.10	131
41.80	71	52.85	257	64.05	3822	71.95	4665
42.95	486	53.10	151	64.80	805	73.00	36709
44.05	5477	54.20	171	65.05	1311	74.00	153301

Average of 14.407 to 14.413 min.: VL039359.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	440576	83.90	99	96.00	53621	110.95	805
76.05	37891	85.85	736	96.95	1921	111.85	920
76.95	4887	86.95	23072	102.60	53	112.50	97
77.85	2456	88.00	23968	102.90	106	112.95	762
78.95	21427	88.80	129	103.90	3044	114.90	1230
79.95	6108	89.50	81	104.95	1387	115.90	2196
80.95	23208	90.95	3623	105.90	3719	116.95	5633
81.95	5803	92.00	23728	106.95	1057	117.80	1669
82.70	331	93.00	36171	109.70	330	118.00	1761
82.95	529	94.00	96072	110.20	116	118.80	1287
83.30	89	95.00	757205	110.50	227	119.00	2566

Average of 14.407 to 14.413 min.: VL039359.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.90	181	128.75	851	135.90	102	144.85	383
122.05	327	129.00	612	136.60	222	145.05	537
122.50	71	129.80	1206	137.05	1304	145.95	1410
122.70	54	129.95	2506	138.55	165	146.60	69
123.10	150	130.70	551	139.00	401	147.05	464
123.70	57	131.00	824	139.65	442	147.70	687
123.95	385	132.00	67	140.00	491	147.90	1110
124.80	308	133.70	75	141.00	7735	149.00	526
126.10	594	133.90	133	141.95	1291	149.70	796
126.80	172	134.80	455	143.00	8705	150.05	271
127.95	3331	134.95	642	143.85	520	152.05	206

Average of 14.407 to 14.413 min.: VL039359.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.60	139	160.90	962	170.80	180	190.10	90
152.95	347	161.80	63	171.00	254	223.80	81
153.20	167	163.10	110	172.05	1590	258.40	64
153.95	655	166.40	164	172.30	953	261.00	105
155.00	1982	167.90	120	174.00	514645	280.10	243
155.70	76	168.50	142	174.95	37183		
156.00	603	168.90	54	176.00	481429		
156.85	1278	169.05	253	176.95	31227		
157.75	358	169.50	194	178.05	1134		
158.80	894	169.85	511	181.40	66		
159.20	262	170.55	394	187.50	100		