

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062922\
 Data File : VL039404.D
 Acq On : 29 Jun 2022 20:17
 Operator : SY/AP
 Sample : QC062022 CAN 10448
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC062022 CAN 10448

Quant Time: Jun 30 05:44:28 2022
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Jun 30 05:40:11 2022
 QLast Update : Thu Jun 30 05:40:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.655	49	1230429	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	7.160	114	3492494	10.000	ppbv	0.00
55) Chlorobenzene-d5	12.069	117	2959658	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.401	95	2238226	10.194	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062922\
Data File : VL039404.D
Acq On : 29 Jun 2022 20:17
Operator : SY/AP
Sample : QC062022 CAN 10448
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC062022 CAN 10448

Quant Time: Jun 30 05:44:28 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Jun 30 05:40:11 2022
QLast Update : Thu Jun 30 05:40:11 2022
Response via : Initial Calibration




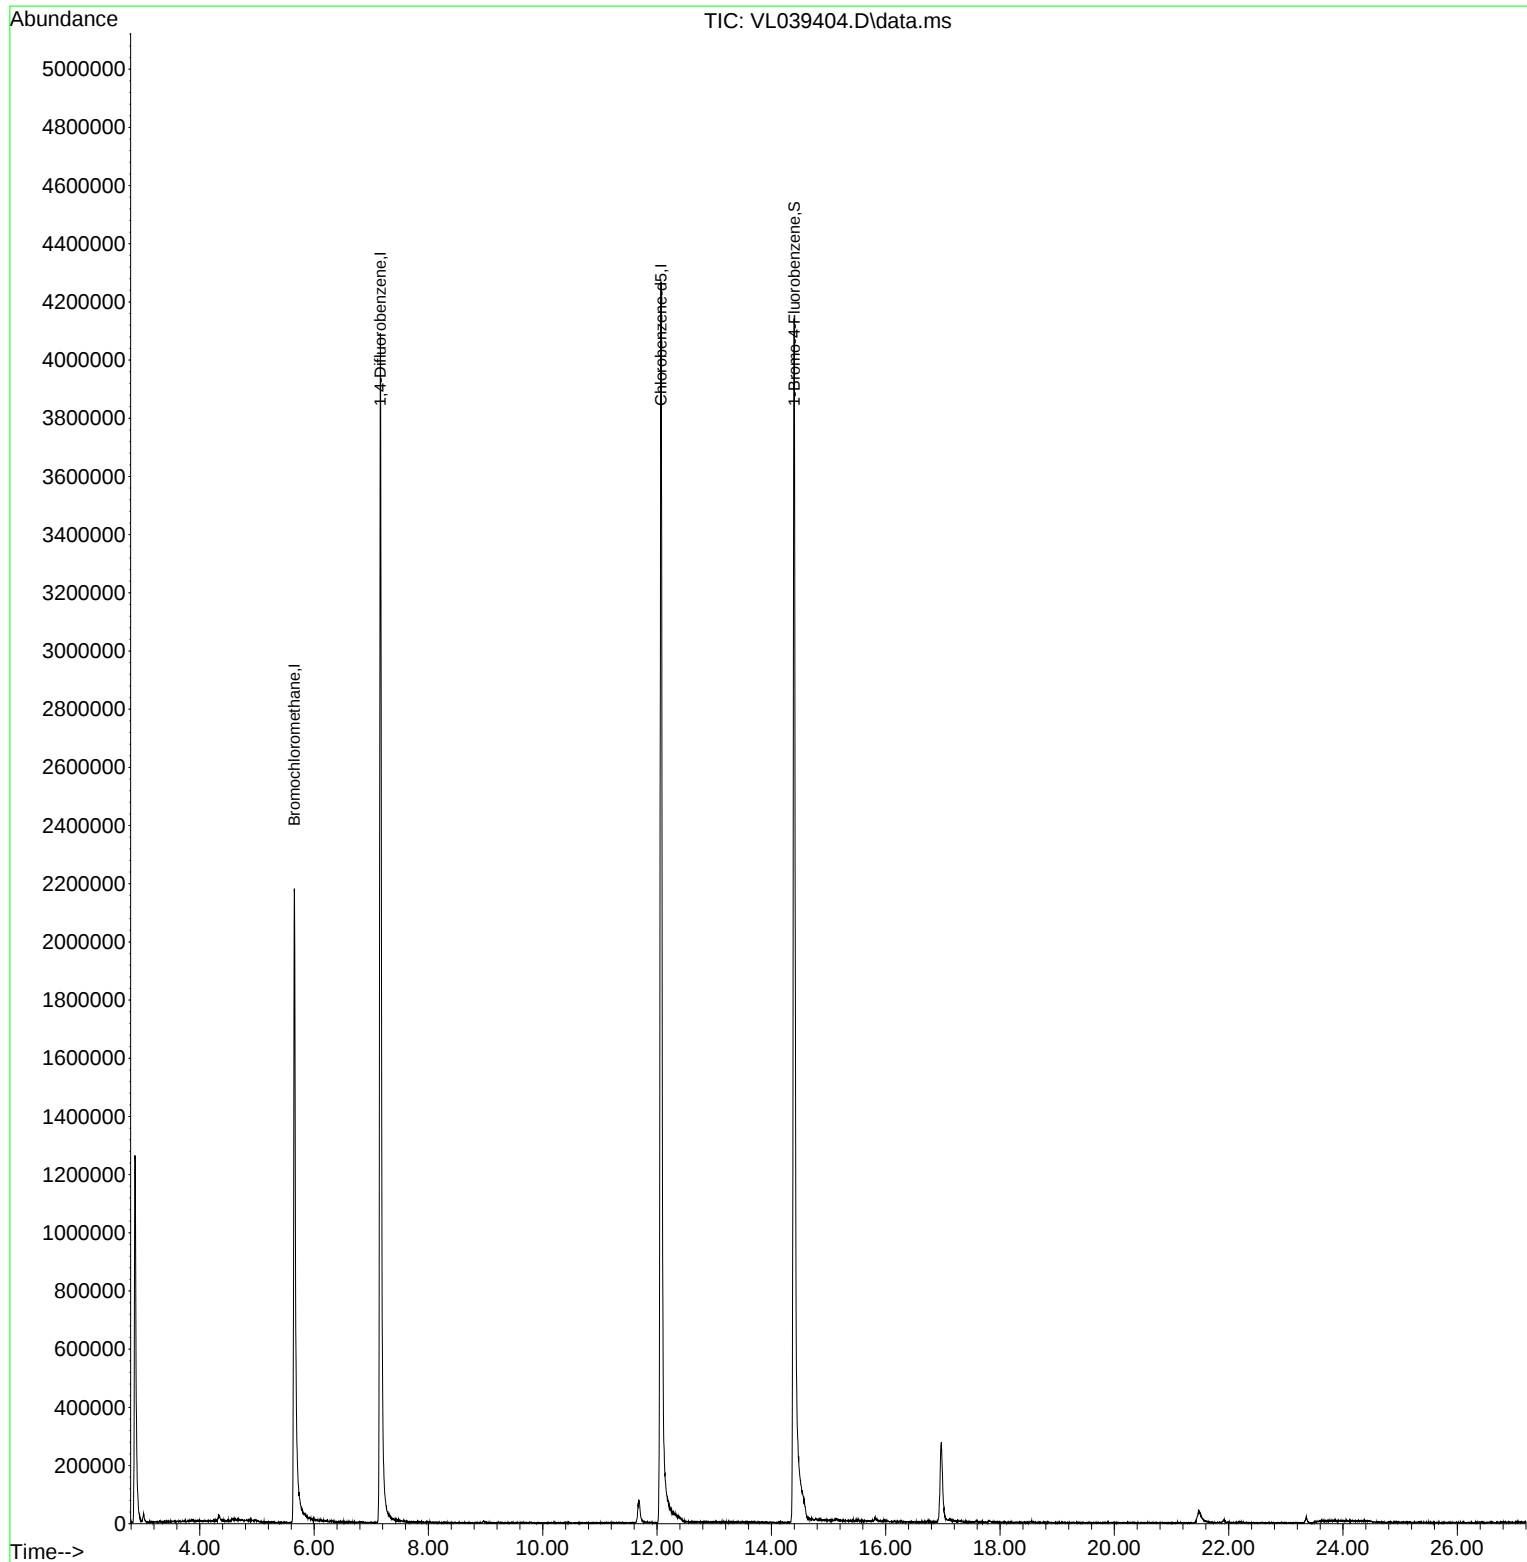


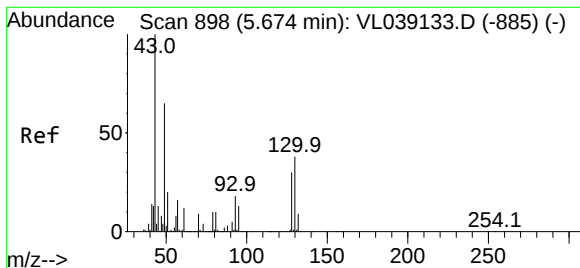

#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.655 min Scan# 898
 Delta R.T. 0.003 min
 Lab File: VL039404.D
 Acq: 29 Jun 2022 20:17




Instrument :
 MSVOA_L
 ClientSampleId :
 QC062022 CAN 10448


Tgt Ion: 49 Resp: 1230429
 Ion Ratio Lower Upper
 49 100
 128 54.8 26.7 80.0
 130 70.4 34.3 102.8

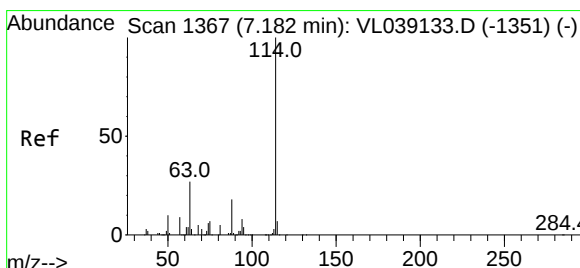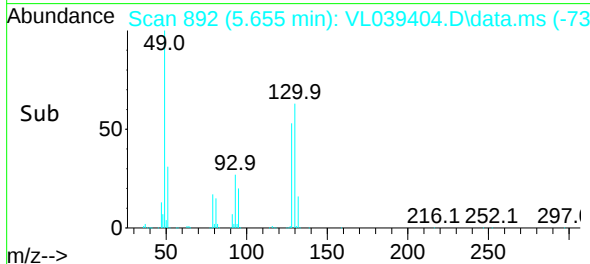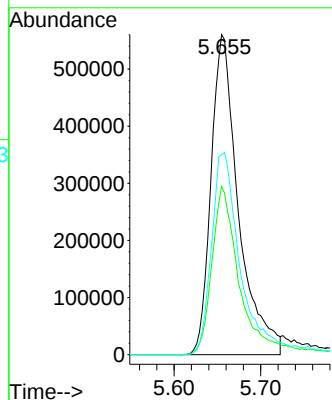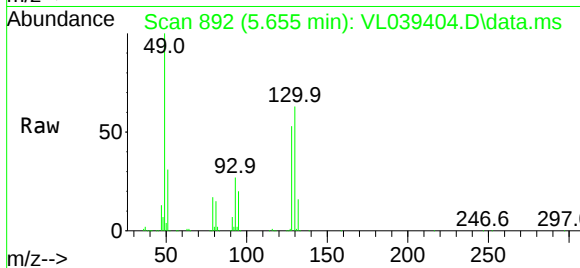

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.160 min Scan# 1360
 Delta R.T. 0.003 min
 Lab File: VL039404.D
 Acq: 29 Jun 2022 20:17

Tgt Ion: 114 Resp: 3492494
 Ion Ratio Lower Upper
 114 100
 63 24.9 20.2 30.4
 88 18.5 14.5 21.7


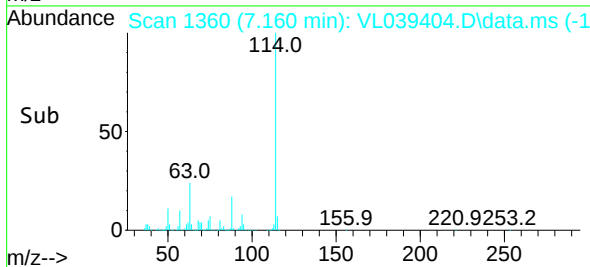
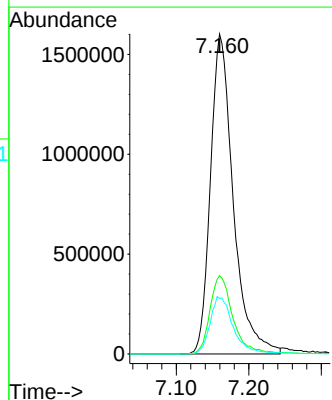
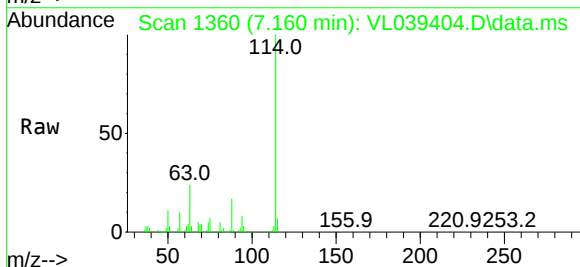


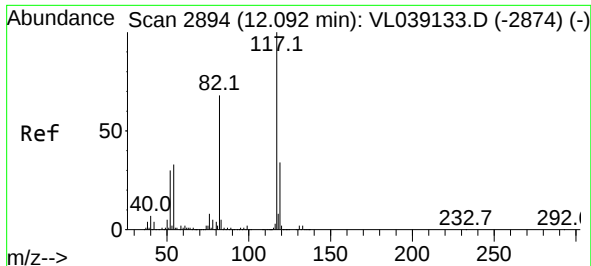

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.069 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL039404.D
Acq: 29 Jun 2022 20:17

Instrument :
MSVOA_L
ClientSampleId :
QC062022 CAN 10448

Tgt Ion:117 Resp: 2959658
Ion Ratio Lower Upper
117 100
82 67.0 50.8 76.2
119 34.3 24.1 36.1

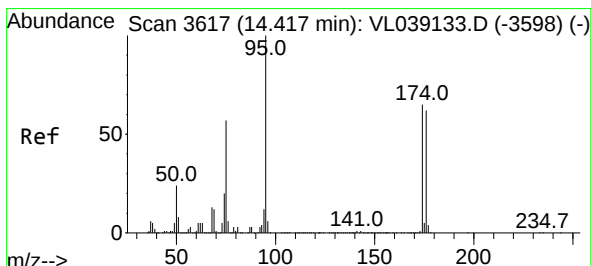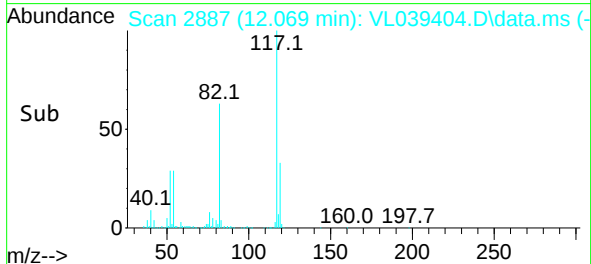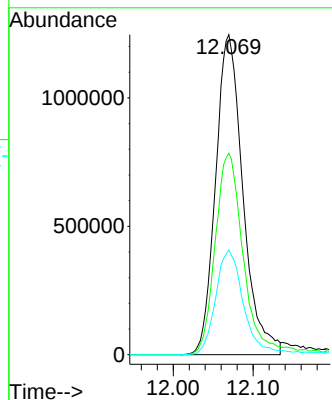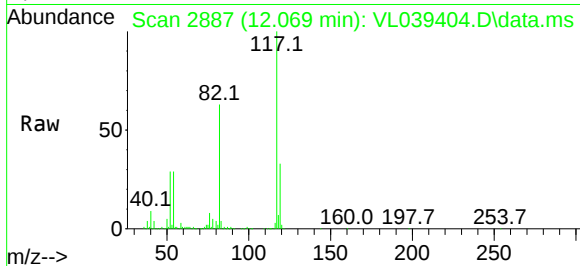

#68
1-Bromo-4-Fluorobenzene
Concen: 10.194 ppbv
RT: 14.401 min Scan# 3612
Delta R.T. 0.010 min
Lab File: VL039404.D
Acq: 29 Jun 2022 20:17

Tgt Ion: 95 Resp: 2238226
Ion Ratio Lower Upper
95 100
174 70.5 55.9 83.9
175 5.3 4.2 6.4

