


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062922\
 Data File : VL039393.D
 Acq On : 29 Jun 2022 11:07
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

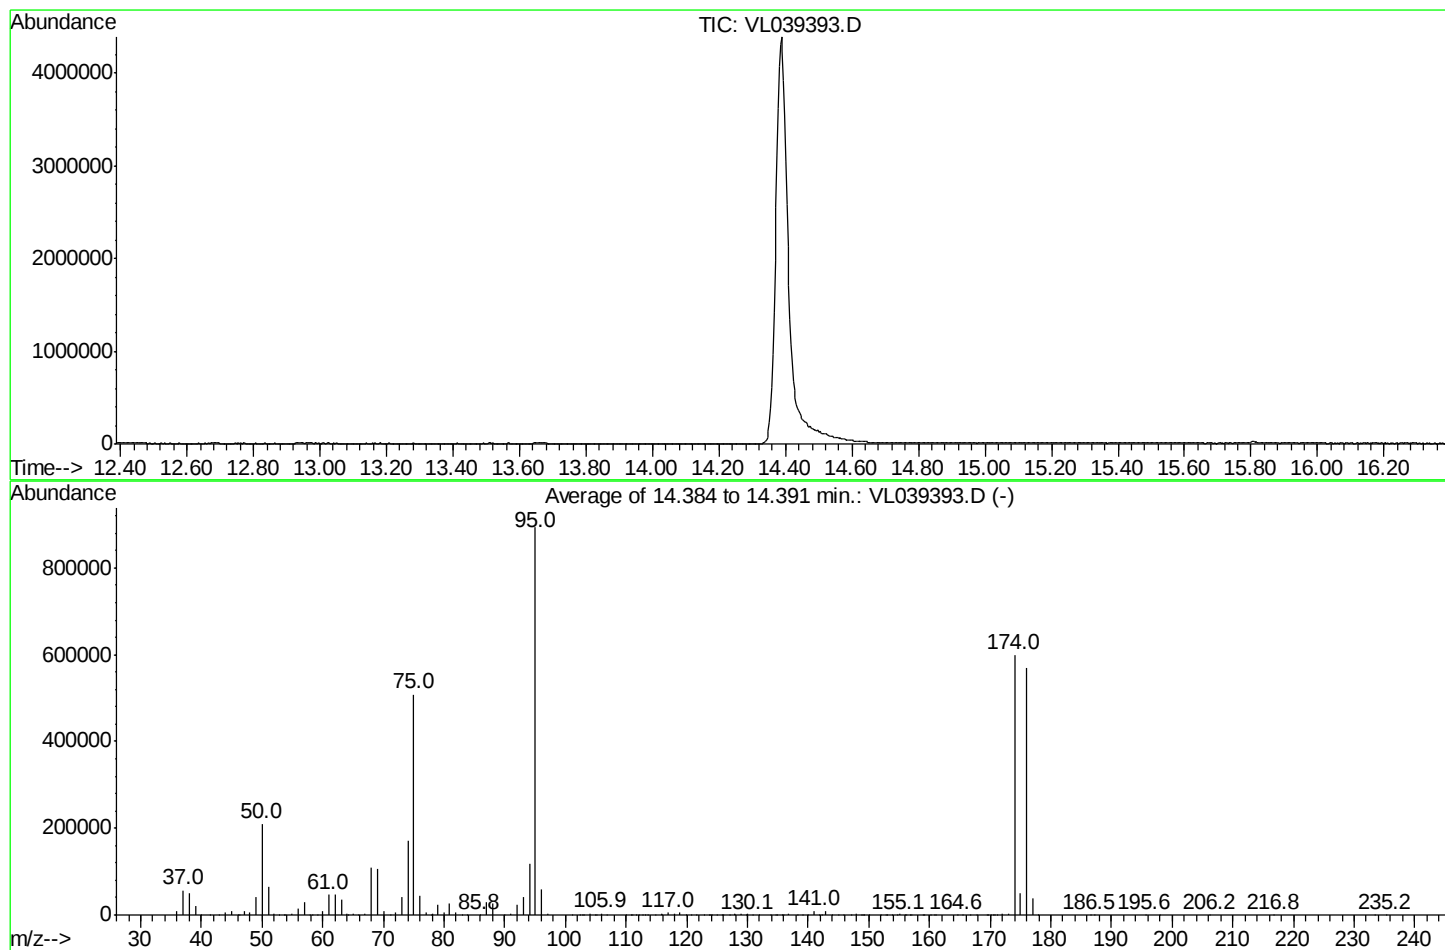

AutoFind: Scans 3607, 3608, 3609; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	210752	PASS
75	95	30	66	56.8	507776	PASS
95	95	100	100	100.0	893461	PASS
96	95	5	9	6.7	60285	PASS
173	174	0.00	2	0.3	1913	PASS
174	95	50	120	67.0	598976	PASS
175	174	4	9	8.1	48792	PASS
176	174	93	101	95.1	569472	PASS
177	176	5	9	6.7	37984	PASS