


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL063020\
 Data File : VL035120.D
 Acq On : 30 Jun 2020 8:57
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL061920AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Sat Jun 20 02:10:36 2020
 Last Update : Sat Jun 20 02:10:36 2020

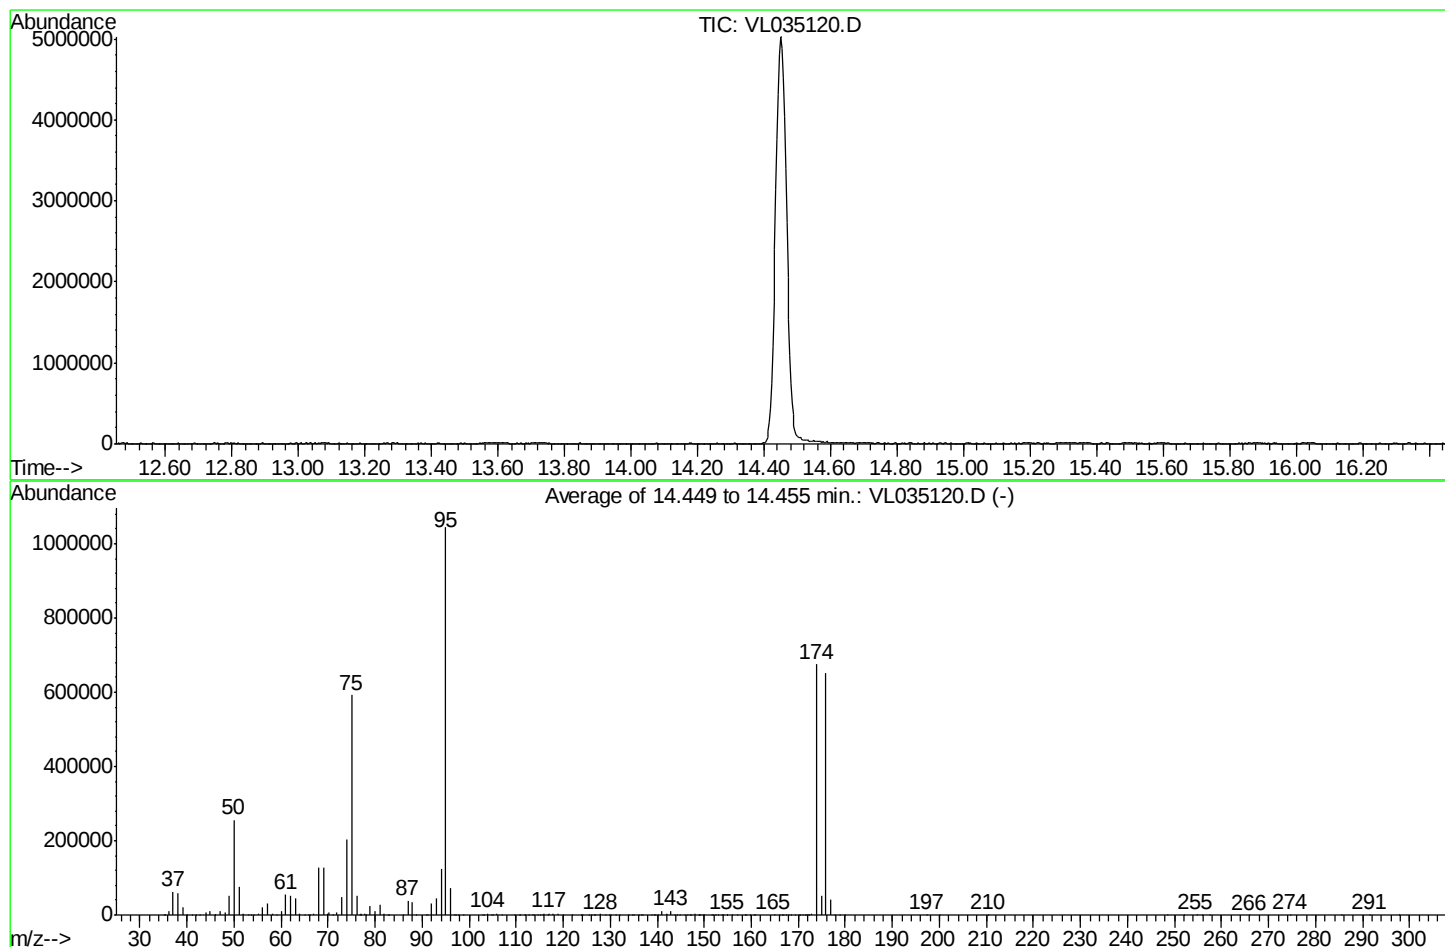

AutoFind: Scans 3627, 3628, 3629; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.5	256128	PASS
75	95	30	66	56.8	592896	PASS
95	95	100	100	100.0	1044266	PASS
96	95	5	9	6.9	72344	PASS
173	174	0.00	2	0.3	2339	PASS
174	95	50	120	64.6	674304	PASS
175	174	4	9	7.7	51720	PASS
176	174	93	101	96.5	650368	PASS
177	176	5	9	6.6	43248	PASS